

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100920\
 Data File : PD059605.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2020 16:24
 Operator : DD\AJ
 Sample : L4330-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 S-2

Manual Integrations
 APPROVED

Ankita

10/13/2020 9:43:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 18:12:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.508	4.024	20568805	30032213	14.266m	13.814
28)	SA Decachlor...	8.313	9.108	12869556	17531295	11.585	10.880m
Target Compounds							
12)	B 4,4'-DDE	5.698	6.365	3779455	4324690	2.229	1.821m
17)	MA 4,4'-DDT	6.460	7.156	8154606	8376041	5.350m	4.273m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100920\
Data File : PD059605.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2020 16:24
Operator : DD\AJ
Sample : L4330-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
S-2



Manual Integrations
APPROVED


Ankita

10/13/2020 9:43:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 18:12:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

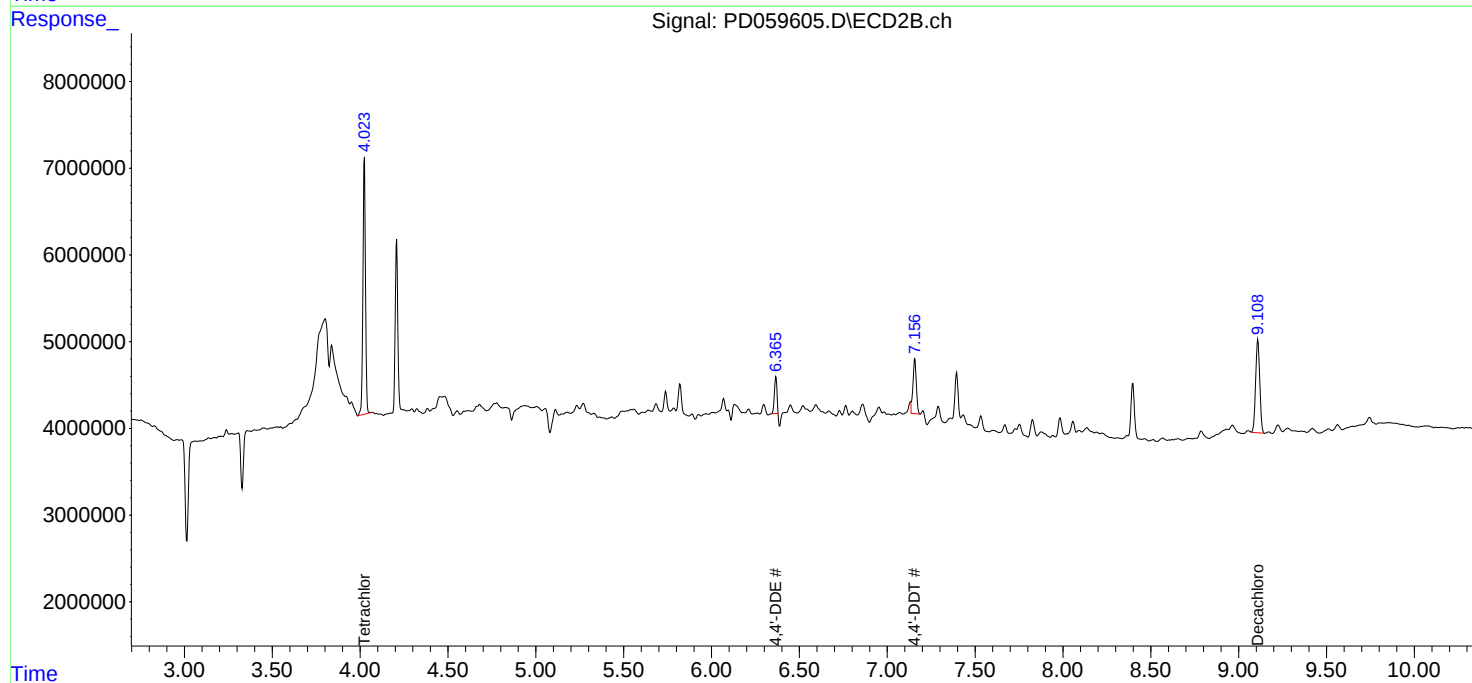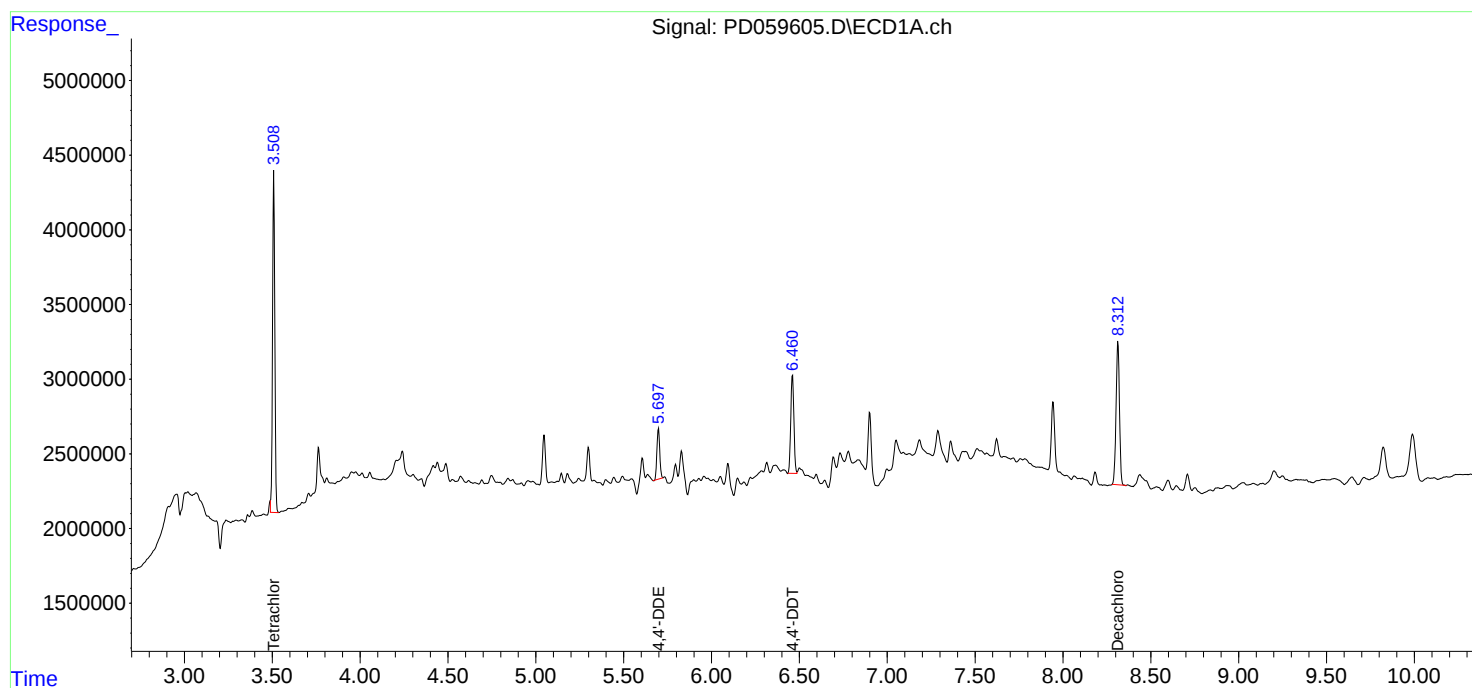

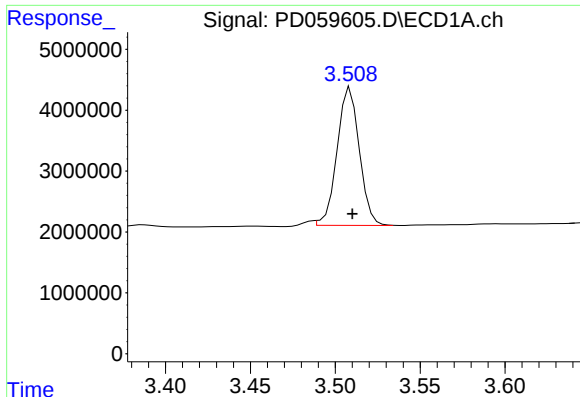

#1 Tetrachloro-m-xylene


R.T.: 3.508 min
Delta R.T.: -0.002 min
Response: 20568805
Conc: 14.27 ng/ml m

Instrument :
ECD_D
ClientSampleId :
S-2

Manual Integrations
APPROVED


Ankita

10/13/2020 9:43:56 AM

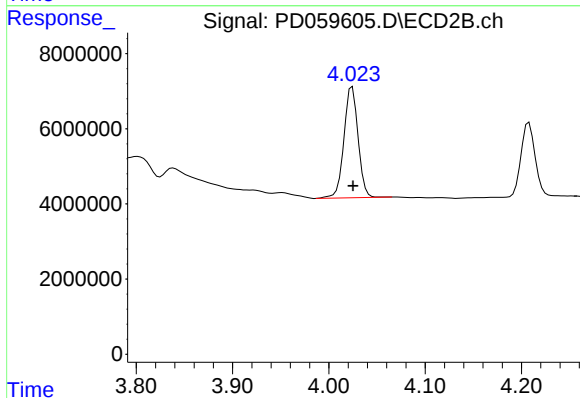


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 30032213
Conc: 13.81 ng/ml

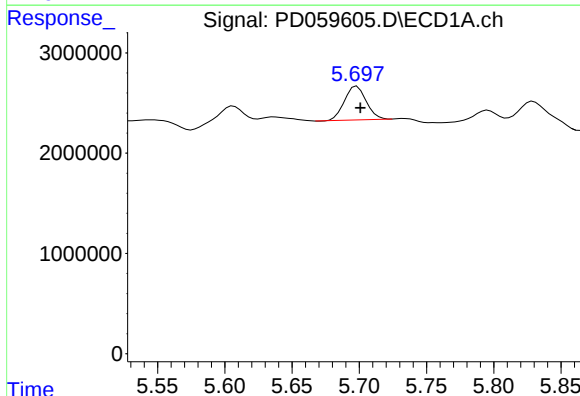


#12 4,4'-DDE

R.T.: 5.698 min
Delta R.T.: -0.003 min
Response: 3779455
Conc: 2.23 ng/ml

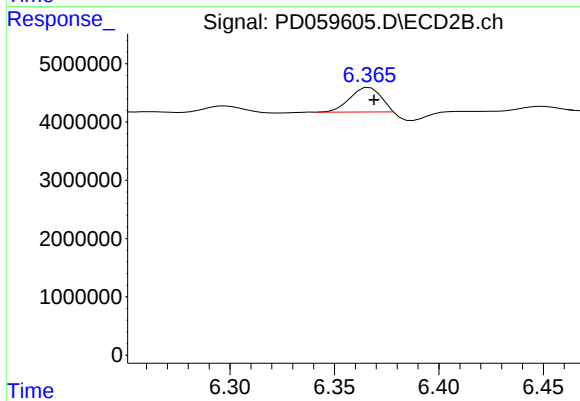

#12 4,4'-DDE

R.T.: 6.365 min
Delta R.T.: -0.003 min
Response: 4324690
Conc: 1.82 ng/ml m

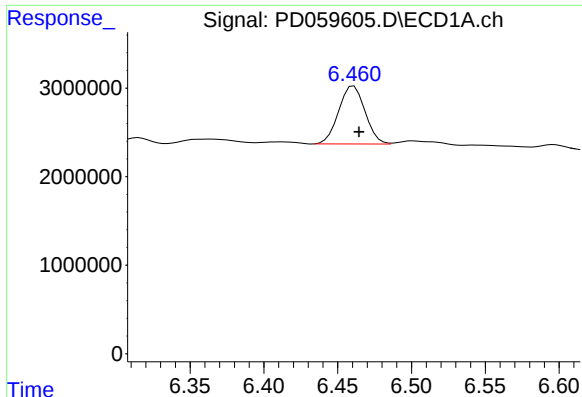

#17 4,4'-DDT


R.T.: 6.460 min
Delta R.T.: -0.005 min
Response: 8154606
Conc: 5.35 ng/ml m

Instrument :
ECD_D
ClientSampleId :
S-2

Manual Integrations
APPROVED


Ankita

10/13/2020 9:43:56 AM

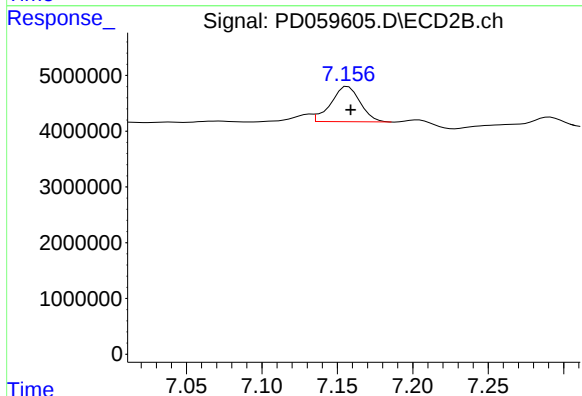


#17 4,4'-DDT

R.T.: 7.156 min
Delta R.T.: -0.003 min
Response: 8376041
Conc: 4.27 ng/ml m

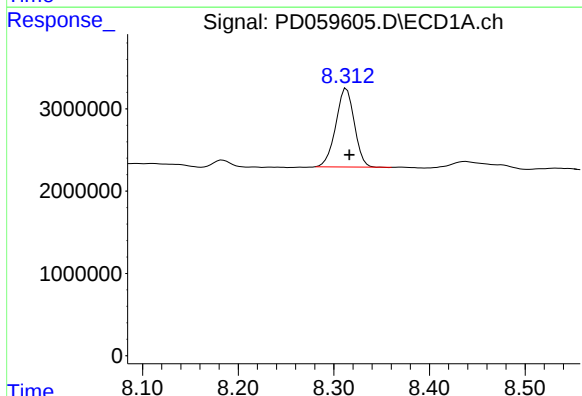

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: -0.003 min
Response: 12869556
Conc: 11.59 ng/ml

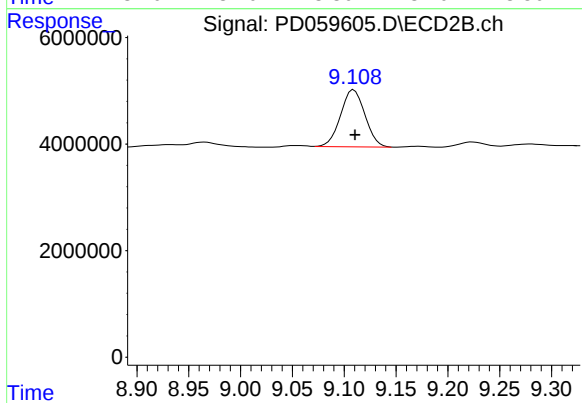

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: -0.003 min
Response: 17531295
Conc: 10.88 ng/ml m