

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078760.D
Acq On : 09 Oct 2023 20:47
Operator : AR\AJ
Sample : RESC009
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Title : GC Extractables
Last Update : Wed Oct 11 01:02:10 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.570	4.027	100.00%
4.027	4.361	100.00%
4.361	4.553	100.00%
4.553	4.803	100.00%
4.803	4.954	100.00%
4.954	5.298	100.00%
5.298	5.725	100.00%
5.725	5.980	100.00%
5.980	6.060	100.00%
6.060	6.111	96.91%
6.111	6.231	100.00%
6.231	6.387	100.00%
6.387	6.617	100.00%
6.617	6.748	100.00%
6.748	6.835	100.00%
6.835	6.965	100.00%
6.965	7.064	100.00%
7.064	7.199	100.00%
7.199	7.538	100.00%
7.538	7.686	100.00%
7.686	9.120	100.00%


Signal #2

2.807	3.311	100.00%
3.311	3.642	100.00%
3.642	3.937	100.00%
3.937	3.986	100.00%
3.986	4.168	100.00%
4.168	4.268	100.00%
4.268	4.770	100.00%
4.770	5.021	100.00%
5.021	5.086	99.62%
5.086	5.141	99.16%
5.141	5.275	100.00%
5.275	5.407	100.00%
5.407	5.682	100.00%
5.682	5.829	100.00%
5.829	5.974	100.00%
5.974	6.081	100.00%
6.081	6.154	100.00%
6.154	6.376	100.00%
6.376	6.658	100.00%
6.658	6.882	100.00%
6.882	7.964	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 20:47
Operator : AR\AJ
Sample : RESC009
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:04:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 01:02:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

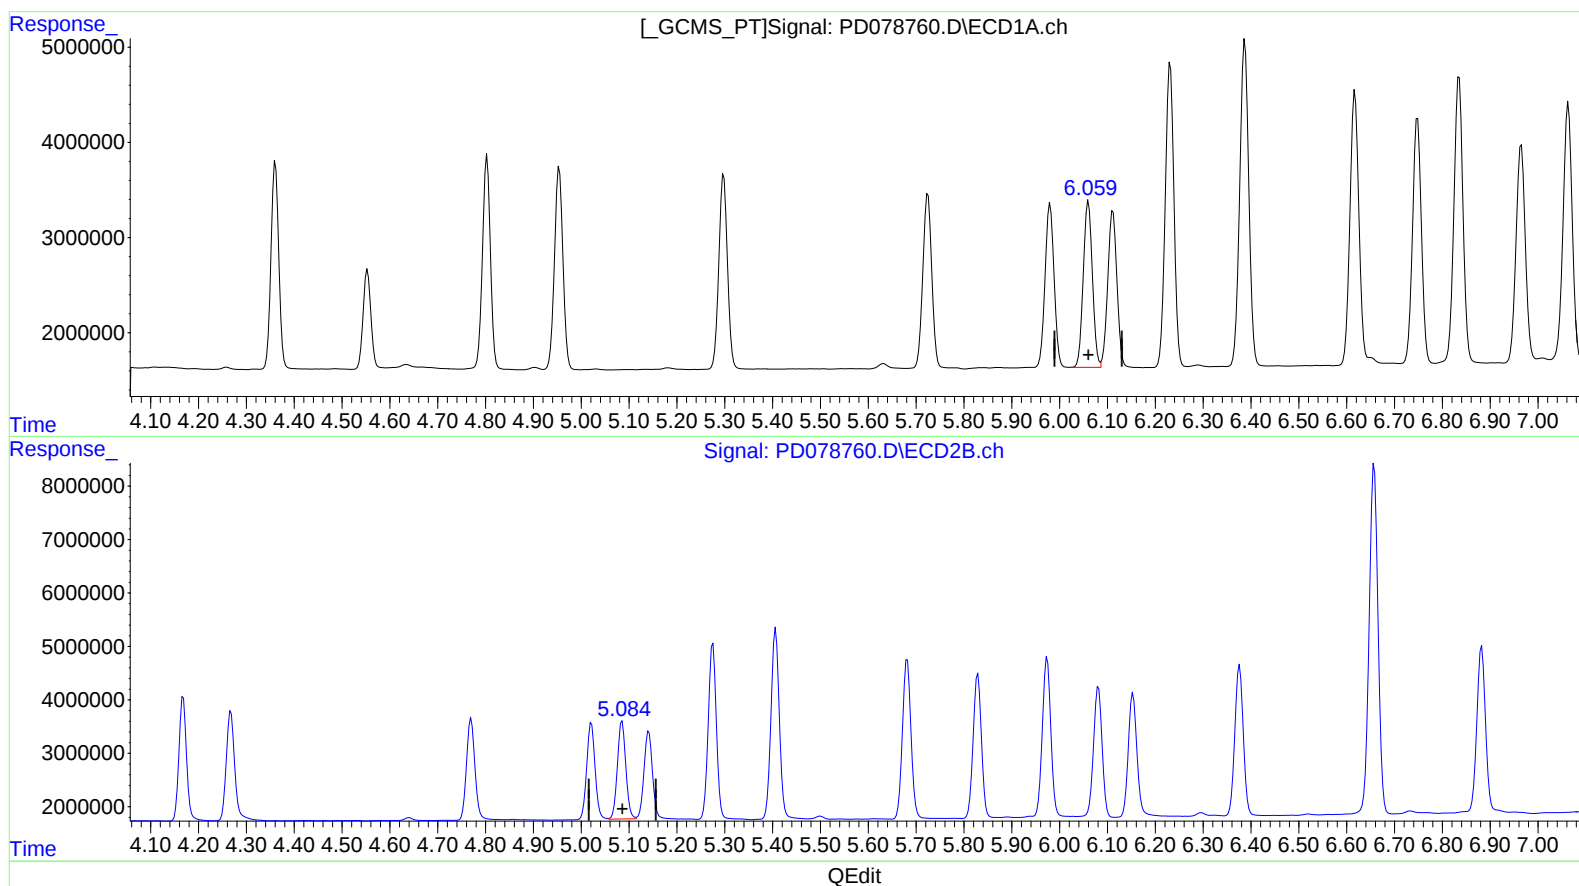

(11) cis-Chlordane (B)

6.060min 10.073 ng/ml

response 23163045

(11) cis-Chlordane #2 (B)


5.086min 9.985 ng/ml

response 22291616

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 20:47
Operator : AR\AJ
Sample : RESC009
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:04:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 01:02:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

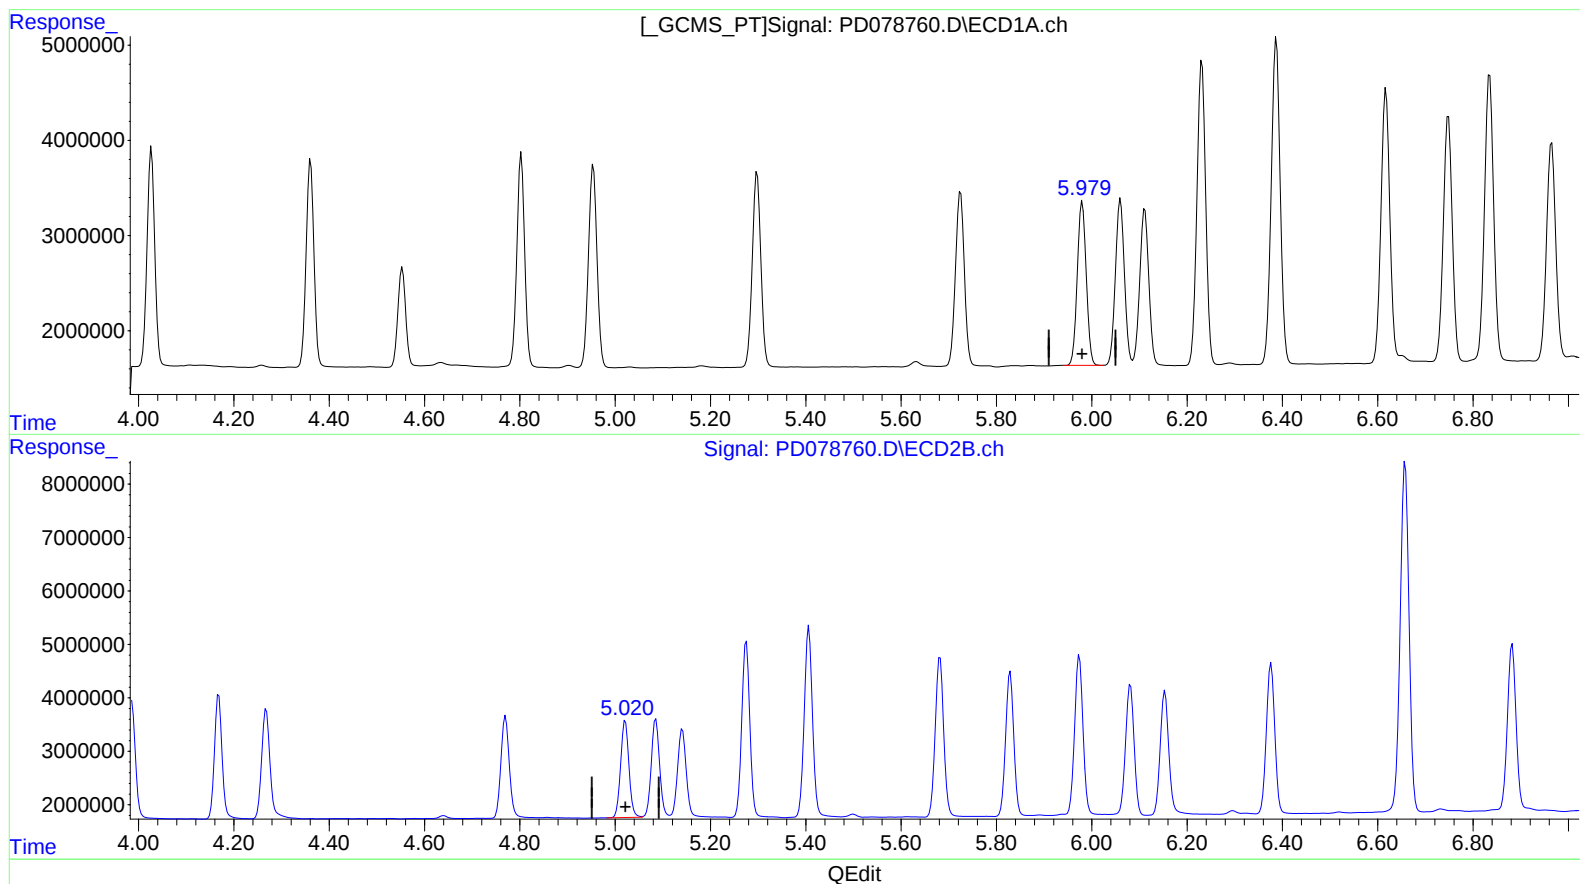

(10) trans-Chlordane (B)

5.980min 9.988 ng/ml

response 22500640

(10) trans-Chlordane #2 (B)


5.021min 10.002 ng/ml

response 21892032

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 20:47
Operator : AR\AJ
Sample : RESC009
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:04:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 01:02:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

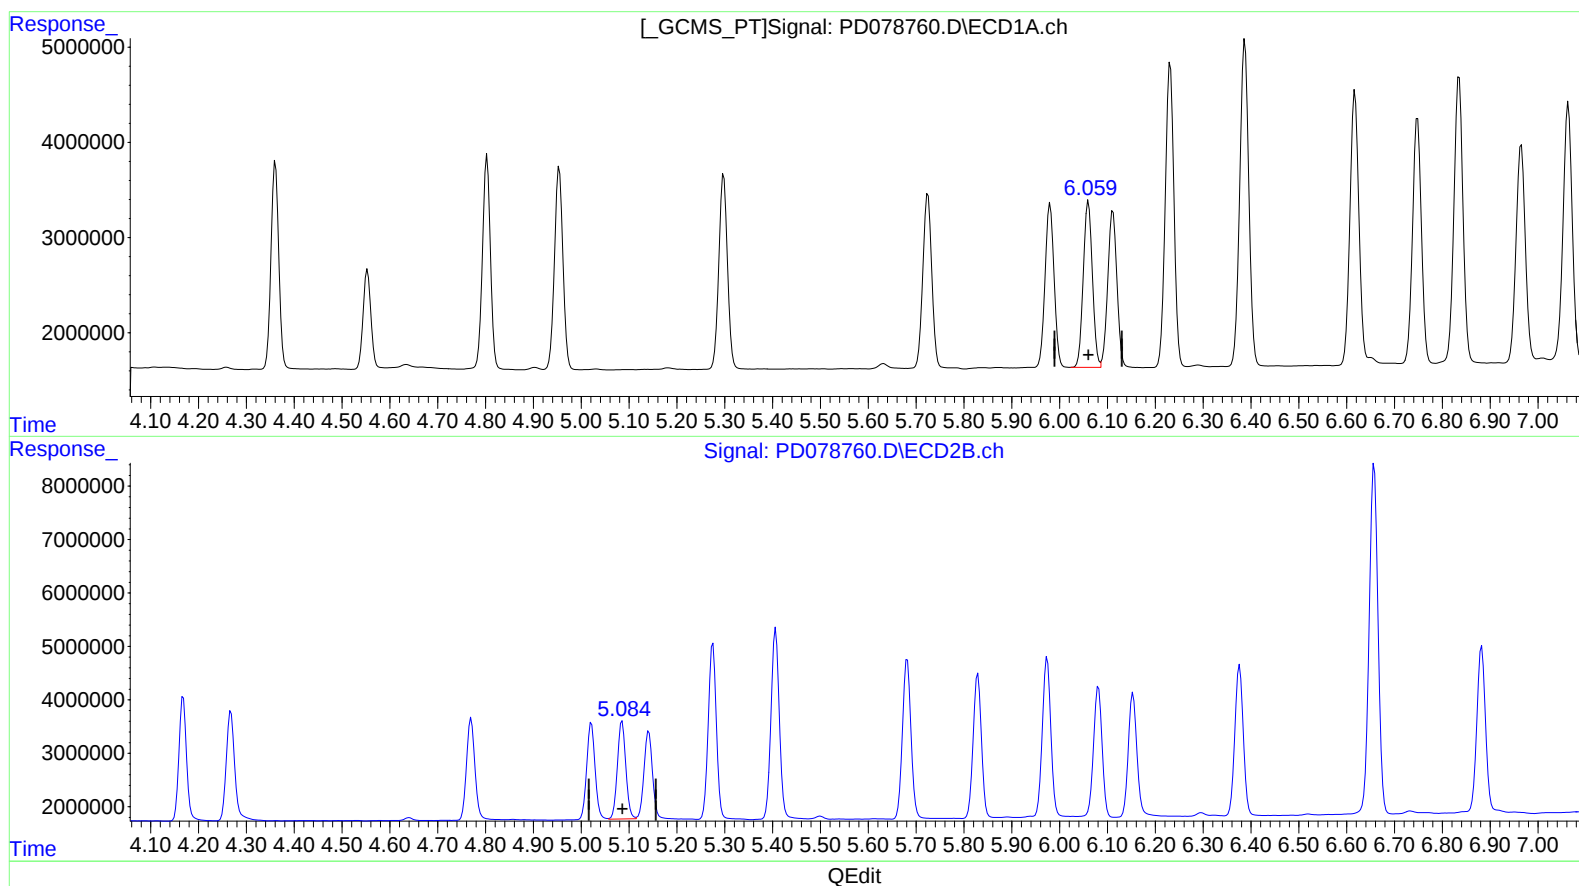

(11) cis-Chlordane (B)

6.060min 10.073 ng/ml

response 23163045

(11) cis-Chlordane #2 (B)

5.086min 9.985 ng/ml

response 22291616