

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
 Data File : PD078767.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2023 22:21
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:59:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 10 01:58:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.807	8219896	10560728	5.238	5.238
27)	SA Decachlor...	9.120	7.964	20476883	16166034	11.096	10.927
Target Compounds							
2)	A alpha-BHC	4.027	3.311	12694863	14394798	4.847	4.798
3)	MA gamma-BHC...	4.361	3.642	12420421	13374790	4.970	4.927
4)	MA Heptachlor	4.954	3.986	13555290	12695854	5.193	5.092
9)	A Endosulfan I	6.111	5.141	11803536	9941725	5.542	4.971
13)	MA Dieldrin	6.387	5.406	23044138	24186135	10.199	11.065
14)	MA Endrin	6.617	5.681	19177415	18527571	10.583	10.263
16)	A 4,4'-DDD	6.748	5.829	16957282	15771303	10.098	10.016
17)	MA 4,4'-DDT	7.063	6.081	18163659	14920529	10.282	10.037
20)	A Methoxychlor	7.537	6.657	49610093	43253345	53.019	53.939


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078767.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 22:21
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:59:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 10 01:58:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

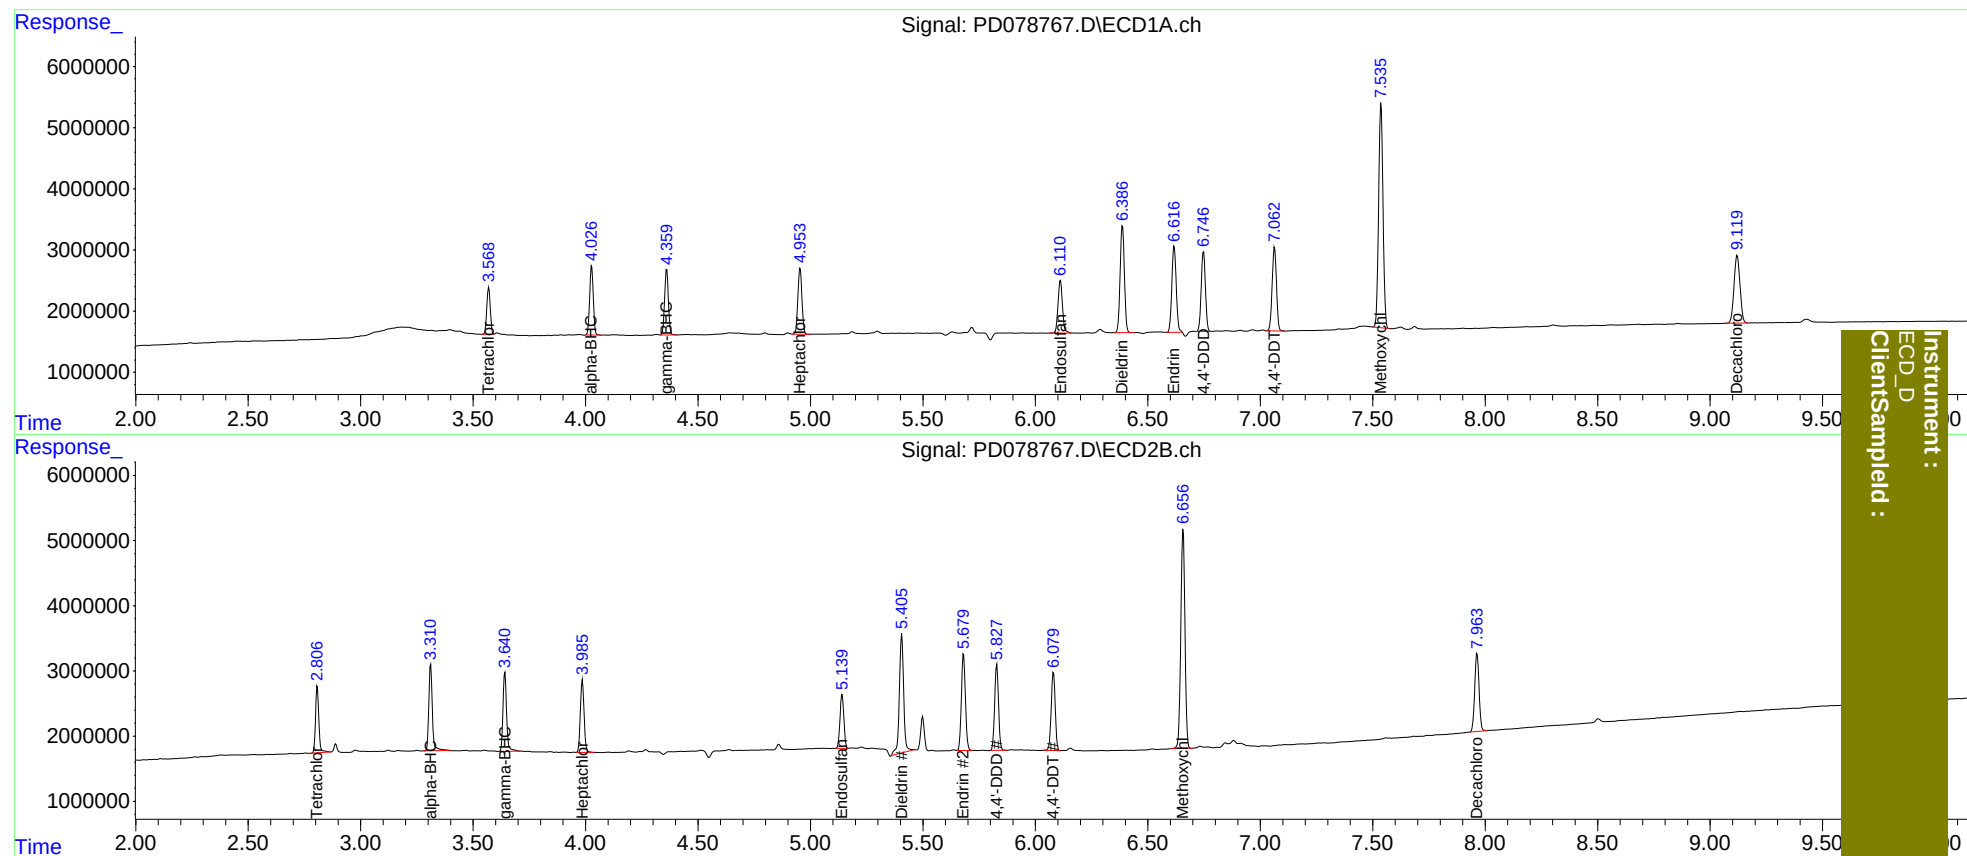


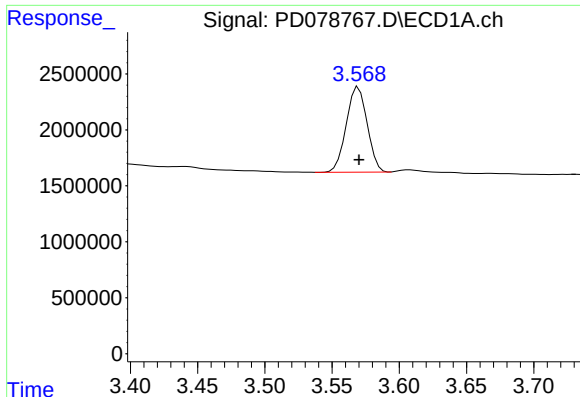

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 8219896
Conc: 5.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

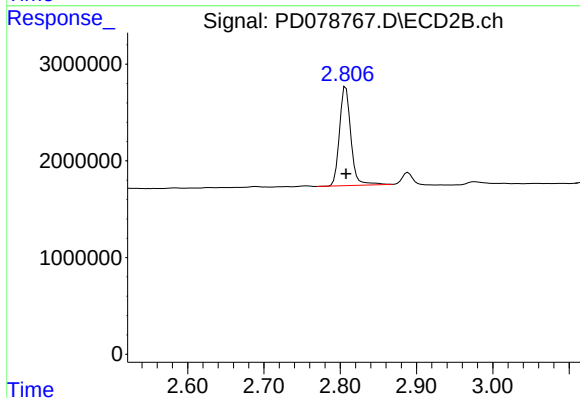


#1 Tetrachloro-m-xylene

R.T.: 2.807 min
Delta R.T.: 0.000 min
Response: 10560728
Conc: 5.24 ng/ml

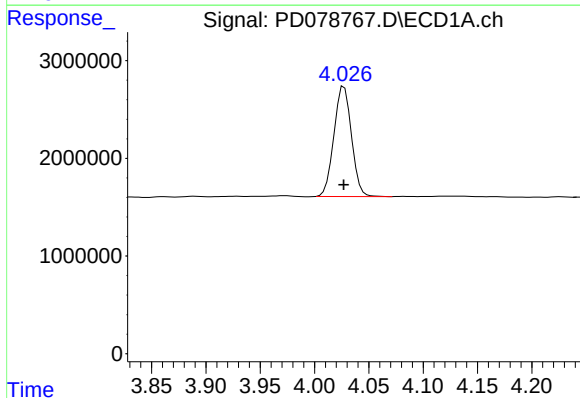


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 12694863
Conc: 4.85 ng/ml

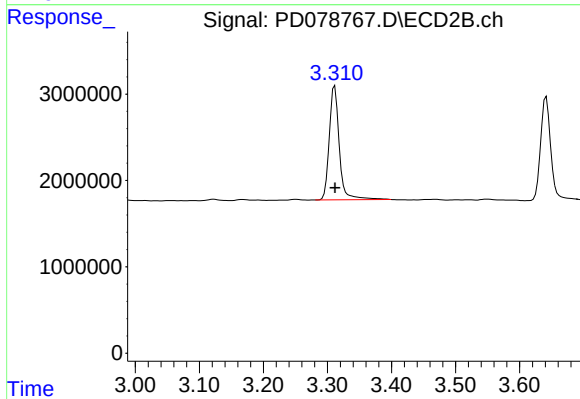

#2 alpha-BHC


R.T.: 3.311 min
Delta R.T.: 0.000 min
Response: 14394798
Conc: 4.80 ng/ml

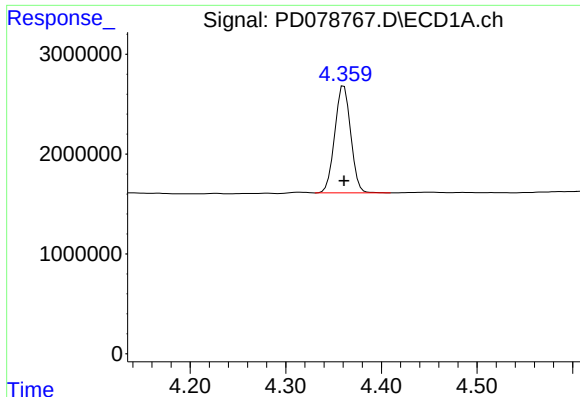

#3 gamma-BHC (Lindane)


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 12420421
Conc: 4.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

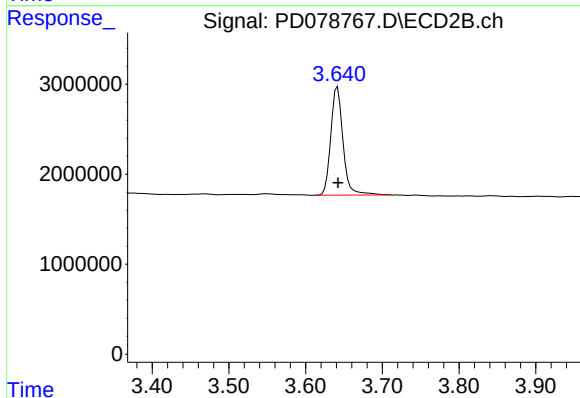


#3 gamma-BHC (Lindane)

R.T.: 3.642 min
Delta R.T.: 0.000 min
Response: 13374790
Conc: 4.93 ng/ml

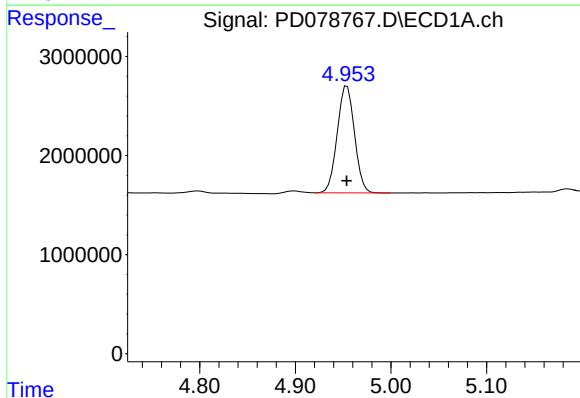


#4 Heptachlor

R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 13555290
Conc: 5.19 ng/ml

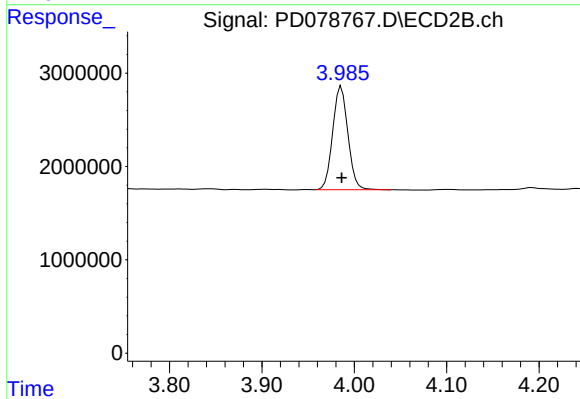

#4 Heptachlor


R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 12695854
Conc: 5.09 ng/ml

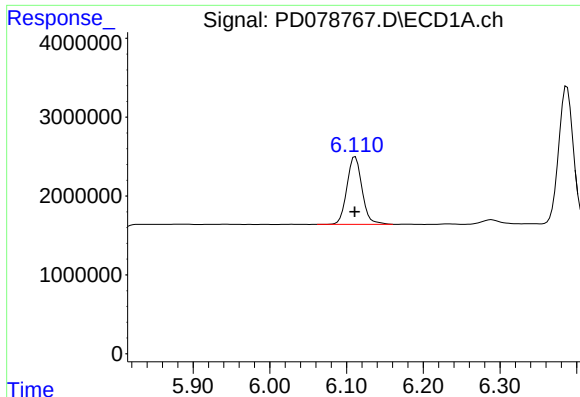

#9 Endosulfan I


R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 11803536
Conc: 5.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

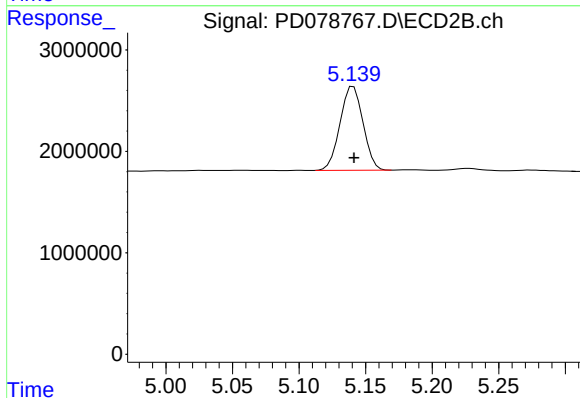


#9 Endosulfan I

R.T.: 5.141 min
Delta R.T.: 0.000 min
Response: 9941725
Conc: 4.97 ng/ml

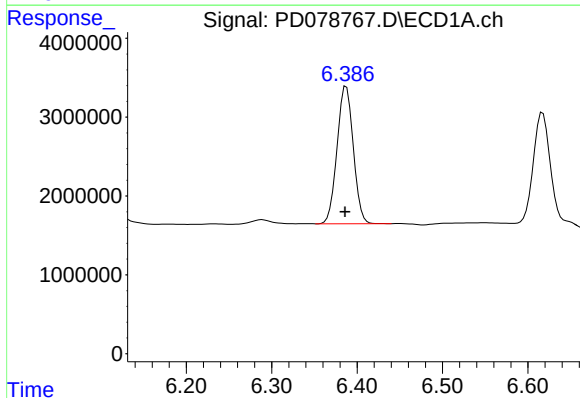


#13 Dieldrin

R.T.: 6.387 min
Delta R.T.: 0.001 min
Response: 23044138
Conc: 10.20 ng/ml

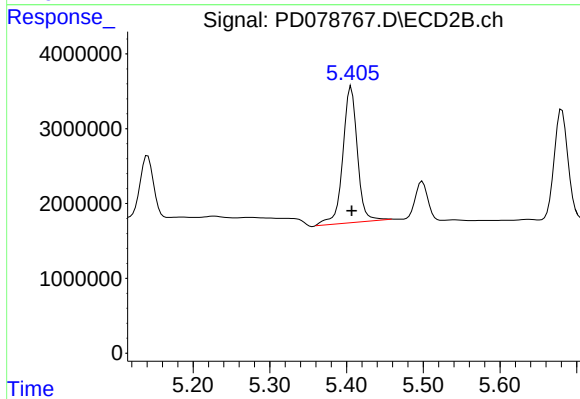

#13 Dieldrin


R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 24186135
Conc: 11.07 ng/ml

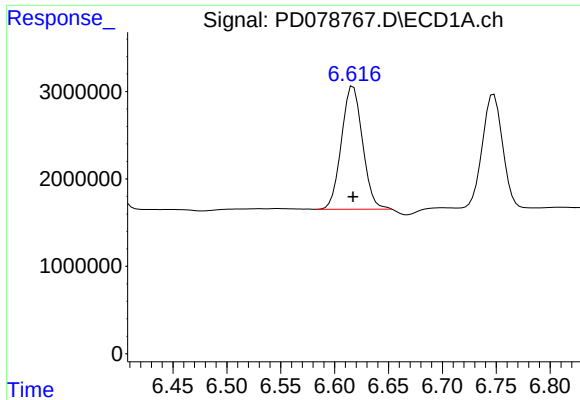

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 19177415
Conc: 10.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

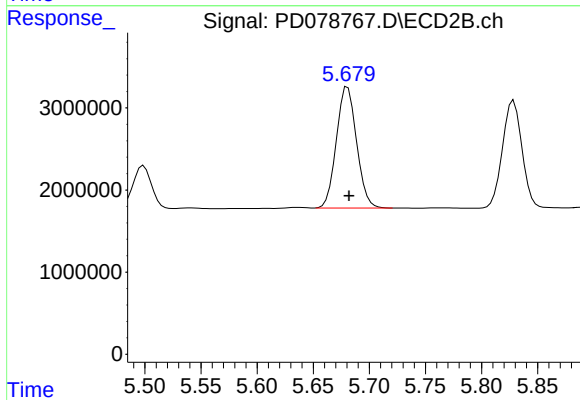


#14 Endrin

R.T.: 5.681 min
Delta R.T.: -0.001 min
Response: 18527571
Conc: 10.26 ng/ml

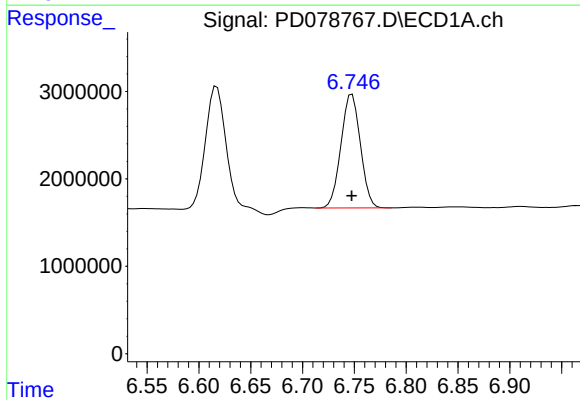


#16 4,4'-DDD

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 16957282
Conc: 10.10 ng/ml

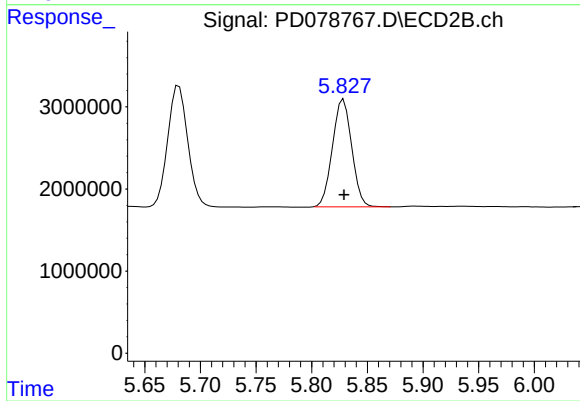

#16 4,4'-DDD


R.T.: 5.829 min
Delta R.T.: 0.000 min
Response: 15771303
Conc: 10.02 ng/ml

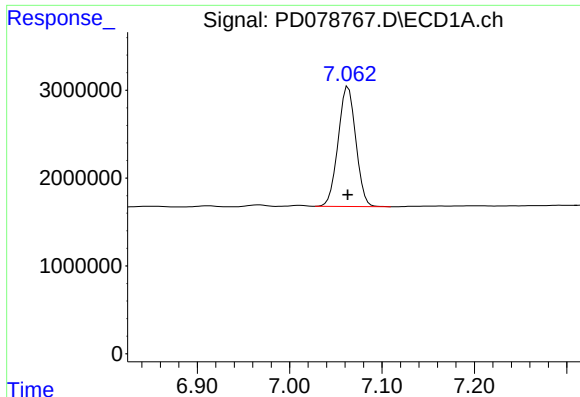

#17 4,4'-DDT


R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 18163659
Conc: 10.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

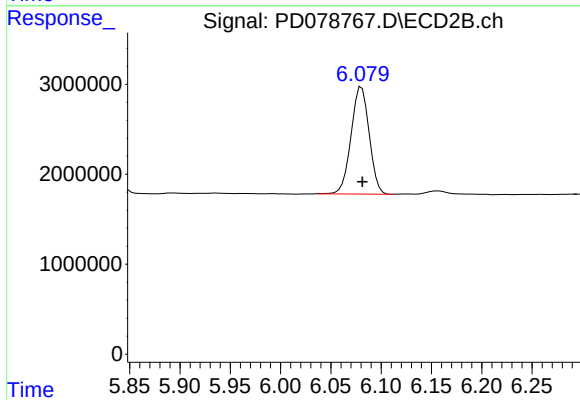


#17 4,4'-DDT

R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 14920529
Conc: 10.04 ng/ml

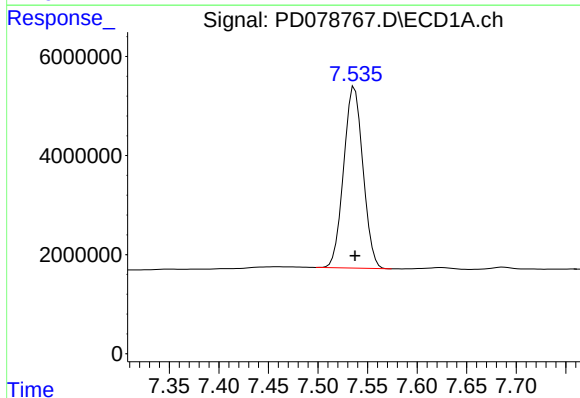


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 49610093
Conc: 53.02 ng/ml

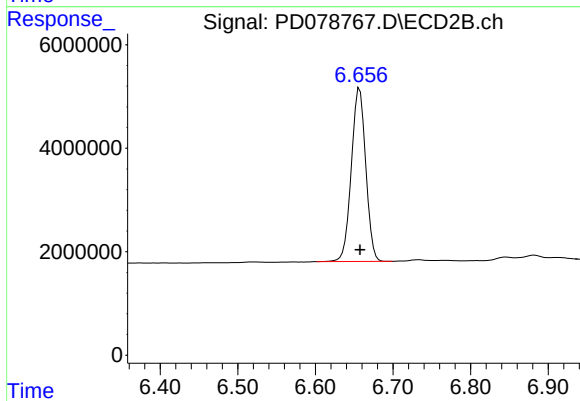

#20 Methoxychlor


R.T.: 6.657 min
Delta R.T.: 0.000 min
Response: 43253345
Conc: 53.94 ng/ml

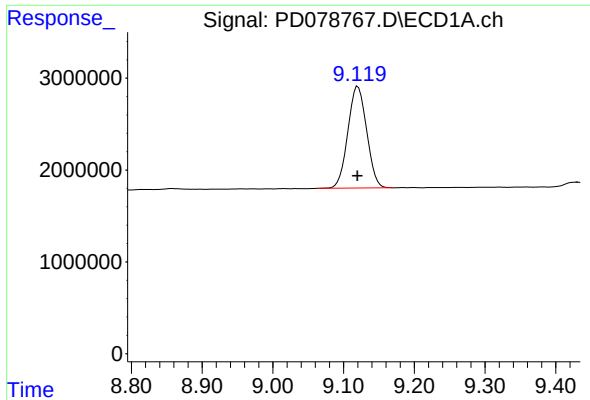

#27 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 20476883
Conc: 11.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

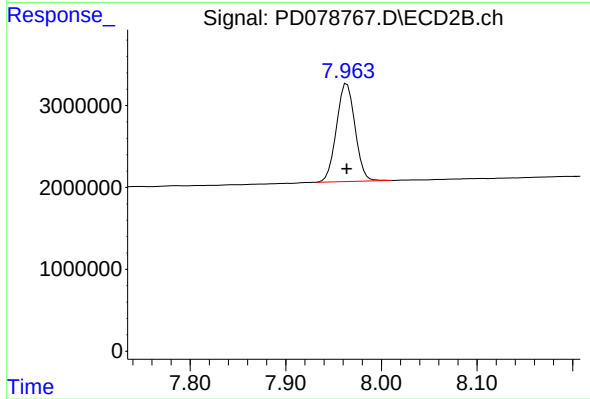

#27 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 16166034
Conc: 10.93 ng/ml