

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
 Data File : PD078769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2023 22:48
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:59:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 10 01:58:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.807	16231304	20862057	10.344	10.347
27)	SA Decachlor...	9.120	7.964	39316663	31144106	21.305	21.052
Target Compounds							
2)	A alpha-BHC	4.027	3.311	25754439	29549435	9.834	9.848
3)	MA gamma-BHC...	4.360	3.642	24983499	27380945	9.996	10.086
4)	MA Heptachlor	4.954	3.986	26771501	25286464	10.256	10.142
9)	A Endosulfan I	6.111	5.141	22210905	20504787	10.429	10.252
13)	MA Dieldrin	6.386	5.406	45934184	43928557	20.331	20.098
14)	MA Endrin	6.617	5.681	36862167	36443117	20.343	20.188
16)	A 4,4'-DDD	6.747	5.829	34081529	31841605	20.296	20.221
17)	MA 4,4'-DDT	7.063	6.081	35878728	29948753	20.311	20.146
20)	A Methoxychlor	7.537	6.657	96518365	83870672	103.150	104.590


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 22:48
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:59:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 10 01:58:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

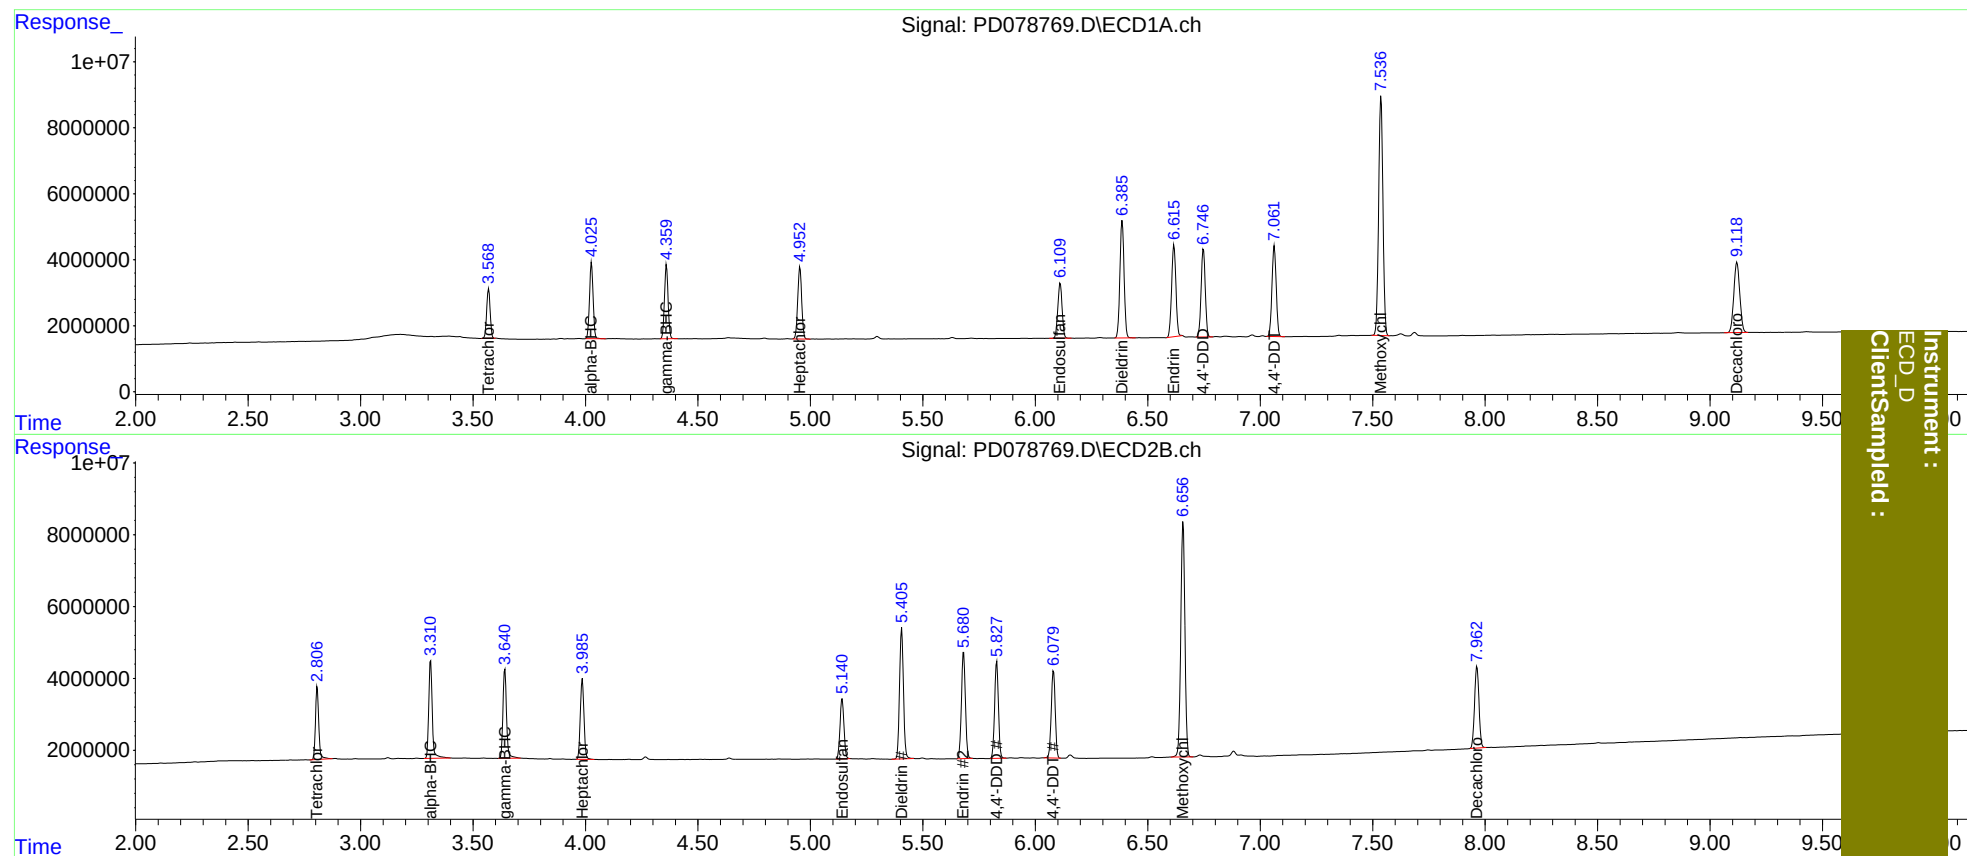


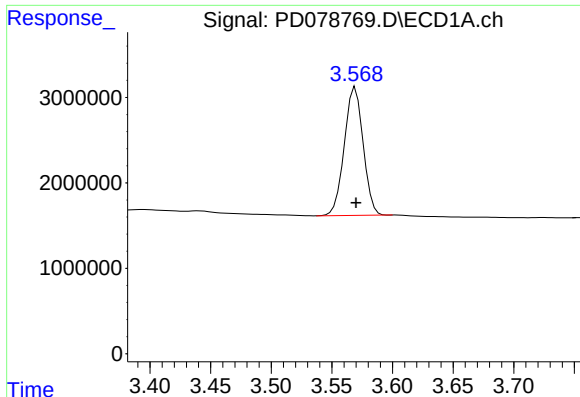

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 16231304
Conc: 10.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

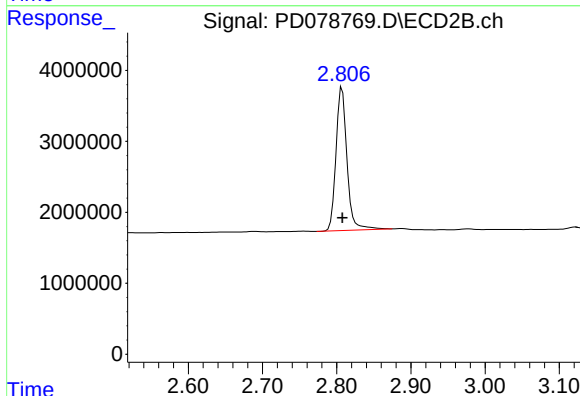


#1 Tetrachloro-m-xylene

R.T.: 2.807 min
Delta R.T.: 0.000 min
Response: 20862057
Conc: 10.35 ng/ml

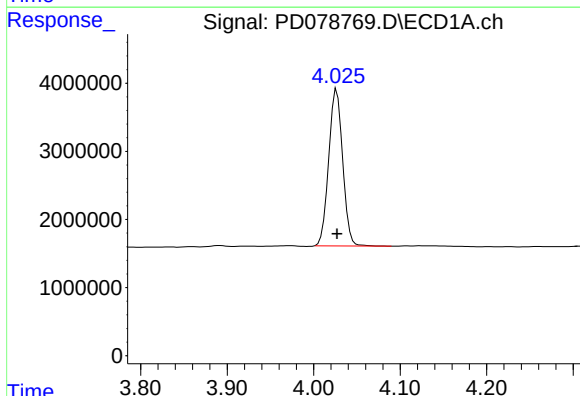


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 25754439
Conc: 9.83 ng/ml

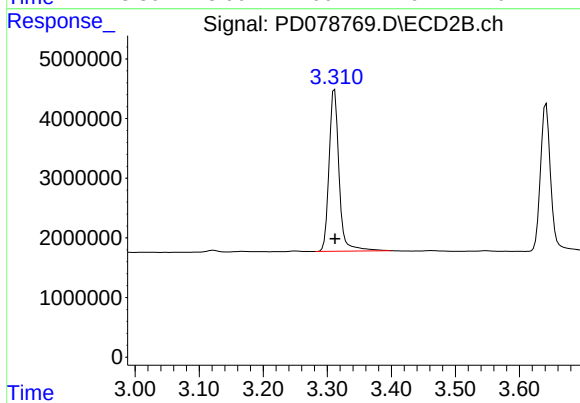

#2 alpha-BHC


R.T.: 3.311 min
Delta R.T.: 0.000 min
Response: 29549435
Conc: 9.85 ng/ml

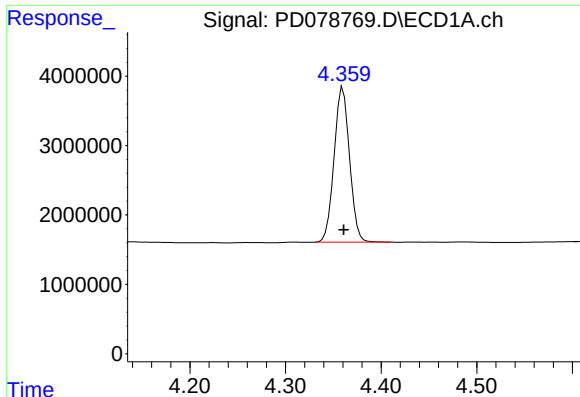

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 24983499
Conc: 10.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

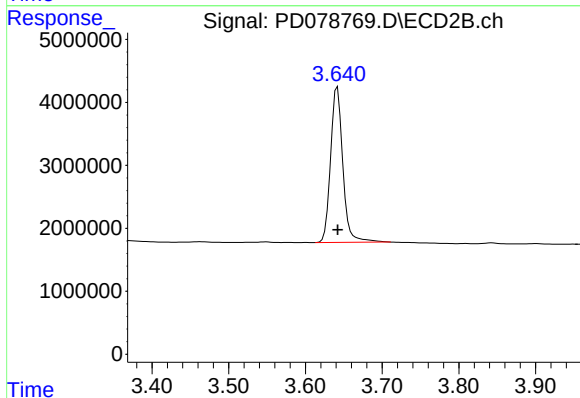


#3 gamma-BHC (Lindane)

R.T.: 3.642 min
Delta R.T.: 0.000 min
Response: 27380945
Conc: 10.09 ng/ml

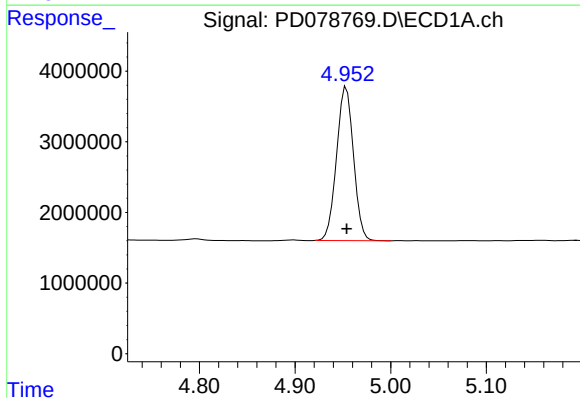


#4 Heptachlor

R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 26771501
Conc: 10.26 ng/ml

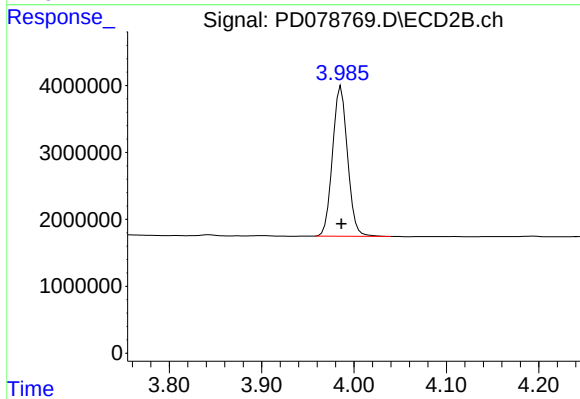

#4 Heptachlor


R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 25286464
Conc: 10.14 ng/ml

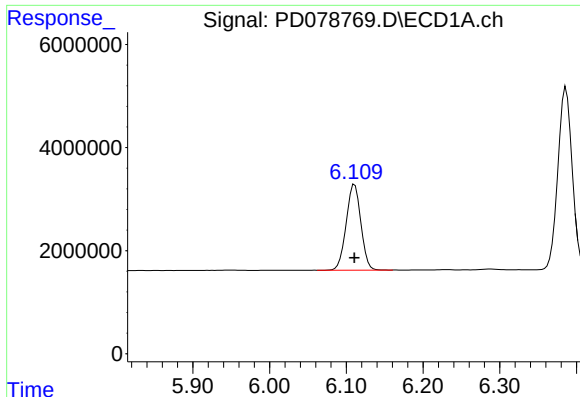

#9 Endosulfan I


R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 22210905
Conc: 10.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

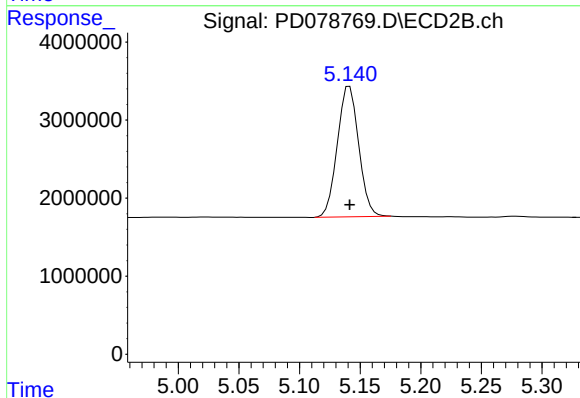


#9 Endosulfan I

R.T.: 5.141 min
Delta R.T.: 0.000 min
Response: 20504787
Conc: 10.25 ng/ml

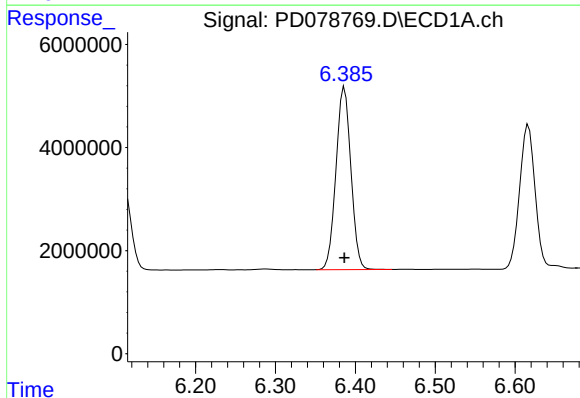


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 45934184
Conc: 20.33 ng/ml

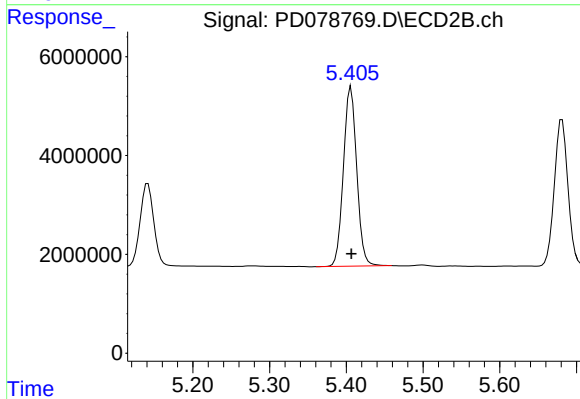

#13 Dieldrin


R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 43928557
Conc: 20.10 ng/ml

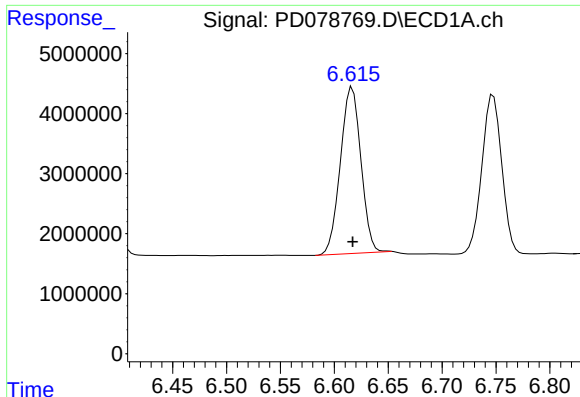

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 36862167
Conc: 20.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

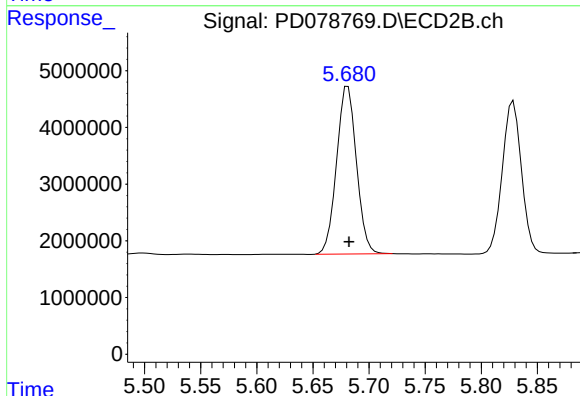


#14 Endrin

R.T.: 5.681 min
Delta R.T.: 0.000 min
Response: 36443117
Conc: 20.19 ng/ml

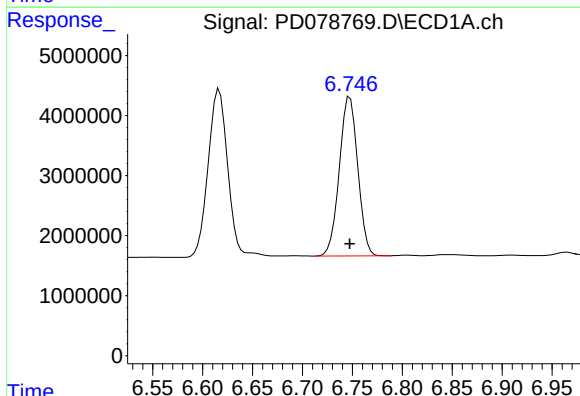


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 34081529
Conc: 20.30 ng/ml

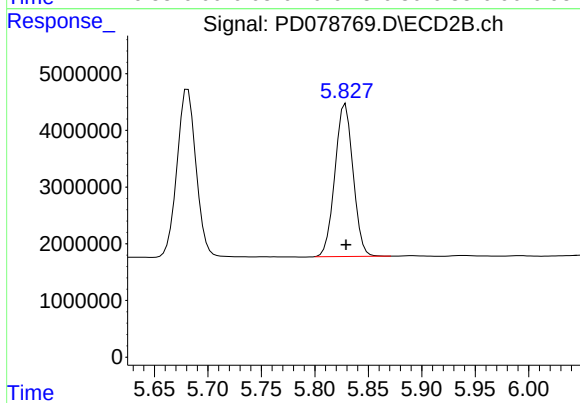

#16 4,4'-DDD


R.T.: 5.829 min
Delta R.T.: 0.000 min
Response: 31841605
Conc: 20.22 ng/ml

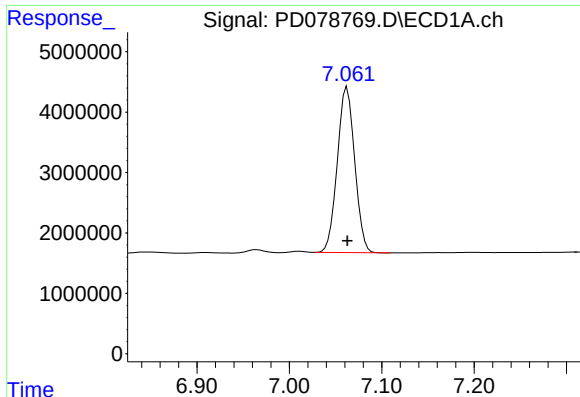

#17 4,4'-DDT


R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 35878728
Conc: 20.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

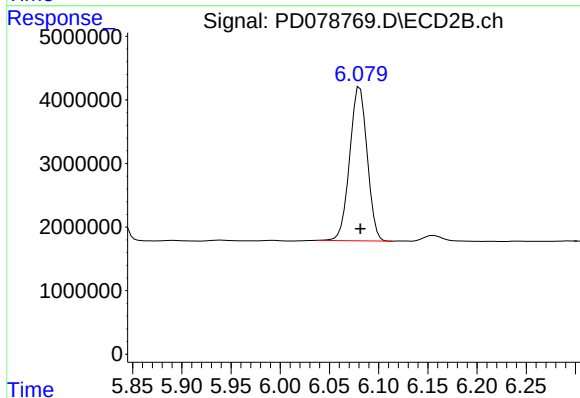


#17 4,4'-DDT

R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 29948753
Conc: 20.15 ng/ml

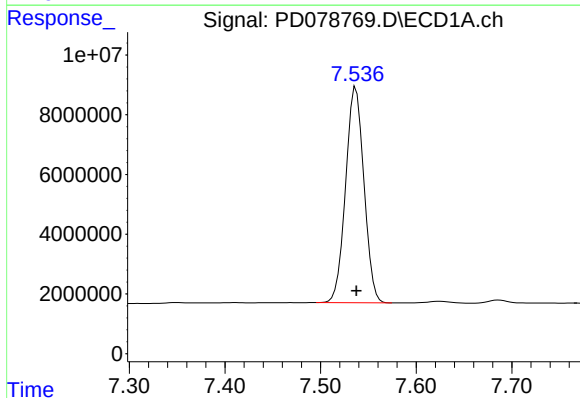


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 96518365
Conc: 103.15 ng/ml

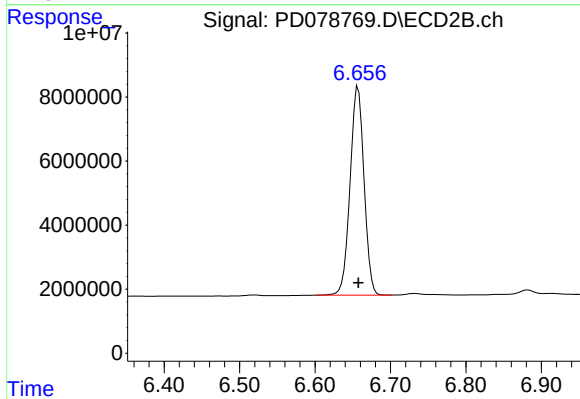

#20 Methoxychlor


R.T.: 6.657 min
Delta R.T.: 0.000 min
Response: 83870672
Conc: 104.59 ng/ml

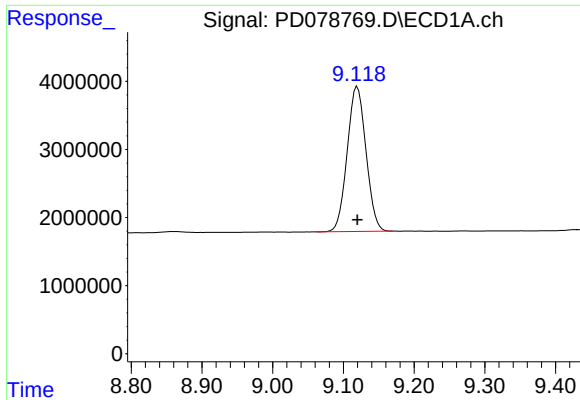

#27 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 39316663
Conc: 21.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

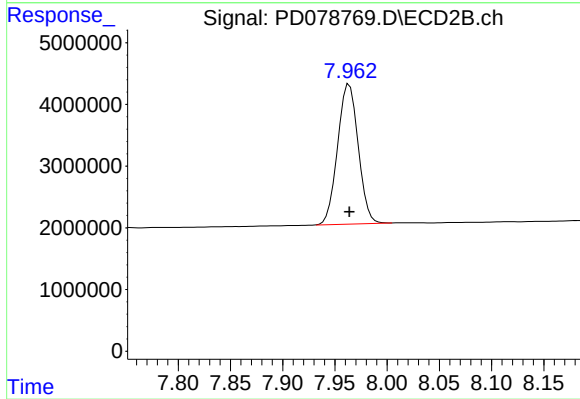

#27 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 31144106
Conc: 21.05 ng/ml