

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
 Data File : PD078771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2023 23:14
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:59:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 10 01:58:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.808	31384021	40323176	20.000	20.000
27)	SA Decachlor...	9.120	7.964	73817689	59176869	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.027	3.312	52380935	60009429	20.000	20.000
3)	MA gamma-BHC...	4.361	3.642	49985504	54294680	20.000	20.000
4)	MA Heptachlor	4.954	3.986	52205512	49862729	20.000	20.000
9)	A Endosulfan I	6.111	5.142	42595942	40001837	20.000	20.000
13)	MA Dieldrin	6.386	5.407	90374725	87430113	40.000	40.000
14)	MA Endrin	6.617	5.682	72481588	72208185	40.000	40.000
16)	A 4,4'-DDD	6.747	5.829	67168945	62986929	40.000	40.000
17)	MA 4,4'-DDT	7.063	6.082	70658841	59463421	40.000	40.000
20)	A Methoxychlor	7.537	6.657	187.1E6	160.4E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 23:14
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:59:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 10 01:58:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

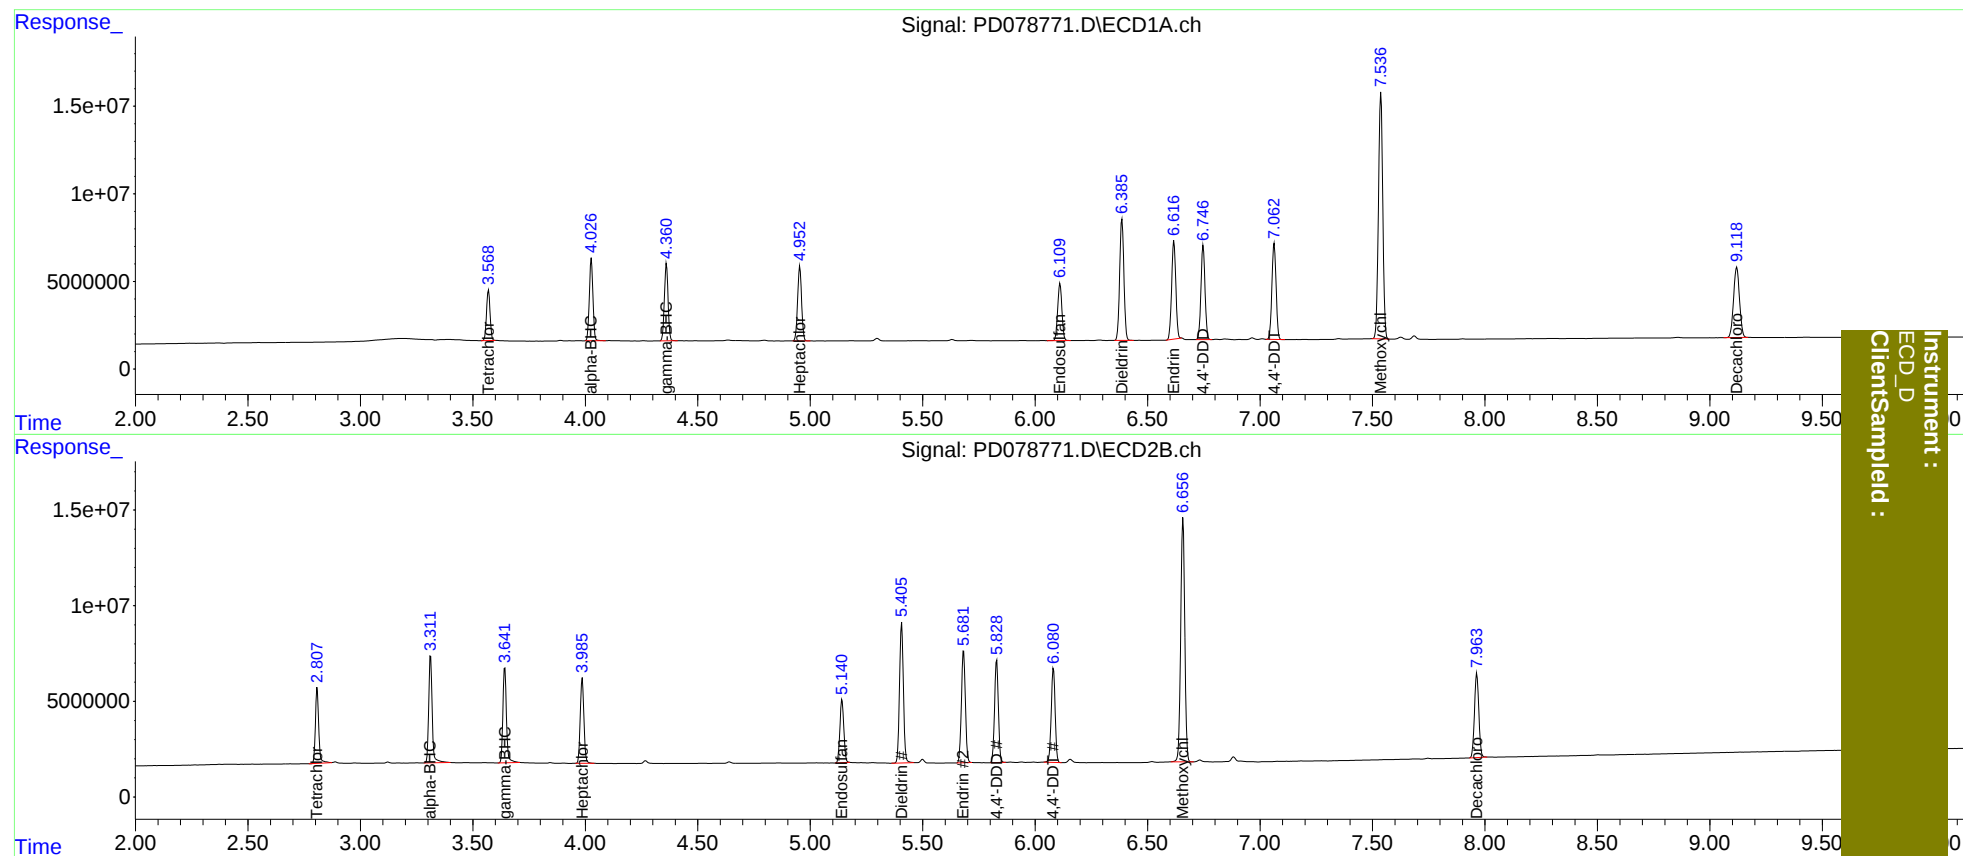


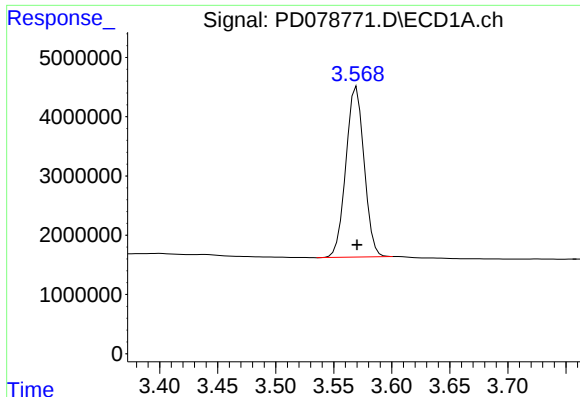

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 31384021
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

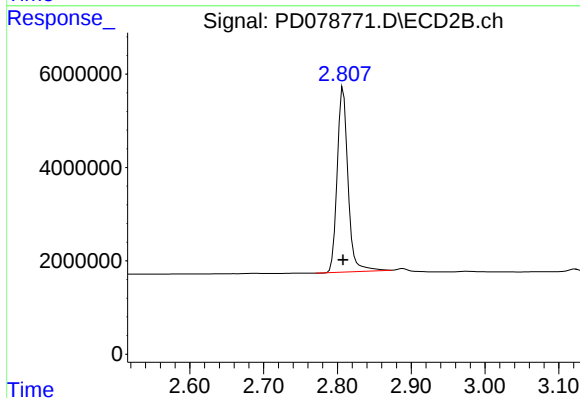


#1 Tetrachloro-m-xylene

R.T.: 2.808 min
Delta R.T.: 0.000 min
Response: 40323176
Conc: 20.00 ng/ml

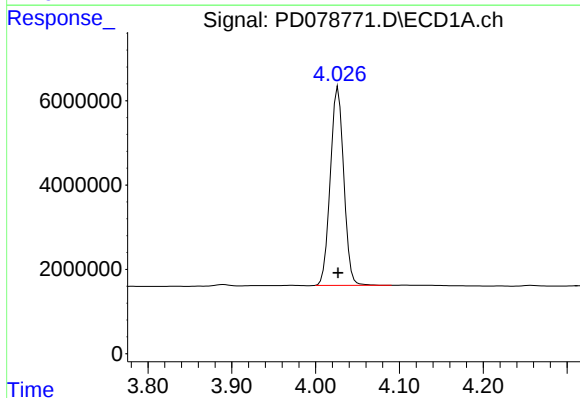


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 52380935
Conc: 20.00 ng/ml

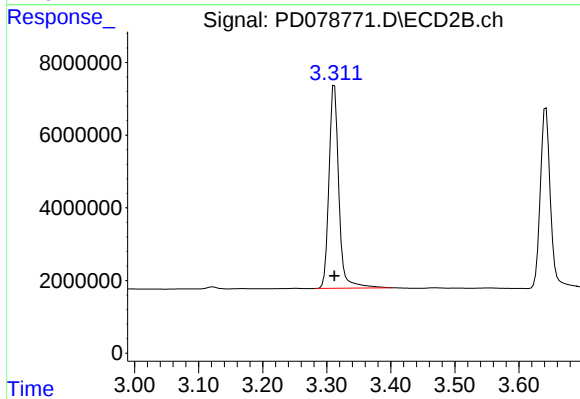

#2 alpha-BHC


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 60009429
Conc: 20.00 ng/ml

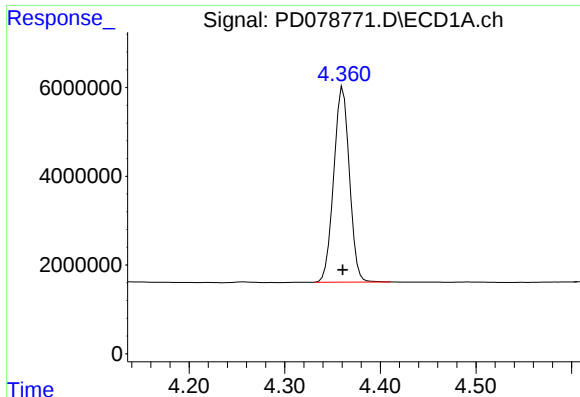

#3 gamma-BHC (Lindane)


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 49985504
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

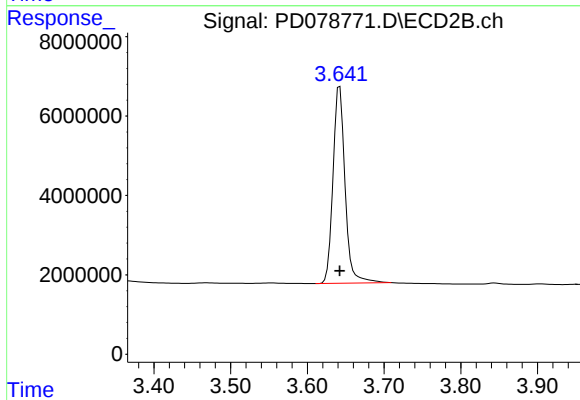


#3 gamma-BHC (Lindane)

R.T.: 3.642 min
Delta R.T.: 0.000 min
Response: 54294680
Conc: 20.00 ng/ml

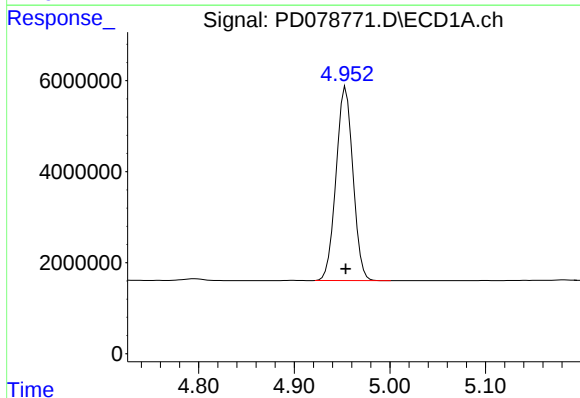


#4 Heptachlor

R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 52205512
Conc: 20.00 ng/ml

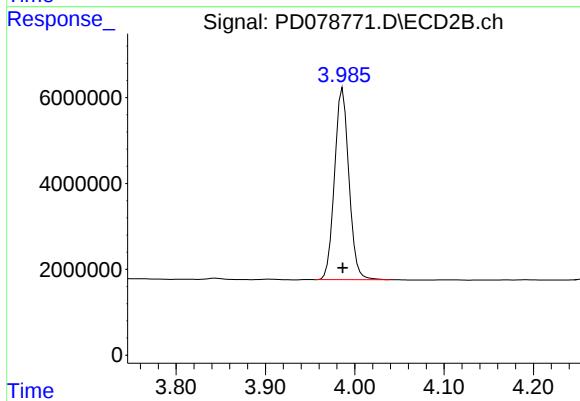

#4 Heptachlor


R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 49862729
Conc: 20.00 ng/ml

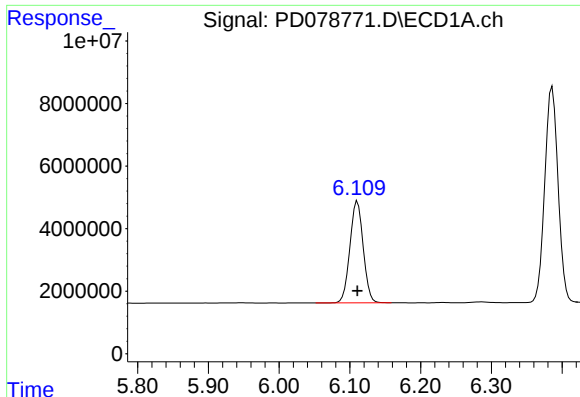

#9 Endosulfan I


R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 42595942
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

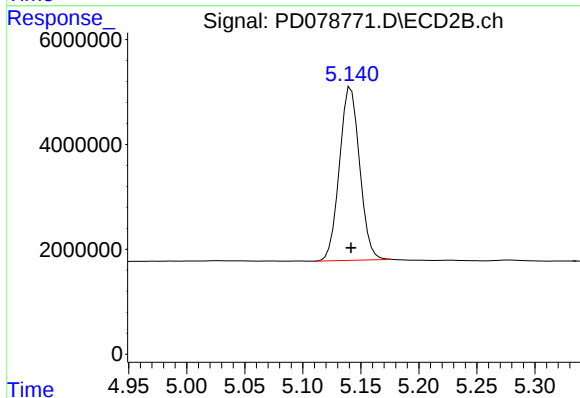


#9 Endosulfan I

R.T.: 5.142 min
Delta R.T.: 0.000 min
Response: 40001837
Conc: 20.00 ng/ml

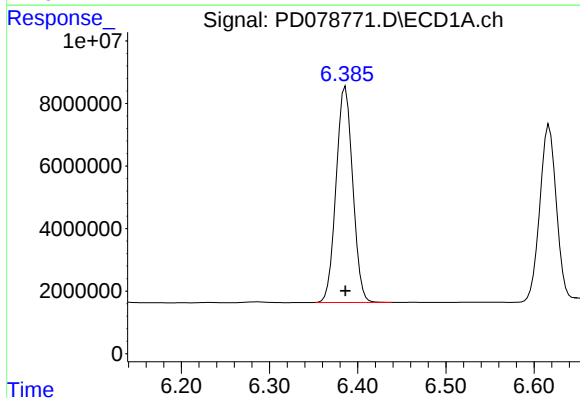


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 90374725
Conc: 40.00 ng/ml

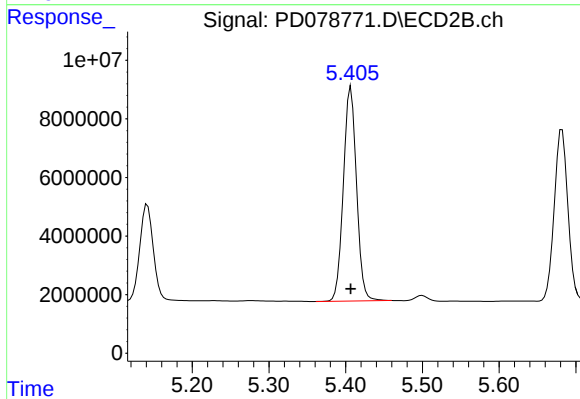

#13 Dieldrin


R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 87430113
Conc: 40.00 ng/ml

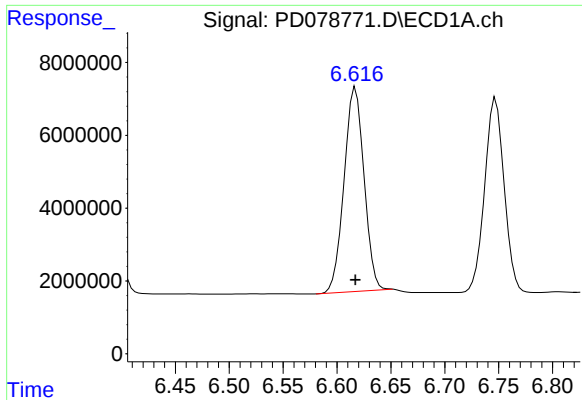

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 72481588
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

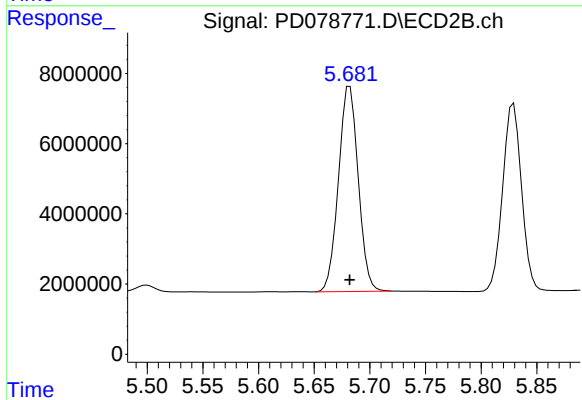


#14 Endrin

R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 72208185
Conc: 40.00 ng/ml

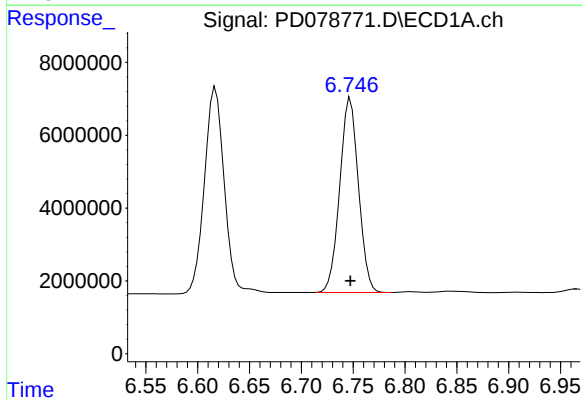


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 67168945
Conc: 40.00 ng/ml

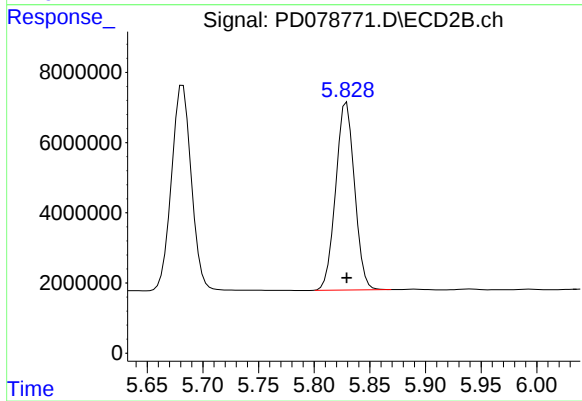

#16 4,4'-DDD


R.T.: 5.829 min
Delta R.T.: 0.000 min
Response: 62986929
Conc: 40.00 ng/ml

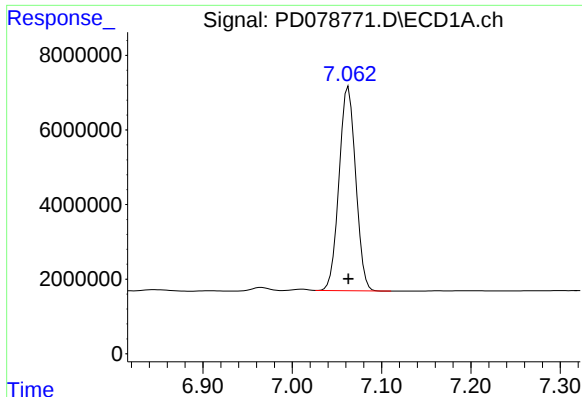

#17 4,4'-DDT


R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 70658841
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

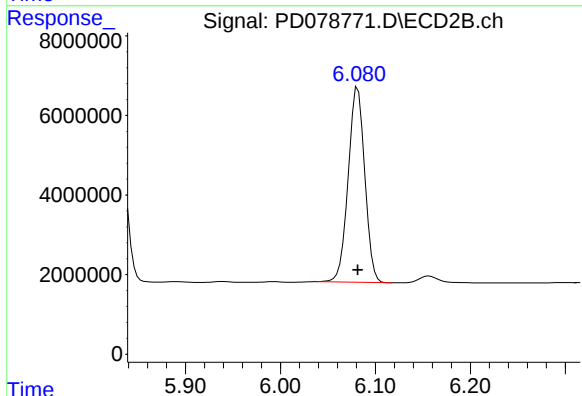


#17 4,4'-DDT

R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 59463421
Conc: 40.00 ng/ml

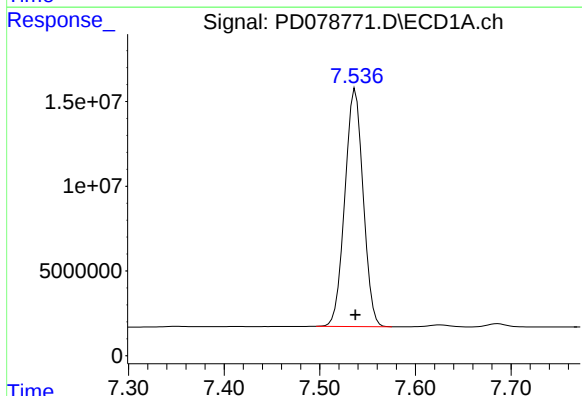


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 187140930
Conc: 200.00 ng/ml

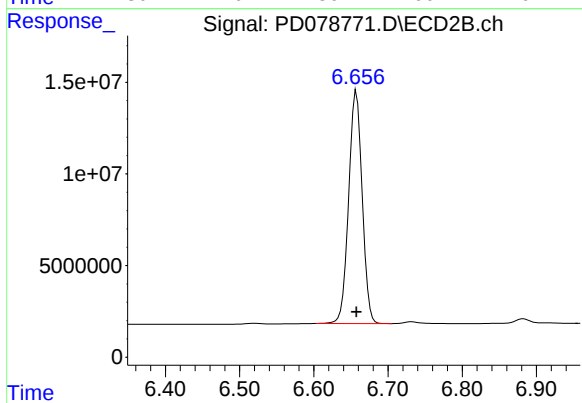

#20 Methoxychlor


R.T.: 6.657 min
Delta R.T.: 0.000 min
Response: 160380178
Conc: 200.00 ng/ml

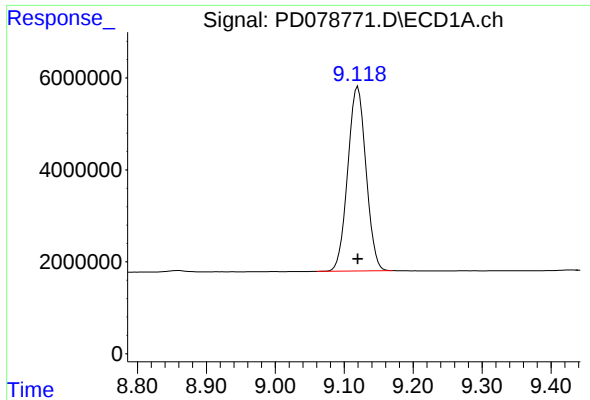

#27 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 73817689
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

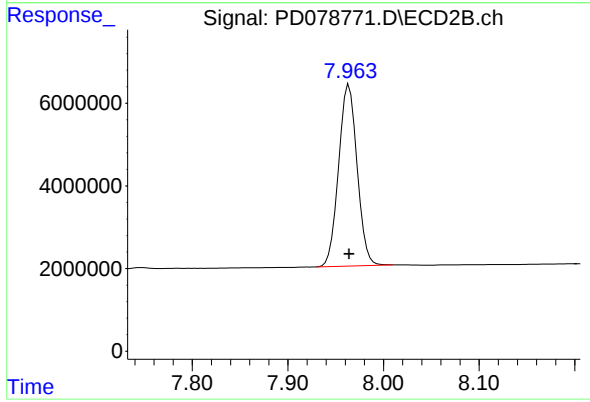

#27 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 59176869
Conc: 40.00 ng/ml