

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
 Data File : PD078773.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2023 23:41
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 01:59:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 10 01:58:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.808	59696288	77374647	38.042	38.377
27)	SA Decachlor...	9.120	7.964	135.2E6	106.9E6	73.272	72.230
Target Compounds							
2)	A alpha-BHC	4.027	3.312	105.3E6	119.7E6	40.205	39.887
3)	MA gamma-BHC...	4.360	3.642	98770588	106.9E6	39.520	39.378
4)	MA Heptachlor	4.954	3.986	108.0E6	96752037	41.366	38.807
9)	A Endosulfan I	6.111	5.141	80323651	76136808	37.714	38.067
13)	MA Dieldrin	6.387	5.407	177.0E6	170.5E6	78.335	77.991
14)	MA Endrin	6.617	5.682	140.9E6	138.4E6	77.783	76.674
16)	A 4,4'-DDD	6.748	5.830	132.1E6	121.4E6	78.663	77.108
17)	MA 4,4'-DDT	7.063	6.082	138.1E6	113.6E6	78.162	76.419
20)	A Methoxychlor	7.537	6.658	362.4E6	288.8E6	387.296	360.085


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078773.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 23:41
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 01:59:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 10 01:58:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

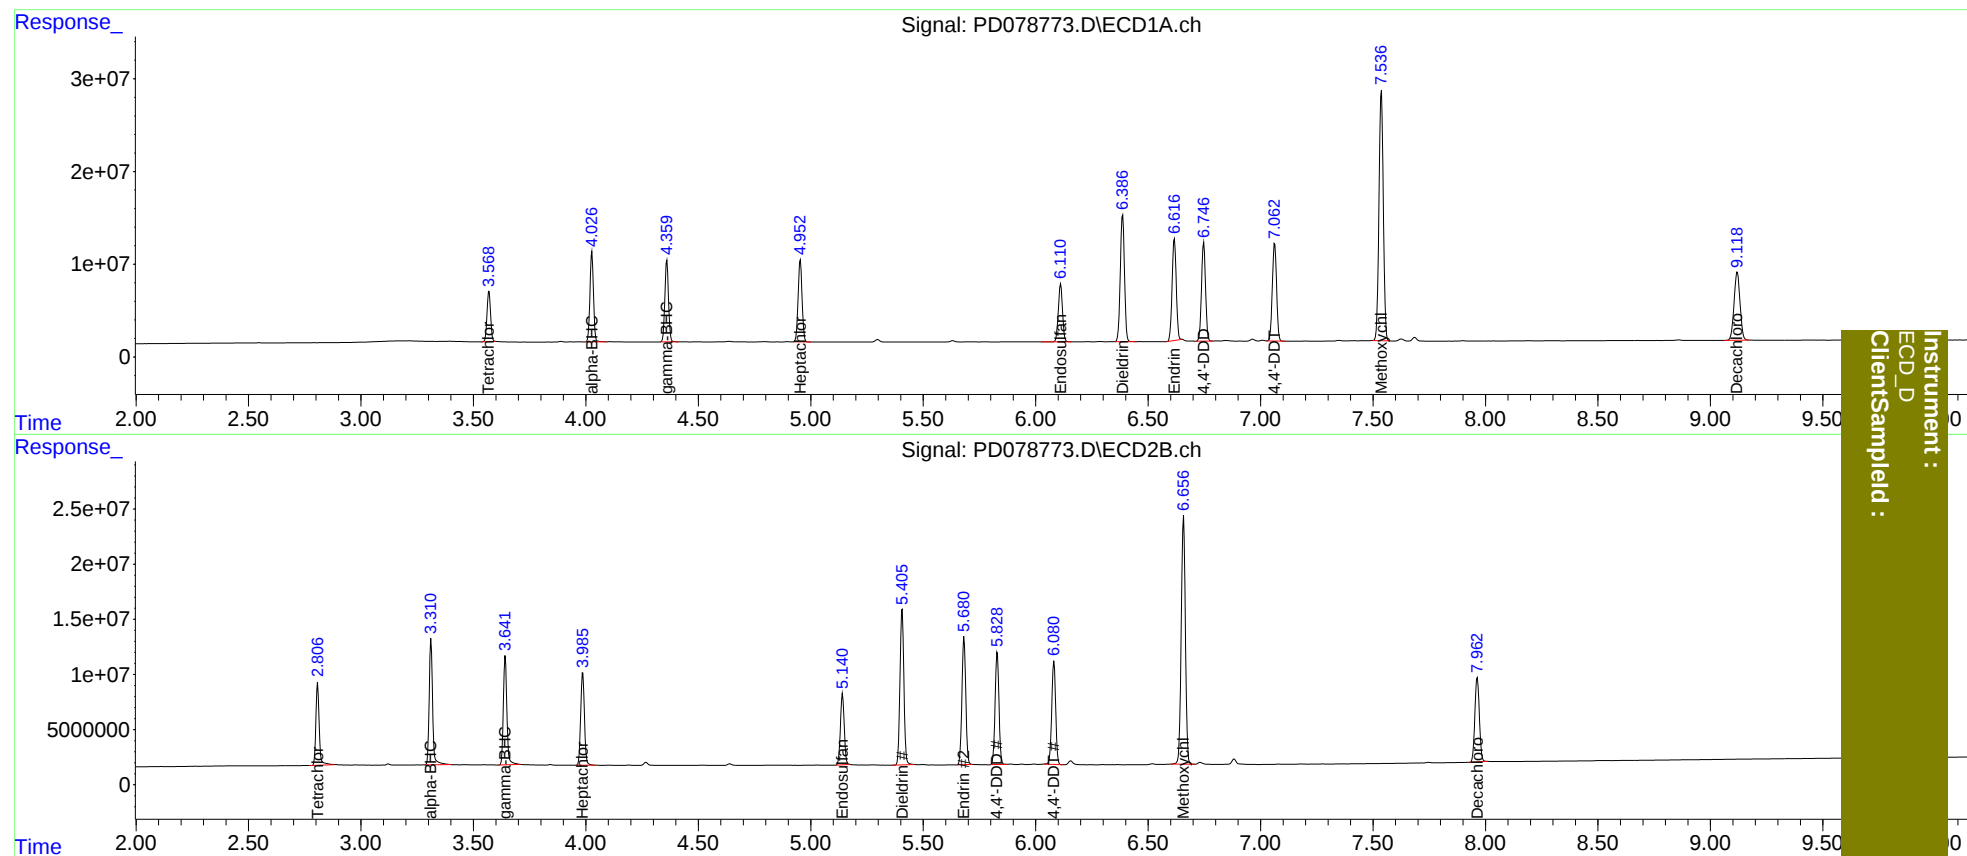


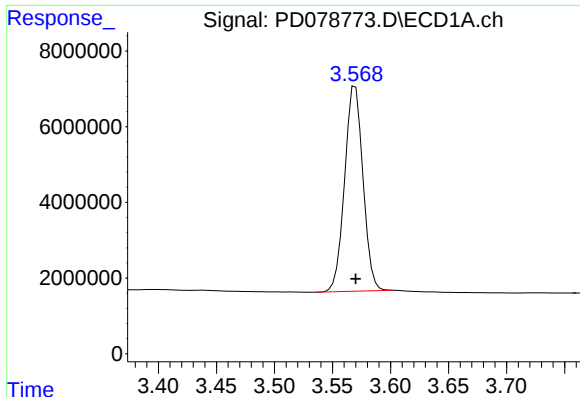

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 59696288
Conc: 38.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

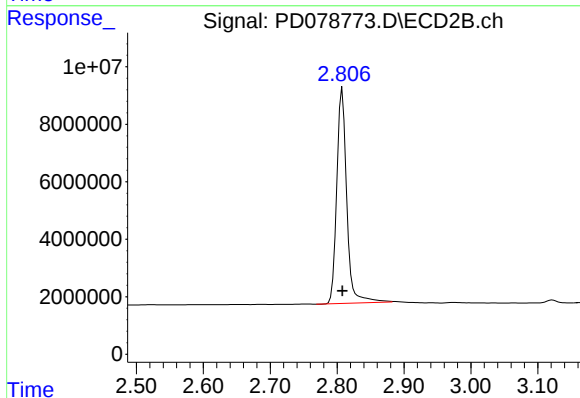


#1 Tetrachloro-m-xylene

R.T.: 2.808 min
Delta R.T.: 0.000 min
Response: 77374647
Conc: 38.38 ng/ml

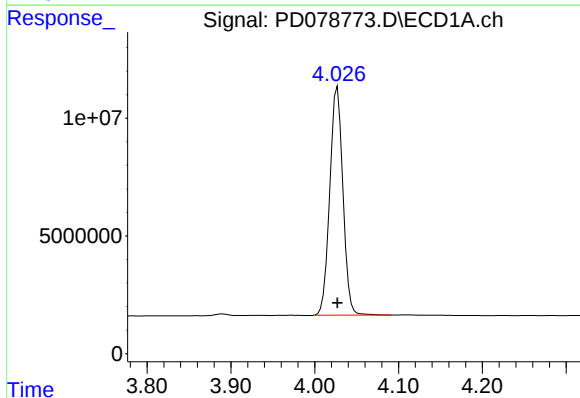


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 105298348
Conc: 40.20 ng/ml

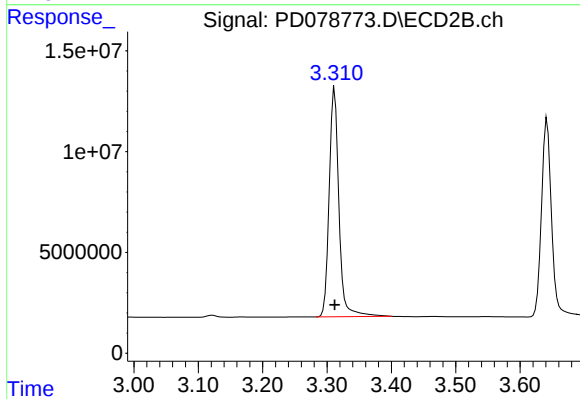

#2 alpha-BHC


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 119678912
Conc: 39.89 ng/ml

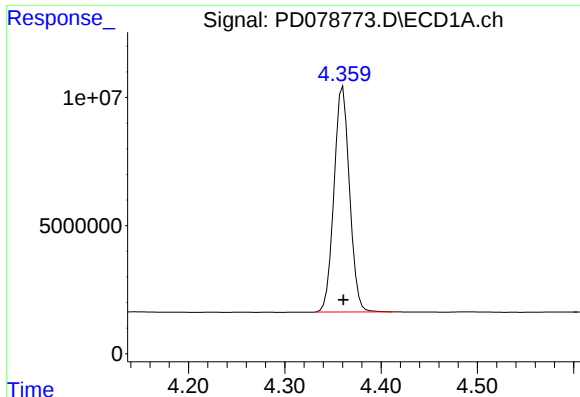

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 98770588
Conc: 39.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

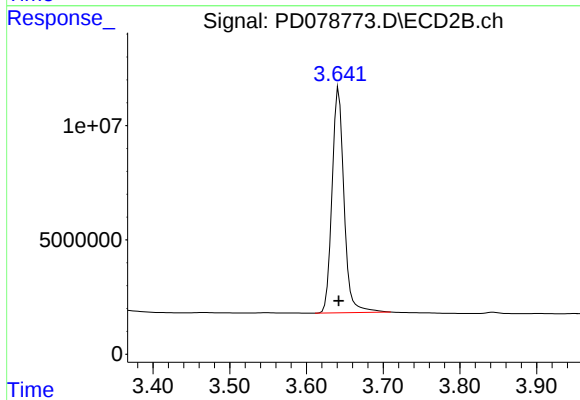


#3 gamma-BHC (Lindane)

R.T.: 3.642 min
Delta R.T.: 0.000 min
Response: 106901650
Conc: 39.38 ng/ml

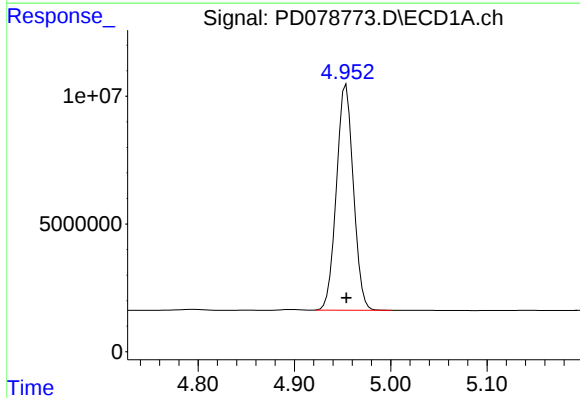


#4 Heptachlor

R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 107977014
Conc: 41.37 ng/ml

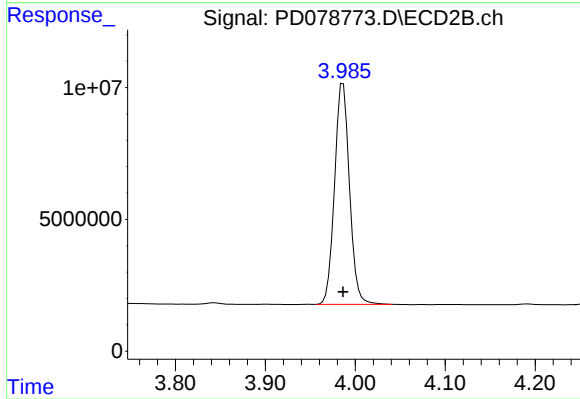

#4 Heptachlor


R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 96752037
Conc: 38.81 ng/ml

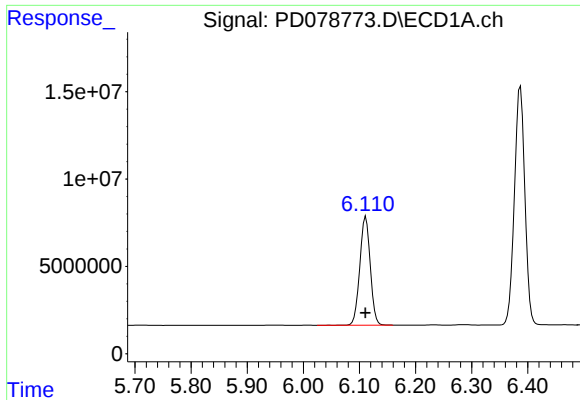

#9 Endosulfan I


R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 80323651
Conc: 37.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

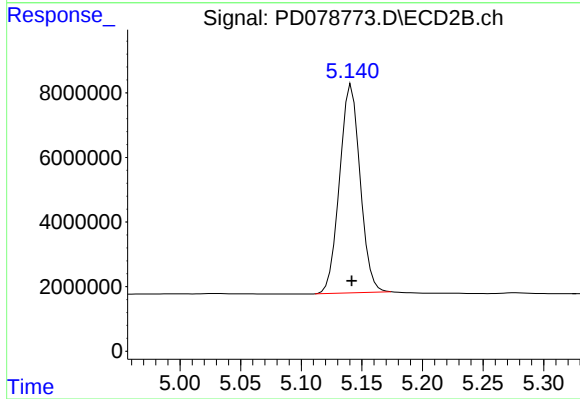


#9 Endosulfan I

R.T.: 5.141 min
Delta R.T.: 0.000 min
Response: 76136808
Conc: 38.07 ng/ml

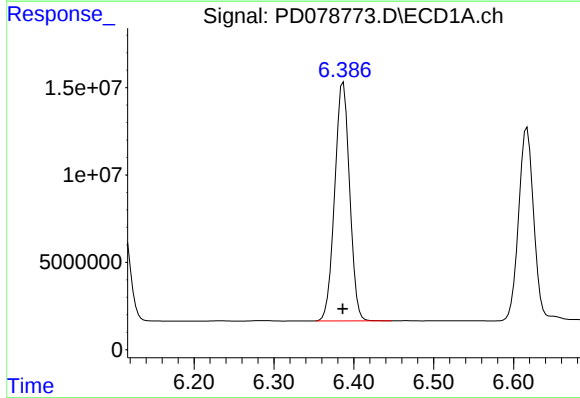


#13 Dieldrin

R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 176987223
Conc: 78.33 ng/ml

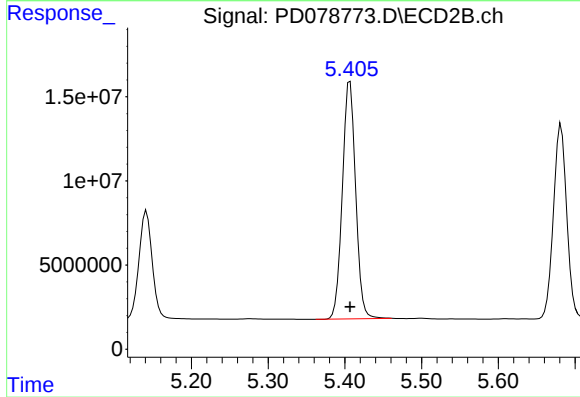

#13 Dieldrin


R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 170470018
Conc: 77.99 ng/ml

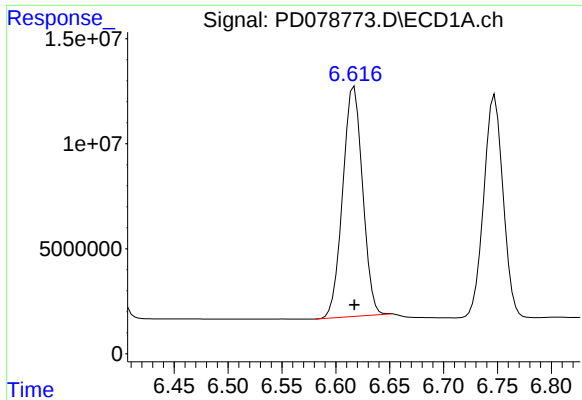

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 140945782
Conc: 77.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

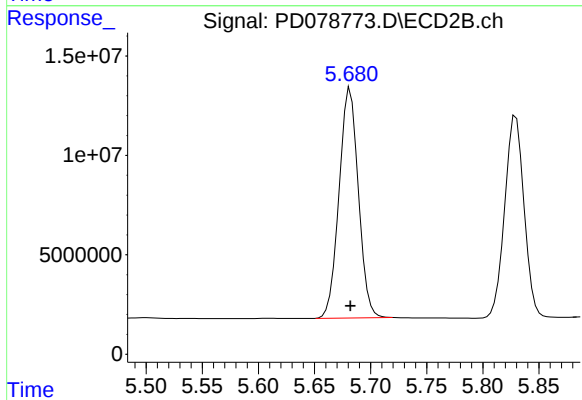


#14 Endrin

R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 138413006
Conc: 76.67 ng/ml

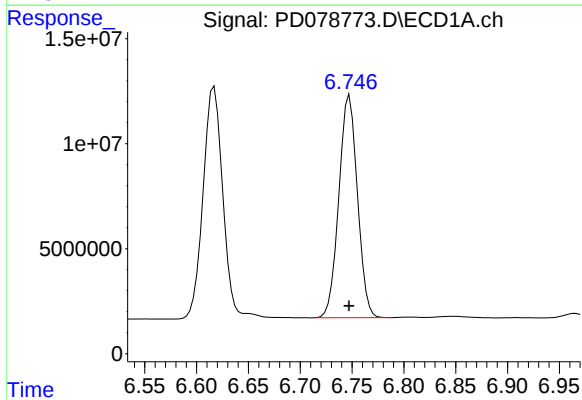


#16 4,4'-DDD

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 132092536
Conc: 78.66 ng/ml

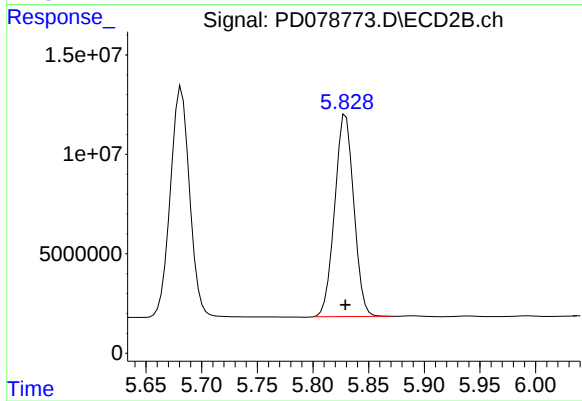

#16 4,4'-DDD


R.T.: 5.830 min
Delta R.T.: 0.000 min
Response: 121420606
Conc: 77.11 ng/ml

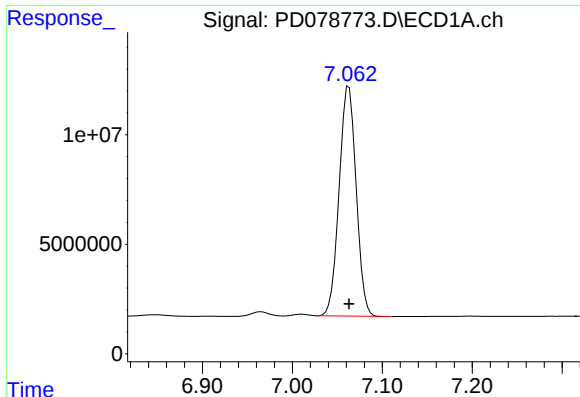

#17 4,4'-DDT


R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 138070161
Conc: 78.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

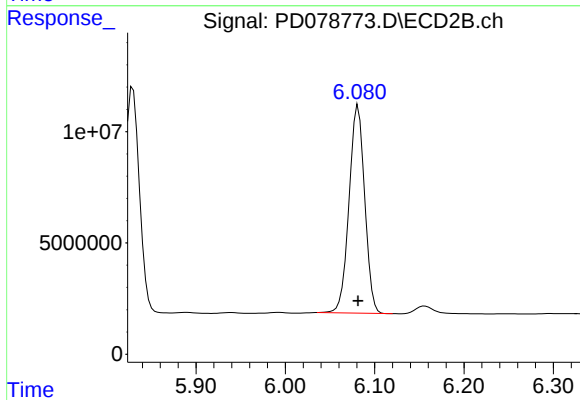


#17 4,4'-DDT

R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 113603378
Conc: 76.42 ng/ml

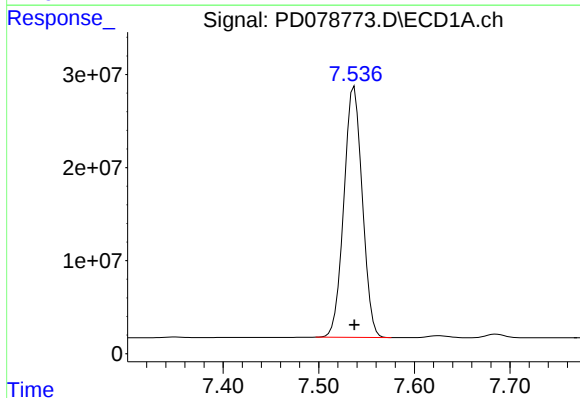


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 362395014
Conc: 387.30 ng/ml

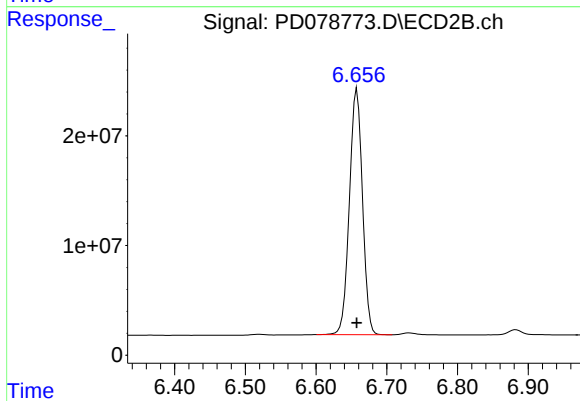

#20 Methoxychlor


R.T.: 6.658 min
Delta R.T.: 0.000 min
Response: 288752635
Conc: 360.09 ng/ml

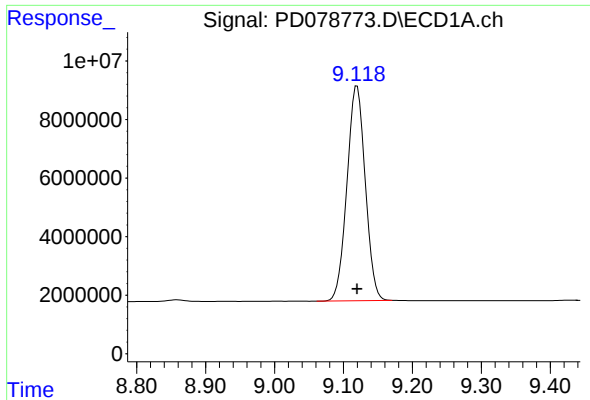

#27 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 135219880
Conc: 73.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

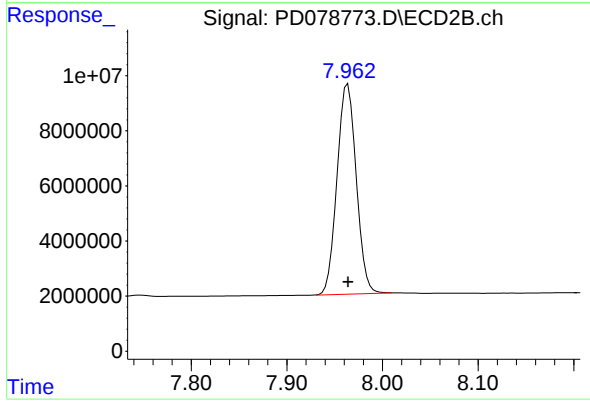

#27 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 106858696
Conc: 72.23 ng/ml