

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
 Data File : PD078775.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2023 00:08
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 02:00:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 10 01:58:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.808	118.4E6	153.7E6	75.453	76.224
27)	SA Decachlor...	9.120	7.964	260.7E6	205.1E6	141.273	138.625
Target Compounds							
2)	A alpha-BHC	4.027	3.312	219.7E6	248.7E6	83.891	82.886
3)	MA gamma-BHC...	4.361	3.643	204.0E6	219.6E6	81.609	80.889
4)	MA Heptachlor	4.955	3.987	220.1E6	196.4E6	84.333	78.770
9)	A Endosulfan I	6.112	5.142	159.4E6	151.9E6	74.833	75.922
13)	MA Dieldrin	6.387	5.407	362.2E6	344.5E6	160.303	157.622
14)	MA Endrin	6.617	5.682	288.5E6	279.3E6	159.210	154.731
16)	A 4,4'-DDD	6.748	5.830	268.4E6	245.9E6	159.864	156.189
17)	MA 4,4'-DDT	7.064	6.082	281.3E6	232.8E6	159.232	156.623
20)	A Methoxychlor	7.537	6.658	717.1E6	545.9E6	766.380	680.723


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078775.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 00:08
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 02:00:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 10 01:58:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

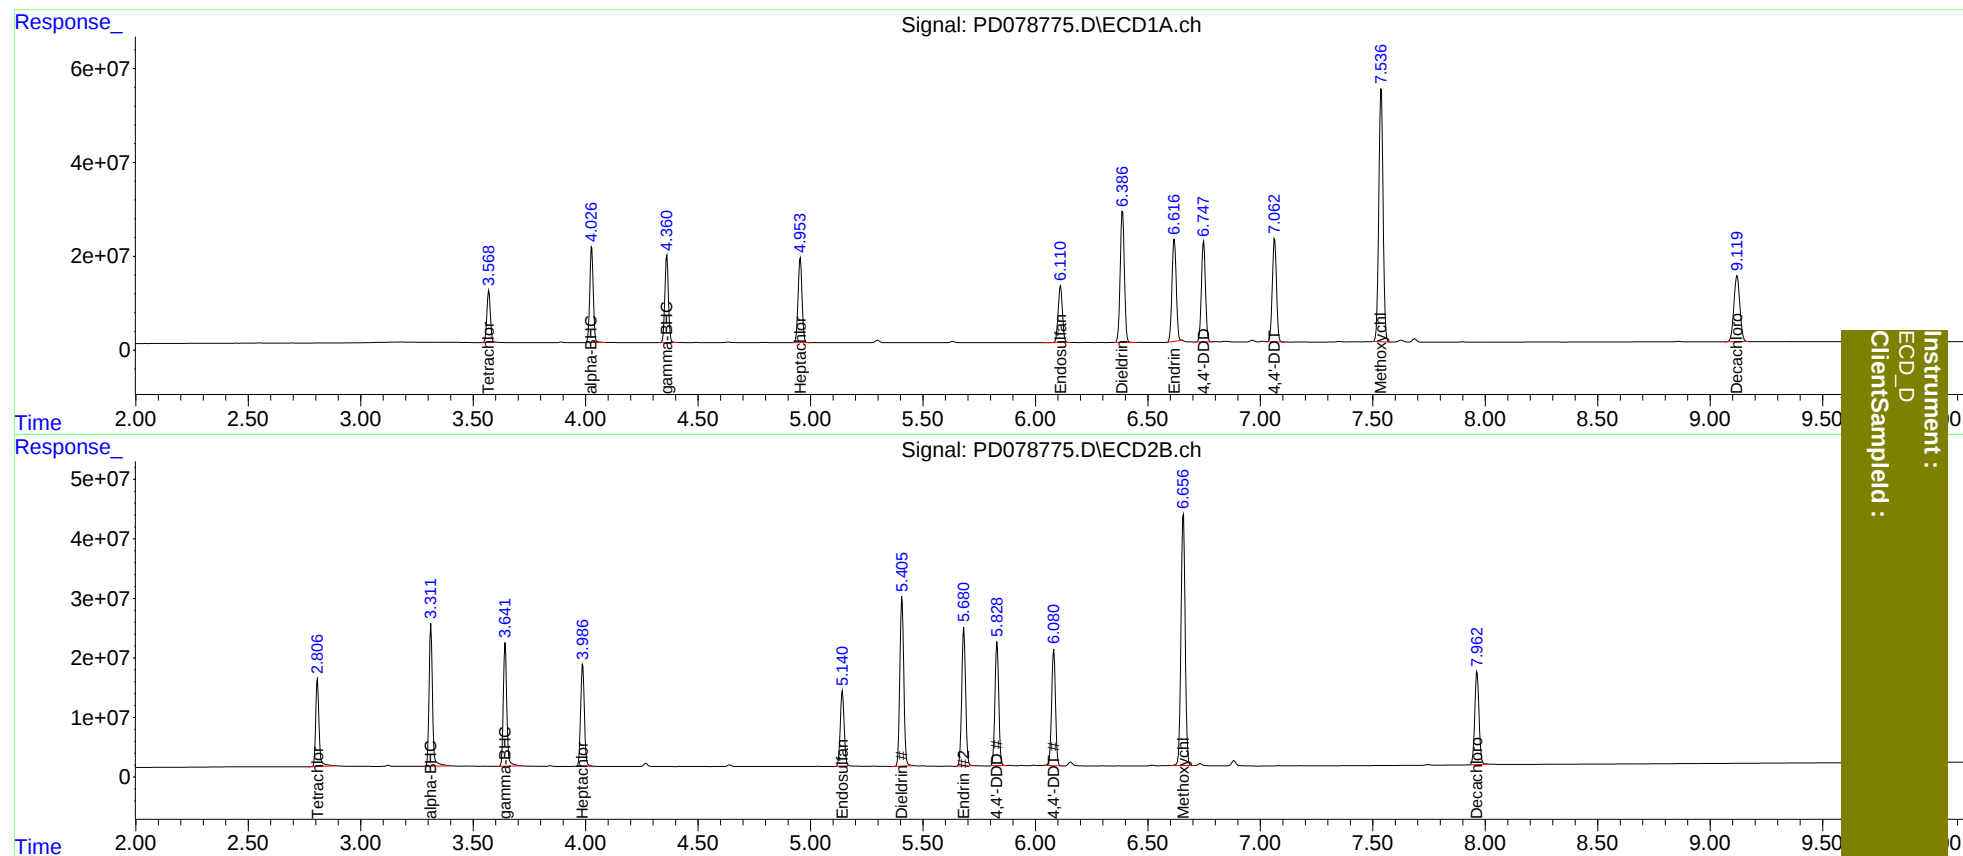


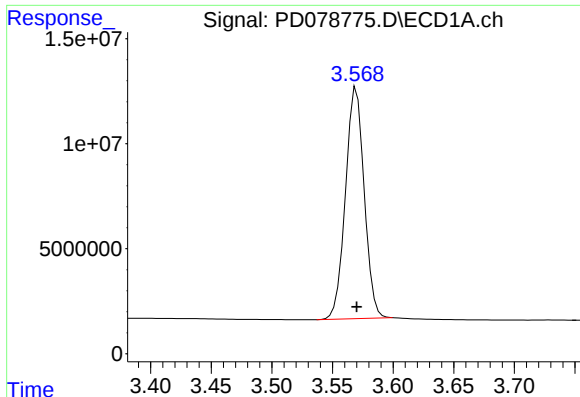

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 118401417
Conc: 75.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

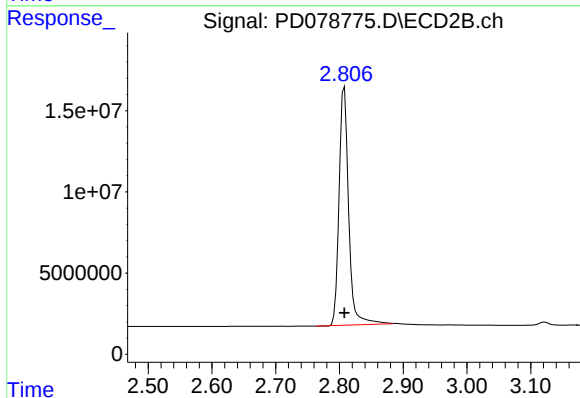


#1 Tetrachloro-m-xylene

R.T.: 2.808 min
Delta R.T.: 0.000 min
Response: 153679903
Conc: 76.22 ng/ml

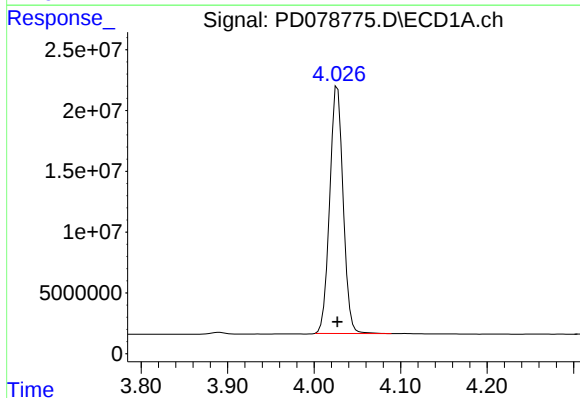


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 219715239
Conc: 83.89 ng/ml

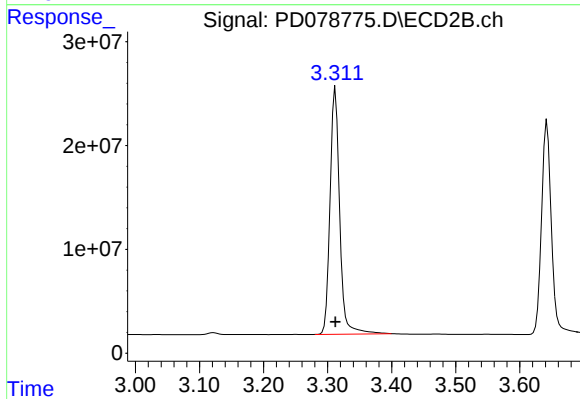

#2 alpha-BHC


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 248698006
Conc: 82.89 ng/ml

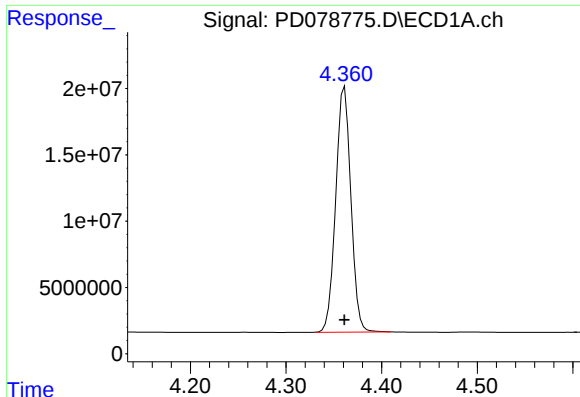

#3 gamma-BHC (Lindane)


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 203964092
Conc: 81.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

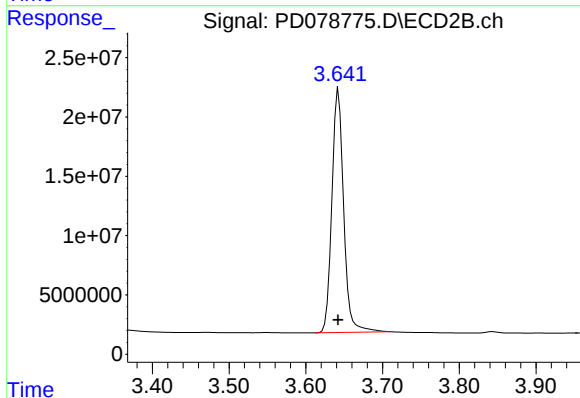


#3 gamma-BHC (Lindane)

R.T.: 3.643 min
Delta R.T.: 0.000 min
Response: 219593387
Conc: 80.89 ng/ml

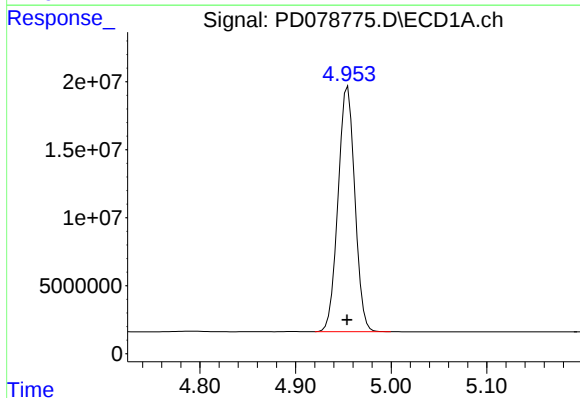


#4 Heptachlor

R.T.: 4.955 min
Delta R.T.: 0.000 min
Response: 220132897
Conc: 84.33 ng/ml

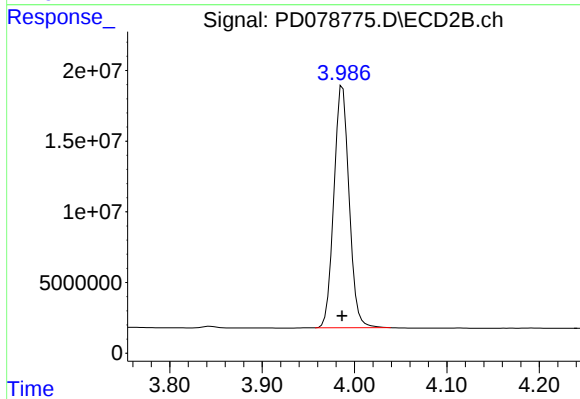

#4 Heptachlor


R.T.: 3.987 min
Delta R.T.: 0.000 min
Response: 196384150
Conc: 78.77 ng/ml

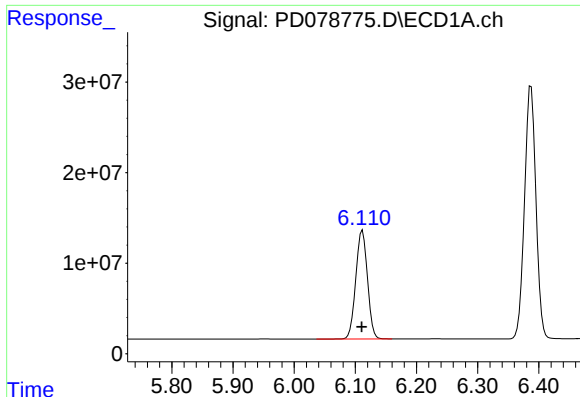

#9 Endosulfan I


R.T.: 6.112 min
Delta R.T.: 0.000 min
Response: 159379188
Conc: 74.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

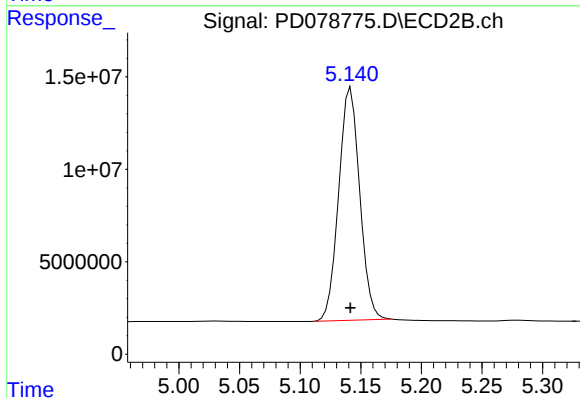


#9 Endosulfan I

R.T.: 5.142 min
Delta R.T.: 0.000 min
Response: 151850329
Conc: 75.92 ng/ml

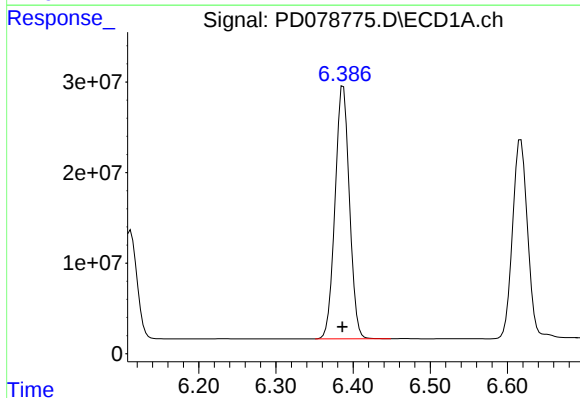


#13 Dieldrin

R.T.: 6.387 min
Delta R.T.: 0.001 min
Response: 362182611
Conc: 160.30 ng/ml

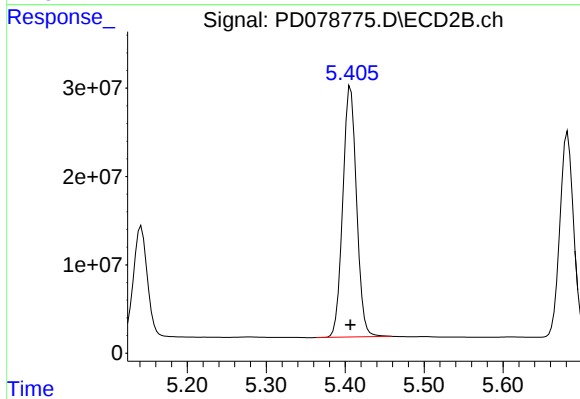

#13 Dieldrin


R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 344522908
Conc: 157.62 ng/ml

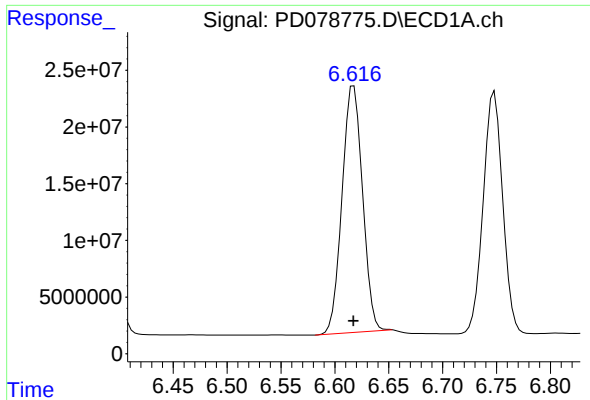

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 288495682
Conc: 159.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

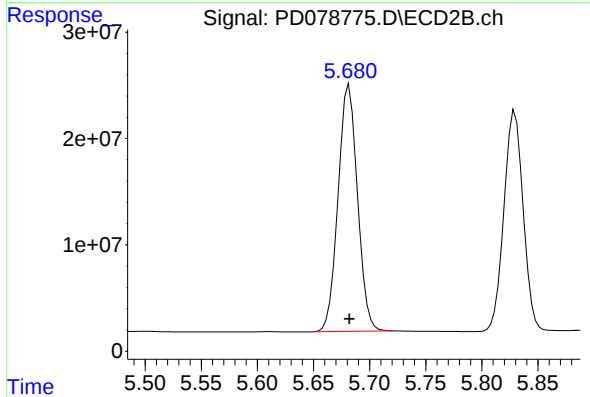


#14 Endrin

R.T.: 5.682 min
Delta R.T.: 0.000 min
Response: 279321318
Conc: 154.73 ng/ml

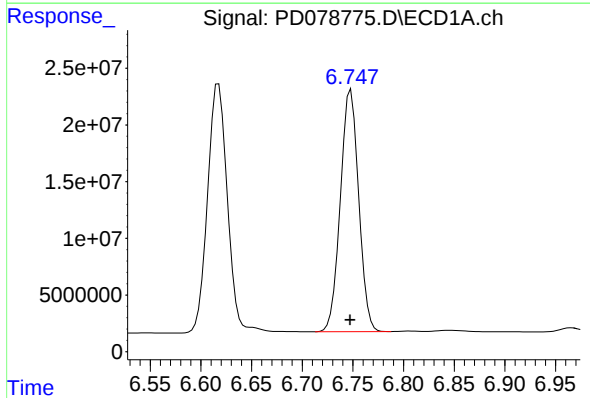


#16 4,4'-DDD

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 268447687
Conc: 159.86 ng/ml

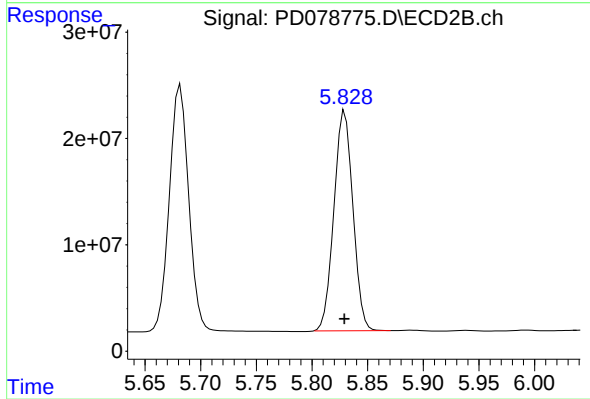

#16 4,4'-DDD


R.T.: 5.830 min
Delta R.T.: 0.000 min
Response: 245946981
Conc: 156.19 ng/ml

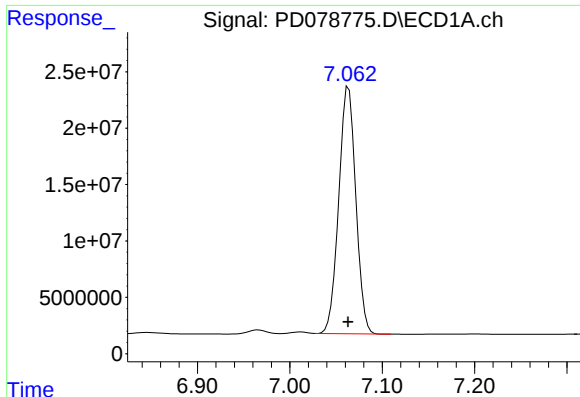

#17 4,4'-DDT


R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 281278171
Conc: 159.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

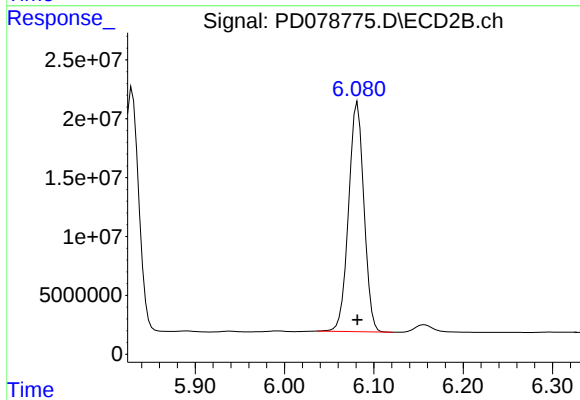


#17 4,4'-DDT

R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 232833060
Conc: 156.62 ng/ml

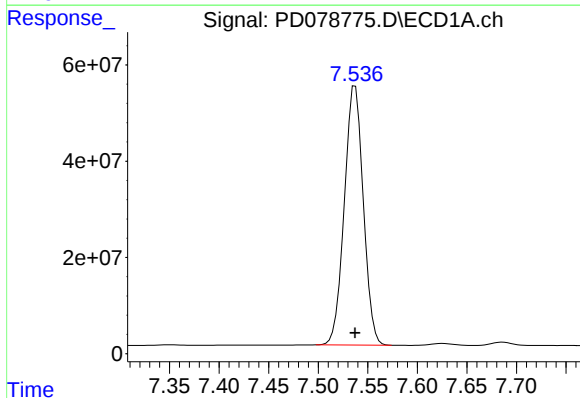


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 717105245
Conc: 766.38 ng/ml

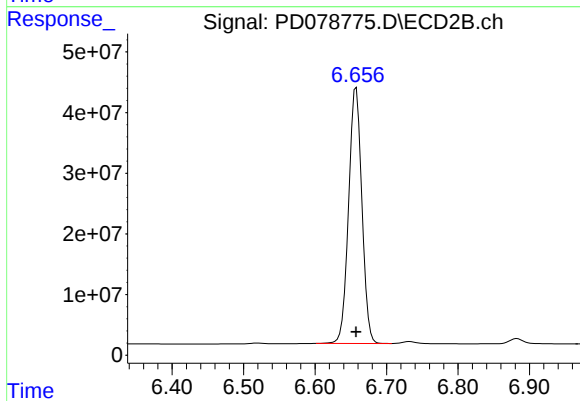

#20 Methoxychlor

R.T.: 6.658 min
Delta R.T.: 0.000 min
Response: 545872086
Conc: 680.72 ng/ml

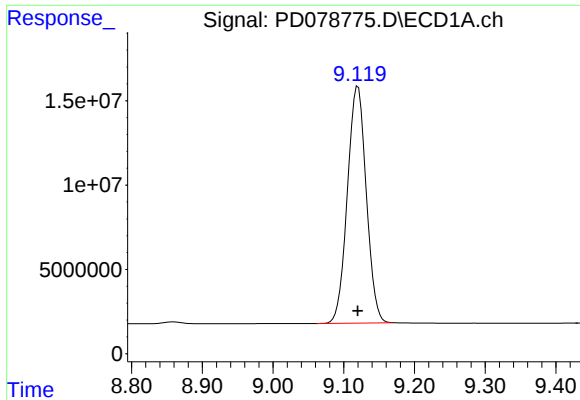

#27 Decachlorobiphenyl


R.T.: 9.120 min

Delta R.T.: 0.000 min

Response: 260711791

Conc: 141.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

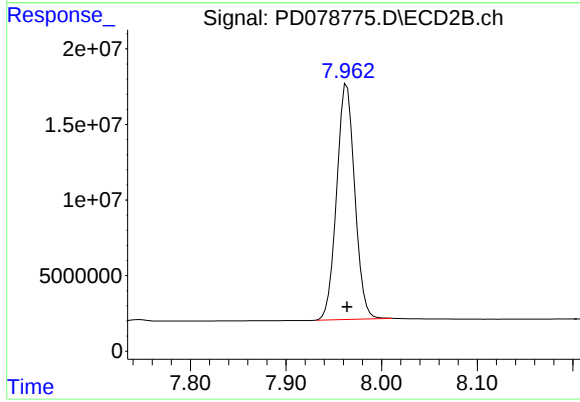

#27 Decachlorobiphenyl

R.T.: 7.964 min

Delta R.T.: 0.000 min

Response: 205085252

Conc: 138.63 ng/ml