

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
 Data File : PD078760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2023 20:47
 Operator : AR\AJ
 Sample : RESC009
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 01:04:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 01:02:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.807	31388459	39131313	20.098	19.430
2)	SA Decachlor...	9.120	7.964	73916426	58005748	40.265	39.890
Target Compounds							
2)	A alpha-BHC	4.027	3.311	25402929	28407678	9.687	9.510
3)	MA gamma-BHC...	4.361	3.642	24771643	26736723	9.908	9.869
4)	MA Heptachlor	4.954	3.986	26430229	24516628	9.826	9.858
5)	MB Aldrin	5.298	4.268	25521440	24926998	10.165	10.100
6)	B beta-BHC	4.553	3.937	11898002	12513559	10.256	10.053
7)	B delta-BHC	4.803	4.168	25624517	25705150	9.213	9.540
8)	B Heptachlo...	5.725	4.770	23700553	23110478	10.062	9.896
9)	A Endosulfan I	6.111	5.141	21928439	20117011	10.236	10.222
10)	B trans-Chl...	5.980	5.021	22500640	21892032	9.988	10.002
11)	B cis-Chlor...	6.060	5.086	23163045	22291616	10.073	9.985
12)	B 4,4'-DDE	6.231	5.275	40536769	39109054	19.298	19.526
13)	MA Dieldrin	6.387	5.407	45118744	43155795	19.900	19.917
14)	MA Endrin	6.617	5.682	36354403	36963611	19.892	20.636
15)	B Endosulfa...	6.835	5.974	39936914	36347456	20.039	20.289
16)	A 4,4'-DDD	6.748	5.829	33555370	32341623	19.954	20.735
17)	MA 4,4'-DDT	7.064	6.081	35717291	30295246	20.155	20.605
18)	B Endrin al...	6.965	6.154	30217550	29363618	19.854	21.557
19)	B Endosulfa...	7.199	6.376	38993219	34422584	20.079	20.910
20)	A Methoxychlor	7.538	6.658	95254315	84474088	101.432	108.026
21)	B Endrin ke...	7.686	6.882	42121072	38290226	20.338	21.113

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 20:47
Operator : AR\AJ
Sample : RESC009
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:04:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 01:02:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

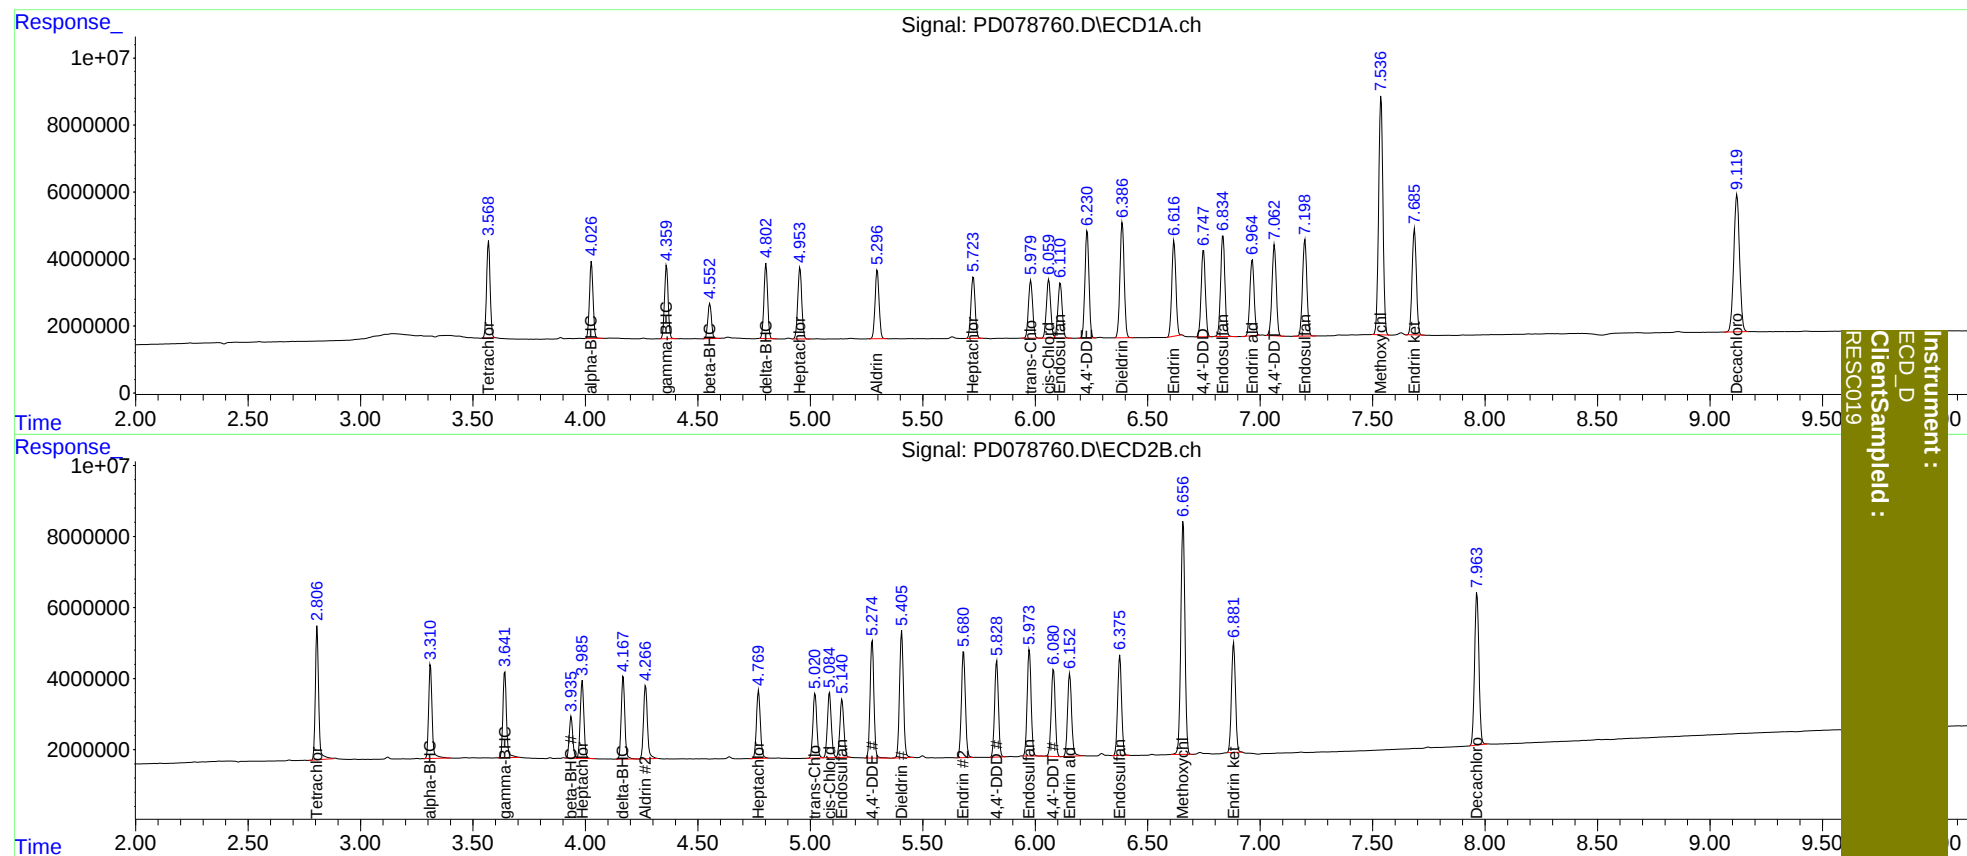

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078760.D
Acq On : 09 Oct 2023 20:47
Operator : AR\AJ
Sample : RESC009
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Title : GC Extractables
Last Update : Wed Oct 11 01:02:10 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.570	4.027	100.00%
4.027	4.361	100.00%
4.361	4.553	100.00%
4.553	4.803	100.00%
4.803	4.954	100.00%
4.954	5.298	100.00%
5.298	5.725	100.00%
5.725	5.980	100.00%
5.980	6.060	100.00%
6.060	6.111	96.91%
6.111	6.231	100.00%
6.231	6.387	100.00%
6.387	6.617	100.00%
6.617	6.748	100.00%
6.748	6.835	100.00%
6.835	6.965	100.00%
6.965	7.064	100.00%
7.064	7.199	100.00%
7.199	7.538	100.00%
7.538	7.686	100.00%
7.686	9.120	100.00%

Signal #2


2.807	3.311	100.00%
3.311	3.642	100.00%
3.642	3.937	100.00%
3.937	3.986	100.00%
3.986	4.168	100.00%
4.168	4.268	100.00%
4.268	4.770	100.00%
4.770	5.021	100.00%
5.021	5.086	99.62%
5.086	5.141	99.16%
5.141	5.275	100.00%
5.275	5.407	100.00%
5.407	5.682	100.00%
5.682	5.829	100.00%
5.829	5.974	100.00%
5.974	6.081	100.00%
6.081	6.154	100.00%
6.154	6.376	100.00%
6.376	6.658	100.00%
6.658	6.882	100.00%
6.882	7.964	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 20:47
Operator : AR\AJ
Sample : RESC009
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:04:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 01:02:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

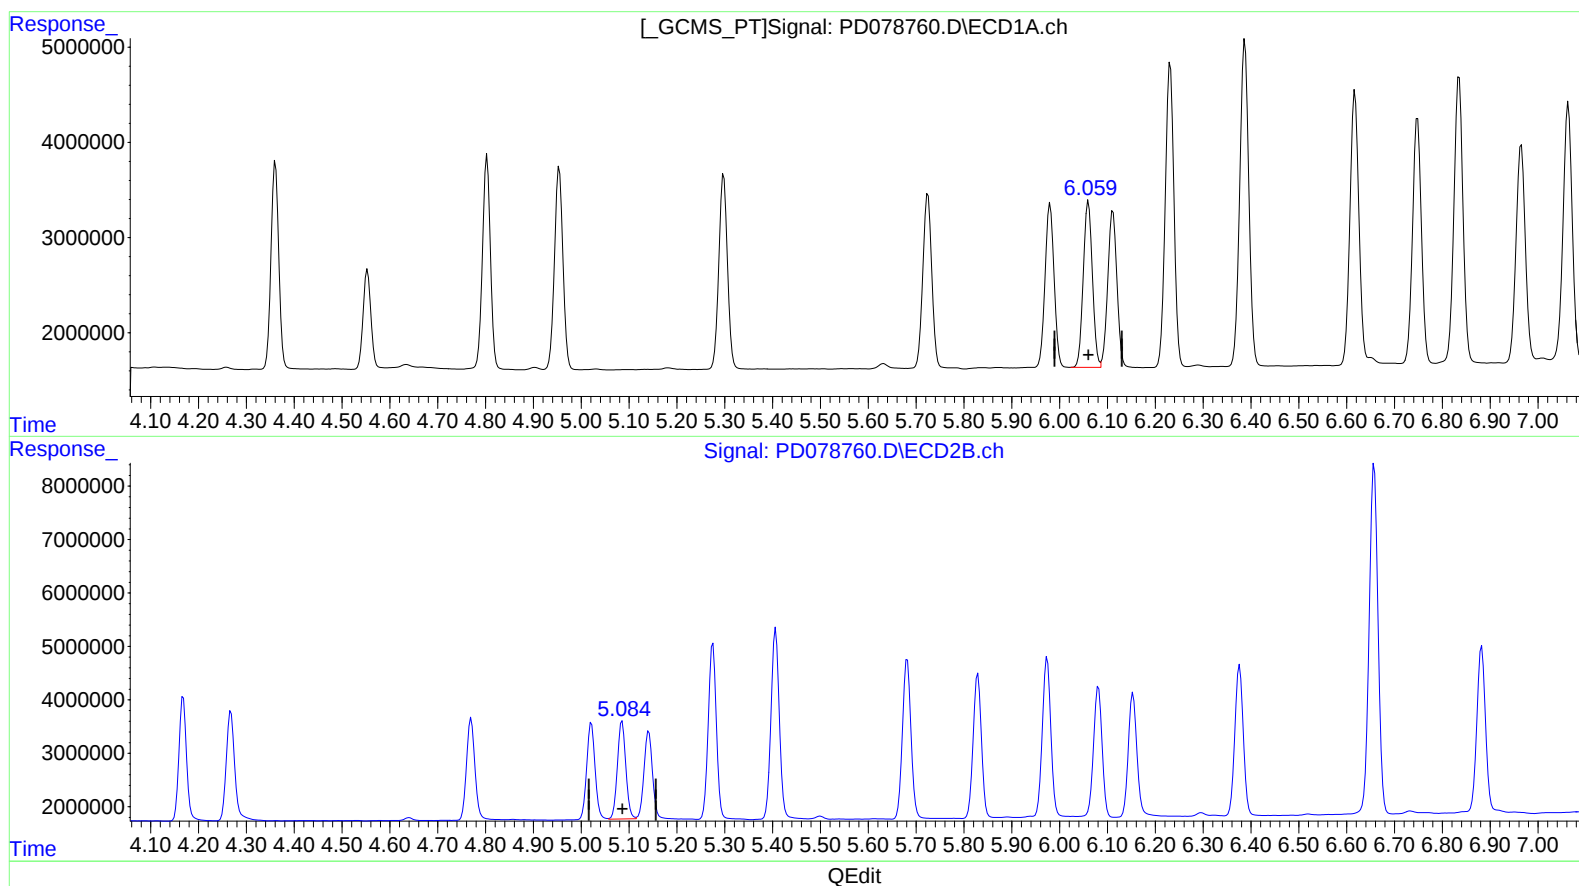

(11) cis-Chlordane (B)

6.060min 10.073 ng/ml

response 23163045

(11) cis-Chlordane #2 (B)

5.086min 9.985 ng/ml


response 22291616

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 20:47
Operator : AR\AJ
Sample : RESC009
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:04:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 01:02:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

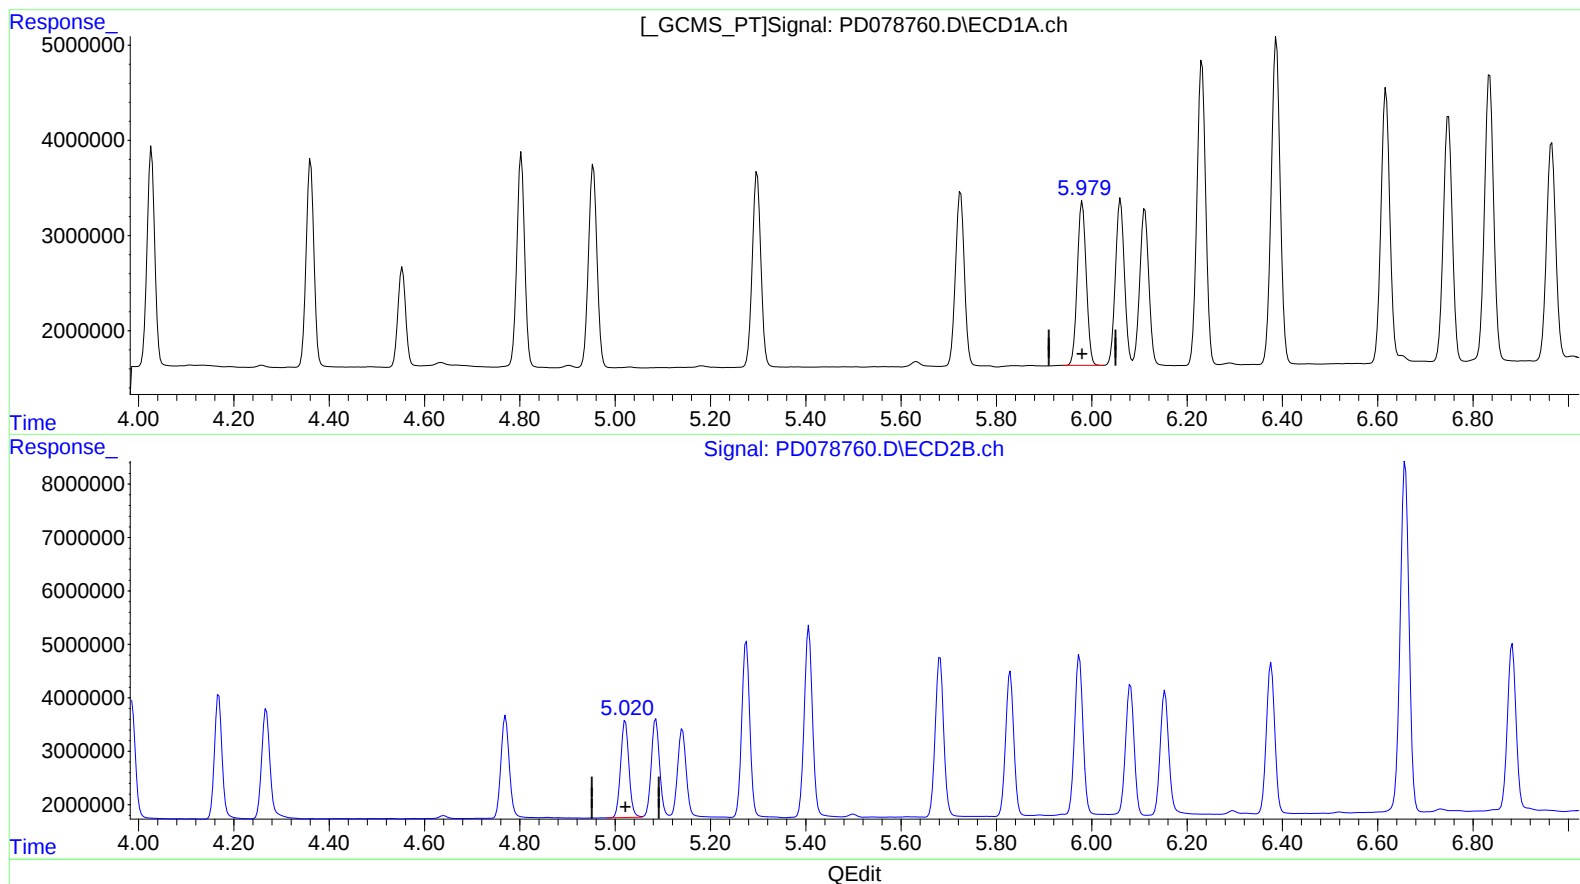

(10) trans-Chlordane (B)

5.980min 9.988 ng/ml

response 22500640

(10) trans-Chlordane #2 (B)

5.021min 10.002 ng/ml


response 21892032

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100923\
Data File : PD078760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2023 20:47
Operator : AR\AJ
Sample : RESC009
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:04:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100923CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 01:02:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

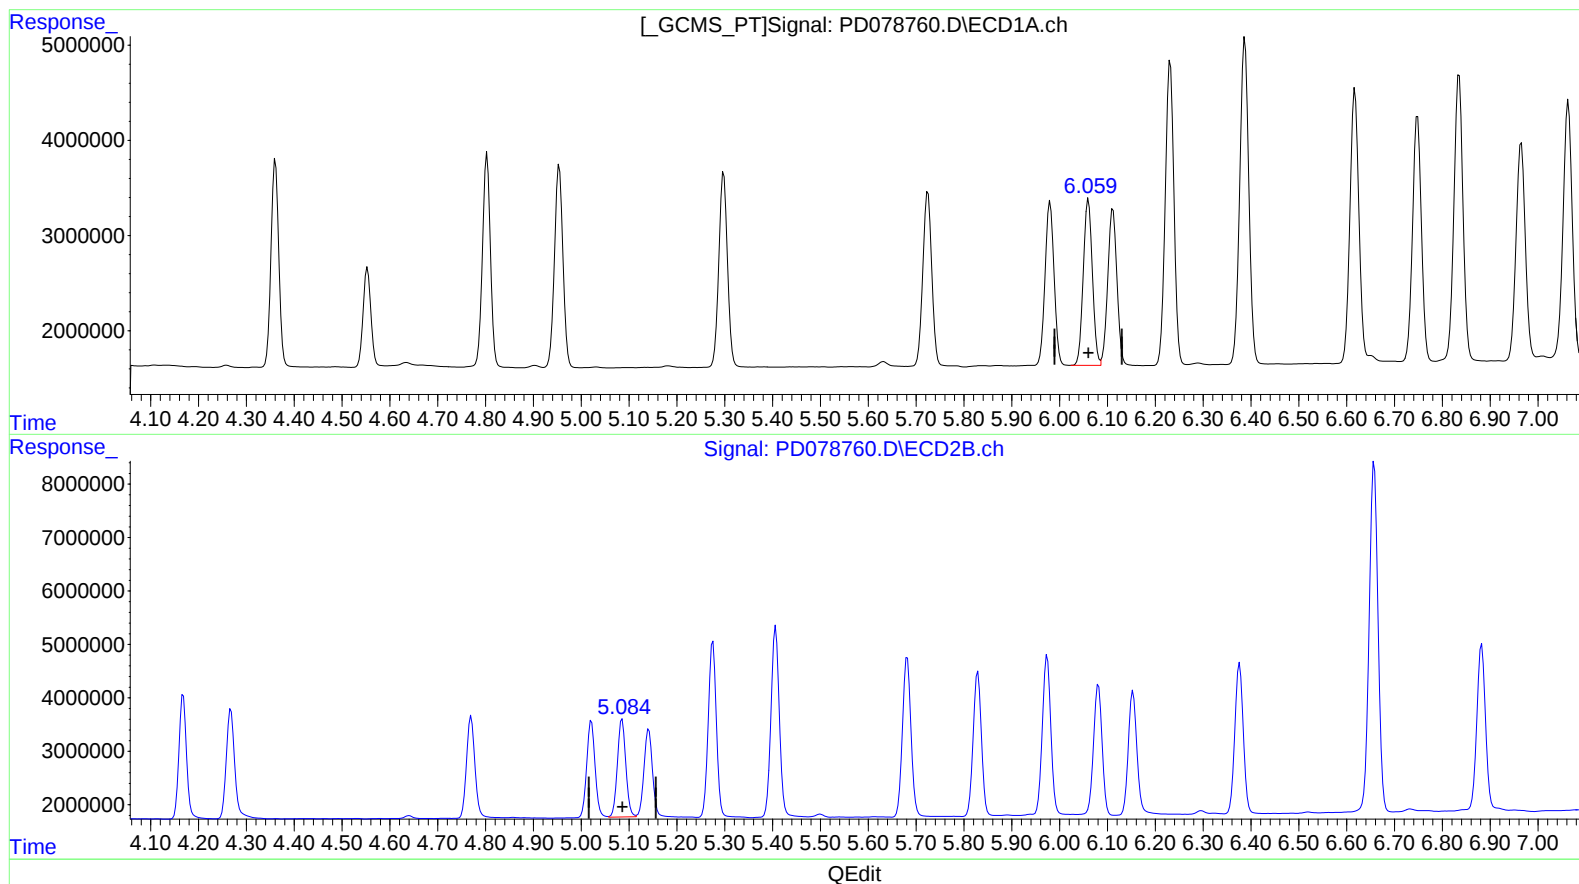

(11) cis-Chlordane (B)

6.060min 10.073 ng/ml

response 23163045

(11) cis-Chlordane #2 (B)

5.086min 9.985 ng/ml

response 22291616