

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100924\
 Data File : PD085946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Oct 2024 13:22
 Operator : AR\AJ
 Sample : RESC049
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC004

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 09 17:24:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 09 17:21:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	2.876	22699966	123.8E6	19.845	19.930
2)	SA Decachlor...	8.899	8.058	75007191	184.2E6	38.891	37.878
Target Compounds							
2)	A alpha-BHC	3.885	3.386	18704824	95343943	9.331	10.332
3)	MA gamma-BHC...	4.212	3.720	19174002	88225763	9.615	10.238
4)	MA Heptachlor	4.805	4.071	17771890	72518255	9.218	9.862
5)	MB Aldrin	5.144	4.357	20136111	87414259	8.369	9.039
6)	B beta-BHC	4.399	4.015	8911927	39539066	8.459	8.767
7)	B delta-BHC	4.643	4.251	17068185	78979569	7.758	8.525
8)	B Heptachlo...	5.564	4.859	18257575	76210186	8.197	8.748
9)	A Endosulfan I	5.944	5.233	18276814	73094423	10.018	10.545
10)	B trans-Chl...	5.818	5.112	18158911	77326325	8.080	8.596
11)	B cis-Chlor...	5.899	5.176	18554326	76846024	8.135	8.560
12)	B 4,4'-DDE	6.071	5.360	29508622	127.6E6	15.475	16.981
13)	MA Dieldrin	6.218	5.499	37267802	150.4E6	18.934	20.318
14)	MA Endrin	6.443	5.776	29498523	121.5E6	19.094	20.598
15)	B Endosulfa...	6.656	6.068	32509933	118.9E6	16.376	16.998
16)	A 4,4'-DDD	6.579	5.915	23470748	95487604	18.815	20.013
17)	MA 4,4'-DDT	6.894	6.170	25785352	95442655	19.109	19.163
18)	B Endrin al...	6.785	6.247	25596991	90566642	16.694	17.483
19)	B Endosulfa...	7.019	6.471	29964285	102.6E6	16.362	16.940
20)	A Methoxychlor	7.368	6.741	76397603	212.4E6	95.549	101.333
21)	B Endrin ke...	7.497	6.981	32909231	126.4E6	16.187	17.358

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100924\
Data File : PD085946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2024 13:22
Operator : AR\AJ
Sample : RESC049
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 17:24:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

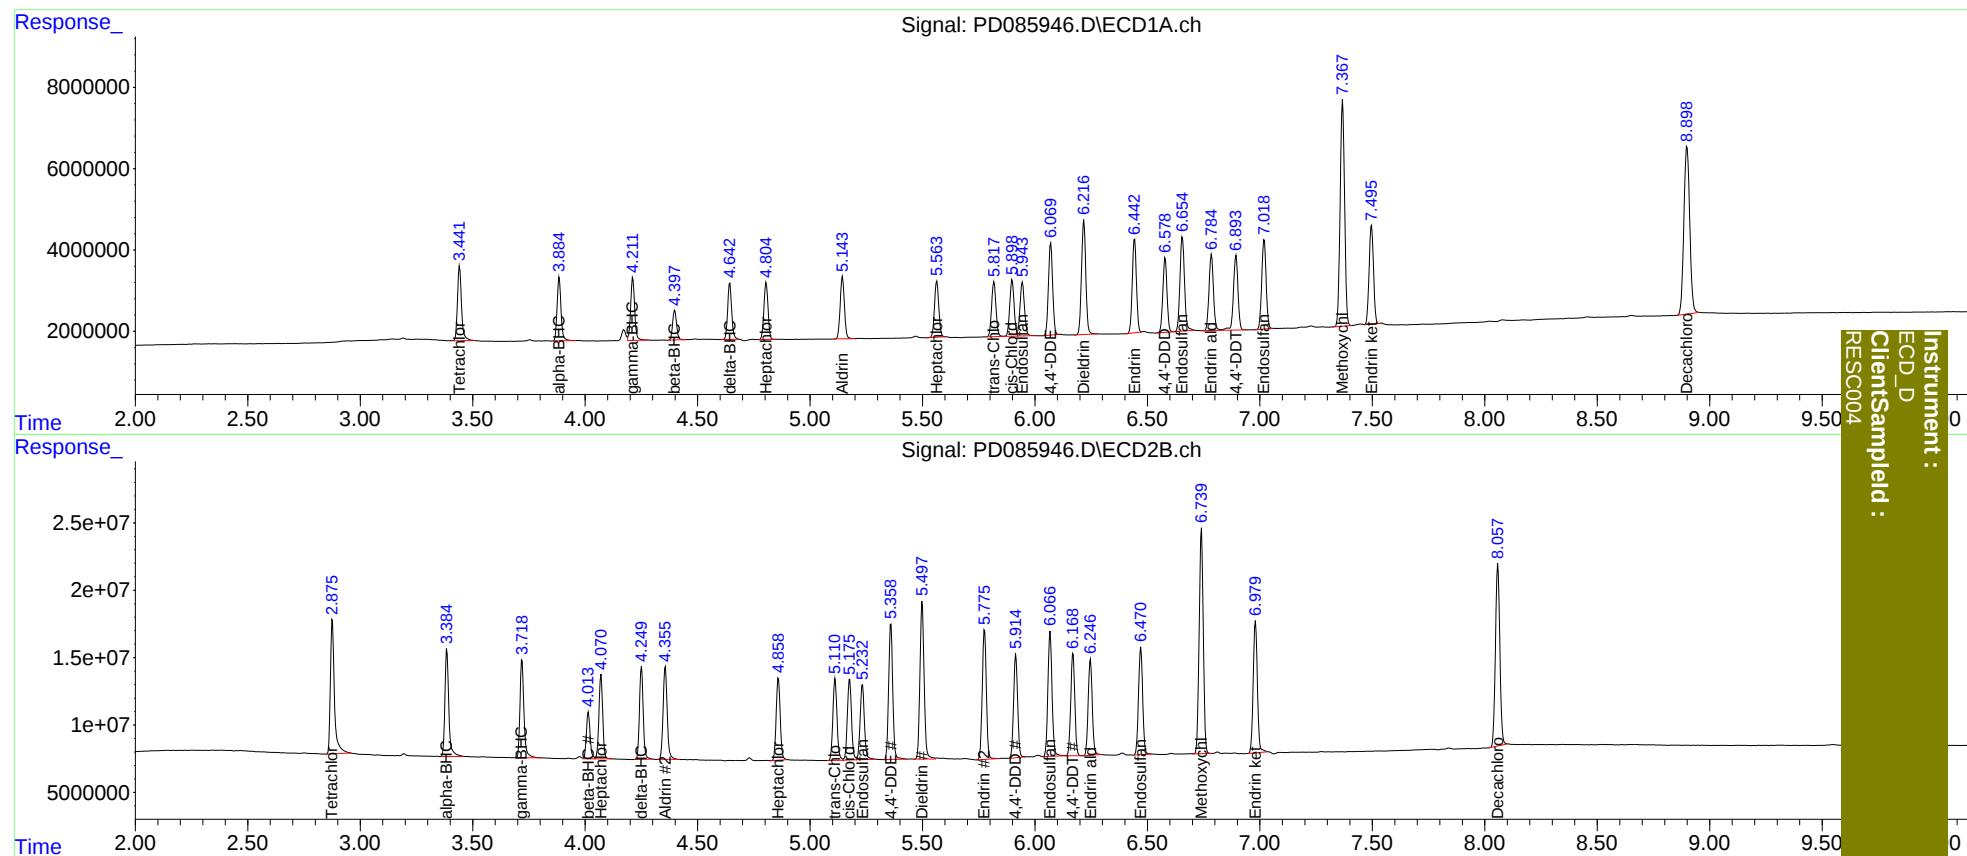

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100924\
Data File : PD085946.D
Acq On : 09 Oct 2024 13:22
Operator : AR\AJ
Sample : RESC049
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Title : GC Extractables
Last Update : Wed Oct 09 17:21:49 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.442	3.885	100.00%
3.885	4.212	100.00%
4.212	4.399	100.00%
4.399	4.643	100.00%
4.643	4.805	100.00%
4.805	5.144	100.00%
5.144	5.564	100.00%
5.564	5.818	100.00%
5.818	5.899	100.00%
5.899	5.944	93.38%
5.944	6.071	100.00%
6.071	6.218	100.00%
6.218	6.443	100.00%
6.443	6.579	100.00%
6.579	6.656	100.00%
6.656	6.785	100.00%
6.785	6.894	100.00%
6.894	7.019	100.00%
7.019	7.368	100.00%
7.368	7.497	100.00%
7.497	8.899	100.00%

Signal #2


2.876	3.386	100.00%
3.386	3.720	100.00%
3.720	4.015	100.00%
4.015	4.071	98.82%
4.071	4.251	100.00%
4.251	4.357	100.00%
4.357	4.859	100.00%
4.859	5.112	100.00%
5.112	5.176	99.40%
5.176	5.233	97.39%
5.233	5.360	100.00%
5.360	5.499	100.00%
5.499	5.776	100.00%
5.776	5.915	100.00%
5.915	6.068	100.00%
6.068	6.170	100.00%
6.170	6.247	100.00%
6.247	6.471	100.00%
6.471	6.741	100.00%
6.741	6.981	100.00%
6.981	8.058	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100924\
Data File : PD085946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2024 13:22
Operator : AR\AJ
Sample : RESC049
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 17:24:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

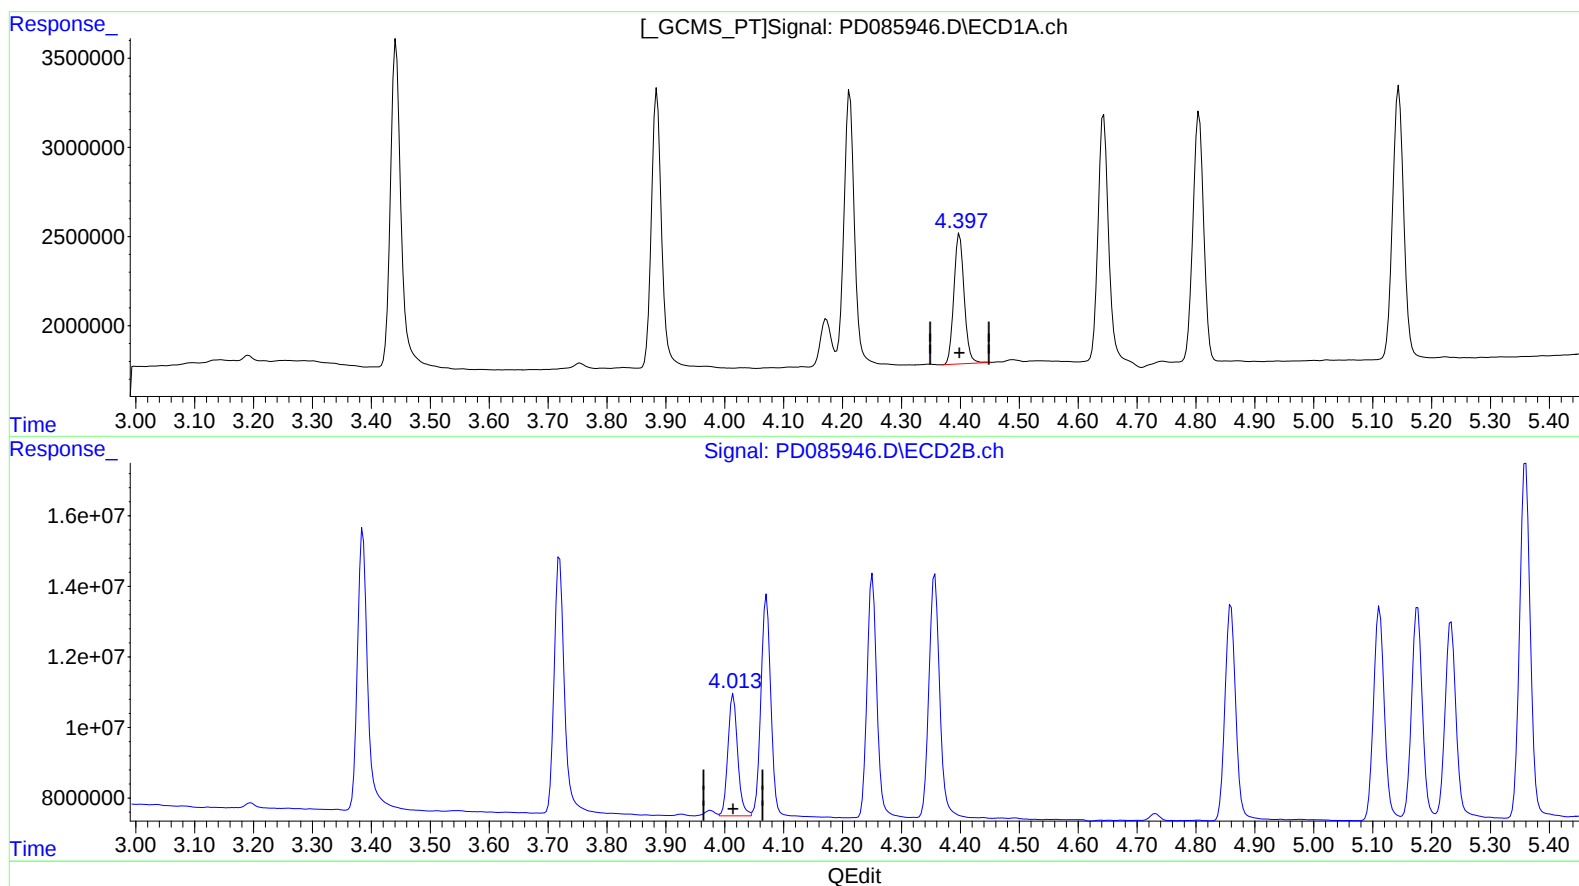

(6) beta-BHC (B)
4.399min 8.459 ng/ml
response 8911927


(6) beta-BHC #2 (B)
4.015min 8.767 ng/ml
response 39539066

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100924\
Data File : PD085946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2024 13:22
Operator : AR\AJ
Sample : RESC049
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 17:24:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

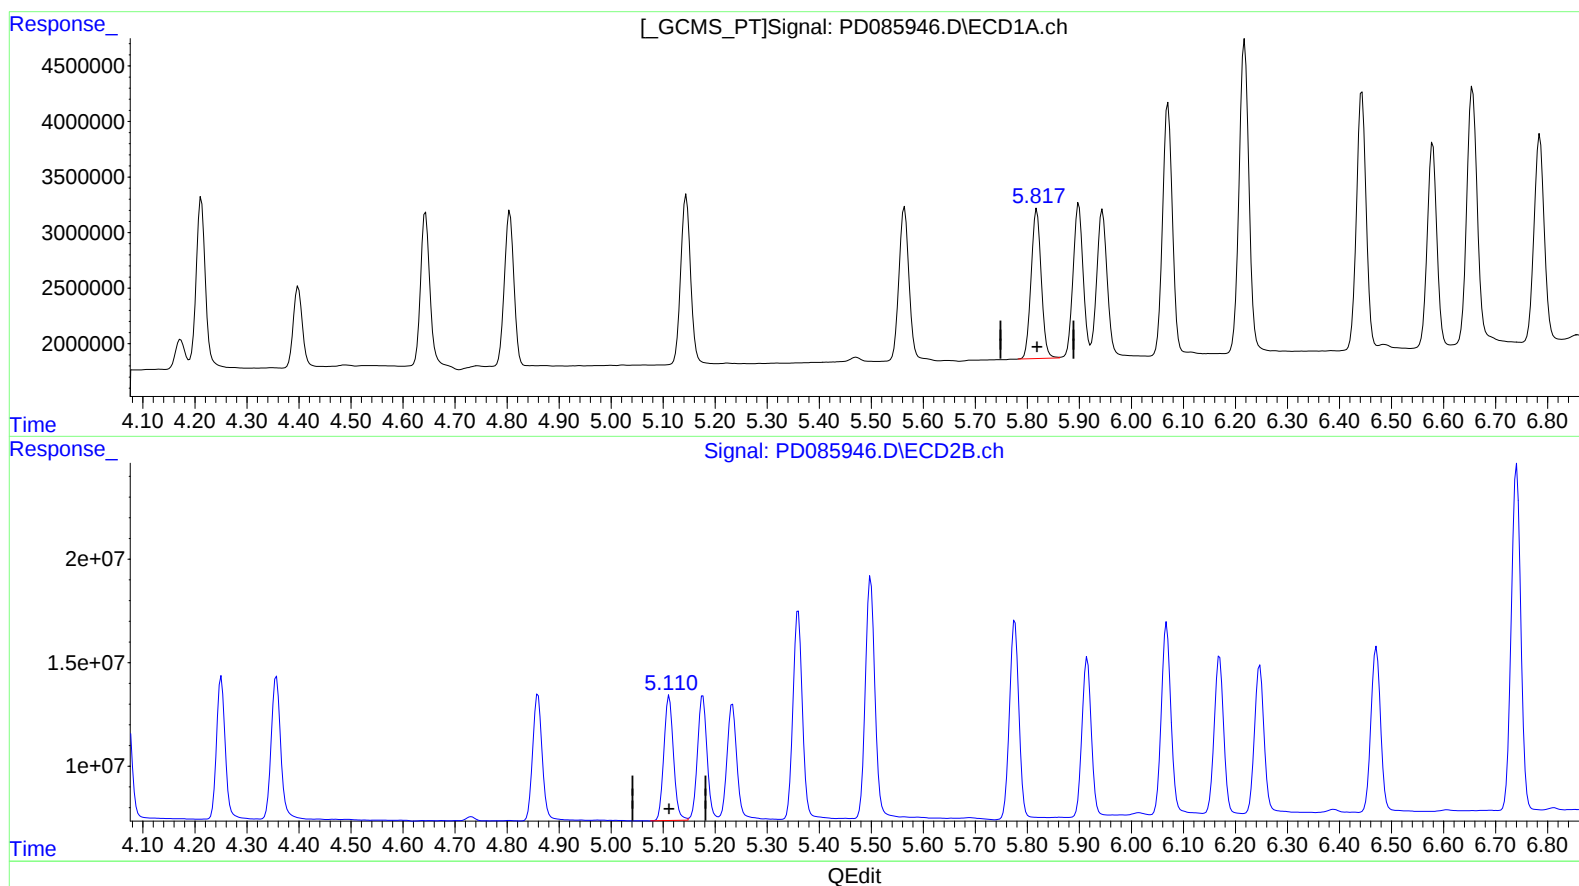

(10) trans-Chlordane (B)

5.818min 8.080 ng/ml

response 18158911

(10) trans-Chlordane #2 (B)

5.112min 8.596 ng/ml


response 77326325

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100924\
Data File : PD085946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Oct 2024 13:22
Operator : AR\AJ
Sample : RESC049
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 09 17:24:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100924CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 09 17:21:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

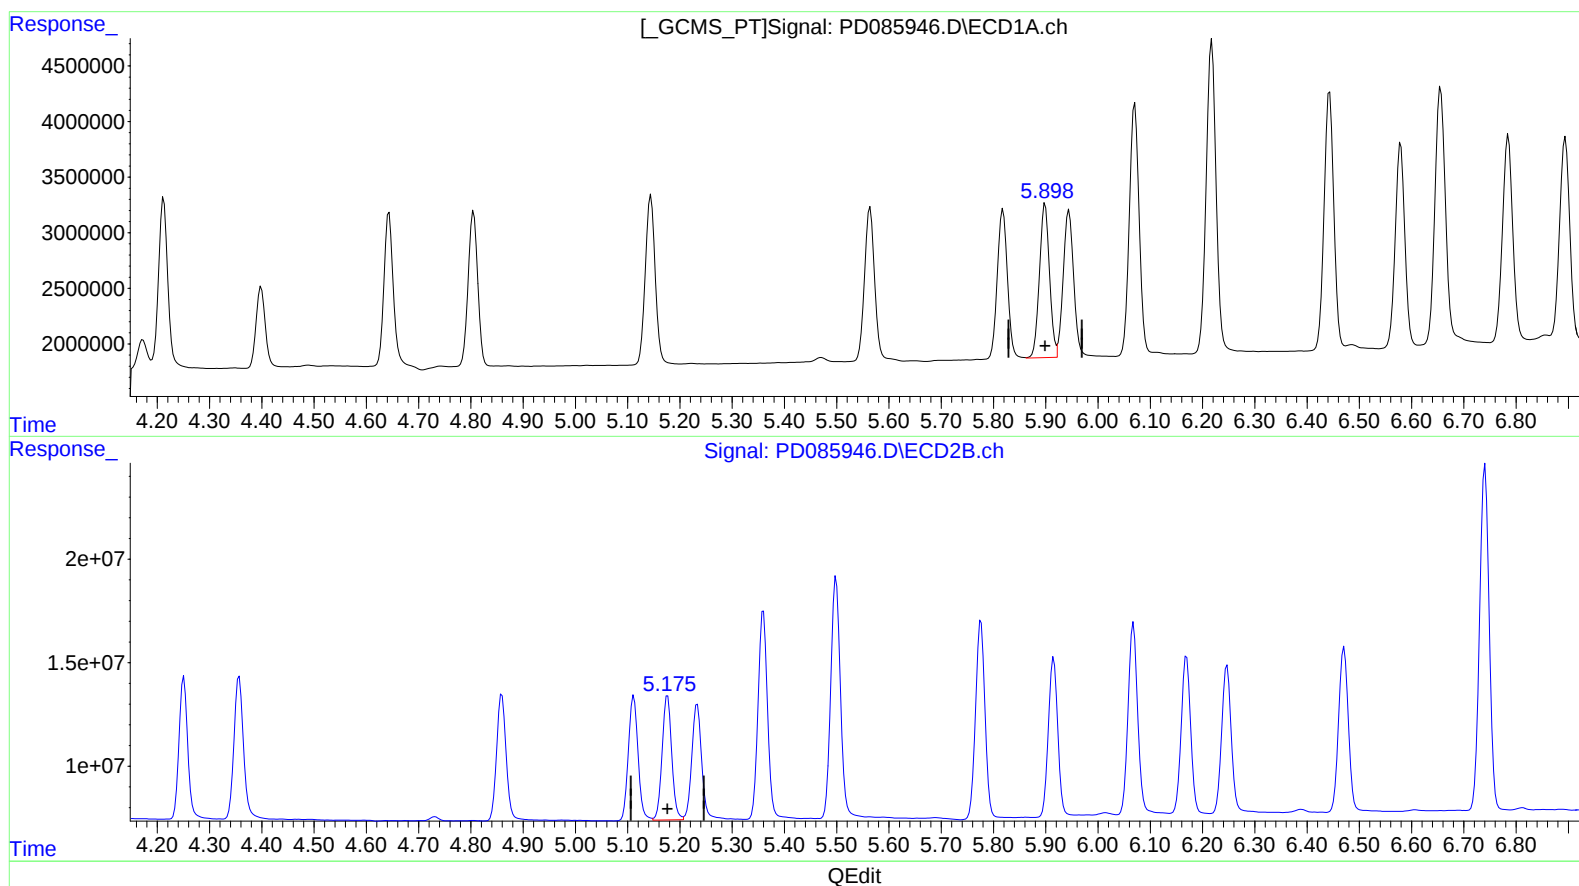

(11) cis-Chlordane (B)

5.899min 8.135 ng/ml

response 18554326

(11) cis-Chlordane #2 (B)

5.176min 8.560 ng/ml

response 76846024