

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
 Data File : PD055233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 16:56
 Operator : SG\AJ
 Sample : K5297-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 01:25:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 06:38:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.291	3.962	12755511	19358794	16.269	16.911
28)	SA Decachlor...	7.968	8.996	9271037	13451889	10.747	11.044
Target Compounds							
5)	MB Aldrin	4.506	0.000	936952	0	0.933	N.D. #
9)	A Endosulfan I	5.260f	0.000	2267415	0	2.557	N.D. #
10)	B gamma-Chl...	0.000	6.062	0	2145827	N.D.	1.401 #
11)	B alpha-Chl...	5.260f	6.131	2267415	2036402	2.342	1.342 #
15)	B Endosulfa...	6.058	6.874	677531	969791	0.767	0.719
17)	MA 4,4'-DDT	6.180f	0.000	274662	0	0.414	N.D. #
25)	Chlordane-3	0.000	6.062	0	2145827	N.D.	10.865 #
26)	Chlordane-4	5.260f	6.131	2267415	2036402	28.260	8.498 #
27)	Chlordane-5	6.058	0.000	677531	0	23.617	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
Data File : PD055233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 16:56
Operator : SG\AJ
Sample : K5297-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:25:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 06:38:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

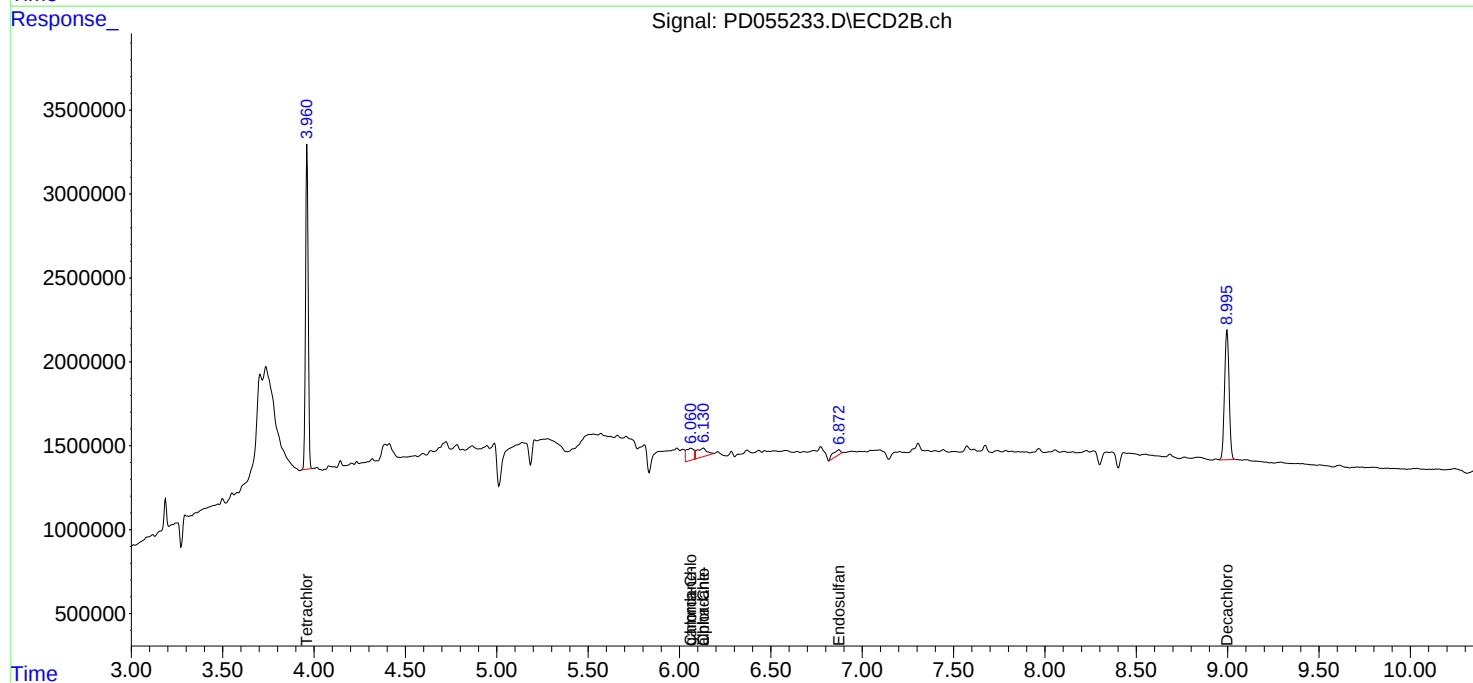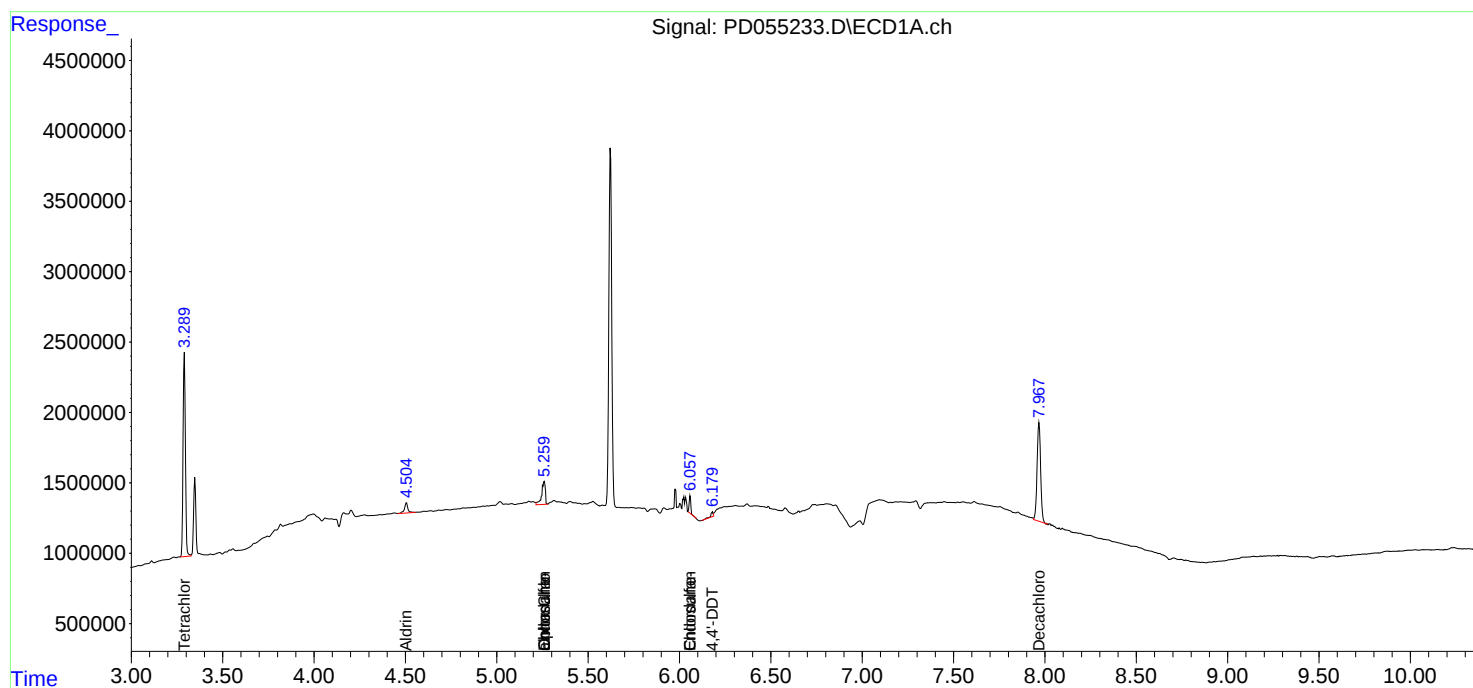


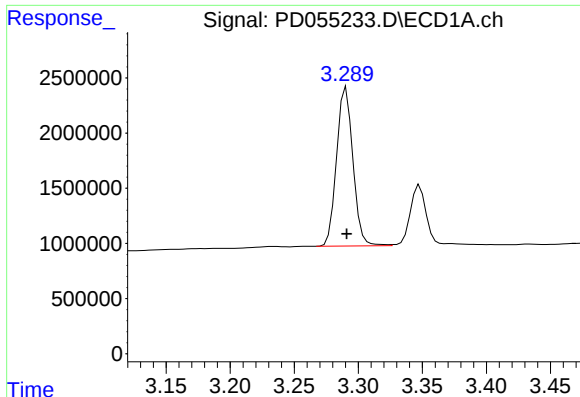

#1 Tetrachloro-m-xylene


R.T.: 3.291 min
Delta R.T.: 0.000 min
Response: 12755511
Conc: 16.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

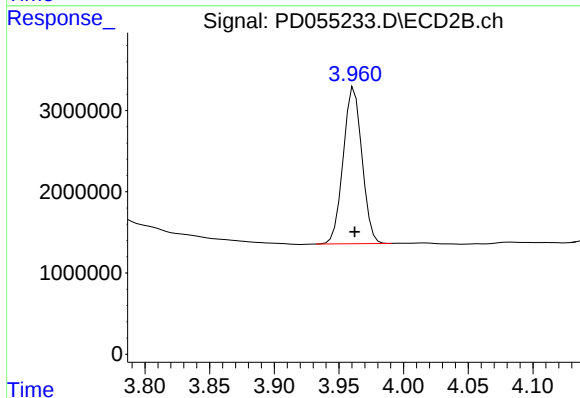


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 19358794
Conc: 16.91 ng/ml

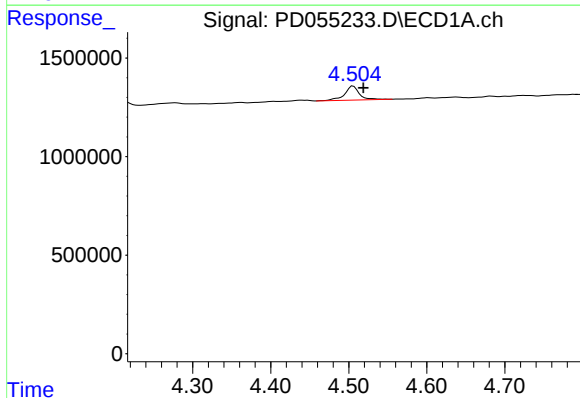


#5 Aldrin

R.T.: 4.506 min
Delta R.T.: -0.013 min
Response: 936952
Conc: 0.93 ng/ml

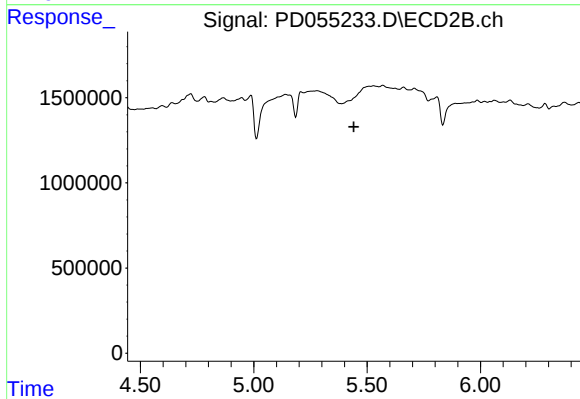

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.441 min
Response: 0
Conc: N.D.

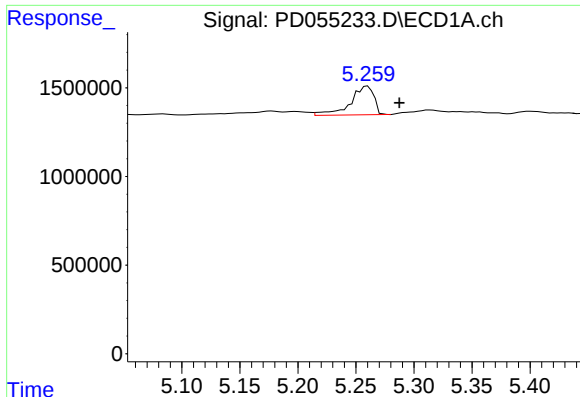

#9 Endosulfan I


R.T.: 5.260 min
Delta R.T.: -0.027 min
Response: 2267415
Conc: 2.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

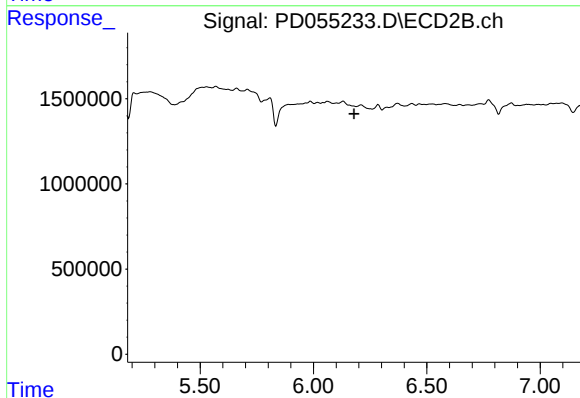


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.180 min
Response: 0
Conc: N.D.

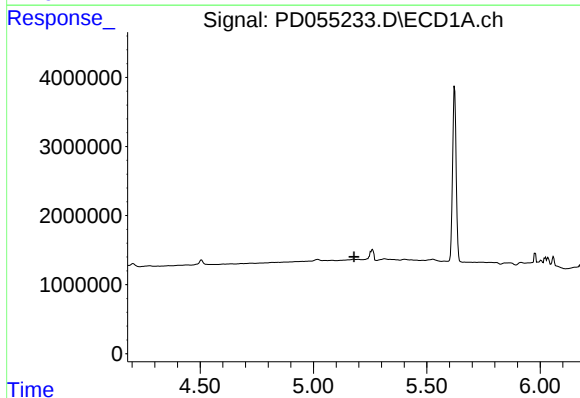


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.179 min
Response: 0
Conc: N.D.

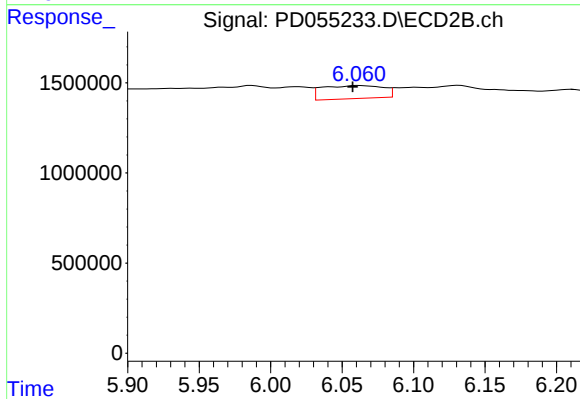

#10 gamma-Chlordane


R.T.: 6.062 min
Delta R.T.: 0.004 min
Response: 2145827
Conc: 1.40 ng/ml

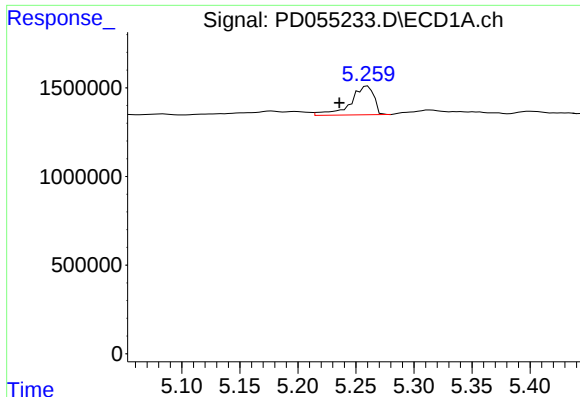

#11 alpha-Chlordane


R.T.: 5.260 min
Delta R.T.: 0.024 min
Response: 2267415
Conc: 2.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

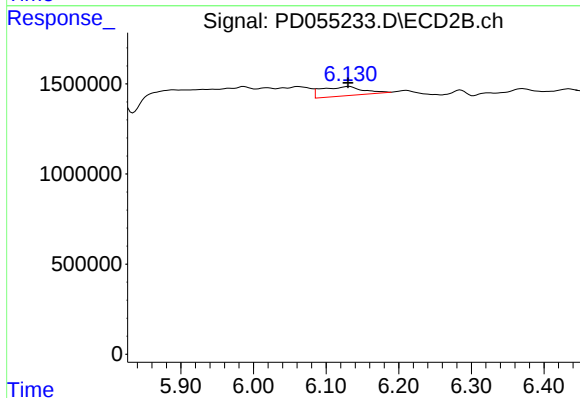


#11 alpha-Chlordane

R.T.: 6.131 min
Delta R.T.: 0.001 min
Response: 2036402
Conc: 1.34 ng/ml

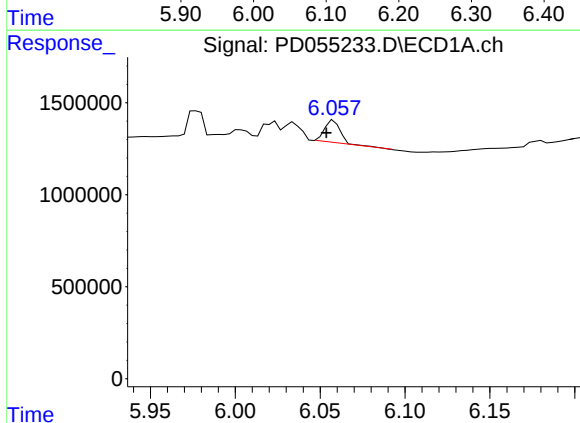


#15 Endosulfan II

R.T.: 6.058 min
Delta R.T.: 0.005 min
Response: 677531
Conc: 0.77 ng/ml

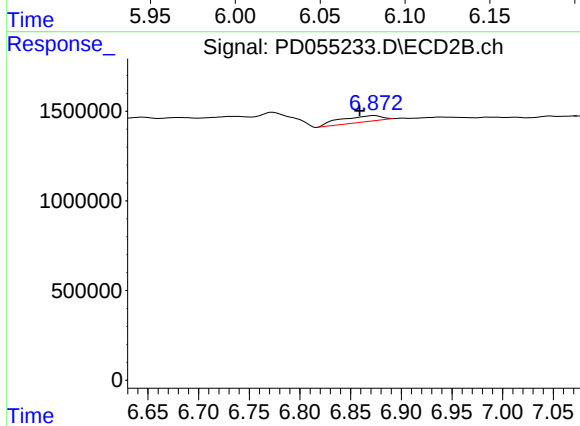

#15 Endosulfan II


R.T.: 6.874 min
Delta R.T.: 0.015 min
Response: 969791
Conc: 0.72 ng/ml

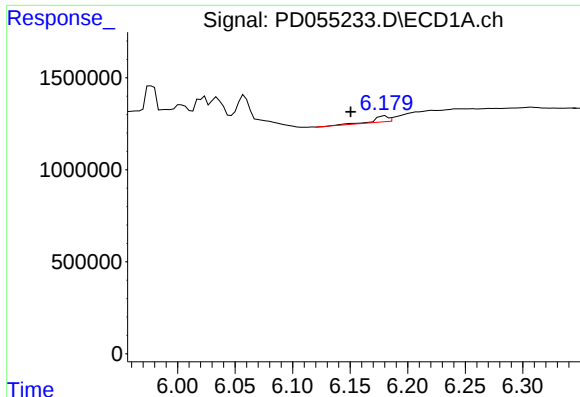

#17 4,4'-DDT


R.T.: 6.180 min
Delta R.T.: 0.030 min
Response: 274662
Conc: 0.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

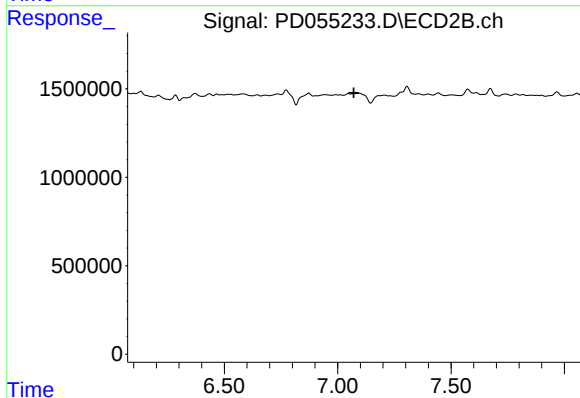


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.072 min
Response: 0
Conc: N.D.

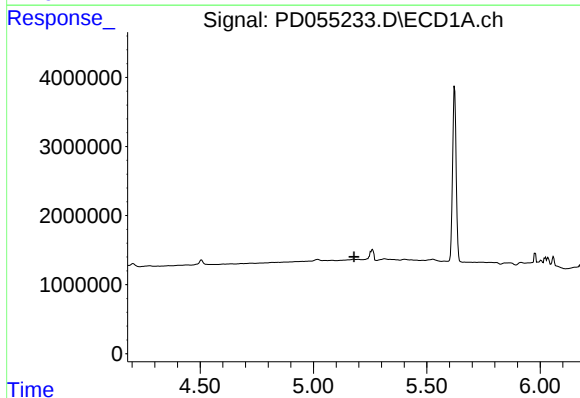


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.179 min
Response: 0
Conc: N.D.

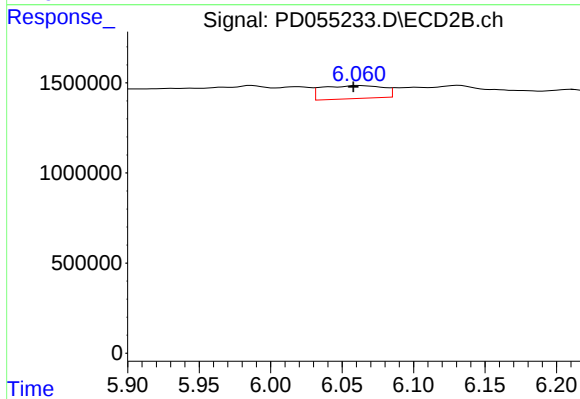

#25 Chlordane-3


R.T.: 6.062 min
Delta R.T.: 0.004 min
Response: 2145827
Conc: 10.87 ng/ml

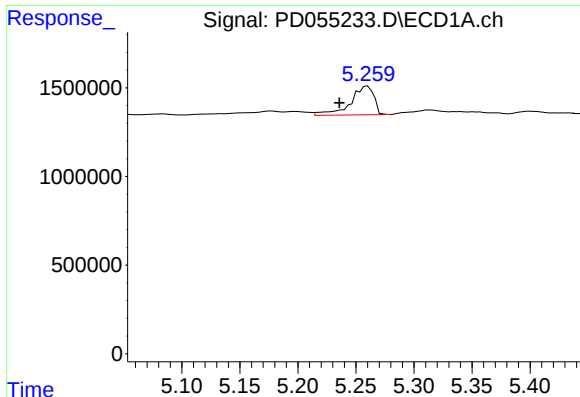

#26 Chlordane-4


R.T.: 5.260 min
Delta R.T.: 0.024 min
Response: 2267415
Conc: 28.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

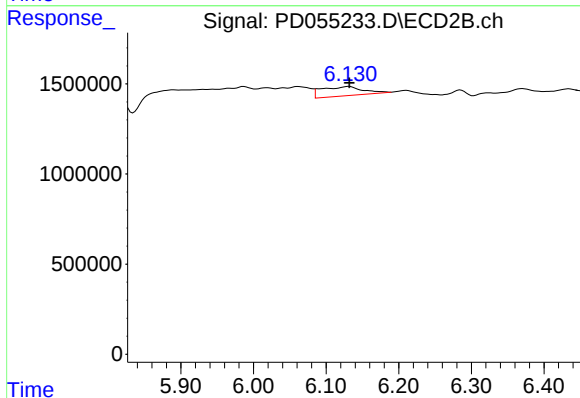


#26 Chlordane-4

R.T.: 6.131 min
Delta R.T.: 0.000 min
Response: 2036402
Conc: 8.50 ng/ml

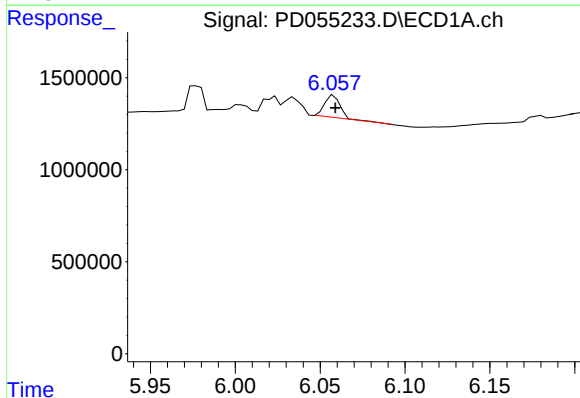


#27 Chlordane-5

R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 677531
Conc: 23.62 ng/ml

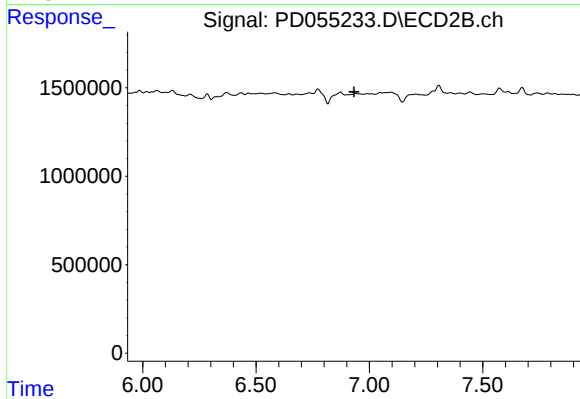

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.932 min
Response: 0
Conc: N.D.

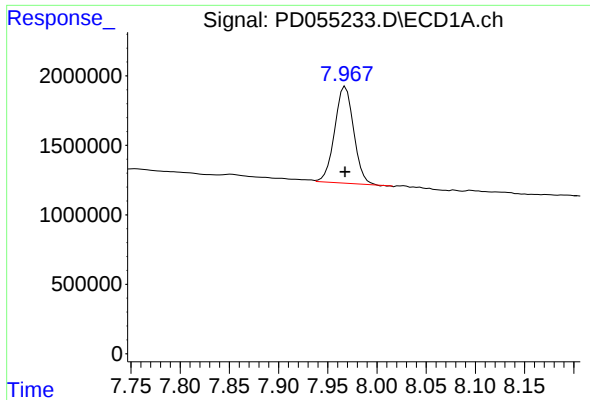

#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 9271037
Conc: 10.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

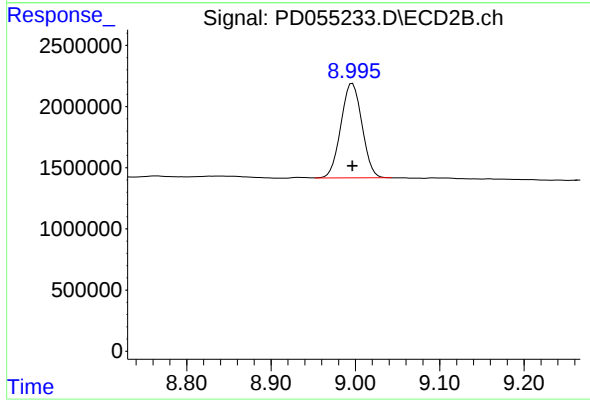

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 13451889
Conc: 11.04 ng/ml