

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
 Data File : PD055238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 18:06
 Operator : SG\AJ
 Sample : K5298-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 01:26:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 06:38:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.962	11731326	18009787	14.963	15.733
28)	SA Decachlor...	7.967	8.996	12962119	18697903	15.026	15.351
Target Compounds							
10)	B gamma-Chl...	0.000	6.037f	0	4058131	N.D.	2.649 #
11)	B alpha-Chl...	0.000	6.102f	0	2496573	N.D.	1.646 #
19)	B Endosulfa...	6.411f	0.000	443226	0	0.548	N.D. #
25)	Chlordane-3	0.000	6.037f	0	4058131	N.D.	20.549 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
Data File : PD055238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 18:06
Operator : SG\AJ
Sample : K5298-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:26:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 06:38:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

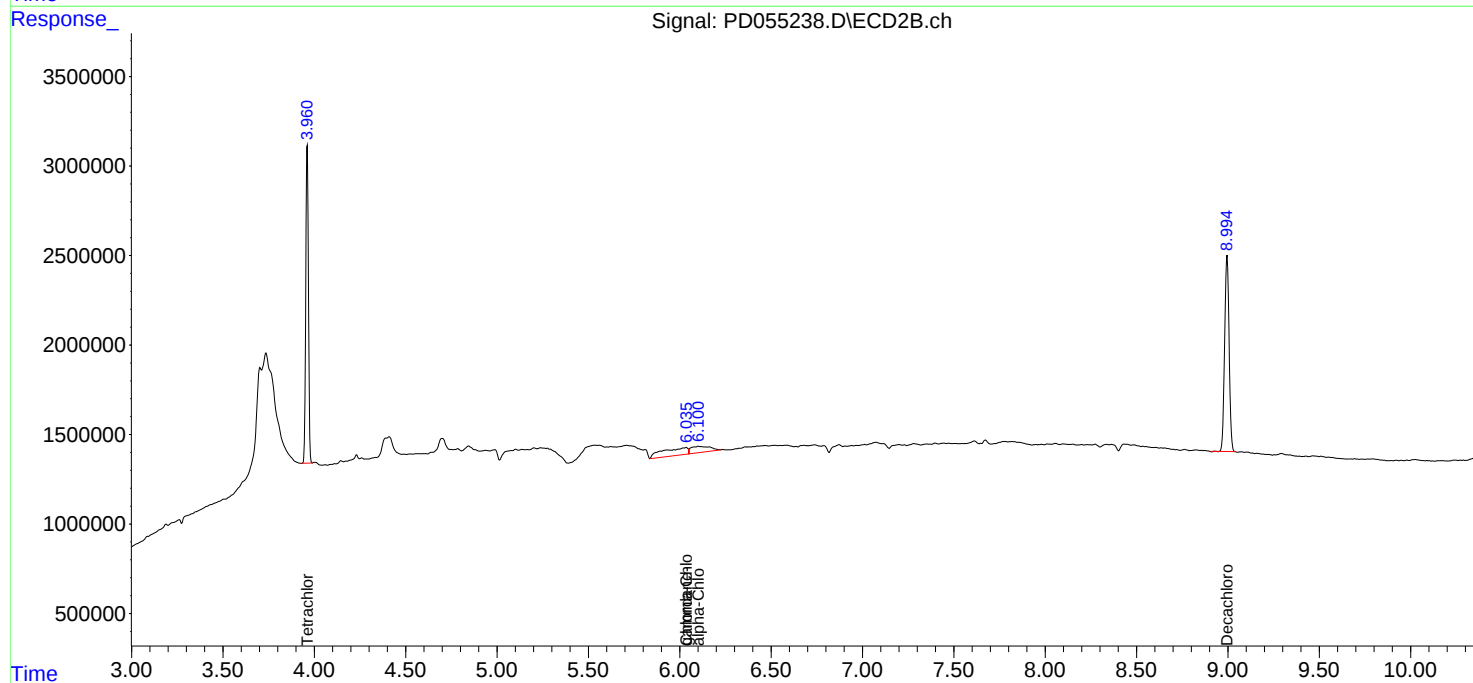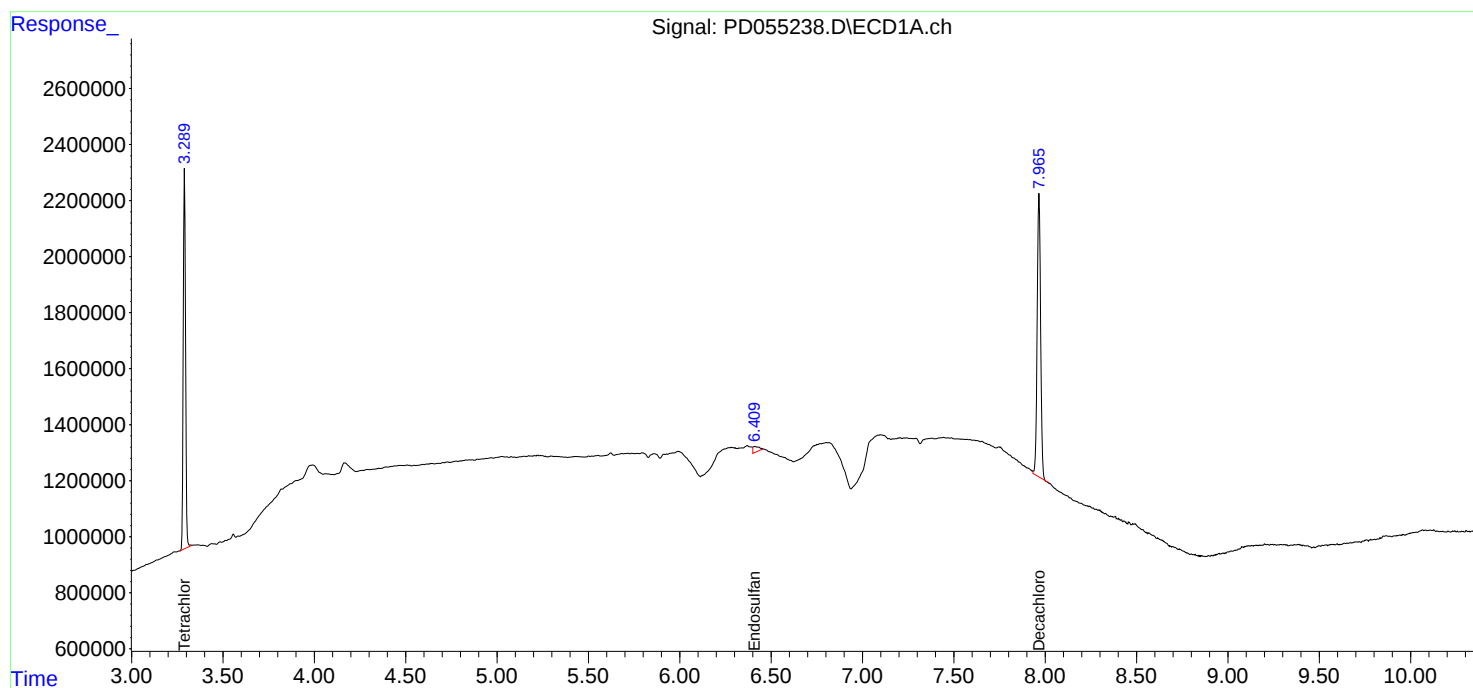


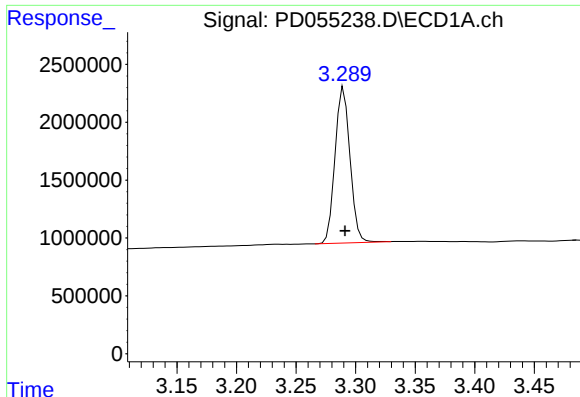

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 11731326
Conc: 14.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

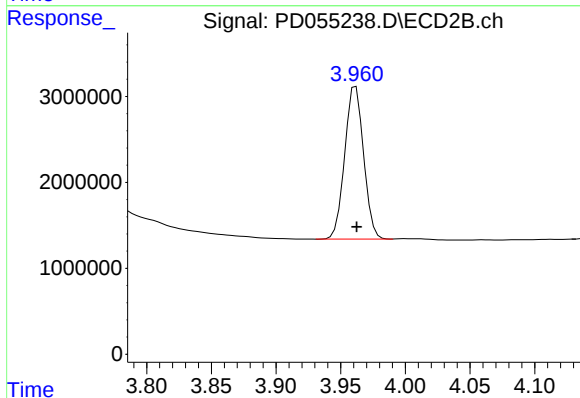


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 18009787
Conc: 15.73 ng/ml

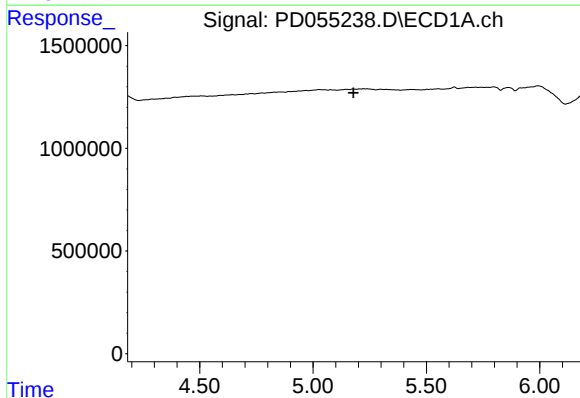


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.179 min
Response: 0
Conc: N.D.

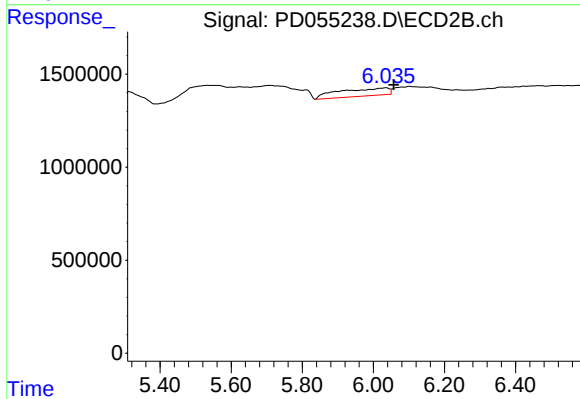

#10 gamma-Chlordane


R.T.: 6.037 min
Delta R.T.: -0.021 min
Response: 4058131
Conc: 2.65 ng/ml

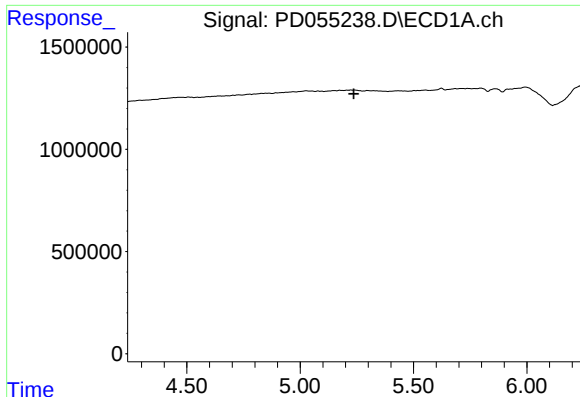

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

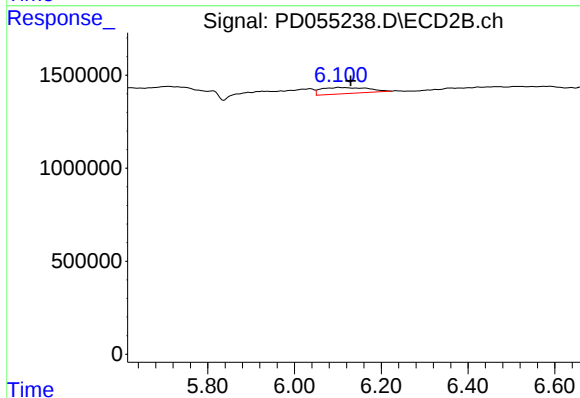


#11 alpha-Chlordane

R.T.: 6.102 min
Delta R.T.: -0.028 min
Response: 2496573
Conc: 1.65 ng/ml

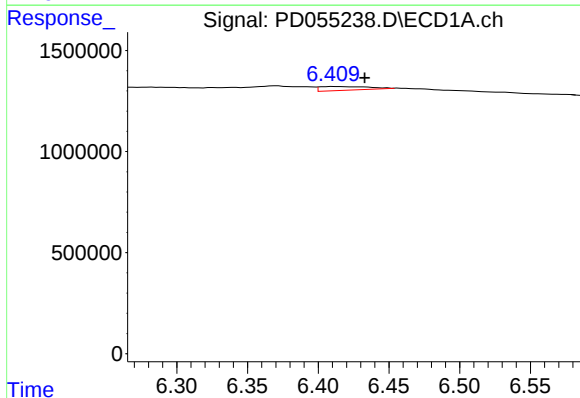


#19 Endosulfan Sulfate

R.T.: 6.411 min
Delta R.T.: -0.022 min
Response: 443226
Conc: 0.55 ng/ml

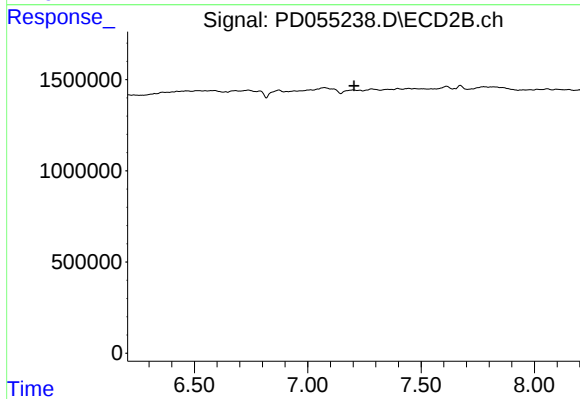

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.205 min
Response: 0
Conc: N.D.

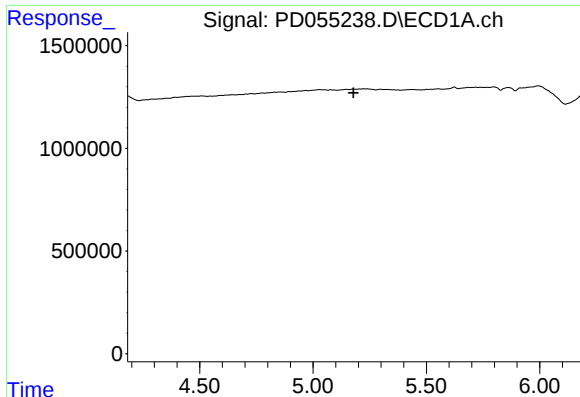

#25 Chloroform-3


R.T.: 0.000 min
Exp R.T.: 5.179 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

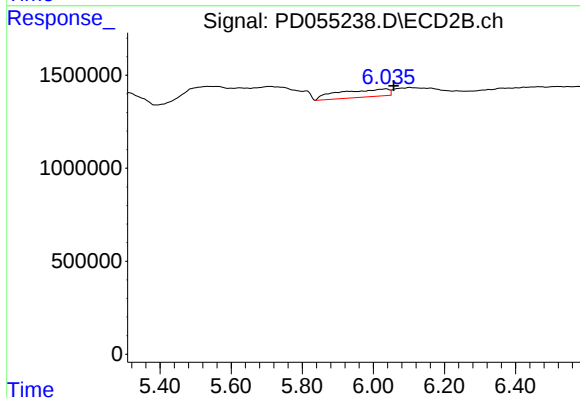


#25 Chloroform-3

R.T.: 6.037 min
Delta R.T.: -0.021 min
Response: 4058131
Conc: 20.55 ng/ml

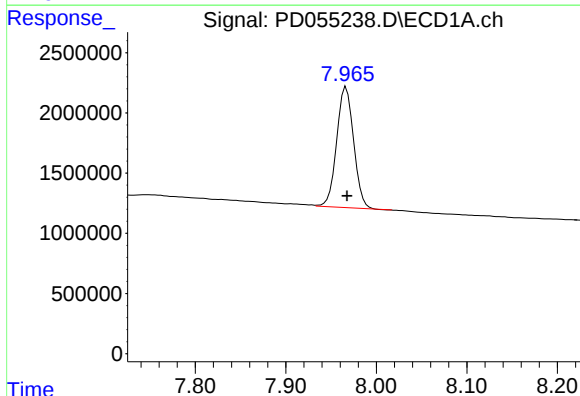

#28 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: -0.001 min
Response: 12962119
Conc: 15.03 ng/ml

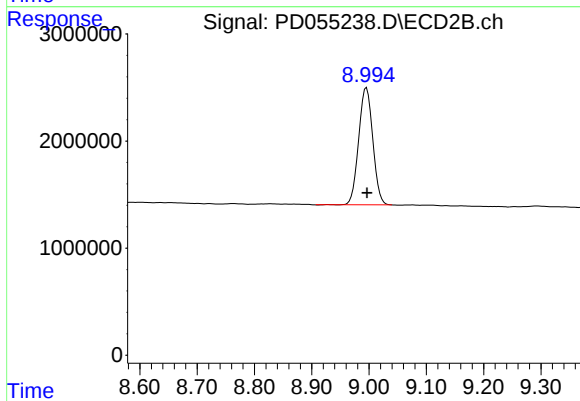

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.000 min
Response: 18697903
Conc: 15.35 ng/ml