

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
 Data File : PD055242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 19:02
 Operator : SG\AJ
 Sample : K5298-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 01:27:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 06:38:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.962	14668995	22560700	18.710	19.709
28)	SA Decachlor...	7.968	8.997	16002208	22647851	18.550	18.594
Target Compounds							
10)	B gamma-Chl...	0.000	6.037f	0	4852453	N.D.	3.168 #
11)	B alpha-Chl...	0.000	6.103f	0	1287461	N.D.	0.849 #
25)	Chlordane-3	0.000	6.037f	0	4852453	N.D.	24.571 #
26)	Chlordane-4	0.000	6.103f	0	1287461	N.D.	5.373 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
Data File : PD055242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 19:02
Operator : SG\AJ
Sample : K5298-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:27:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 06:38:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

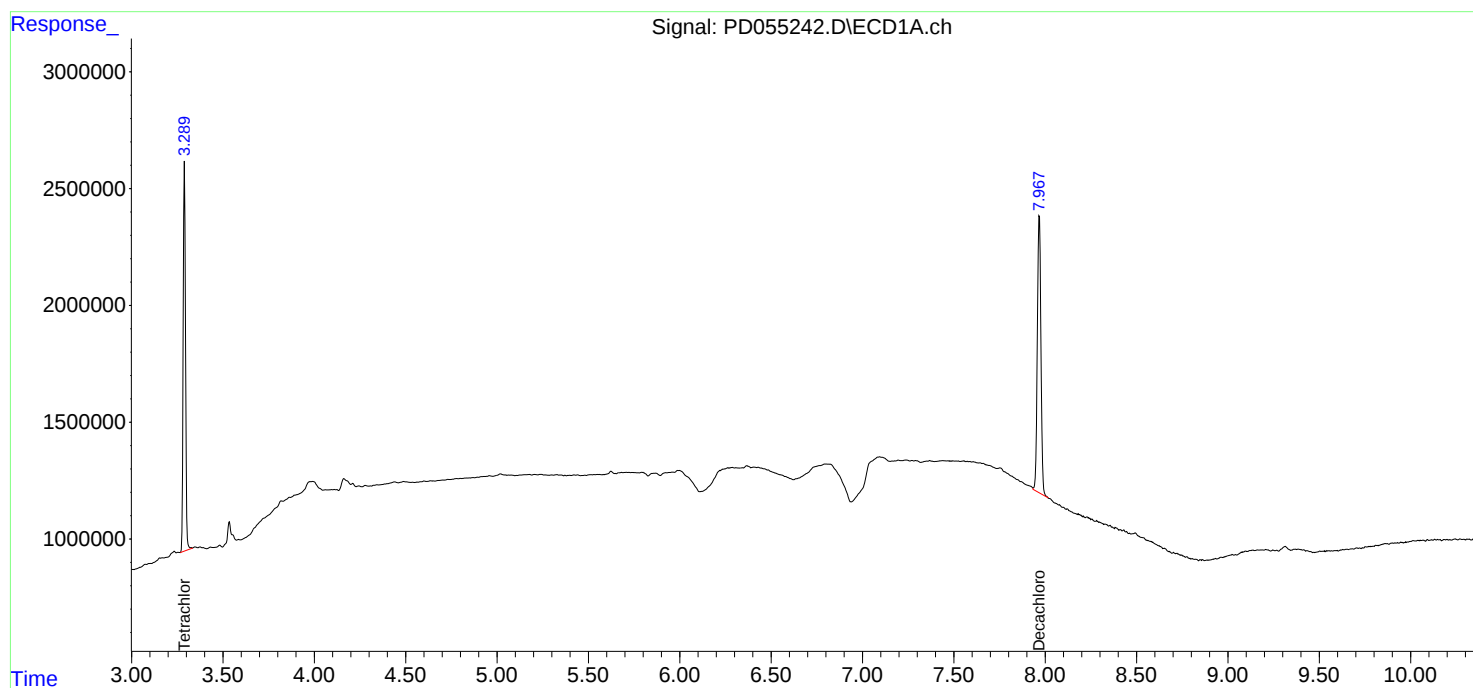


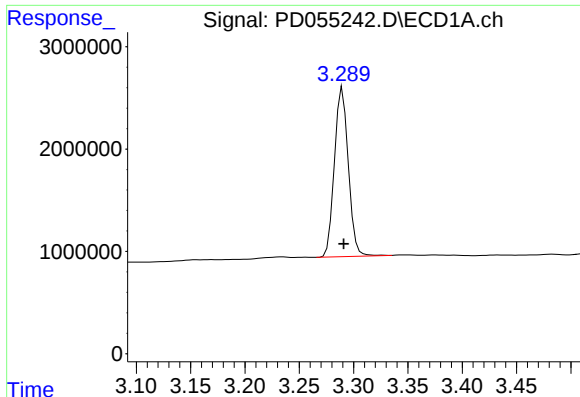

#1 Tetrachloro-m-xylene


R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 14668995
Conc: 18.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

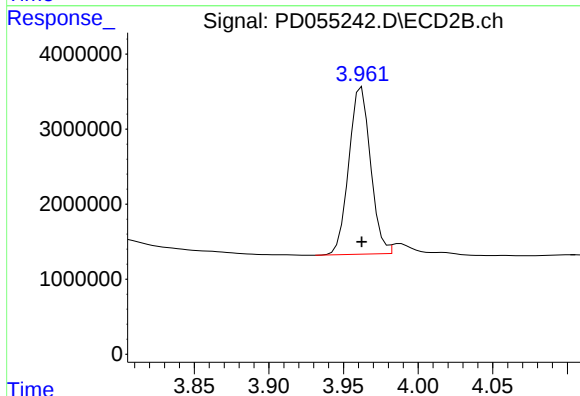


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 22560700
Conc: 19.71 ng/ml

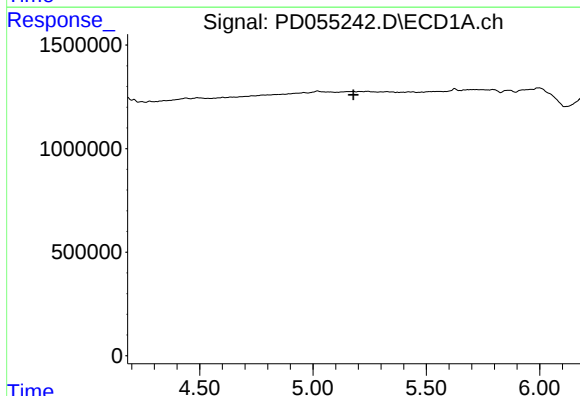


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.179 min
Response: 0
Conc: N.D.

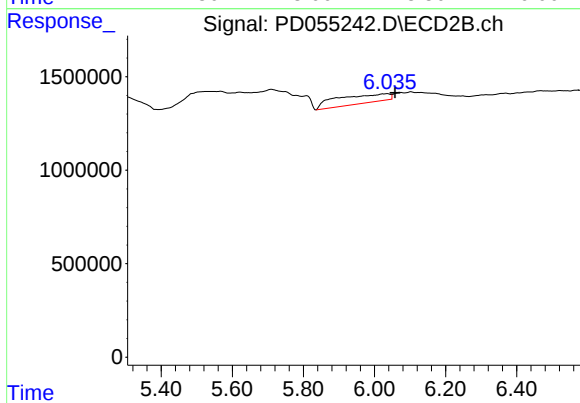

#10 gamma-Chlordane


R.T.: 6.037 min
Delta R.T.: -0.021 min
Response: 4852453
Conc: 3.17 ng/ml

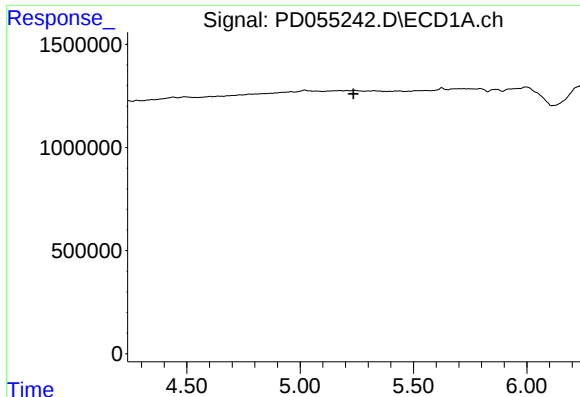

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

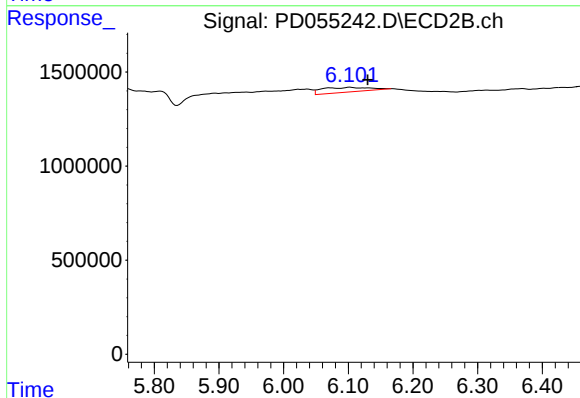


#11 alpha-Chlordane

R.T.: 6.103 min
Delta R.T.: -0.027 min
Response: 1287461
Conc: 0.85 ng/ml

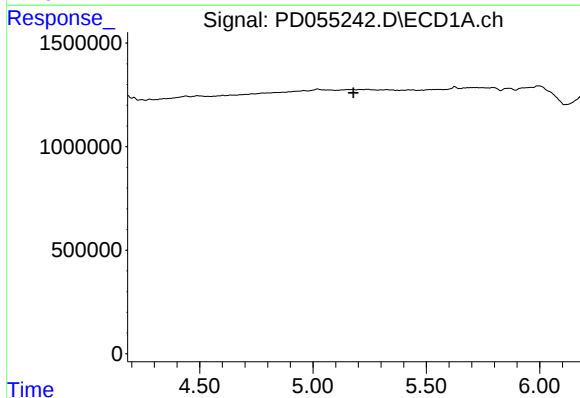


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.179 min
Response: 0
Conc: N.D.

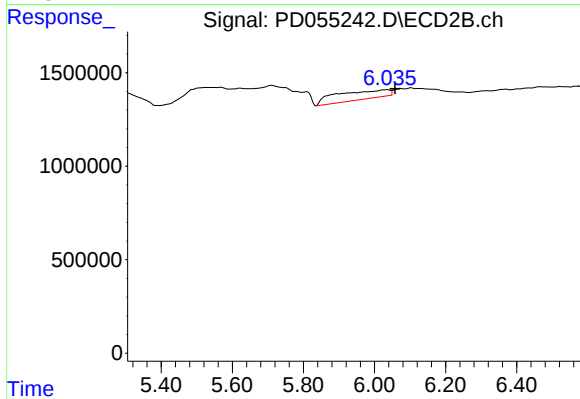

#25 Chlordane-3


R.T.: 6.037 min
Delta R.T.: -0.021 min
Response: 4852453
Conc: 24.57 ng/ml

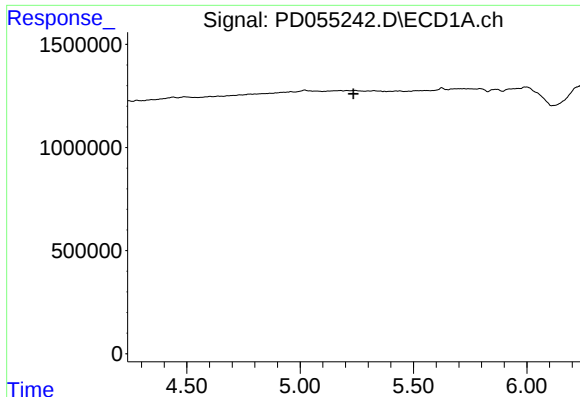

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

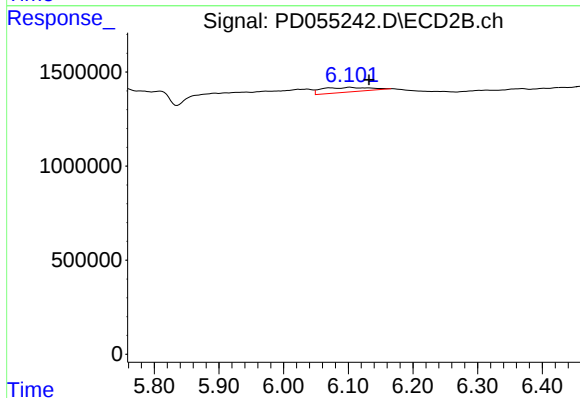


#26 Chlordane-4

R.T.: 6.103 min
Delta R.T.: -0.029 min
Response: 1287461
Conc: 5.37 ng/ml

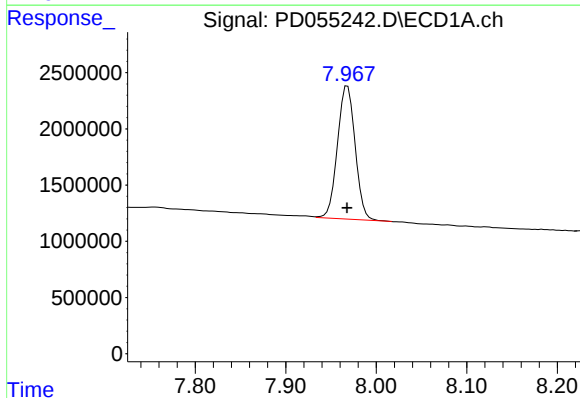

#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 16002208
Conc: 18.55 ng/ml

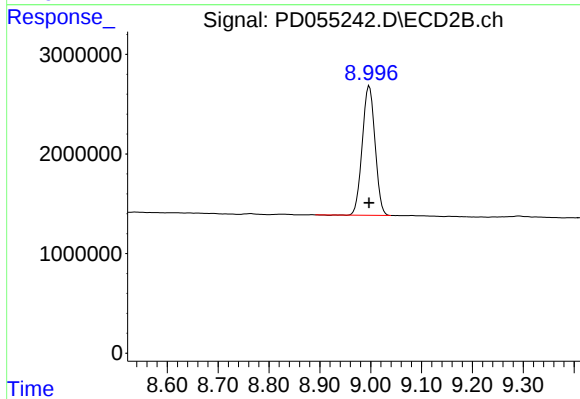

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 22647851
Conc: 18.59 ng/ml