

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
 Data File : PD055224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 14:11
 Operator : SG\AJ
 Sample : K5292-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20190855-AMENDED-COMP-B

Manual Integrations
 APPROVED

Ankita
 10/11/2019 2:09:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 01:24:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 06:38:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.962	7480550	11183785	9.541	9.770
28)	SA Decachlor...	7.967	8.995	4510872	7267369	5.229	5.967m
Target Compounds							
12)	B 4,4'-DDE	5.401	6.285	728923	1315386	0.814m	0.941

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
Data File : PD055224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 14:11
Operator : SG\AJ
Sample : K5292-03
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
20190855-AMENDED-COMP-B


Manual Integrations
APPROVED

Ankita
10/11/2019 2:09:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:24:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 06:38:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

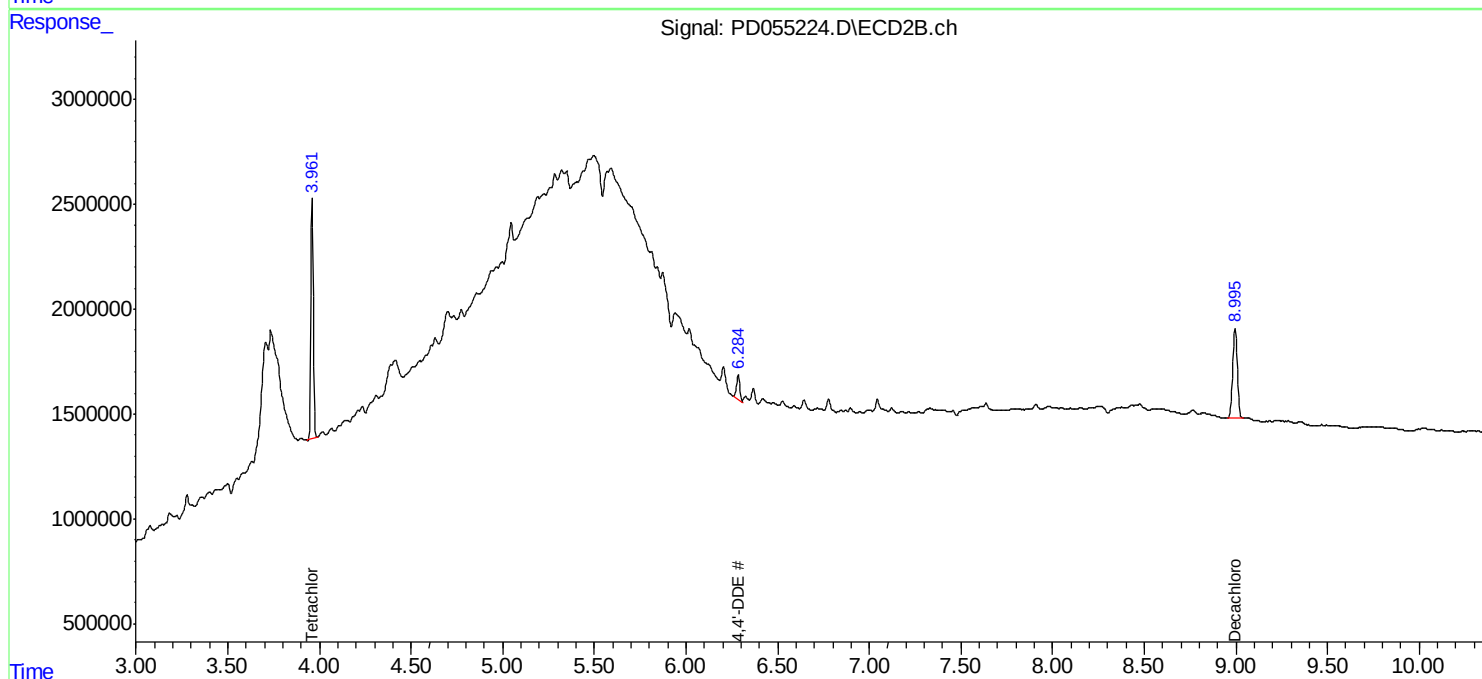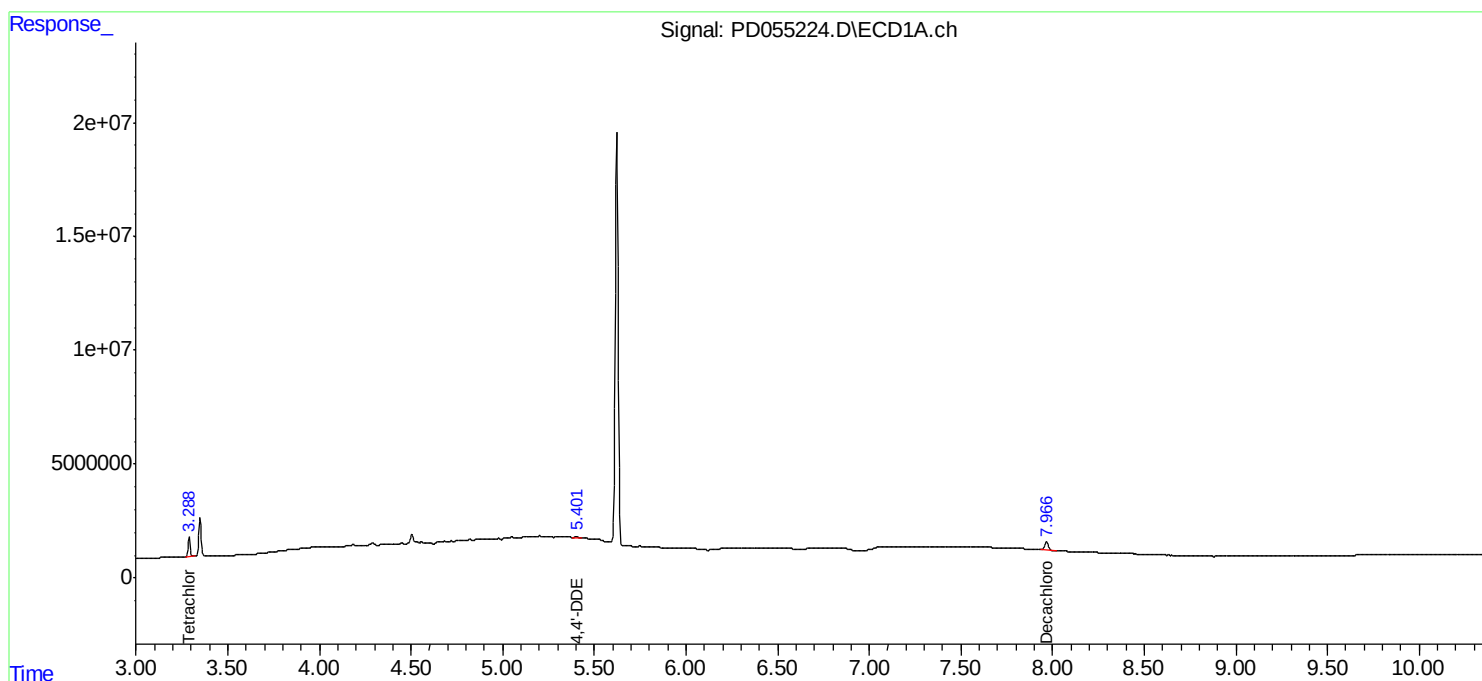

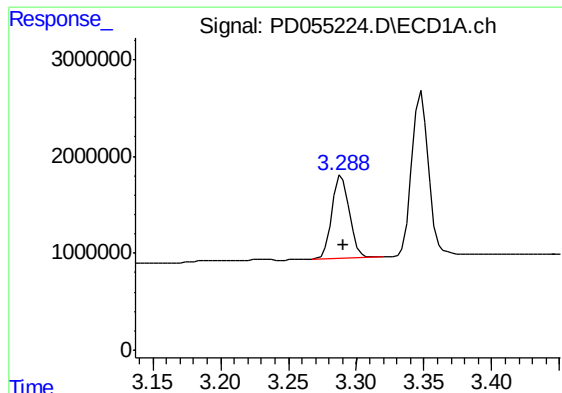


#1 Tetrachloro-m-xylene

R.T.: 3.290 min
Delta R.T.: -0.001 min
Response: 7480550
Conc: 9.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
20190855-AMENDED-COMP-B


Manual Integrations
APPROVED

Ankita
10/11/2019 2:09:25 PM

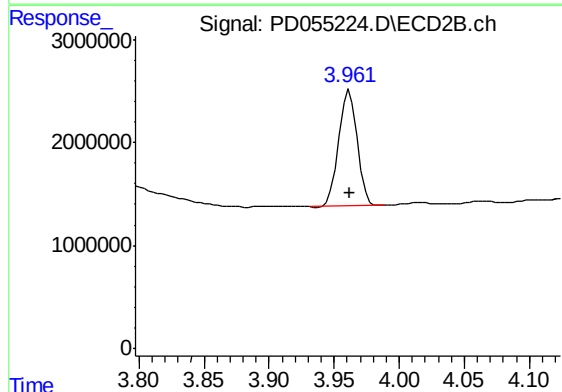


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 11183785
Conc: 9.77 ng/ml

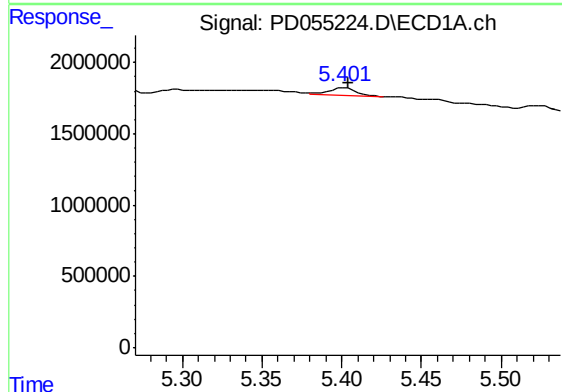


#12 4,4'-DDE

R.T.: 5.401 min
Delta R.T.: -0.003 min
Response: 728923
Conc: 0.81 ng/ml m

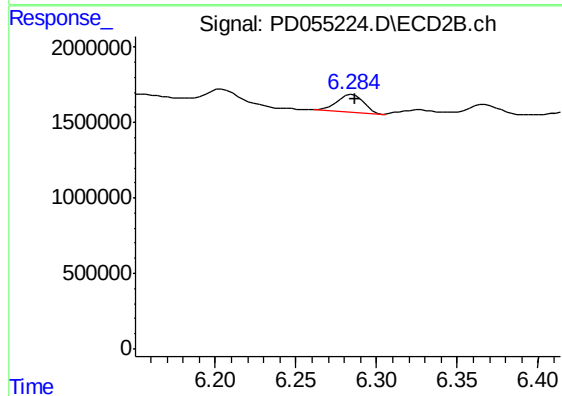

#12 4,4'-DDE

R.T.: 6.285 min
Delta R.T.: -0.001 min
Response: 1315386
Conc: 0.94 ng/ml

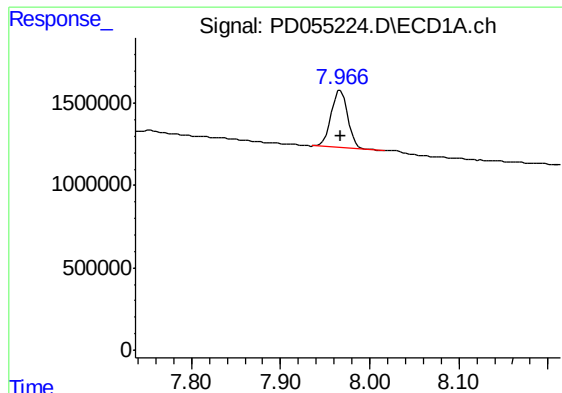


#28 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: 0.000 min
Response: 4510872
Conc: 5.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
20190855-AMENDED-COMP-B

Manual Integrations
APPROVED

Ankita
10/11/2019 2:09:25 PM

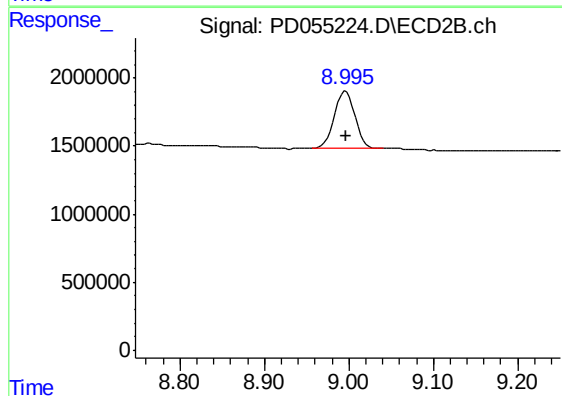

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.002 min
Response: 7267369
Conc: 5.97 ng/ml m