

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
 Data File : PD055226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 14:39
 Operator : SG\AJ
 Sample : K5292-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20190858-AMENDED-COMP-E

Manual Integrations
 APPROVED

Ankita
 10/11/2019 2:09:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 01:24:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 06:38:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.961	7584685	11728773	9.674	10.246
28)	SA Decachlor...	7.966	8.995	7710584	8907077	8.938m	7.313

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
Data File : PD055226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 14:39
Operator : SG\AJ
Sample : K5292-05
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
20190858-AMENDED-COMP-E


Manual Integrations
APPROVED

Ankita
10/11/2019 2:09:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:24:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 06:38:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

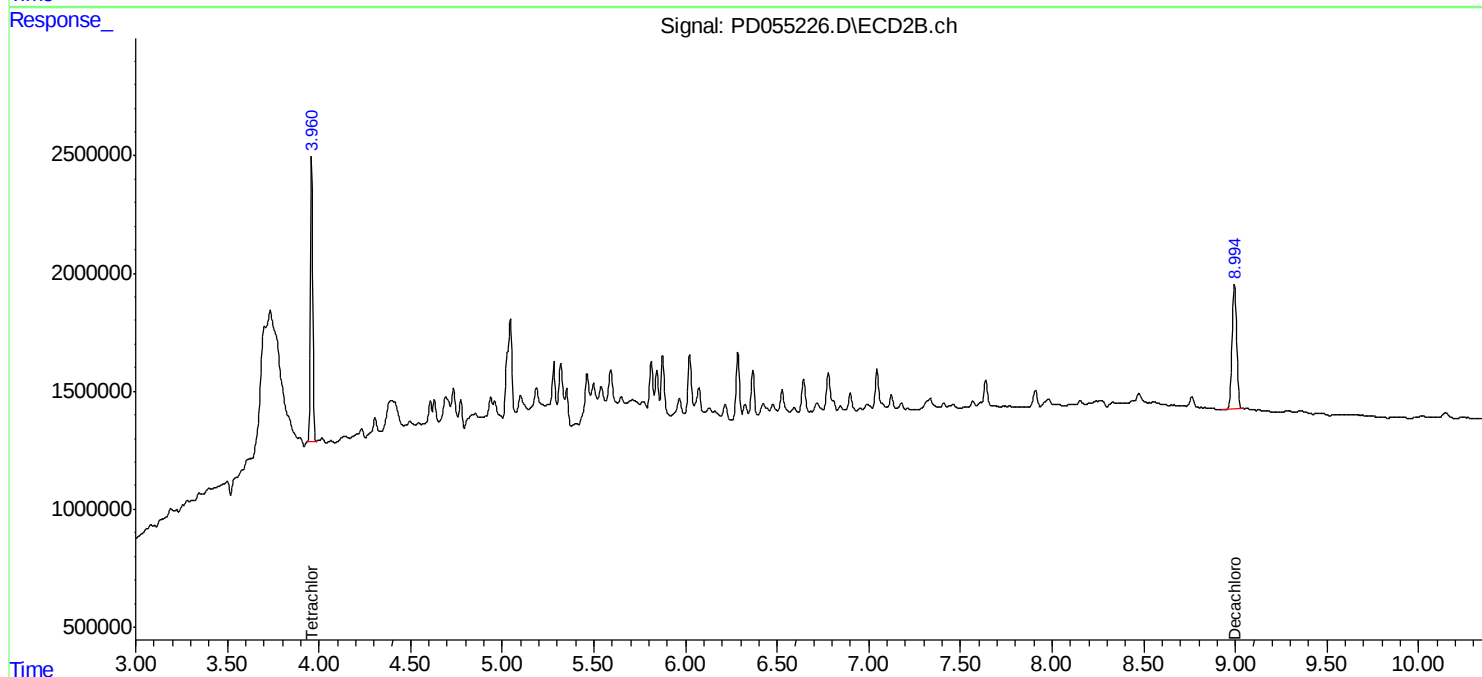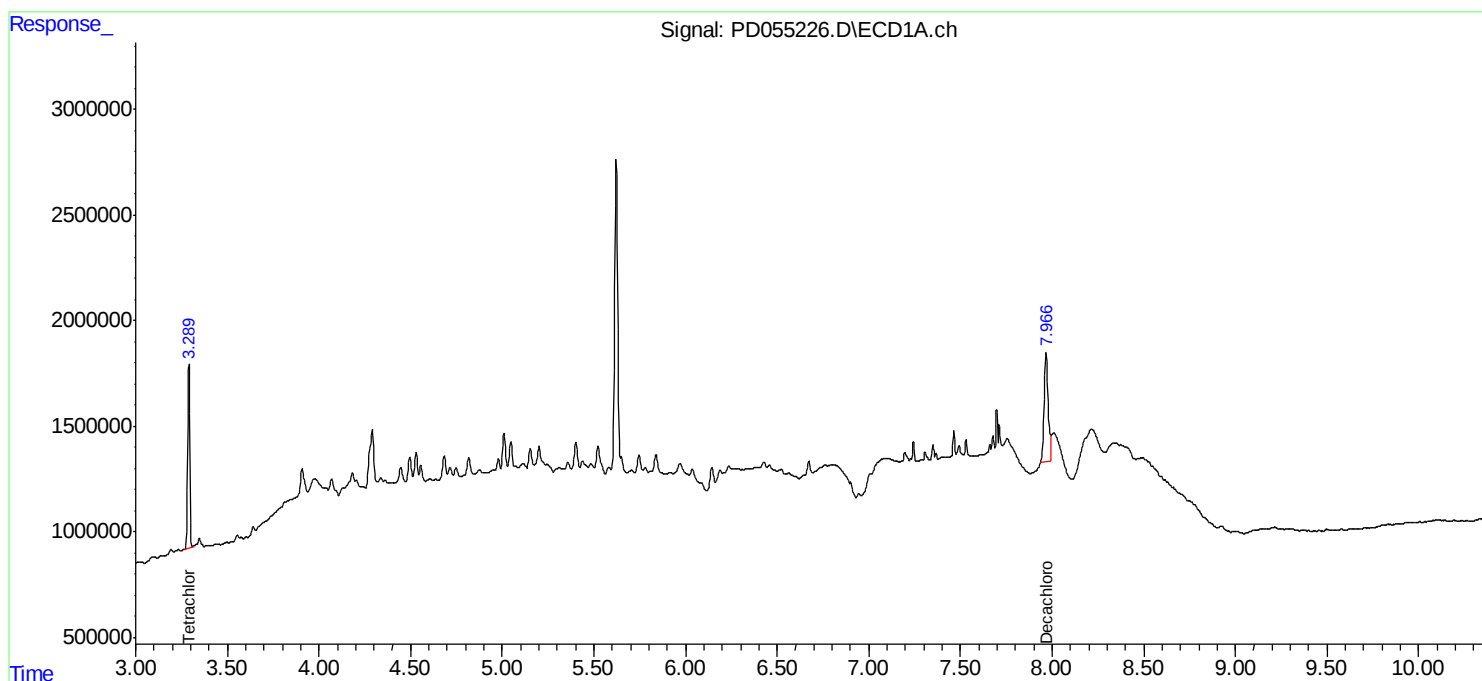

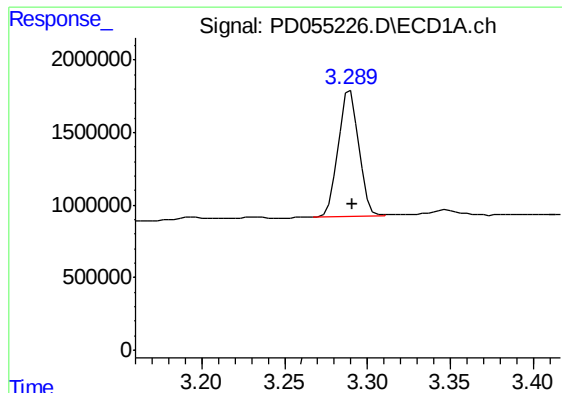


#1 Tetrachloro-m-xylene

R.T.: 3.290 min
Delta R.T.: -0.001 min
Response: 7584685
Conc: 9.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
20190858-AMENDED-COMP-E


Manual Integrations
APPROVED

Ankita
10/11/2019 2:09:27 PM

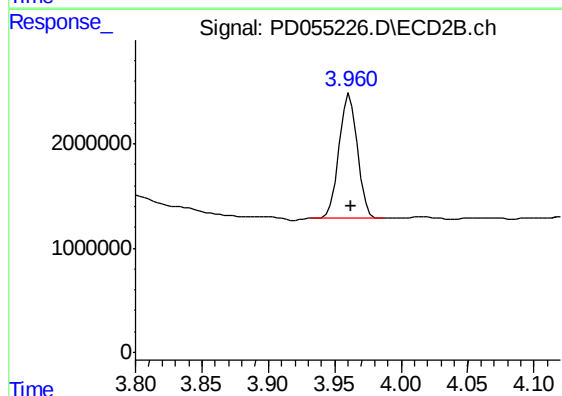


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 11728773
Conc: 10.25 ng/ml

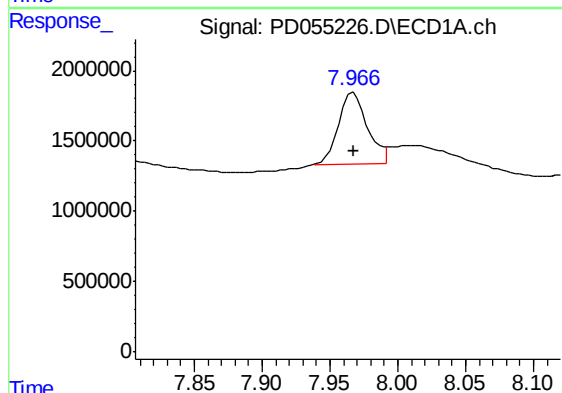

#28 Decachlorobiphenyl

R.T.: 7.966 min
Delta R.T.: -0.002 min
Response: 7710584
Conc: 8.94 ng/ml m

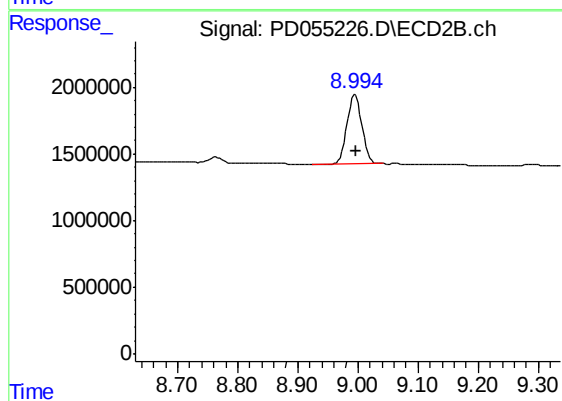

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.001 min
Response: 8907077
Conc: 7.31 ng/ml