

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
 Data File : PD055236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 17:38
 Operator : SG\AJ
 Sample : K5297-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-7

Manual Integrations
 APPROVED

Ankita
 10/11/2019 2:09:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 01:25:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 06:38:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.962	14410992	22021380	18.381	19.237
28)	SA Decachlor...	7.968	8.997	9901720	14842457	11.478	12.186
Target Compounds							
16)	A 4,4'-DDD	5.914	6.773	705060	941211	0.957m	0.780m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
Data File : PD055236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 17:38
Operator : SG\AJ
Sample : K5297-16
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-7


Manual Integrations
APPROVED

Ankita
10/11/2019 2:09:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:25:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 06:38:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

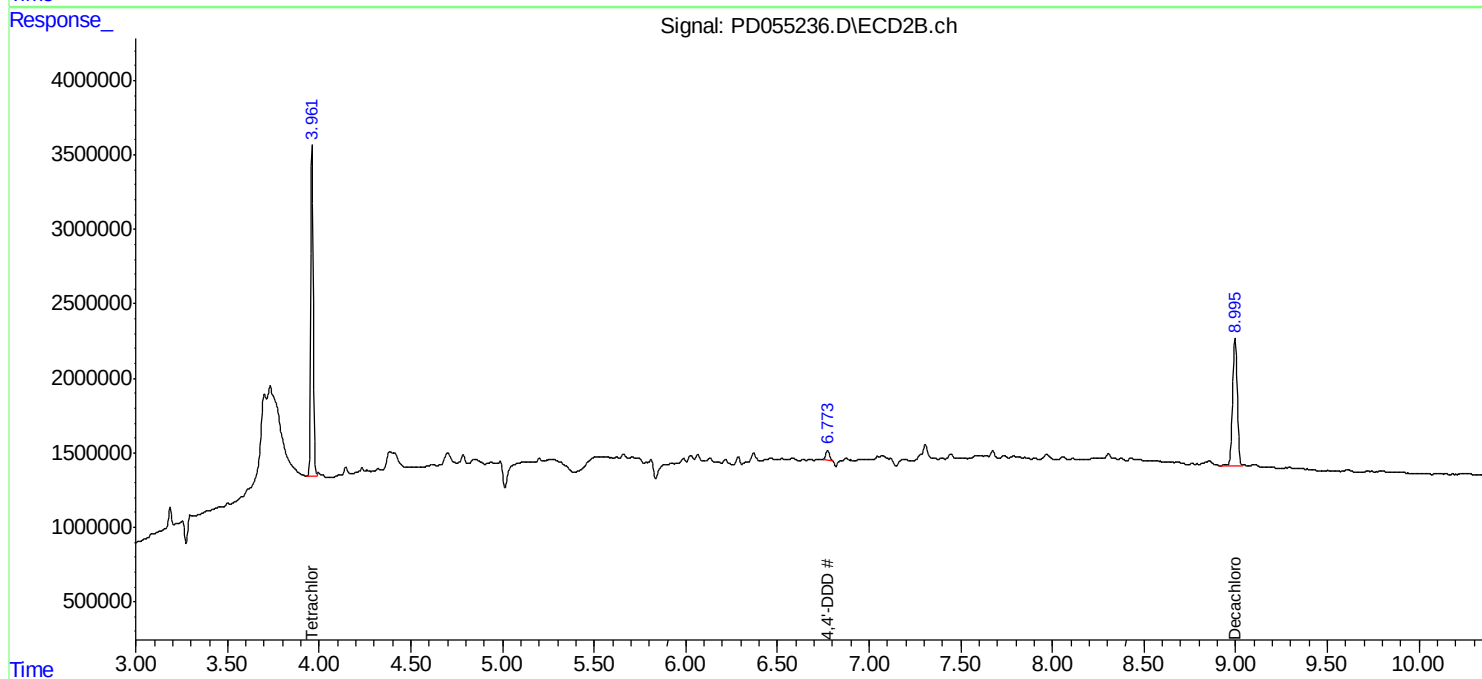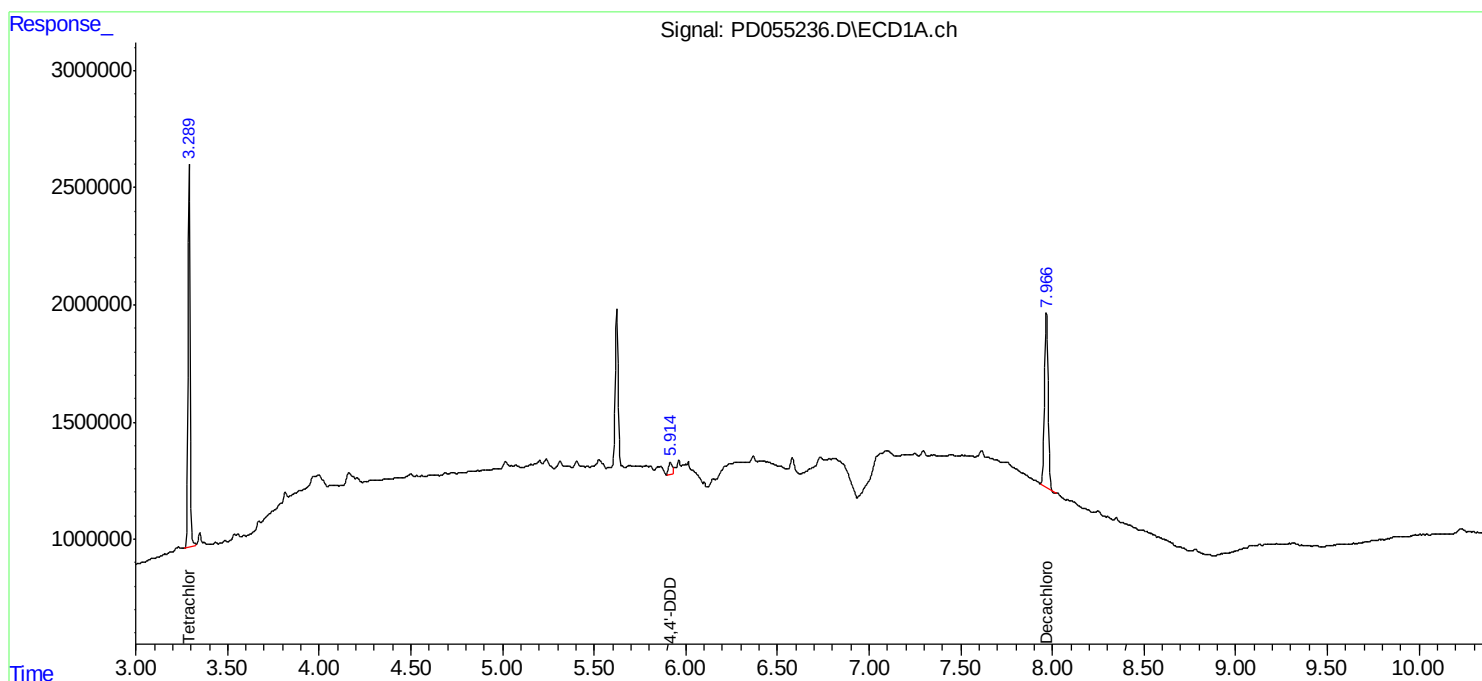

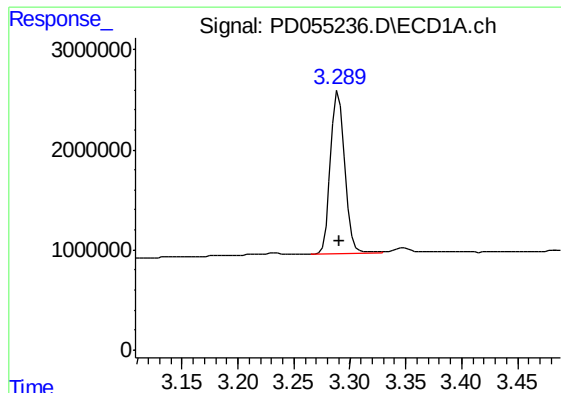


#1 Tetrachloro-m-xylene

R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 14410992
Conc: 18.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-7


Manual Integrations
APPROVED

Ankita
10/11/2019 2:09:36 PM

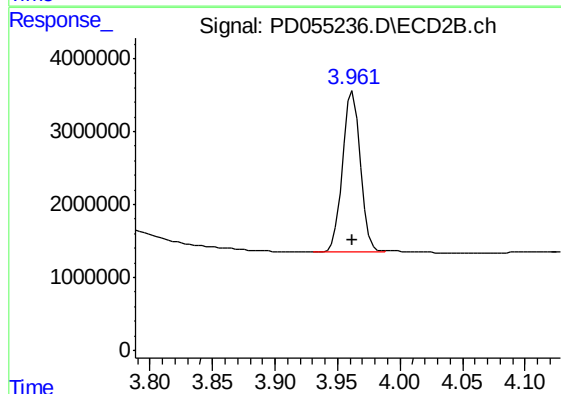


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 22021380
Conc: 19.24 ng/ml

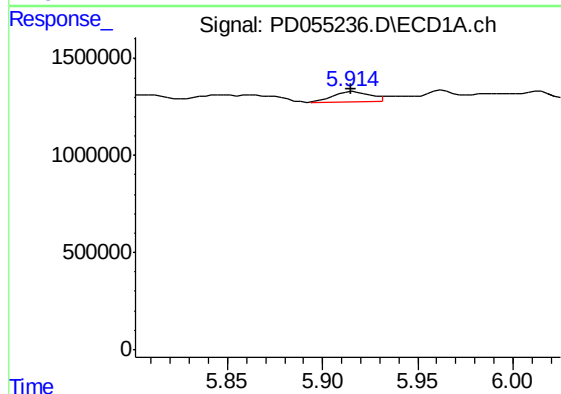


#16 4,4'-DDD

R.T.: 5.914 min
Delta R.T.: 0.000 min
Response: 705060
Conc: 0.96 ng/ml m

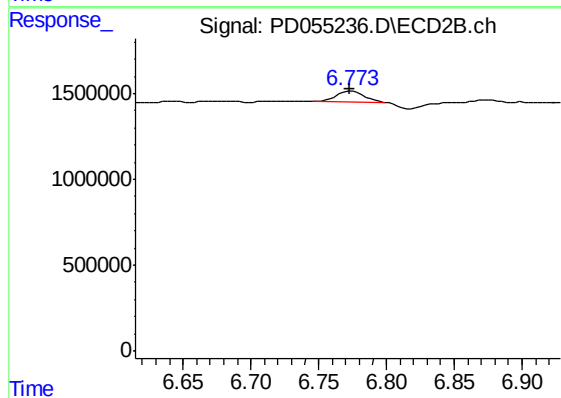

#16 4,4'-DDD

R.T.: 6.773 min
Delta R.T.: 0.000 min
Response: 941211
Conc: 0.78 ng/ml m

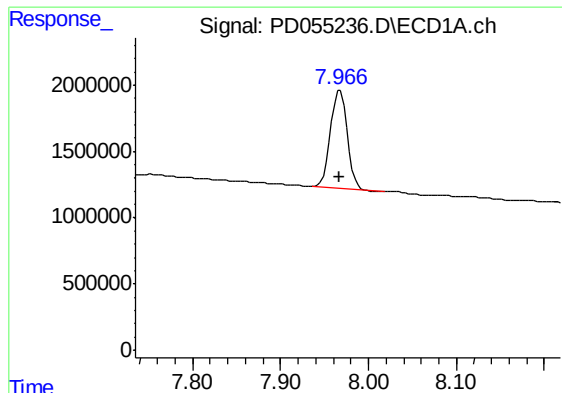


#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 9901720
Conc: 11.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-7

Manual Integrations
APPROVED

Ankita
10/11/2019 2:09:36 PM

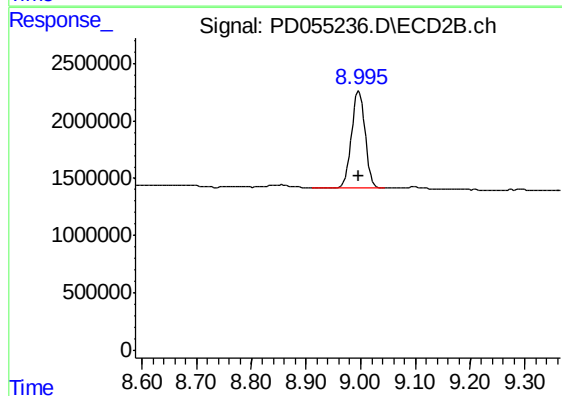

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 14842457
Conc: 12.19 ng/ml