

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
 Data File : PD055243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2019 19:16
 Operator : SG\AJ
 Sample : K5298-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-11

Manual Integrations
 APPROVED

Ankita
 10/11/2019 2:09:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 01:27:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 06:38:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.962	12332986	18933405	15.730	16.540
28)	SA Decachlor...	7.967	8.997	14327951	20994597	16.609	17.237
Target Compounds							
12)	B 4,4'-DDE	5.402	6.284	552499	1490437	0.617	1.067m#
17)	MA 4,4'-DDT	6.145	7.070	956448	756802	1.441	0.635m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101019\
Data File : PD055243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2019 19:16
Operator : SG\AJ
Sample : K5298-05
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-11


Manual Integrations
APPROVED

Ankita
10/11/2019 2:09:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:27:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD093019.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 06:38:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

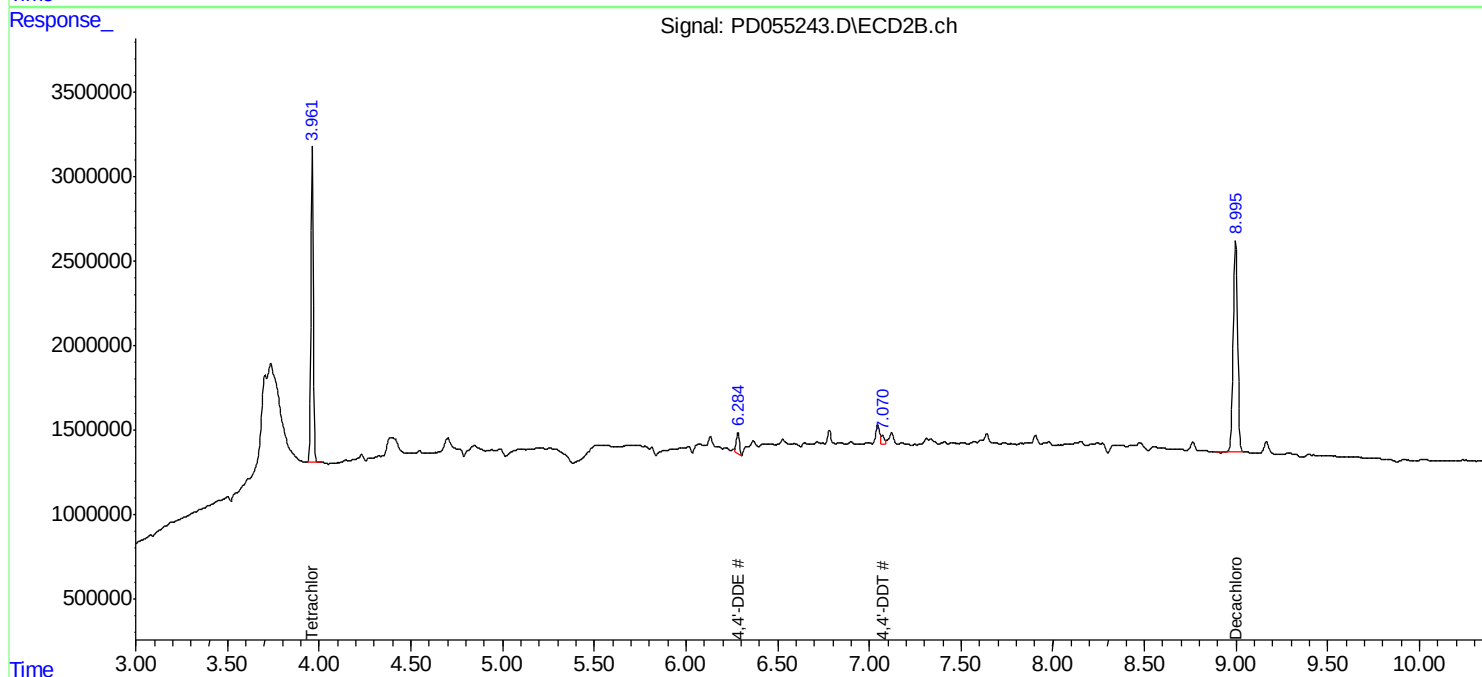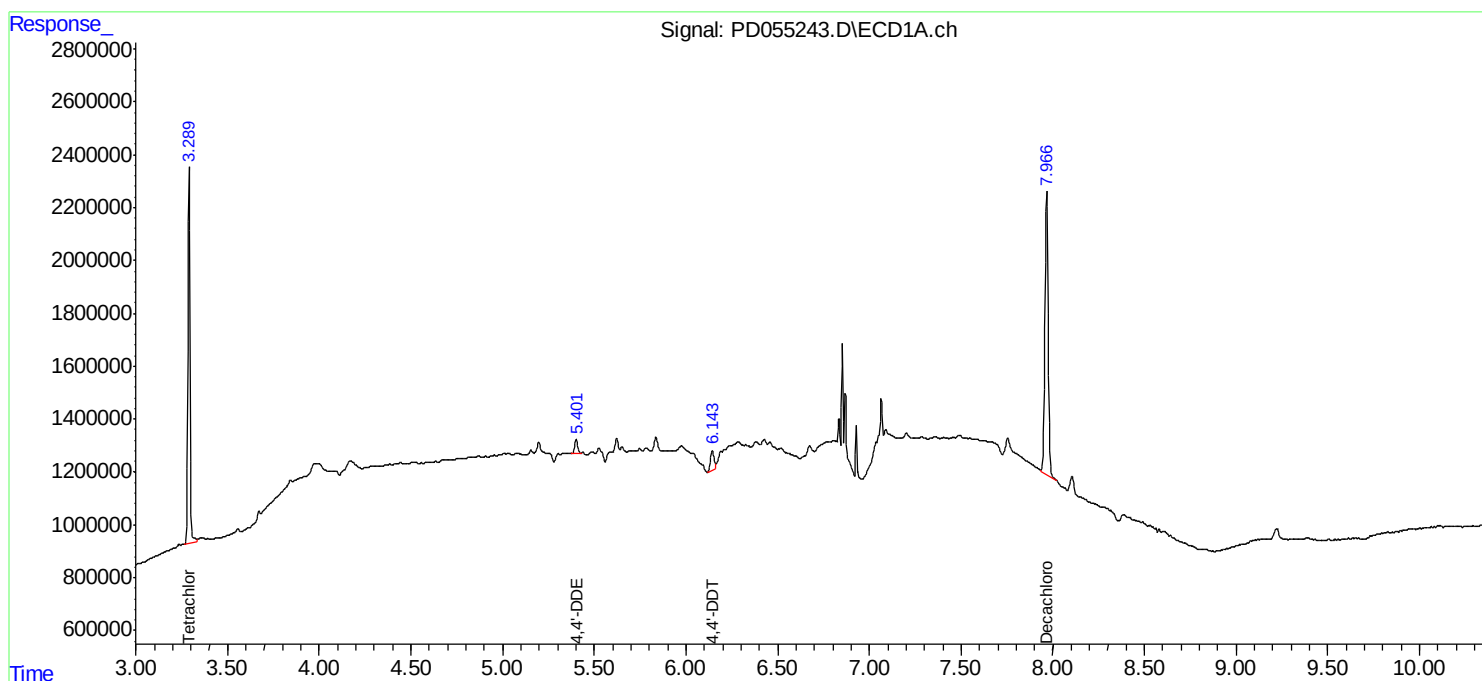

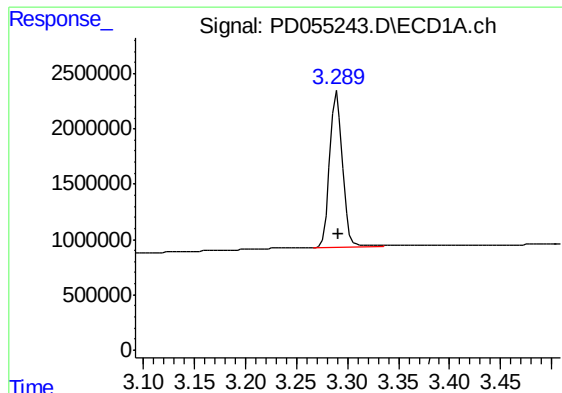


#1 Tetrachloro-m-xylene

R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 12332986
Conc: 15.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-11


Manual Integrations
APPROVED

Ankita
10/11/2019 2:09:42 PM

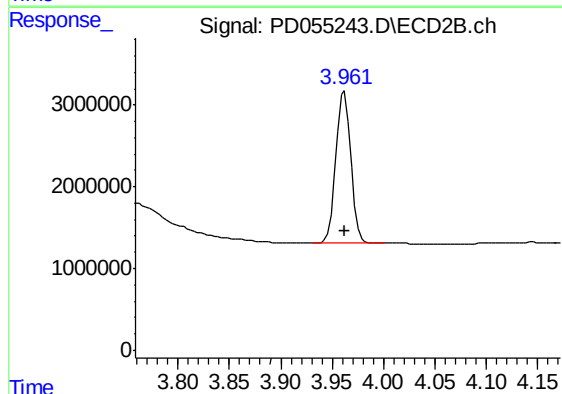


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 18933405
Conc: 16.54 ng/ml

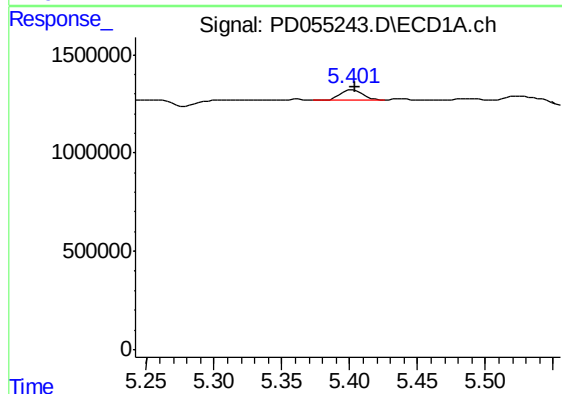


#12 4,4'-DDE

R.T.: 5.402 min
Delta R.T.: -0.002 min
Response: 552499
Conc: 0.62 ng/ml

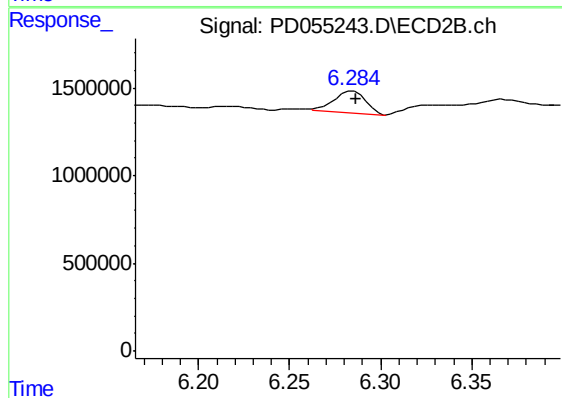

#12 4,4'-DDE

R.T.: 6.284 min
Delta R.T.: -0.003 min
Response: 1490437
Conc: 1.07 ng/ml m

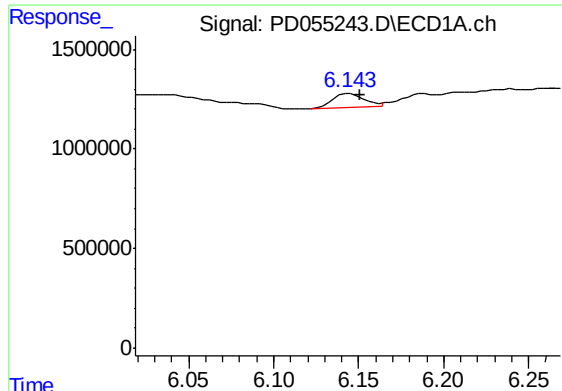


#17 4,4'-DDT

R.T.: 6.145 min
Delta R.T.: -0.006 min
Response: 956448
Conc: 1.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-11


Manual Integrations
APPROVED

Ankita
10/11/2019 2:09:42 PM

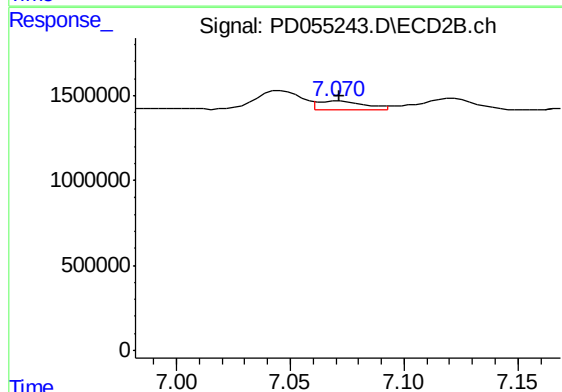


#17 4,4'-DDT

R.T.: 7.070 min
Delta R.T.: -0.002 min
Response: 756802
Conc: 0.63 ng/ml m

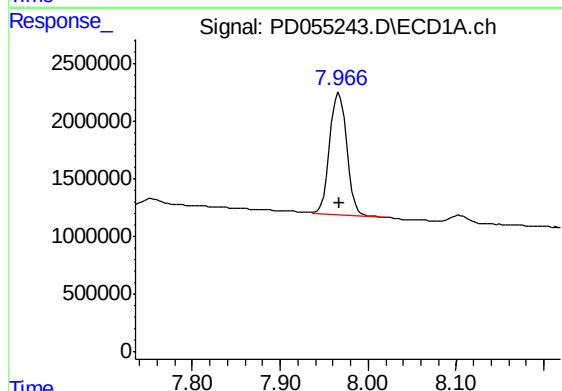

#28 Decachlorobiphenyl

R.T.: 7.967 min
Delta R.T.: 0.000 min
Response: 14327951
Conc: 16.61 ng/ml

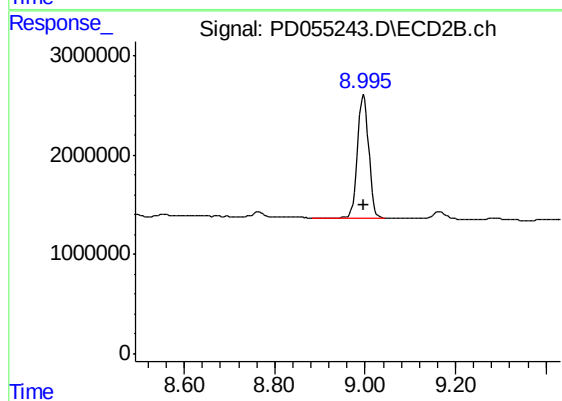

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 20994597
Conc: 17.24 ng/ml