

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101020\
 Data File : PD059655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2020 15:00
 Operator : DD\AJ
 Sample : L4184-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AN1

Manual Integrations
 APPROVED

Ankita
 10/12/2020 2:38:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 01:16:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:21:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.510	4.025	37042199	52670016	25.644	26.518
27) SA Decachlor...	8.314	9.111	52329918	70924333	48.839	47.670
Target Compounds						
10) B trans-Chl...	5.473	6.129	1688567	4823386	1.039m	2.161m#
11) B cis-Chlor...	5.533	6.215	1403973	2526368	0.867	1.155 #
12) B 4,4'-DDE	5.698	6.369	5665562	8528054	3.677	4.078
16) A 4,4'-DDD	6.218	6.860	4500270	7511658	3.442	4.339 #
17) MA 4,4'-DDT	6.462	7.159	9654528	12819114	7.194	7.987

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101020\
Data File : PD059655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2020 15:00
Operator : DD\AJ
Sample : L4184-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 01:16:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

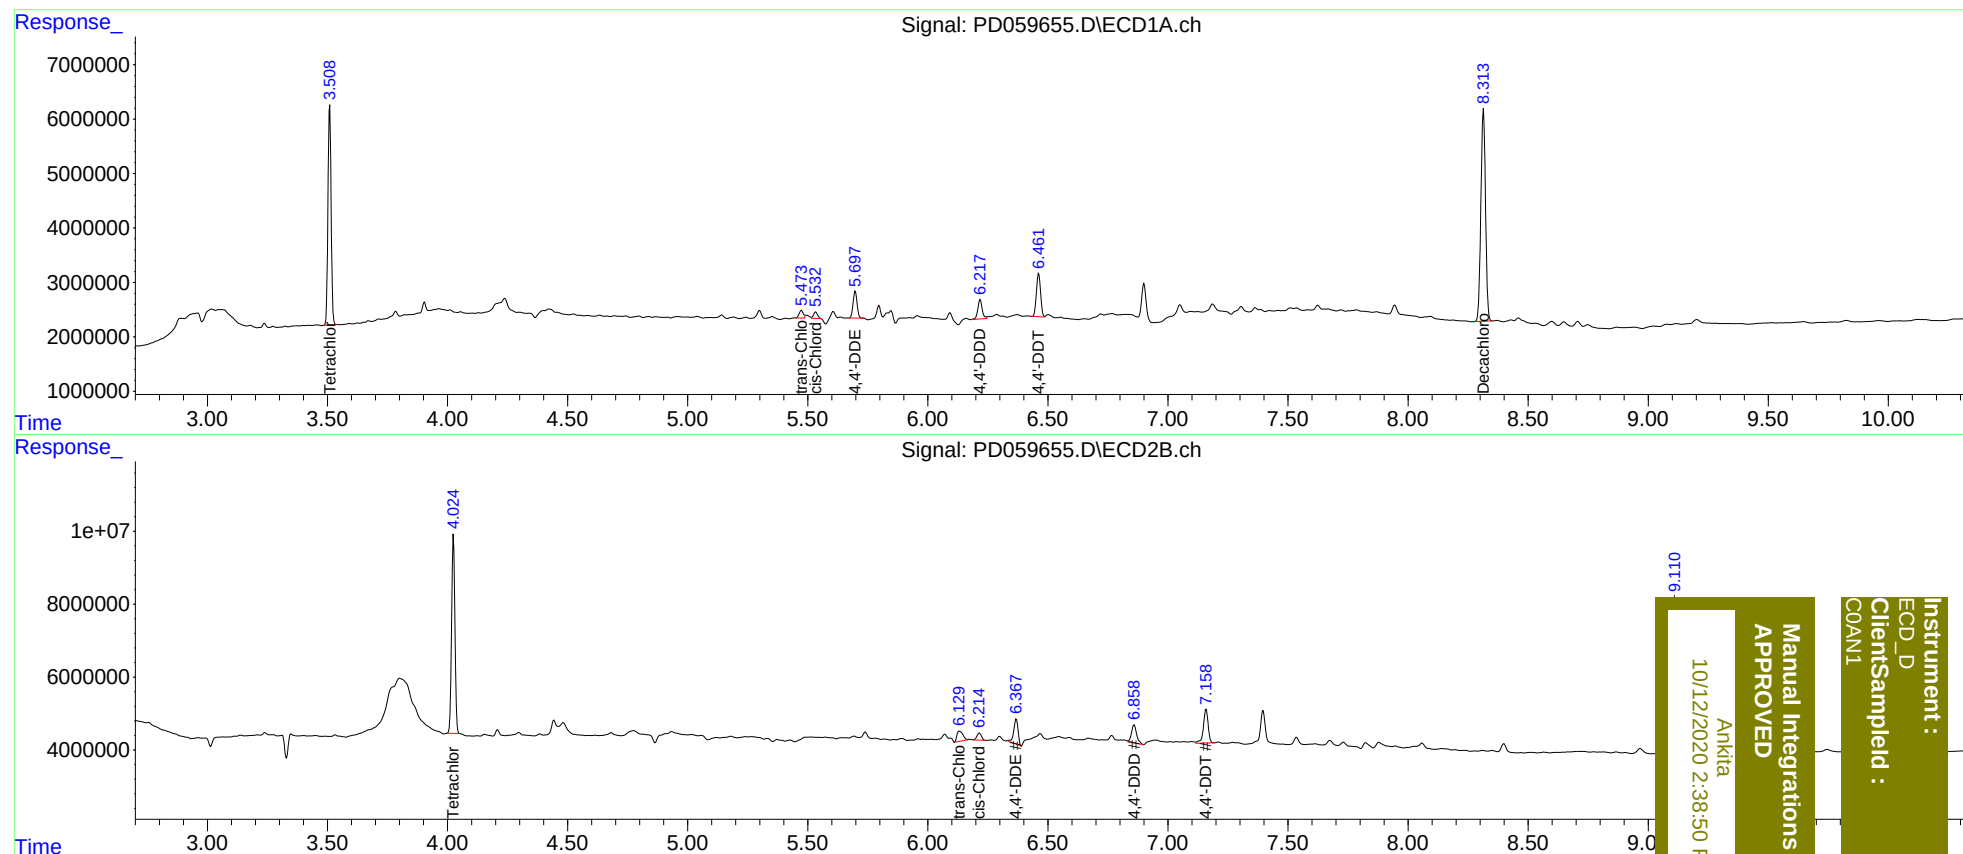

Manual Integrations
APPROVED

Ankita
10/12/2020 2:38:50 PM

Instrument :
ECD_D
Client Sampled :
COAN1