

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101020\
 Data File : PD059649.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2020 13:35
 Operator : DD\AJ
 Sample : L4184-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AJ7

Manual Integrations
 APPROVED

Ankita
 10/12/2020 2:37:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 01:13:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:21:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.510	4.024	17703466	25810425	12.256	12.995m
27) SA Decachlor...	8.314	9.111	27263678	35942707	25.445	24.158
Target Compounds						
12) B 4,4'-DDE	5.699	6.370	2487527	4188849	1.614	2.003
17) MA 4,4'-DDT	6.462	7.159	2171876	2570236	1.618	1.601
20) A Methoxychlor	7.012	7.616	96186303	134.6E6	156.759	162.232

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101020\
Data File : PD059649.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2020 13:35
Operator : DD\AJ
Sample : L4184-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 01:13:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

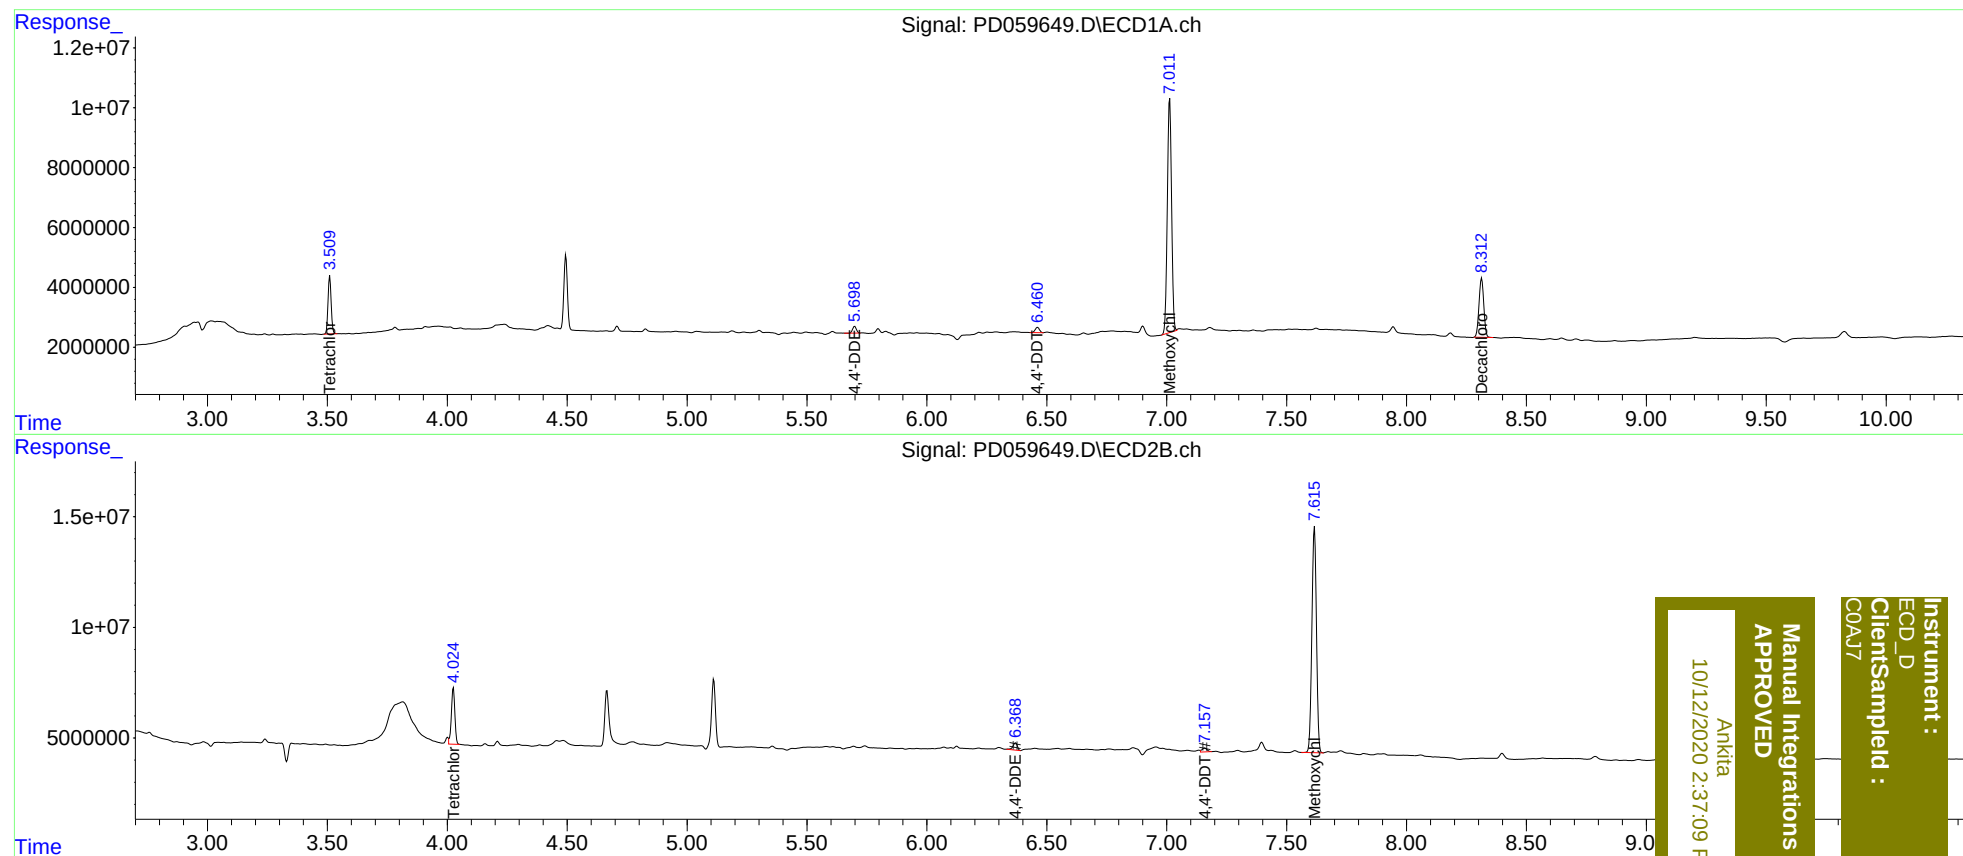

Manual Integrations
APPROVED

Ankita
10/12/2020 2:37:09 PM

Instrument :
ECD_D
ClientSampleId :
C0A37