

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101020\
 Data File : PD059658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2020 15:43
 Operator : DD\AJ
 Sample : L4184-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AL7

Manual Integrations
 APPROVED

Ankita
 10/12/2020 2:38:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 01:17:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 02 04:21:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.510	4.025	29072457	41448327	20.126	20.868
27)	SA Decachlor...	8.314	9.111	43464248	57600458	40.565	38.715m
Target Compounds							
10)	B trans-Chl...	5.474	6.126	2033760	17918307	1.252m	8.029 #
11)	B cis-Chlor...	5.535	6.216	2784306	7583669	1.720	3.467 #
12)	B 4,4'-DDE	5.698	6.370	22297862	30448350	14.472m	14.559
16)	A 4,4'-DDD	6.218	6.860	9747998	20636517	7.456	11.920 #
17)	MA 4,4'-DDT	6.462	7.160	38607890	52213121	28.770	32.530

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101020\
Data File : PD059658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2020 15:43
Operator : DD\AJ
Sample : L4184-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 01:17:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 02 04:21:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

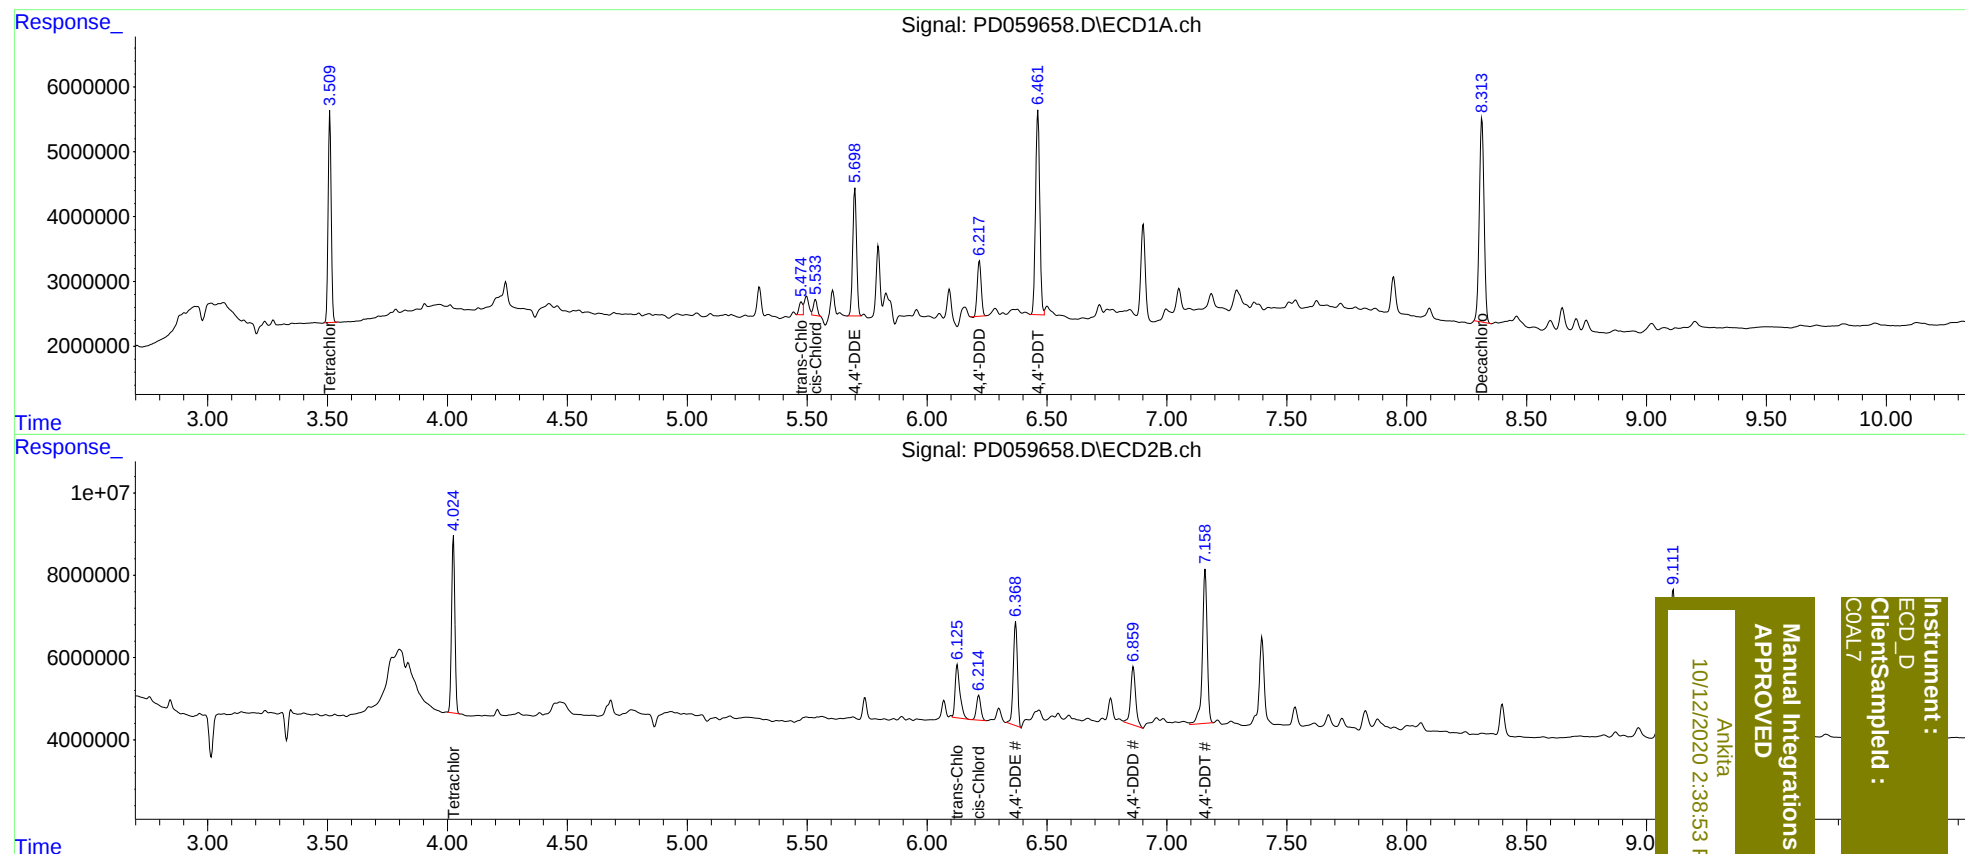

11.116

Manual Integrations
APPROVED

Ankita

10/12/2020 2:38:53 PM

Instrument :
ECD_D
ClientSampleId :
COAL7