

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101118\
 Data File : PD049798.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Oct 2018 9:10
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 11:29:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 11:29:27 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

9) A	Endosulfan I	5.196f	6.242	578184	7016043	0.321	0.282
10) B	gamma-Chl...	5.140	0.000	635191	0	0.318	N.D. #
11) B	alpha-Chl...	5.196	6.242	578184	7016043	0.294	0.266
13) MA	Dieldrin	5.461	0.000	827557	0	0.424	N.D. #
14) MA	Endrin	0.000	6.696f	0	23823239	N.D.	1.310 #
16) A	4,4'-DDD	5.854	0.000	1120528	0	0.777	N.D. #
18) B	Endrin al...	0.000	7.065	0	12439535	N.D.	0.662 #
20) A	Methoxychlor	0.000	7.577f	0	58381383	N.D.	7.068 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101118\
Data File : PD049798.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Oct 2018 9:10
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 11:29:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 11:29:27 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

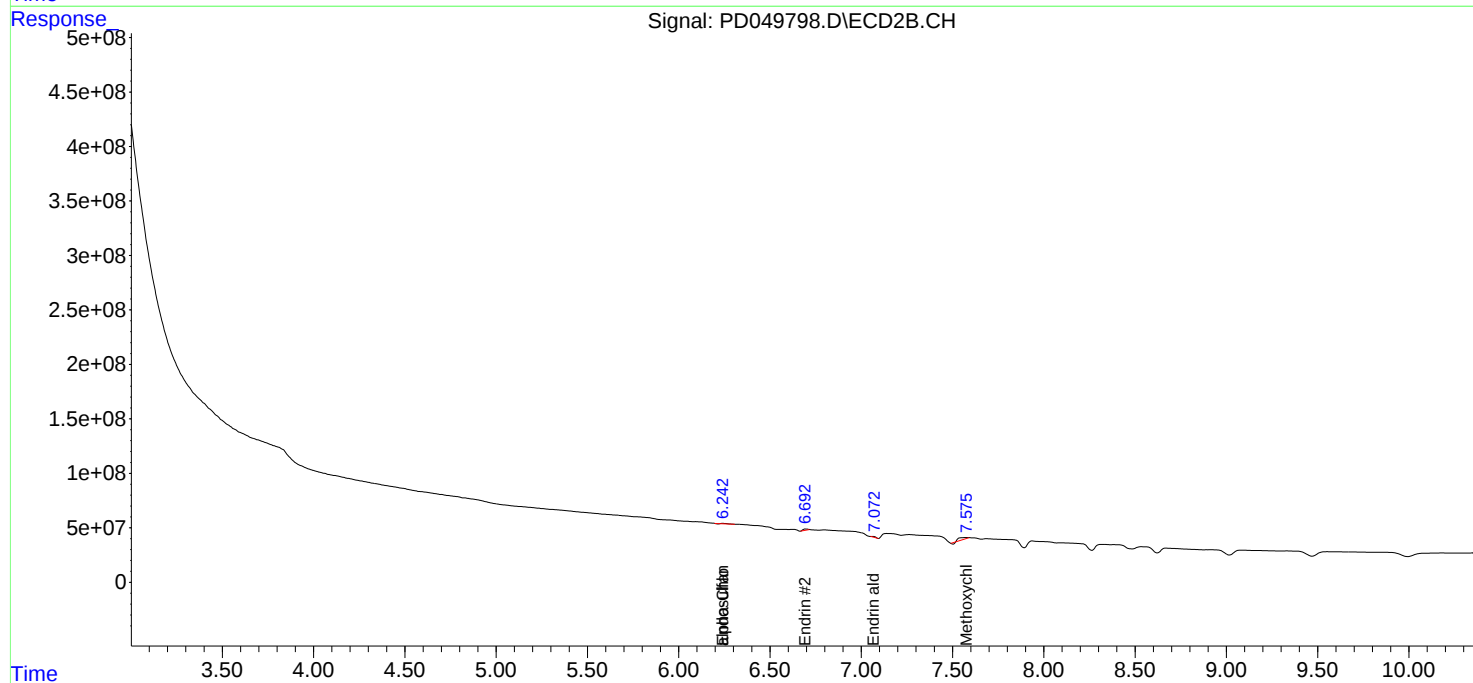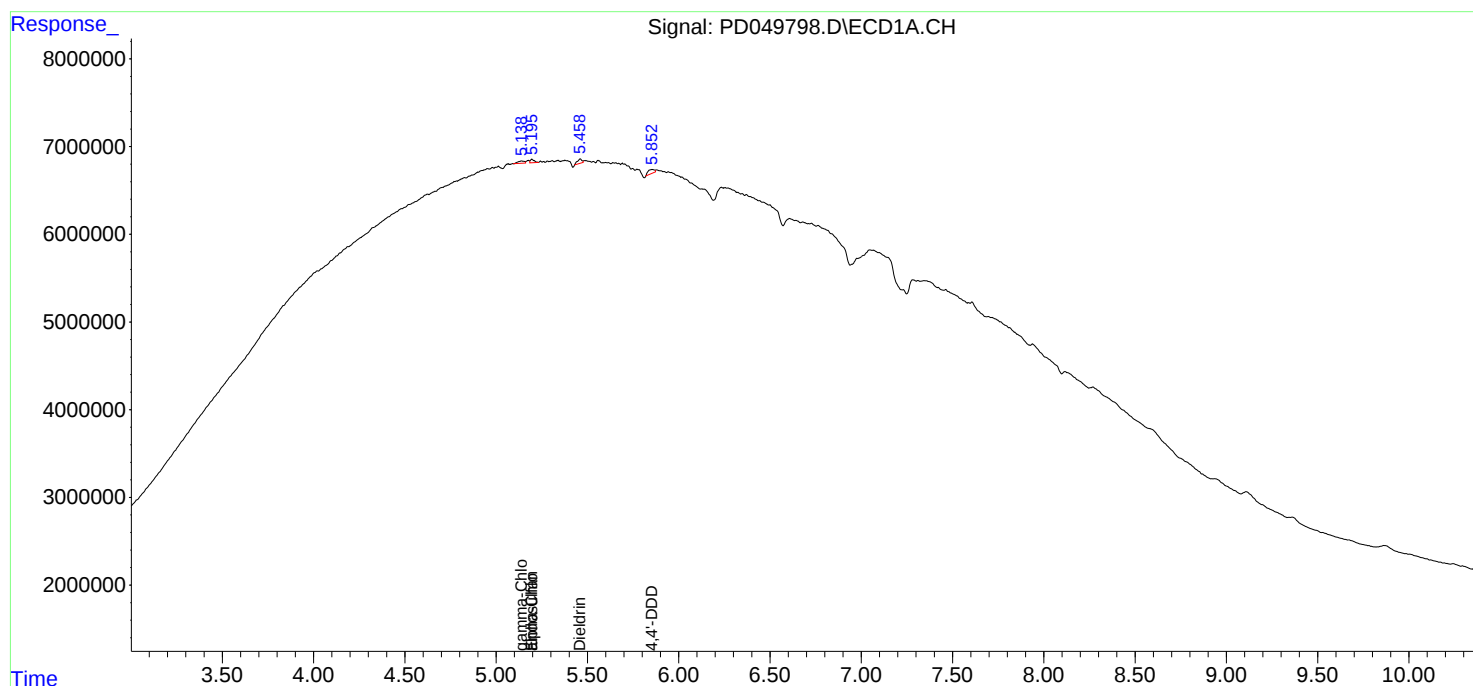


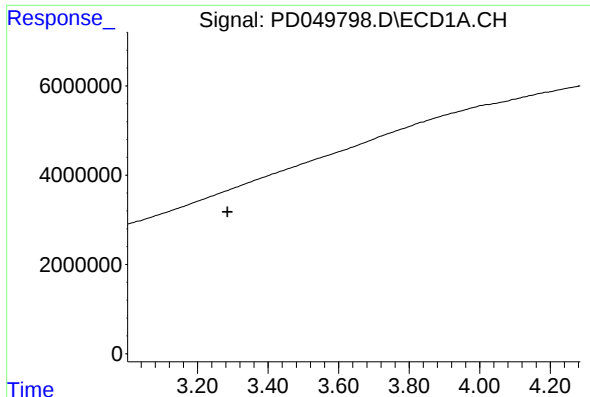

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.285 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

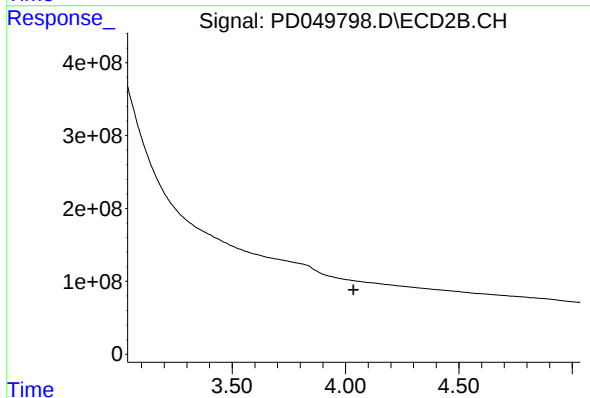


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.036 min
Response: 0
Conc: N.D.

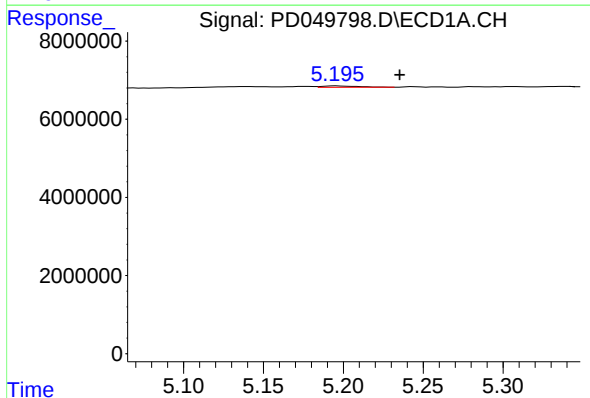


#9 Endosulfan I

R.T.: 5.196 min
Delta R.T.: -0.039 min
Response: 578184
Conc: 0.32 ng/ml

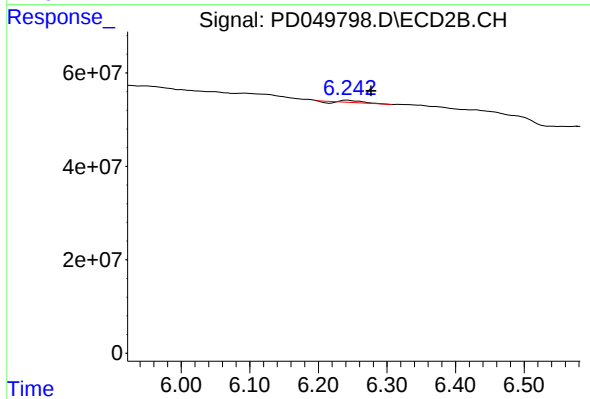

#9 Endosulfan I


R.T.: 6.242 min
Delta R.T.: -0.035 min
Response: 7016043
Conc: 0.28 ng/ml

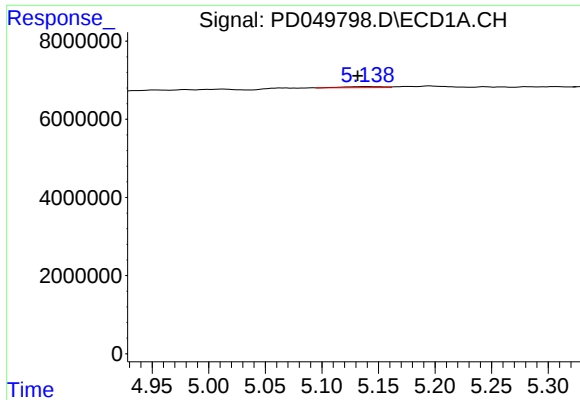

#10 gamma-Chlordane


R.T.: 5.140 min
Delta R.T.: 0.008 min
Response: 635191
Conc: 0.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

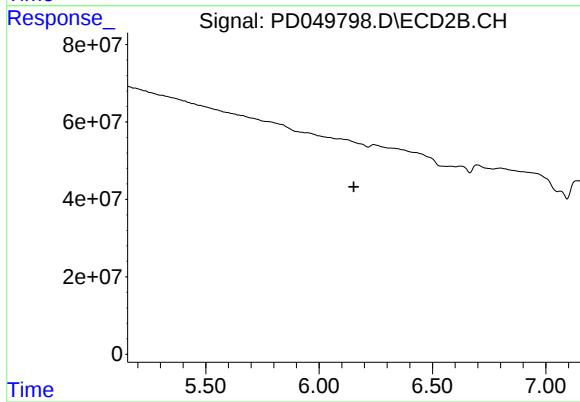


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.153 min
Response: 0
Conc: N.D.

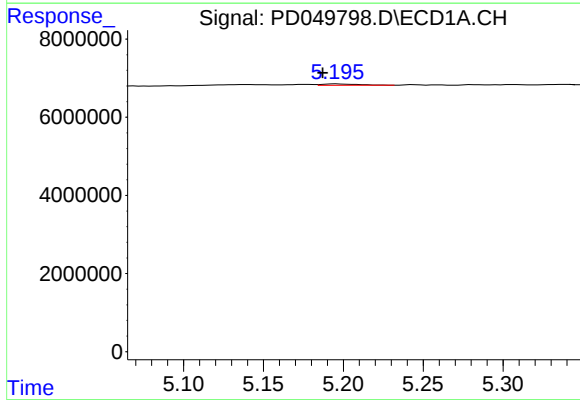


#11 alpha-Chlordane

R.T.: 5.196 min
Delta R.T.: 0.009 min
Response: 578184
Conc: 0.29 ng/ml

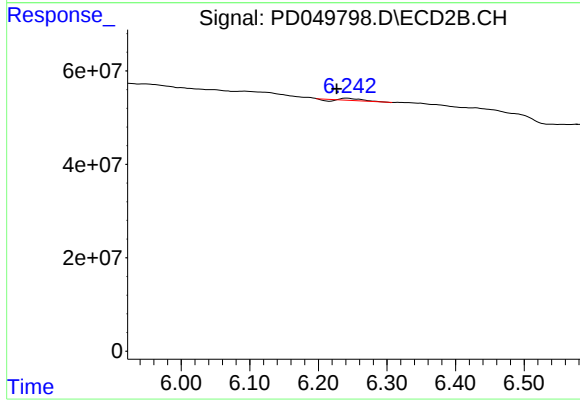

#11 alpha-Chlordane


R.T.: 6.242 min
Delta R.T.: 0.015 min
Response: 7016043
Conc: 0.27 ng/ml

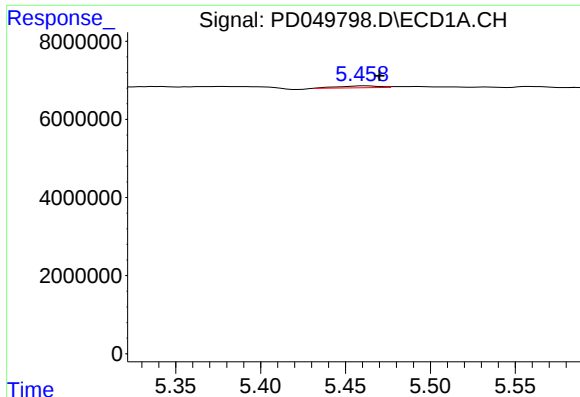

#13 Dieldrin


R.T.: 5.461 min
Delta R.T.: -0.009 min
Response: 827557
Conc: 0.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

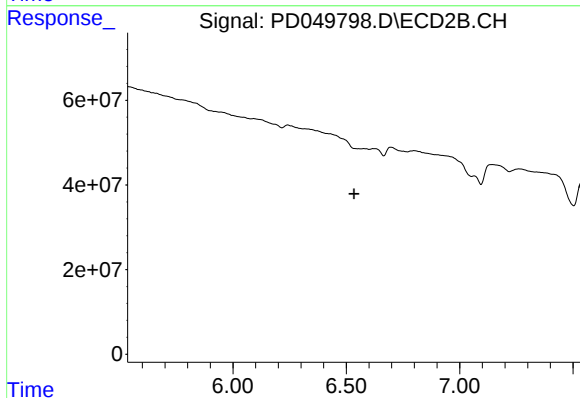


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.535 min
Response: 0
Conc: N.D.

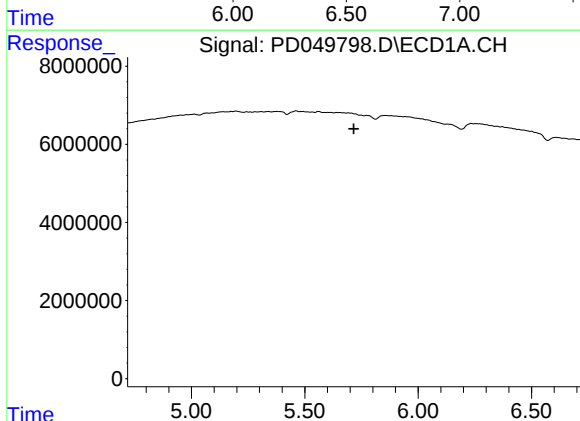


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.716 min
Response: 0
Conc: N.D.

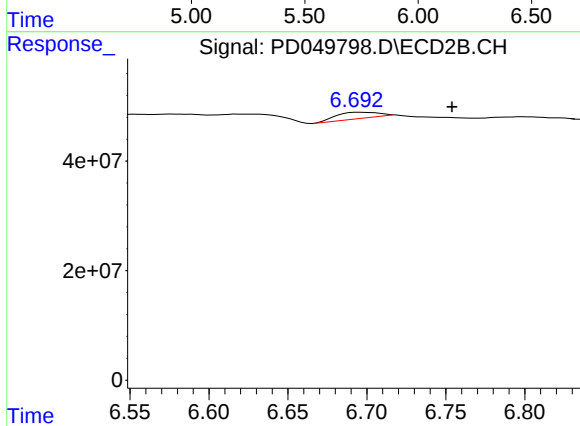

#14 Endrin


R.T.: 6.696 min
Delta R.T.: -0.058 min
Response: 23823239
Conc: 1.31 ng/ml

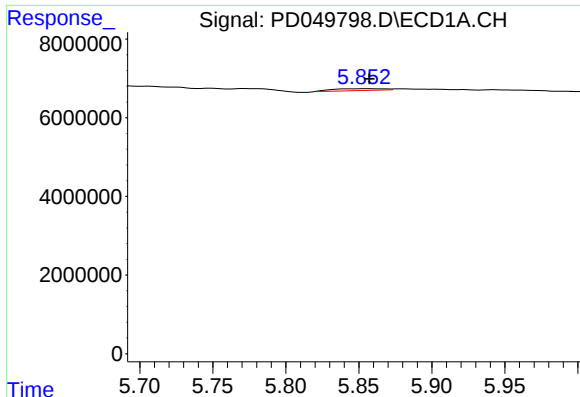

#16 4,4'-DDD


R.T.: 5.854 min
Delta R.T.: -0.003 min
Response: 1120528
Conc: 0.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

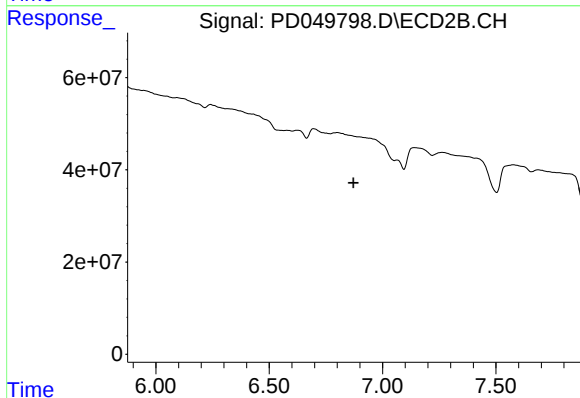


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.872 min
Response: 0
Conc: N.D.

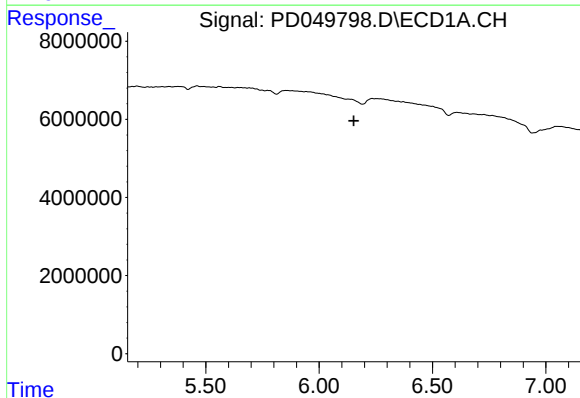


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.153 min
Response: 0
Conc: N.D.

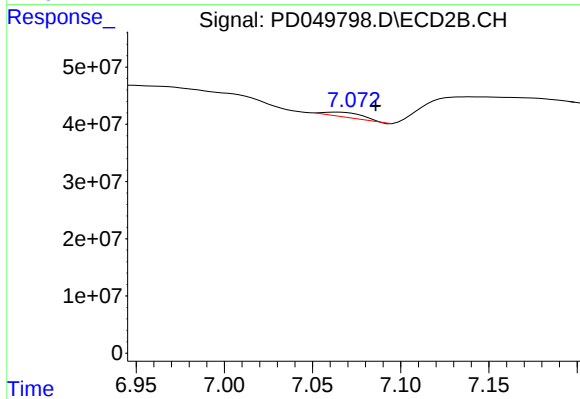

#18 Endrin aldehyde


R.T.: 7.065 min
Delta R.T.: -0.021 min
Response: 12439535
Conc: 0.66 ng/ml

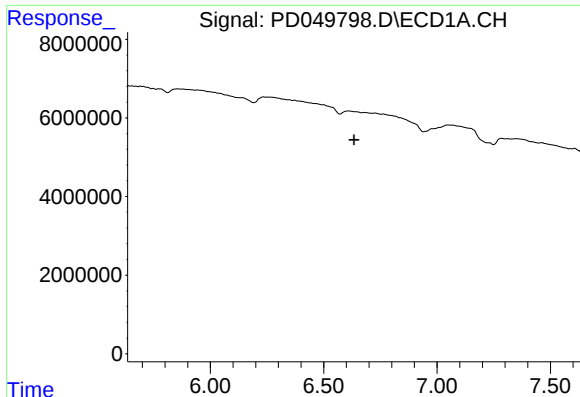

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

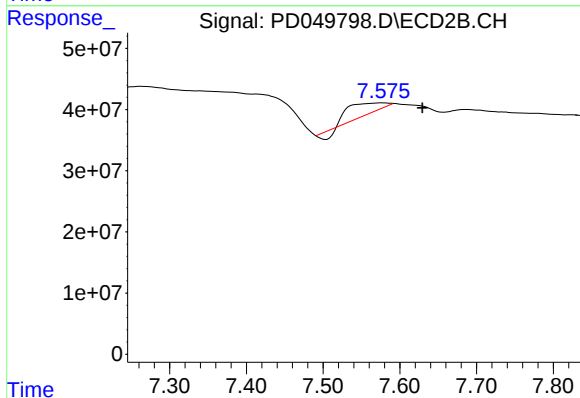


#20 Methoxychlor

R.T.: 7.577 min
Delta R.T.: -0.052 min
Response: 58381383
Conc: 7.07 ng/ml

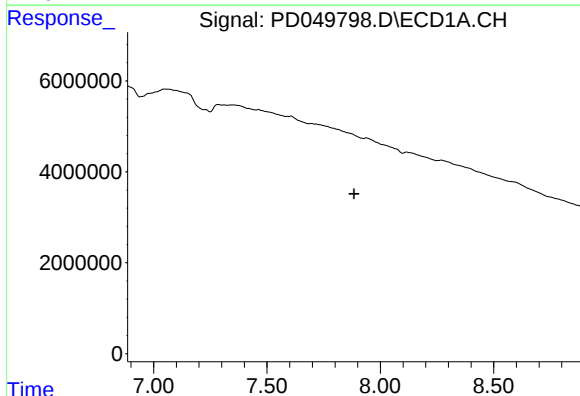

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.884 min
Response: 0
Conc: N.D.

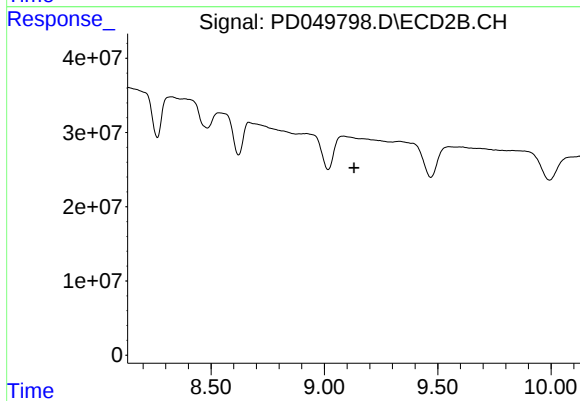

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.131 min
Response: 0
Conc: N.D.