

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101118\
 Data File : PD049812.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Oct 2018 12:36
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 13:14:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 12:26:45 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	4.036	30007498	512.8E6	20.745	21.847
28)	SA Decachlor...	7.885	9.133	32952803	435.7E6	22.031	22.293
Target Compounds							
2)	A alpha-BHC	0.000	4.492f	0	58796598	N.D.	1.638 #
3)	MA gamma-BHC...	3.995	0.000	1551866	0	0.714	N.D. #
6)	B beta-BHC	4.170f	4.927f	658956	23721179	0.761	1.759 #
8)	B Heptachlo...	0.000	5.920	0	8055759	N.D.	0.296 #
12)	B 4,4'-DDE	0.000	6.451f	0	2764721	N.D.	0.106 #
14)	MA Endrin	0.000	6.693f	0	2940648	N.D.	0.162 #
16)	A 4,4'-DDD	5.794f	0.000	391307	0	0.271	N.D. #
20)	A Methoxychlor	0.000	7.571f	0	1929145	N.D.	0.234 #
23)	Chlordane-1	4.144	0.000	587109	0	9.148	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101118\
Data File : PD049812.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Oct 2018 12:36
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 13:14:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 12:26:45 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

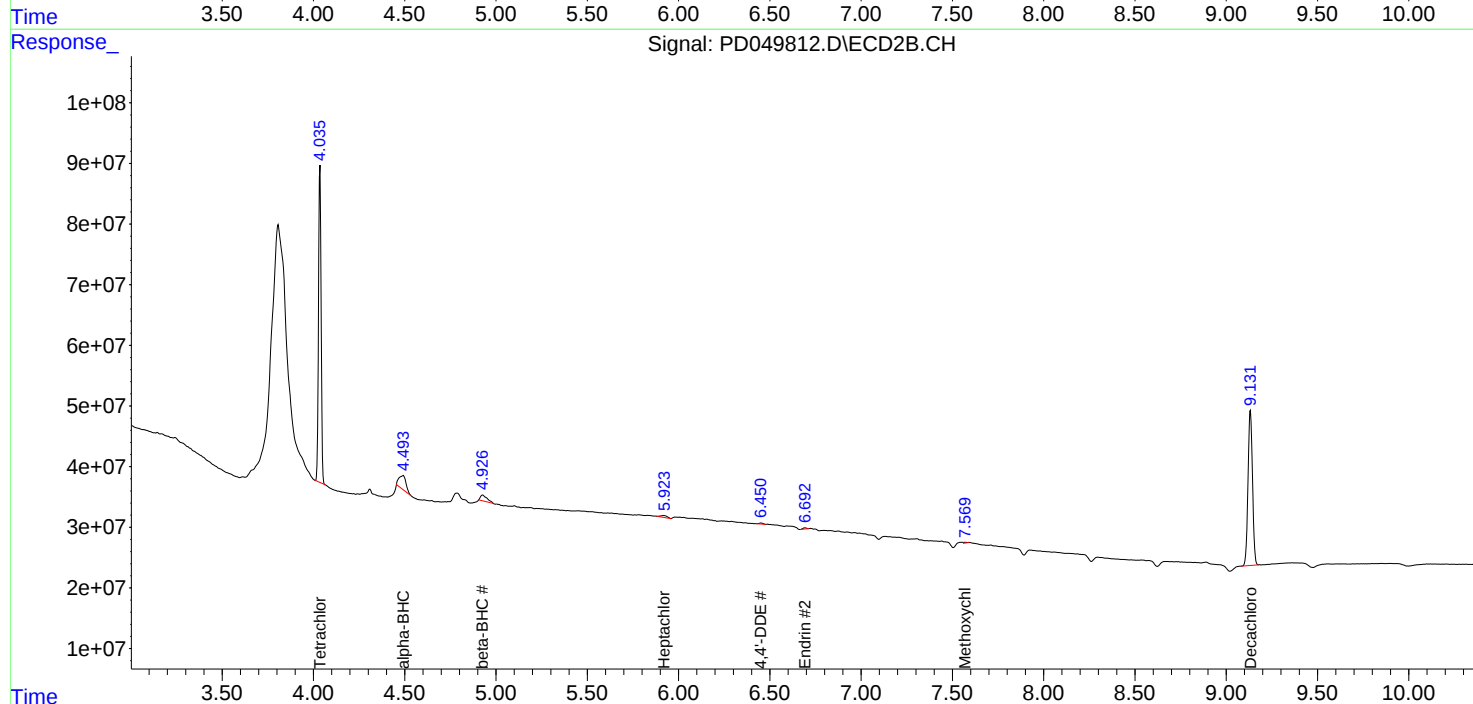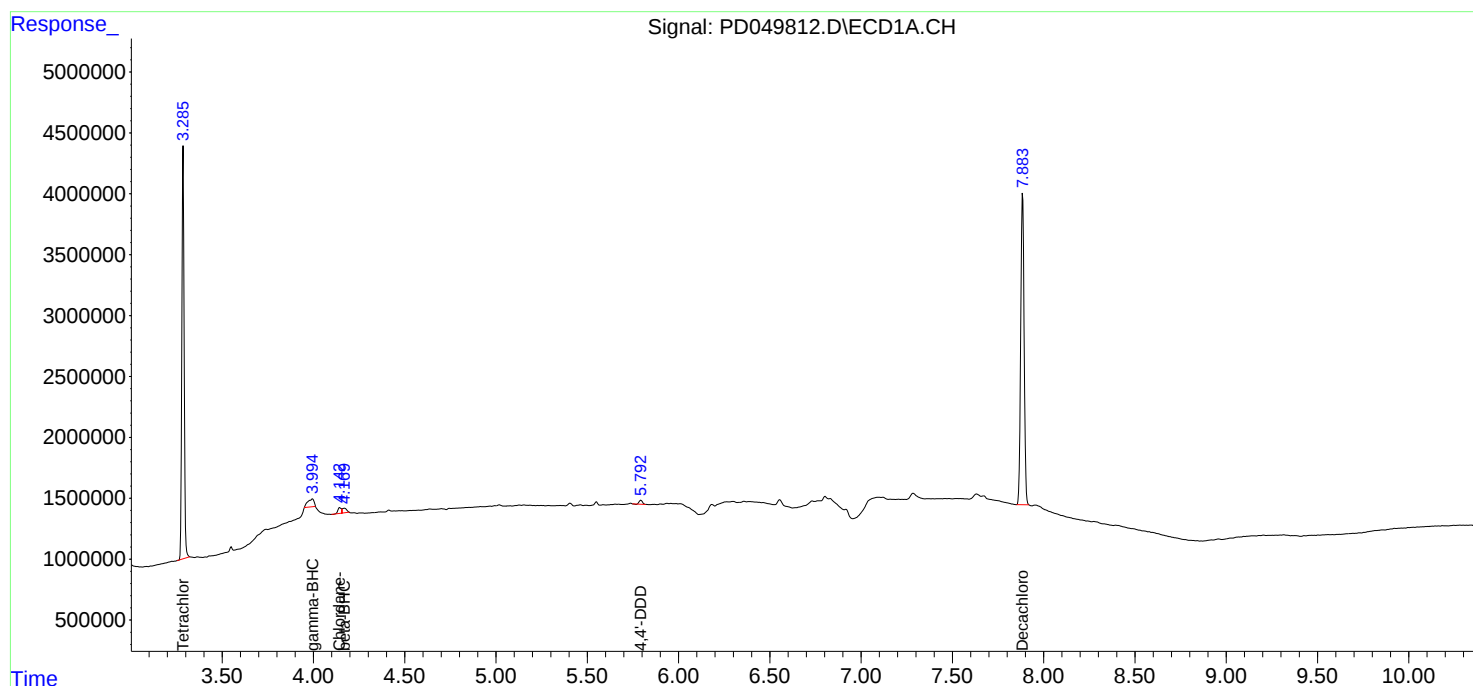


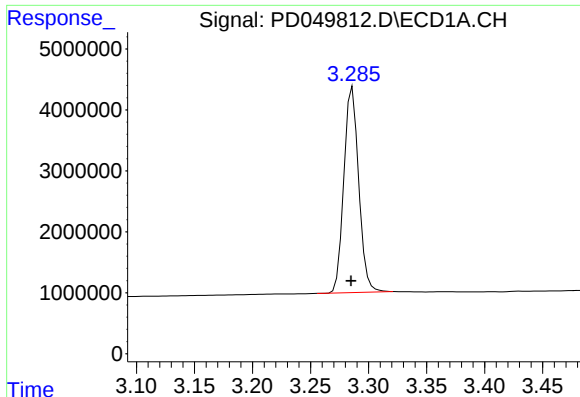

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: 0.001 min
Response: 30007498
Conc: 20.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

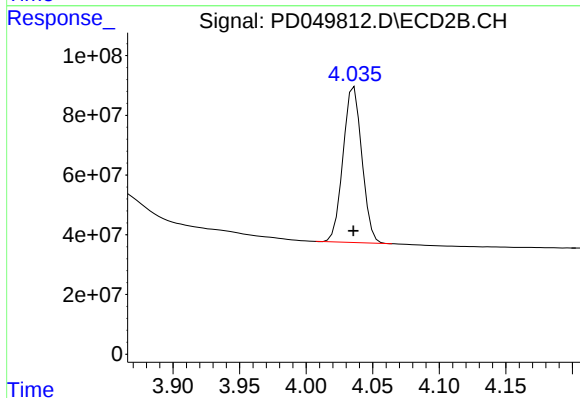


#1 Tetrachloro-m-xylene

R.T.: 4.036 min
Delta R.T.: 0.000 min
Response: 512752127
Conc: 21.85 ng/ml

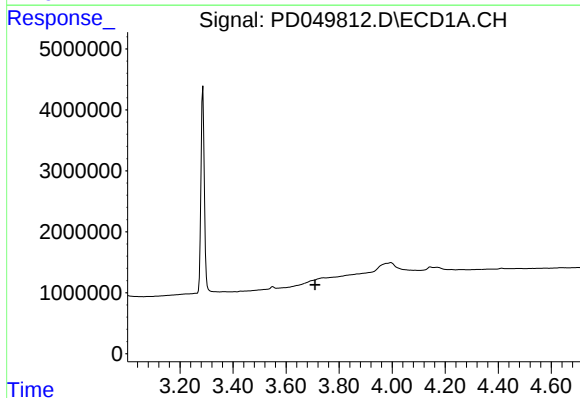


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.709 min
Response: 0
Conc: N.D.

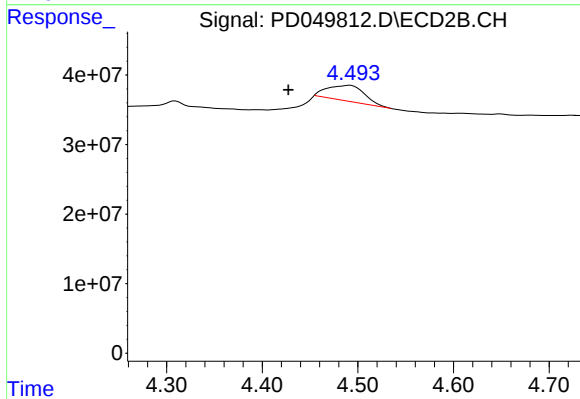

#2 alpha-BHC

R.T.: 4.492 min
Delta R.T.: 0.064 min
Response: 58796598
Conc: 1.64 ng/ml

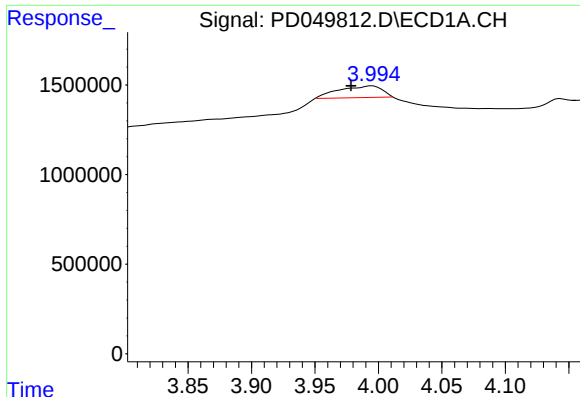

#3 gamma-BHC (Lindane)


R.T.: 3.995 min

Delta R.T.: 0.017 min

Response: 1551866

Conc: 0.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

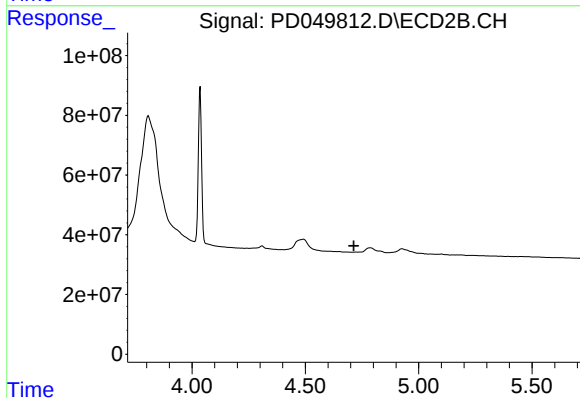


#3 gamma-BHC (Lindane)

R.T.: 0.000 min

Exp R.T. : 4.714 min

Response: 0

Conc: N.D.

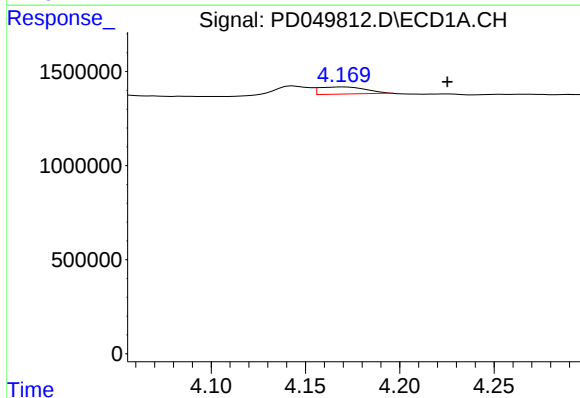


#6 beta-BHC

R.T.: 4.170 min

Delta R.T.: -0.055 min

Response: 658956

Conc: 0.76 ng/ml

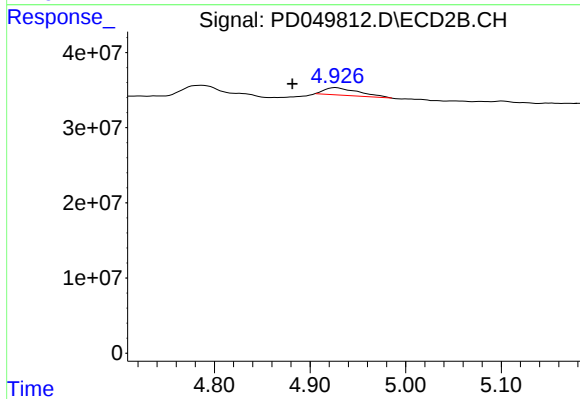


#6 beta-BHC

R.T.: 4.927 min

Delta R.T.: 0.046 min

Response: 23721179


Conc: 1.76 ng/ml

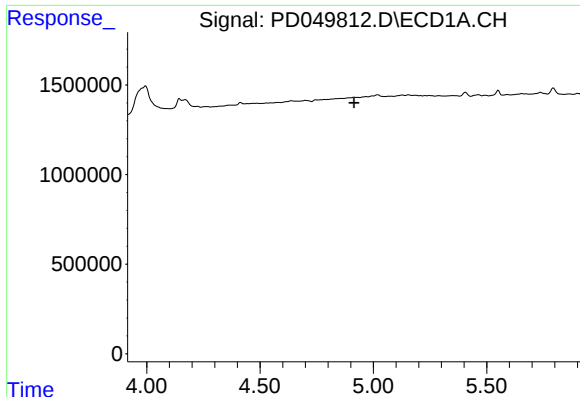

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.915 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

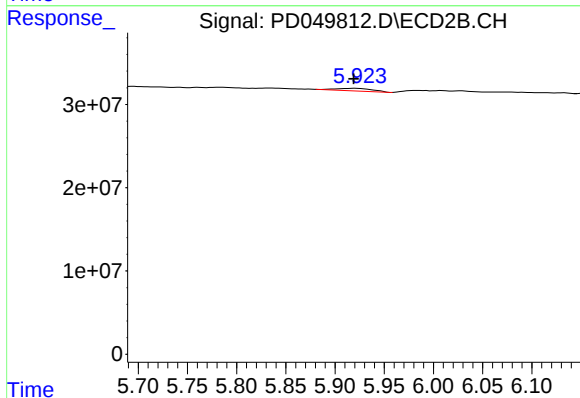


#8 Heptachlor epoxide

R.T.: 5.920 min
Delta R.T.: 0.001 min
Response: 8055759
Conc: 0.30 ng/ml

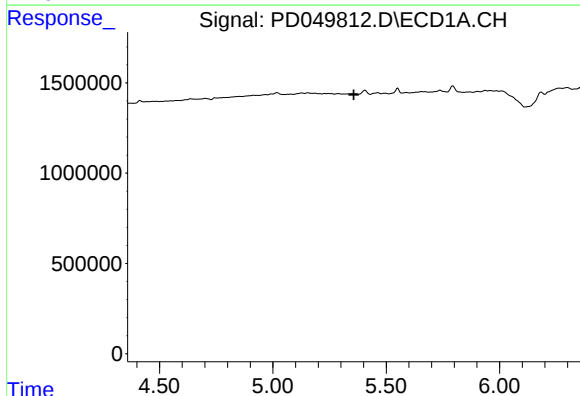


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.358 min
Response: 0
Conc: N.D.

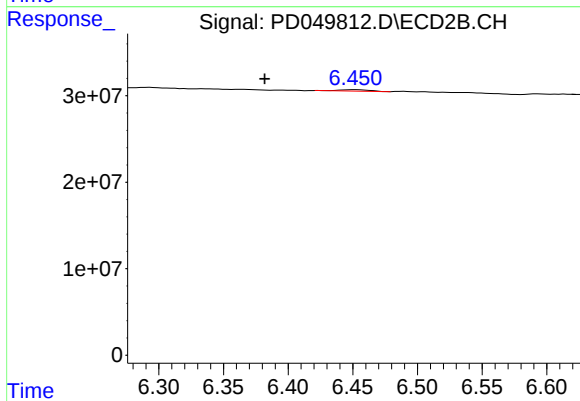

#12 4,4'-DDE


R.T.: 6.451 min
Delta R.T.: 0.070 min
Response: 2764721
Conc: 0.11 ng/ml

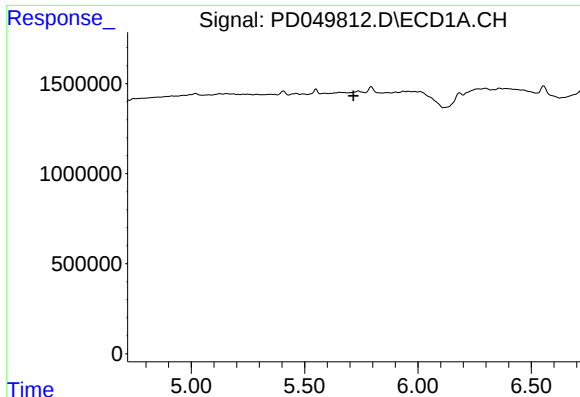

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.716 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

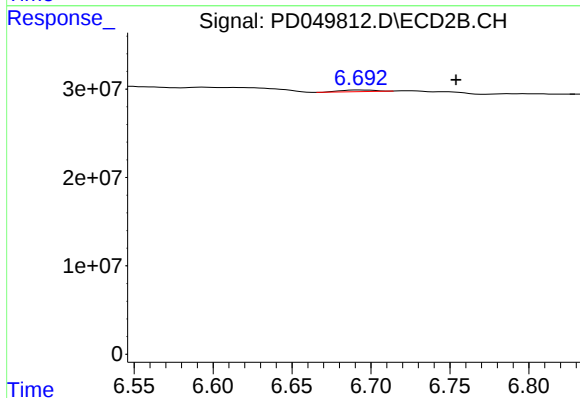


#14 Endrin

R.T.: 6.693 min
Delta R.T.: -0.061 min
Response: 2940648
Conc: 0.16 ng/ml

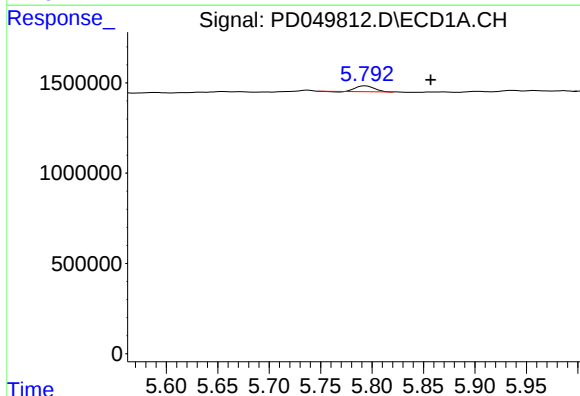


#16 4,4'-DDD

R.T.: 5.794 min
Delta R.T.: -0.063 min
Response: 391307
Conc: 0.27 ng/ml

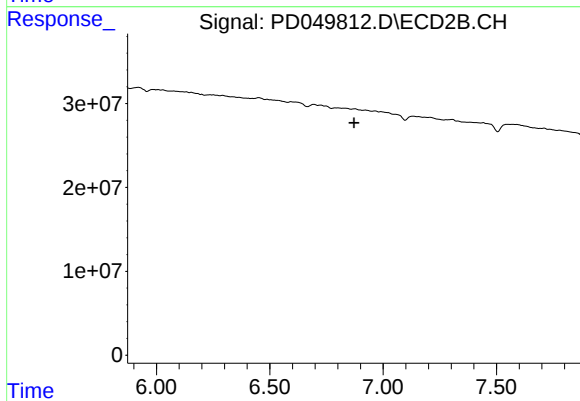

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.872 min
Response: 0
Conc: N.D.

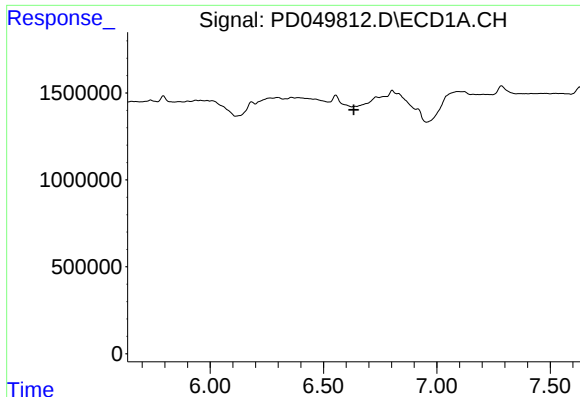

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

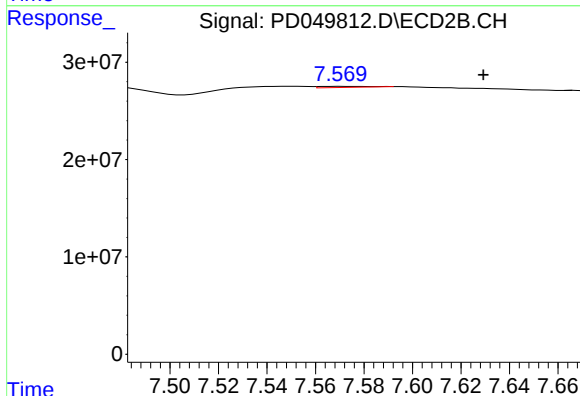


#20 Methoxychlor

R.T.: 7.571 min
Delta R.T.: -0.059 min
Response: 1929145
Conc: 0.23 ng/ml

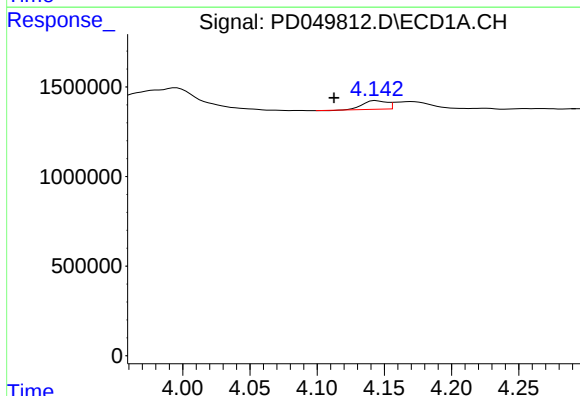


#23 Chlordane-1

R.T.: 4.144 min
Delta R.T.: 0.031 min
Response: 587109
Conc: 9.15 ng/ml

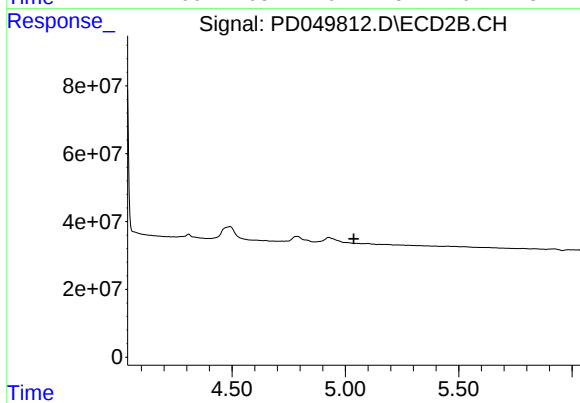

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.037 min
Response: 0
Conc: N.D.

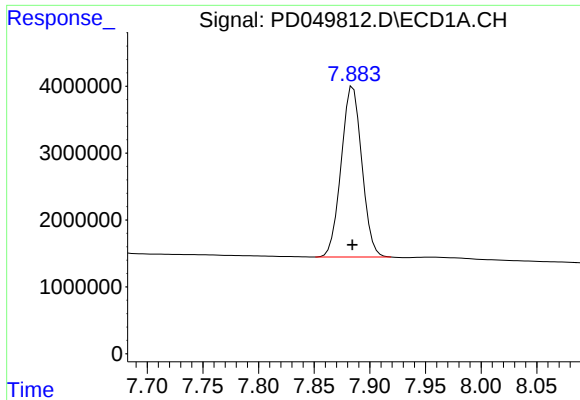

#28 Decachlorobiphenyl

R.T.: 7.885 min
Delta R.T.: 0.000 min
Response: 32952803
Conc: 22.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

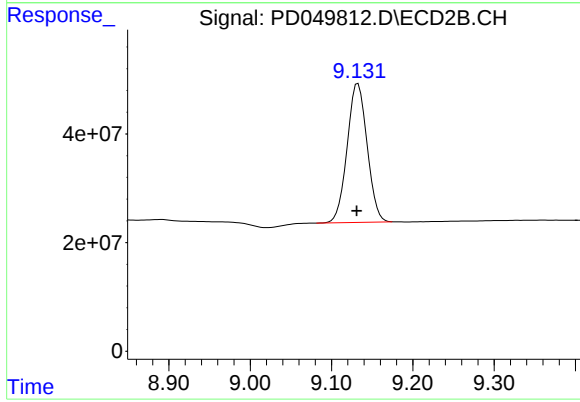

#28 Decachlorobiphenyl

R.T.: 9.133 min
Delta R.T.: 0.002 min
Response: 435727506
Conc: 22.29 ng/ml