

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2022 13:35
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 15:00:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 11 14:59:36 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.710	3.471	25404942	260.6E6	10.360	10.770
27)	SA Decachlor...	7.846	8.930	41536770	108.1E6	21.292	21.095
Target Compounds							
2)	A alpha-BHC	3.215	3.936	35461833	323.6E6	9.862	10.574
3)	MA gamma-BHC...	3.546	4.270	29182964	285.7E6	9.759	11.103
4)	MA Heptachlor	3.879	4.837	32930201	185.5E6	9.974	10.722
9)	A Endosulfan I	5.033	5.993	26695855	99916335	10.237	10.275
13)	MA Dieldrin	5.300	6.271	57301386	199.9E6	19.768	20.636
14)	MA Endrin	5.576	6.502	50101050	166.4E6	19.964	20.779
16)	A 4,4'-DDD	5.724	6.636	45178754	149.8E6	19.938	20.992
17)	MA 4,4'-DDT	5.973	6.944	43014376	141.8E6	19.832	20.765
20)	A Methoxychlor	6.556	7.424	121.6E6	339.2E6	102.606	105.458


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2022 13:35
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 15:00:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 11 14:59:36 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

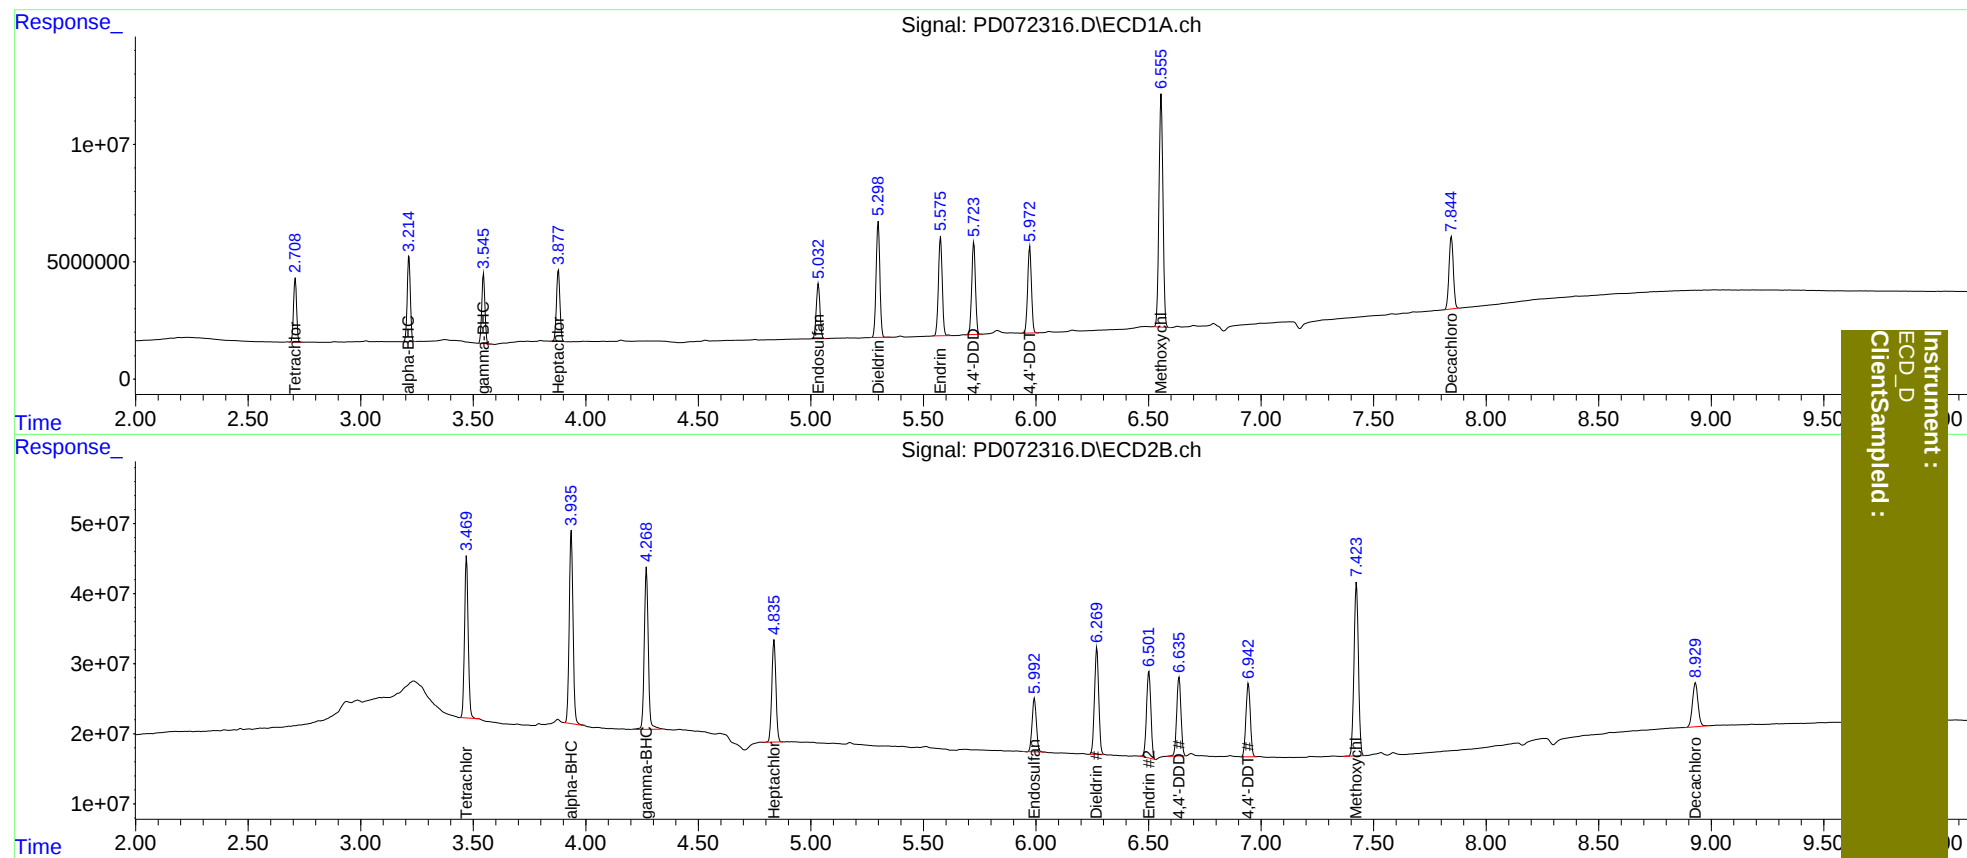


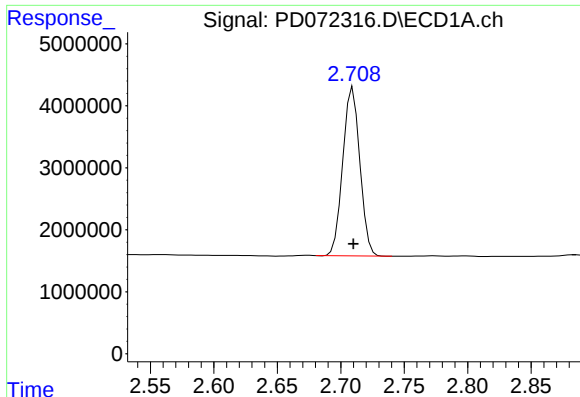

#1 Tetrachloro-m-xylene


R.T.: 2.710 min
Delta R.T.: 0.000 min
Response: 25404942
Conc: 10.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

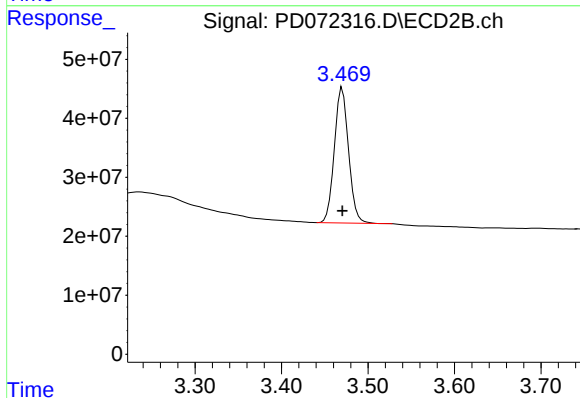


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: 0.000 min
Response: 260611890
Conc: 10.77 ng/ml

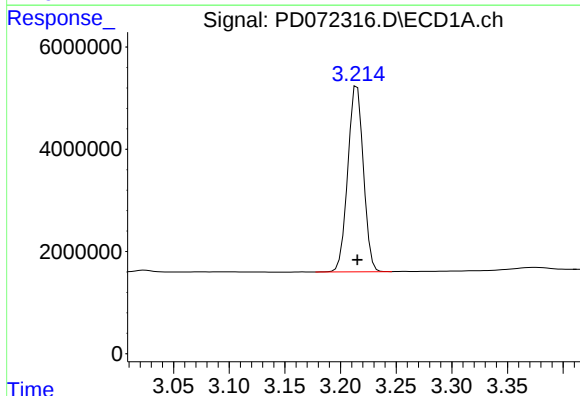


#2 alpha-BHC

R.T.: 3.215 min
Delta R.T.: 0.000 min
Response: 35461833
Conc: 9.86 ng/ml

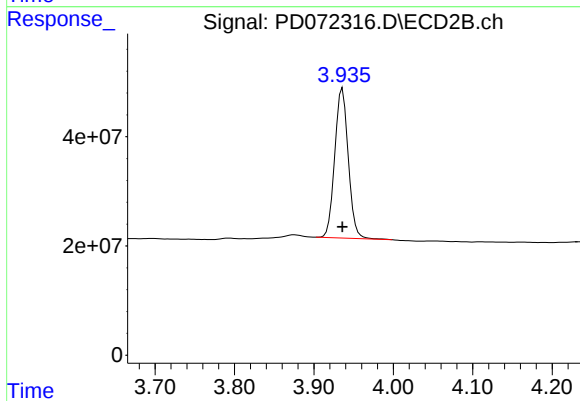

#2 alpha-BHC


R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 323575000
Conc: 10.57 ng/ml

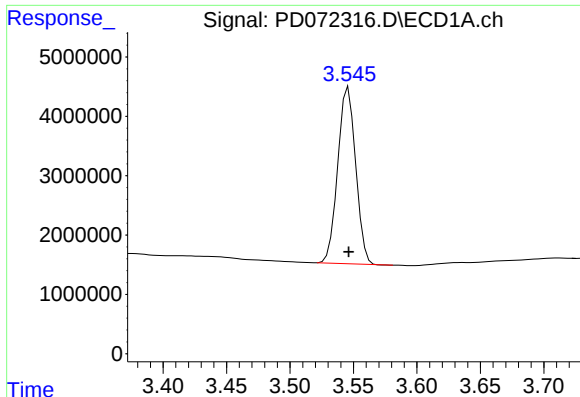

#3 gamma-BHC (Lindane)


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 29182964
Conc: 9.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

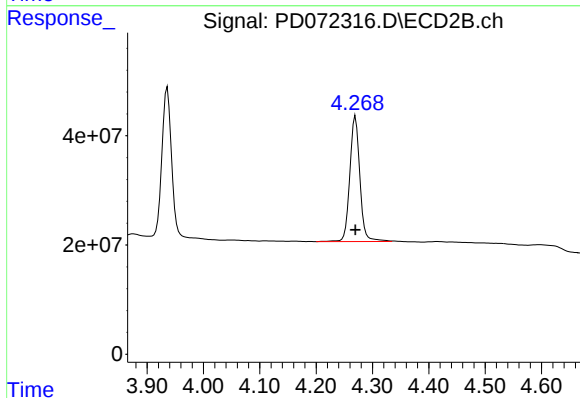


#3 gamma-BHC (Lindane)

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 285659918
Conc: 11.10 ng/ml

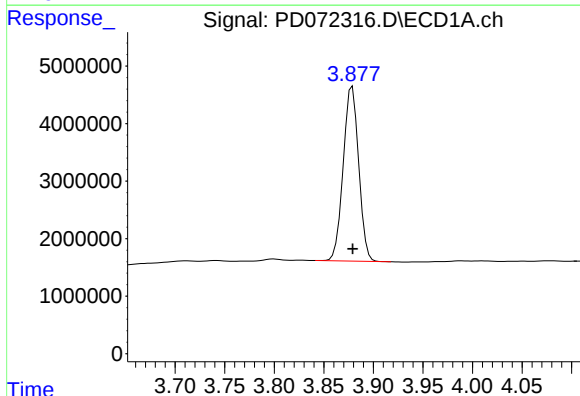


#4 Heptachlor

R.T.: 3.879 min
Delta R.T.: 0.000 min
Response: 32930201
Conc: 9.97 ng/ml

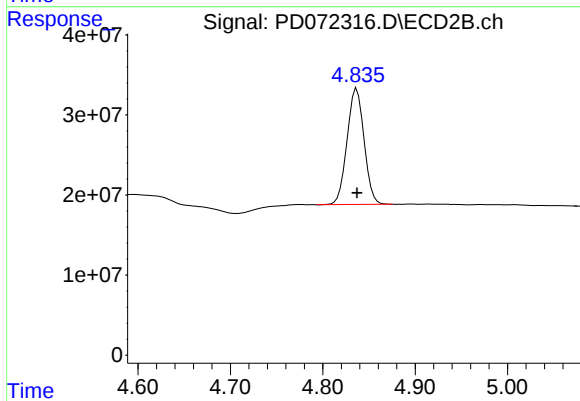

#4 Heptachlor


R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 185470100
Conc: 10.72 ng/ml

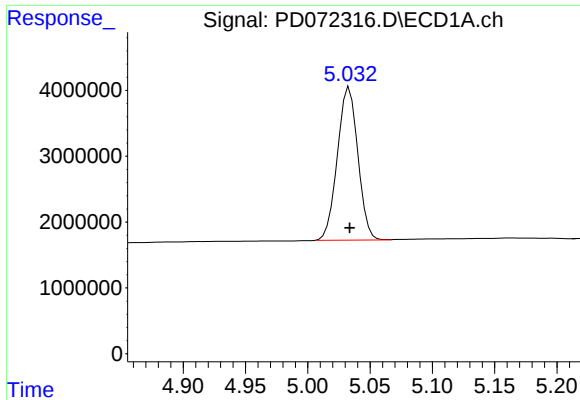

#9 Endosulfan I


R.T.: 5.033 min
Delta R.T.: 0.000 min
Response: 26695855
Conc: 10.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

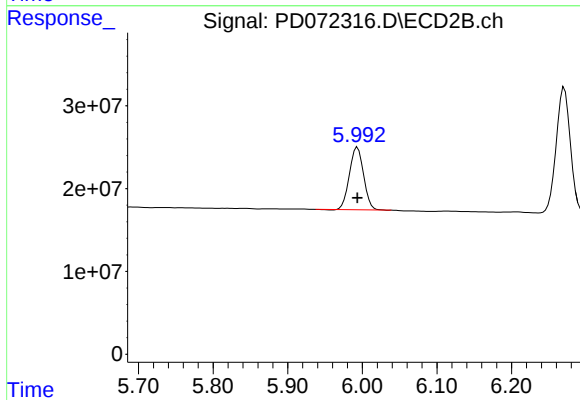


#9 Endosulfan I

R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 99916335
Conc: 10.28 ng/ml

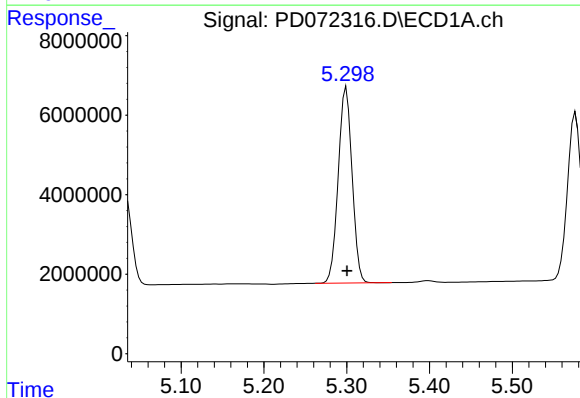


#13 Dieldrin

R.T.: 5.300 min
Delta R.T.: 0.000 min
Response: 57301386
Conc: 19.77 ng/ml

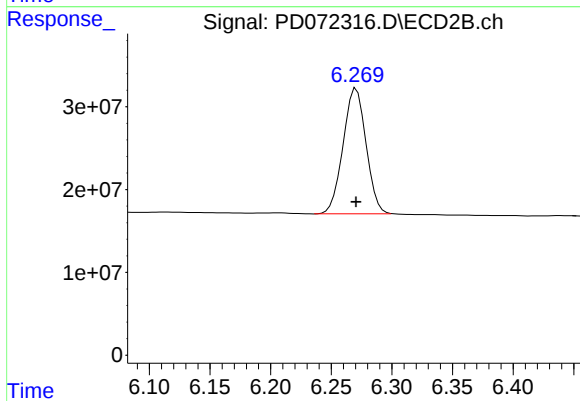

#13 Dieldrin


R.T.: 6.271 min
Delta R.T.: 0.000 min
Response: 199947195
Conc: 20.64 ng/ml

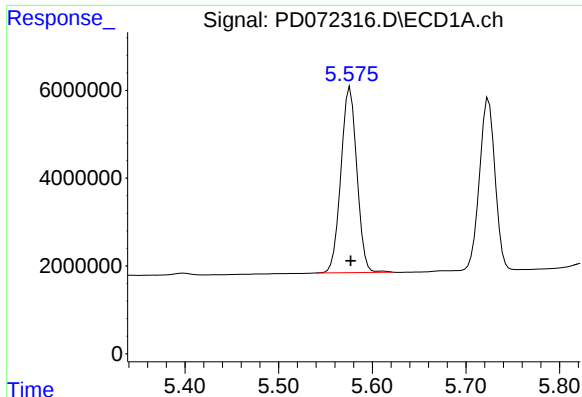

#14 Endrin


R.T.: 5.576 min
Delta R.T.: 0.000 min
Response: 50101050
Conc: 19.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

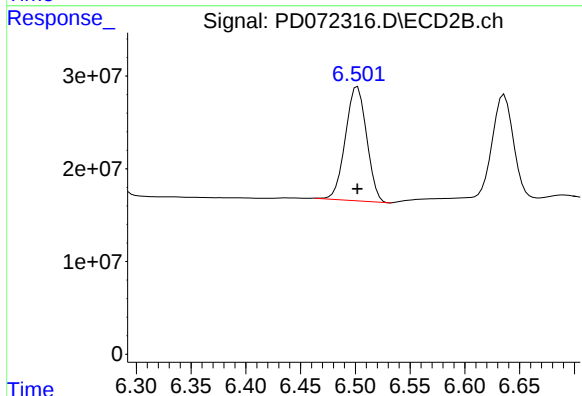


#14 Endrin

R.T.: 6.502 min
Delta R.T.: 0.000 min
Response: 166444823
Conc: 20.78 ng/ml

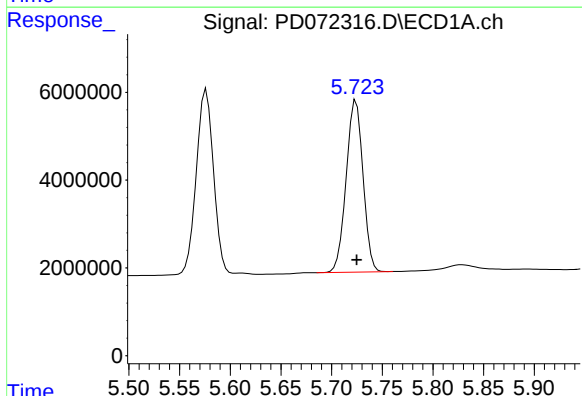


#16 4,4'-DDD

R.T.: 5.724 min
Delta R.T.: 0.000 min
Response: 45178754
Conc: 19.94 ng/ml

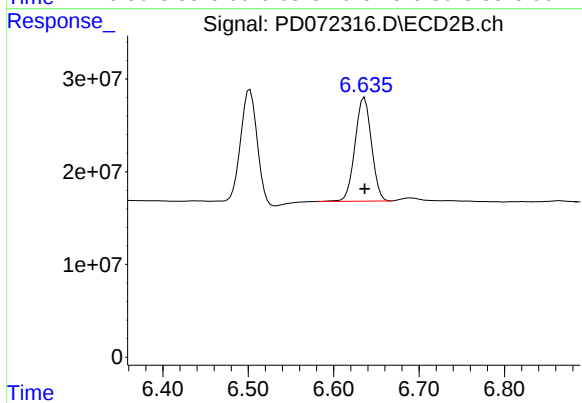

#16 4,4'-DDD


R.T.: 6.636 min
Delta R.T.: 0.000 min
Response: 149784473
Conc: 20.99 ng/ml

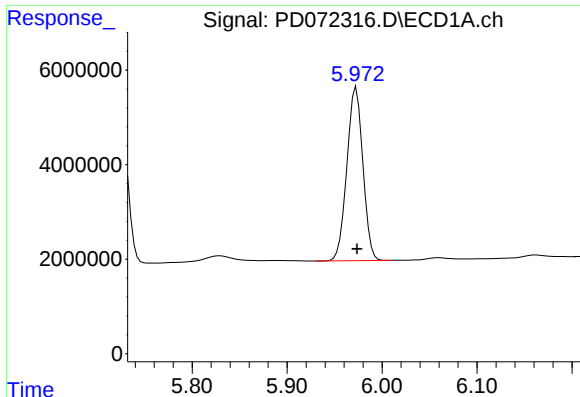

#17 4,4'-DDT


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 43014376
Conc: 19.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

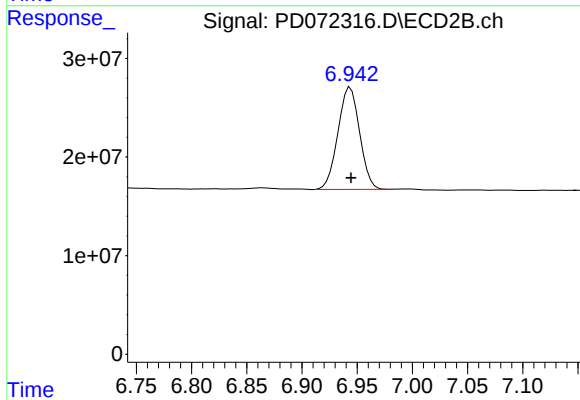


#17 4,4'-DDT

R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 141774307
Conc: 20.77 ng/ml

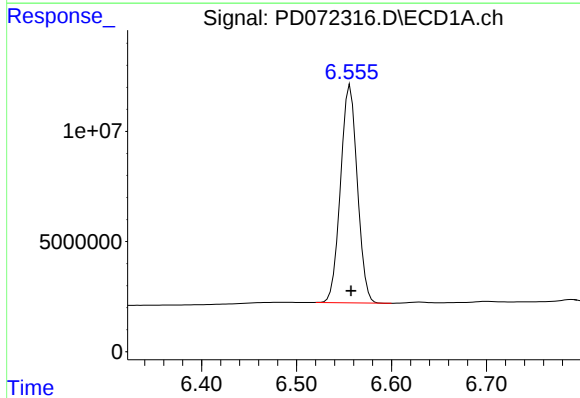


#20 Methoxychlor

R.T.: 6.556 min
Delta R.T.: 0.000 min
Response: 121604370
Conc: 102.61 ng/ml

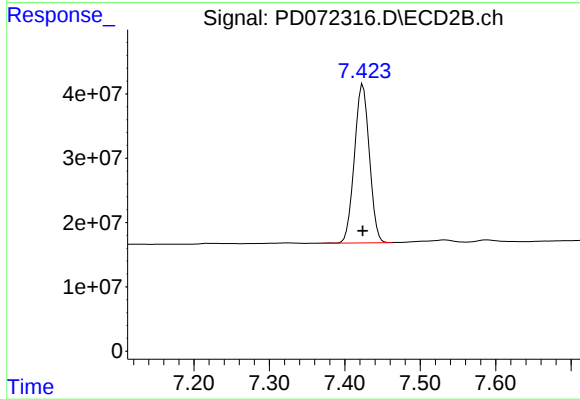

#20 Methoxychlor


R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 339211808
Conc: 105.46 ng/ml

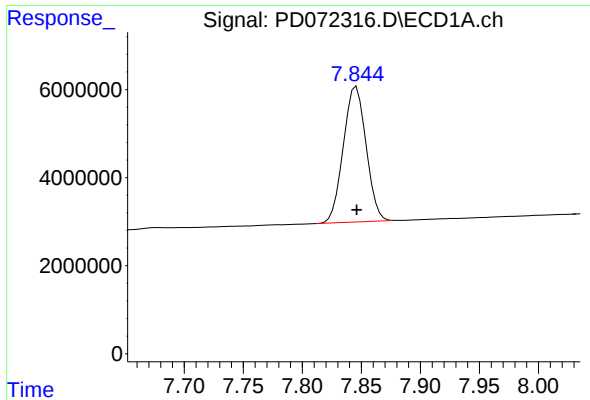

#27 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: 0.000 min
Response: 41536770
Conc: 21.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

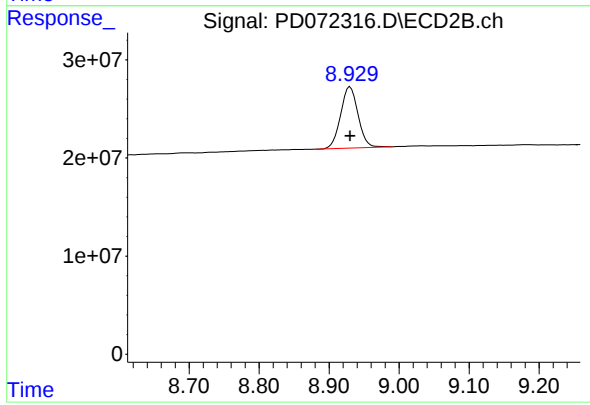

#27 Decachlorobiphenyl

R.T.: 8.930 min
Delta R.T.: 0.000 min
Response: 108057930
Conc: 21.09 ng/ml