

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2022 14:01
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 15:01:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 11 14:59:36 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.710	3.471	49043263	483.9E6	20.000	20.000
27)	SA Decachlor...	7.846	8.930	78031708	204.9E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.215	3.936	71913800	612.0E6	20.000	20.000
3)	MA gamma-BHC...	3.546	4.270	59805169	514.6E6	20.000	20.000
4)	MA Heptachlor	3.879	4.837	66032496	346.0E6	20.000	20.000
9)	A Endosulfan I	5.034	5.993	52154356	194.5E6	20.000	20.000
13)	MA Dieldrin	5.300	6.271	115.9E6	387.6E6	40.000	40.000
14)	MA Endrin	5.577	6.502	100.4E6	320.4E6	40.000	40.000
16)	A 4,4'-DDD	5.725	6.636	90636296	285.4E6	40.000	40.000
17)	MA 4,4'-DDT	5.974	6.944	86757966	273.1E6	40.000	40.000
20)	A Methoxychlor	6.557	7.424	237.0E6	643.3E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2022 14:01
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 15:01:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 11 14:59:36 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

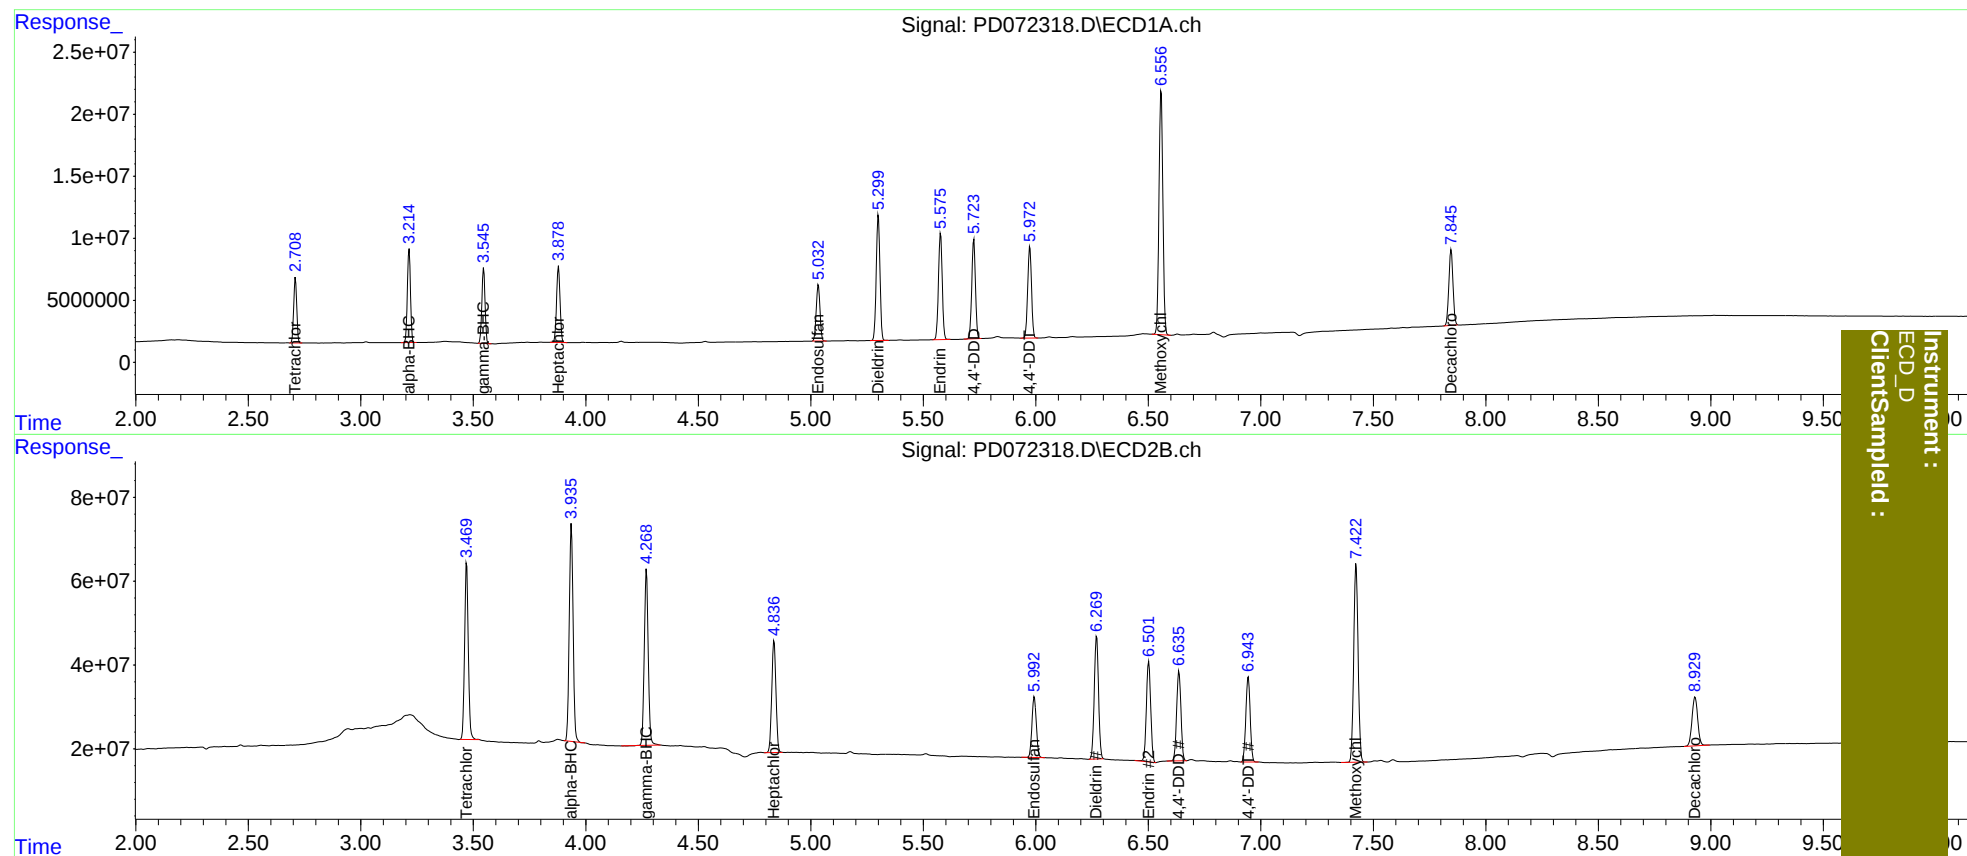


Instrument :
ECD_D
ClientSampled :
7.422

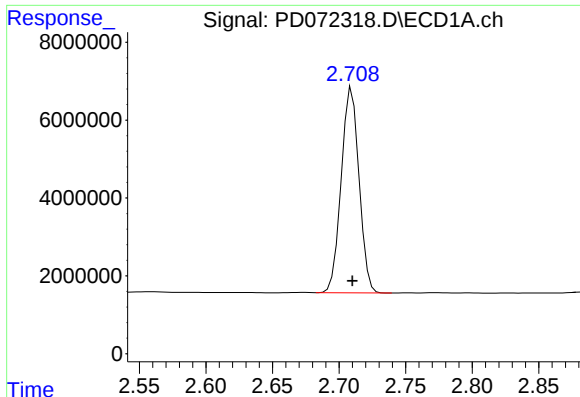

#1 Tetrachloro-m-xylene


R.T.: 2.710 min
Delta R.T.: 0.000 min
Response: 49043263
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

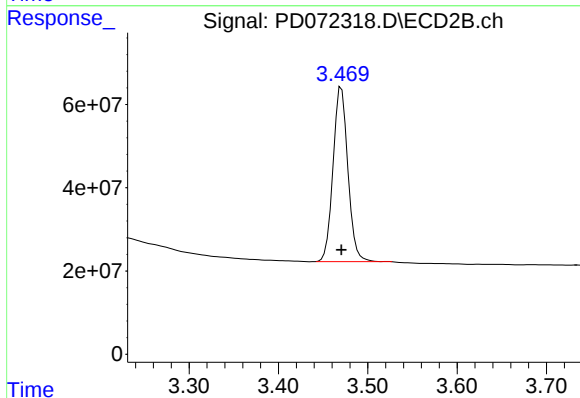


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: 0.000 min
Response: 483940088
Conc: 20.00 ng/ml

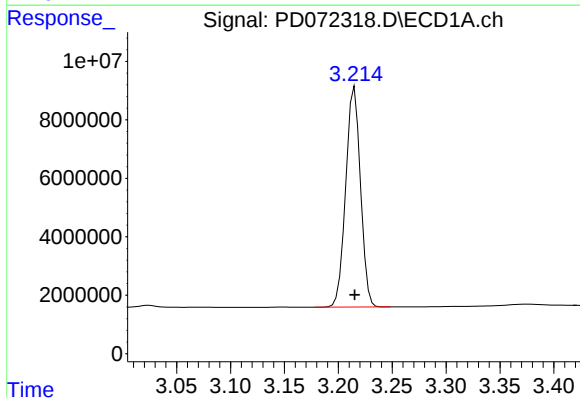


#2 alpha-BHC

R.T.: 3.215 min
Delta R.T.: 0.000 min
Response: 71913800
Conc: 20.00 ng/ml

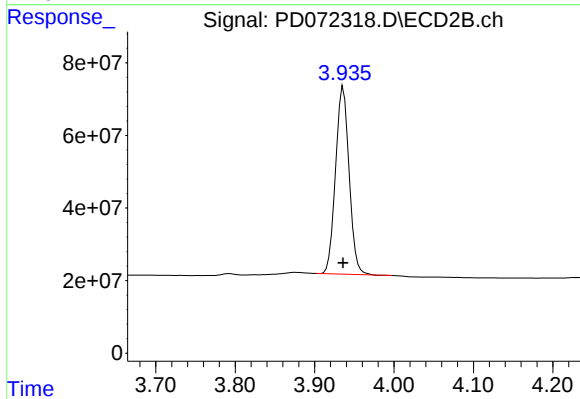

#2 alpha-BHC


R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 612048455
Conc: 20.00 ng/ml

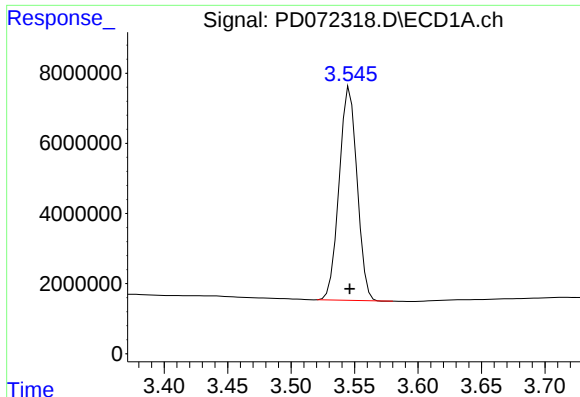

#3 gamma-BHC (Lindane)


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 59805169
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

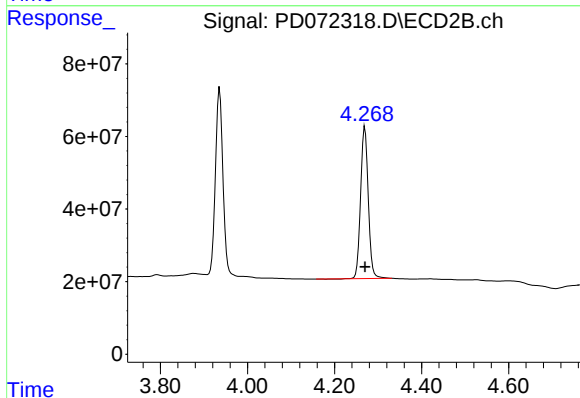


#3 gamma-BHC (Lindane)

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 514557015
Conc: 20.00 ng/ml

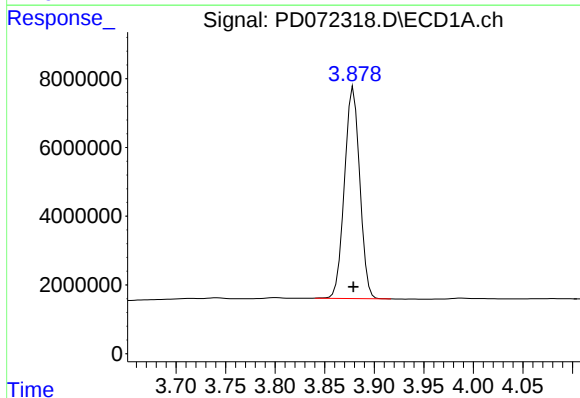


#4 Heptachlor

R.T.: 3.879 min
Delta R.T.: 0.000 min
Response: 66032496
Conc: 20.00 ng/ml

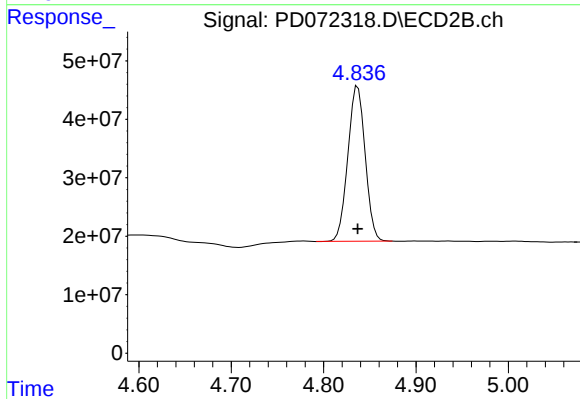

#4 Heptachlor


R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 345964600
Conc: 20.00 ng/ml

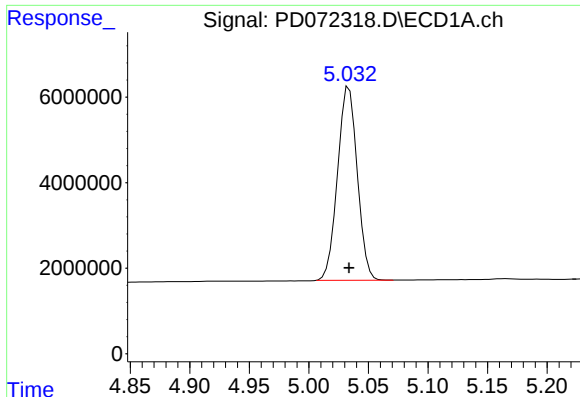

#9 Endosulfan I


R.T.: 5.034 min
Delta R.T.: 0.000 min
Response: 52154356
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

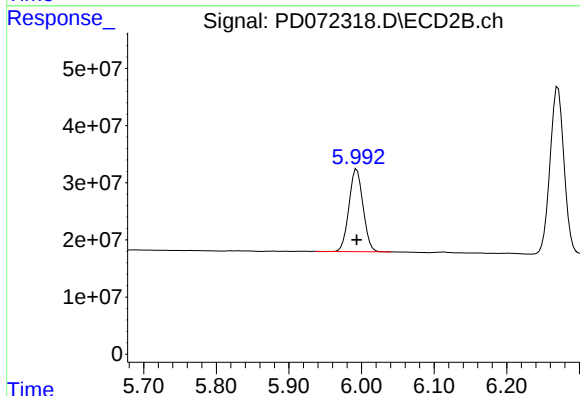


#9 Endosulfan I

R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 194476128
Conc: 20.00 ng/ml

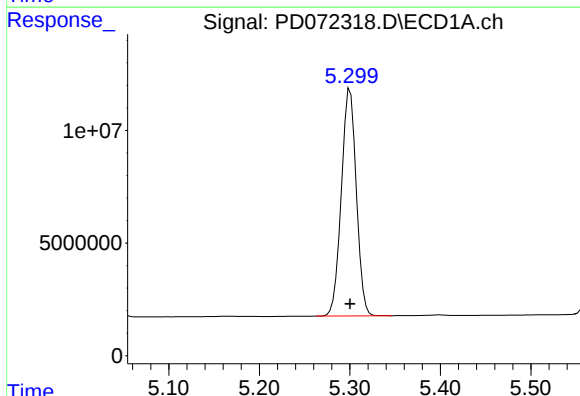


#13 Dieldrin

R.T.: 5.300 min
Delta R.T.: 0.000 min
Response: 115945332
Conc: 40.00 ng/ml

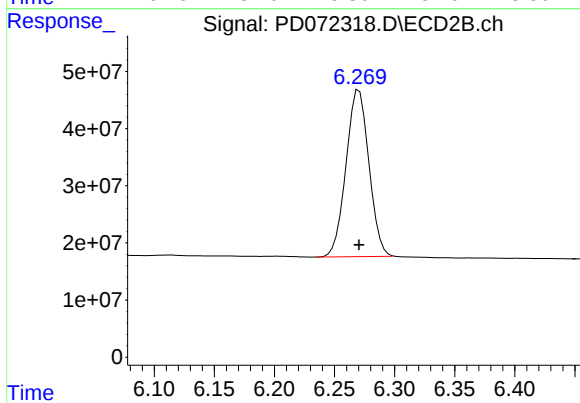

#13 Dieldrin


R.T.: 6.271 min
Delta R.T.: 0.000 min
Response: 387577283
Conc: 40.00 ng/ml

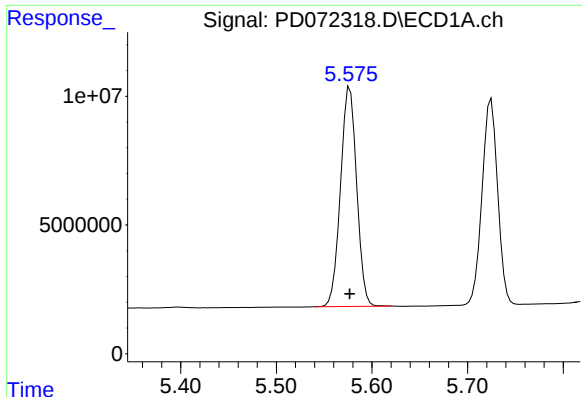

#14 Endrin


R.T.: 5.577 min
Delta R.T.: 0.000 min
Response: 100381935
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

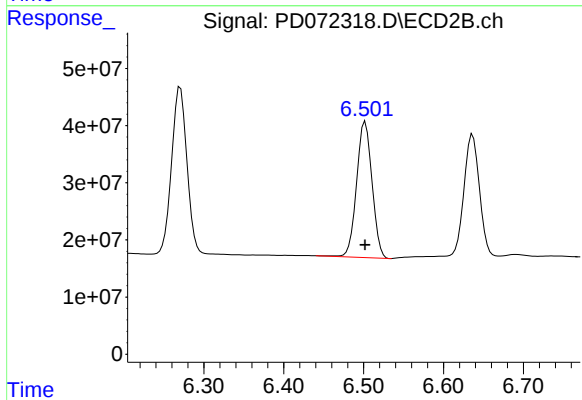


#14 Endrin

R.T.: 6.502 min
Delta R.T.: 0.000 min
Response: 320416025
Conc: 40.00 ng/ml

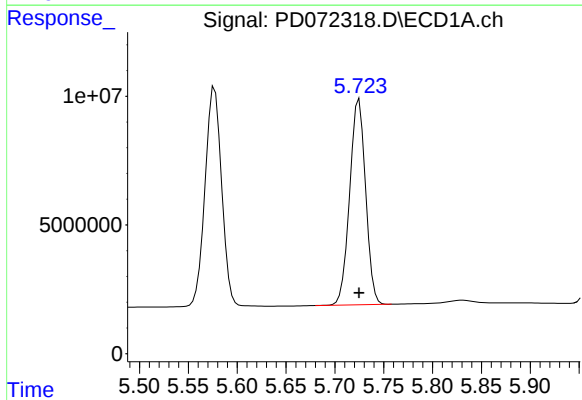


#16 4,4'-DDD

R.T.: 5.725 min
Delta R.T.: 0.000 min
Response: 90636296
Conc: 40.00 ng/ml

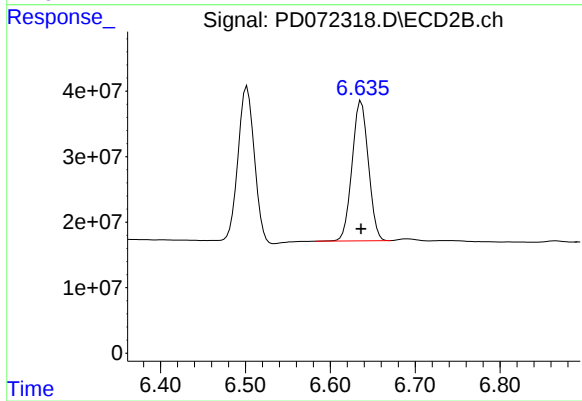

#16 4,4'-DDD


R.T.: 6.636 min
Delta R.T.: 0.000 min
Response: 285416534
Conc: 40.00 ng/ml

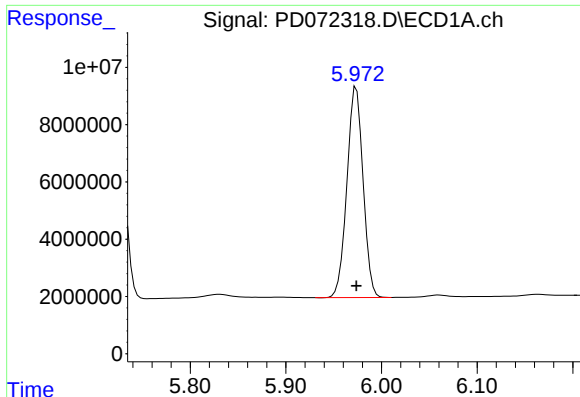

#17 4,4'-DDT


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 86757966
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

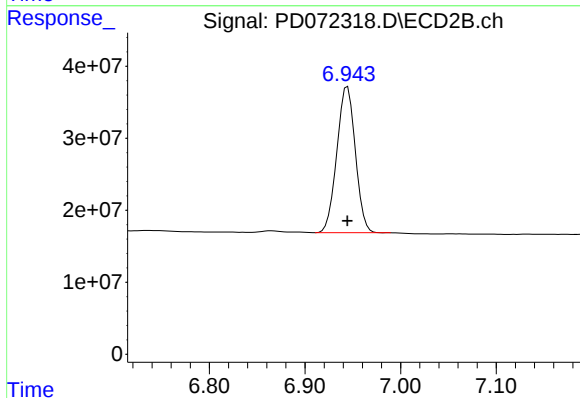


#17 4,4'-DDT

R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 273098757
Conc: 40.00 ng/ml

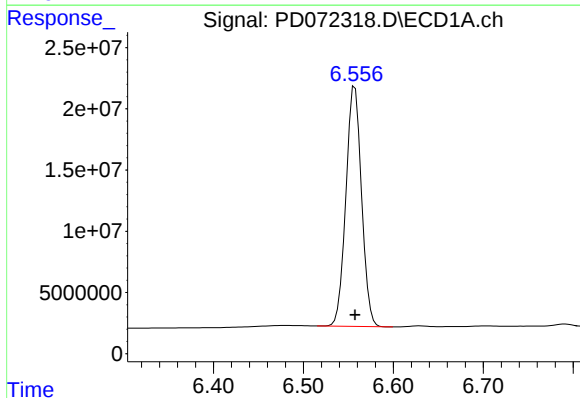


#20 Methoxychlor

R.T.: 6.557 min
Delta R.T.: 0.000 min
Response: 237031165
Conc: 200.00 ng/ml

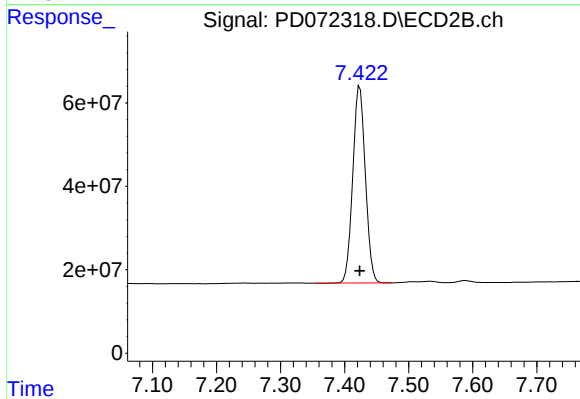

#20 Methoxychlor


R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 643312933
Conc: 200.00 ng/ml

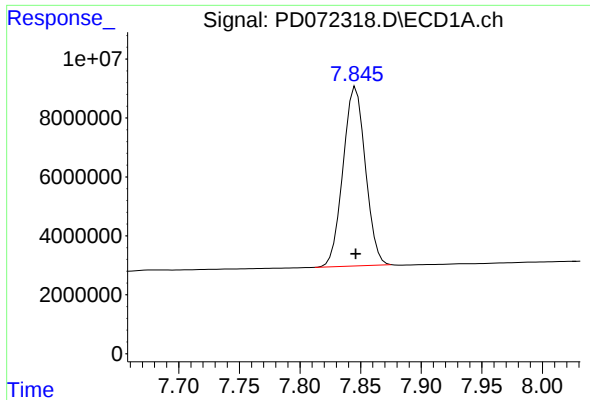

#27 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: 0.000 min
Response: 78031708
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

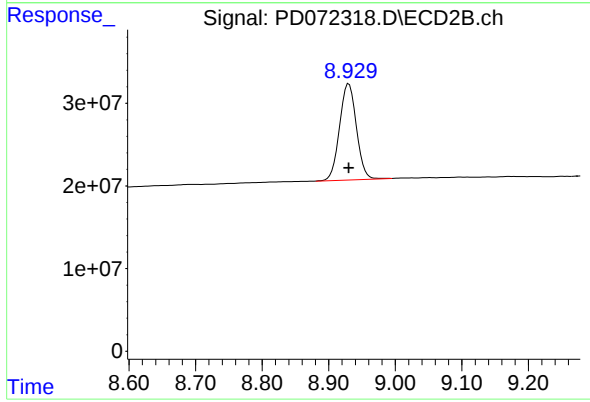

#27 Decachlorobiphenyl

R.T.: 8.930 min
Delta R.T.: 0.000 min
Response: 204898411
Conc: 40.00 ng/ml