

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2022 14:28
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 15:01:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 11 14:59:36 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.710	3.471	94122170	886.5E6	38.383	36.638
27)	SA Decachlor...	7.846	8.930	145.7E6	379.7E6	74.702	74.127
Target Compounds							
2)	A alpha-BHC	3.215	3.936	144.8E6	1128.4E6	40.278	36.874
3)	MA gamma-BHC...	3.547	4.270	120.1E6	935.0E6	40.165	36.344
4)	MA Heptachlor	3.879	4.837	130.1E6	623.5E6	39.406	36.045
9)	A Endosulfan I	5.034	5.993	101.2E6	354.6E6	38.817	36.466
13)	MA Dieldrin	5.300	6.271	230.0E6	708.2E6	79.351	73.085
14)	MA Endrin	5.577	6.502	197.9E6	583.3E6	78.863	72.816
16)	A 4,4'-DDD	5.724	6.636	179.2E6	529.4E6	79.095	74.195
17)	MA 4,4'-DDT	5.973	6.944	173.3E6	511.0E6	79.901	74.847
20)	A Methoxychlor	6.557	7.424	455.7E6	1194.5E6	384.488	371.356


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2022 14:28
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 15:01:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 11 14:59:36 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

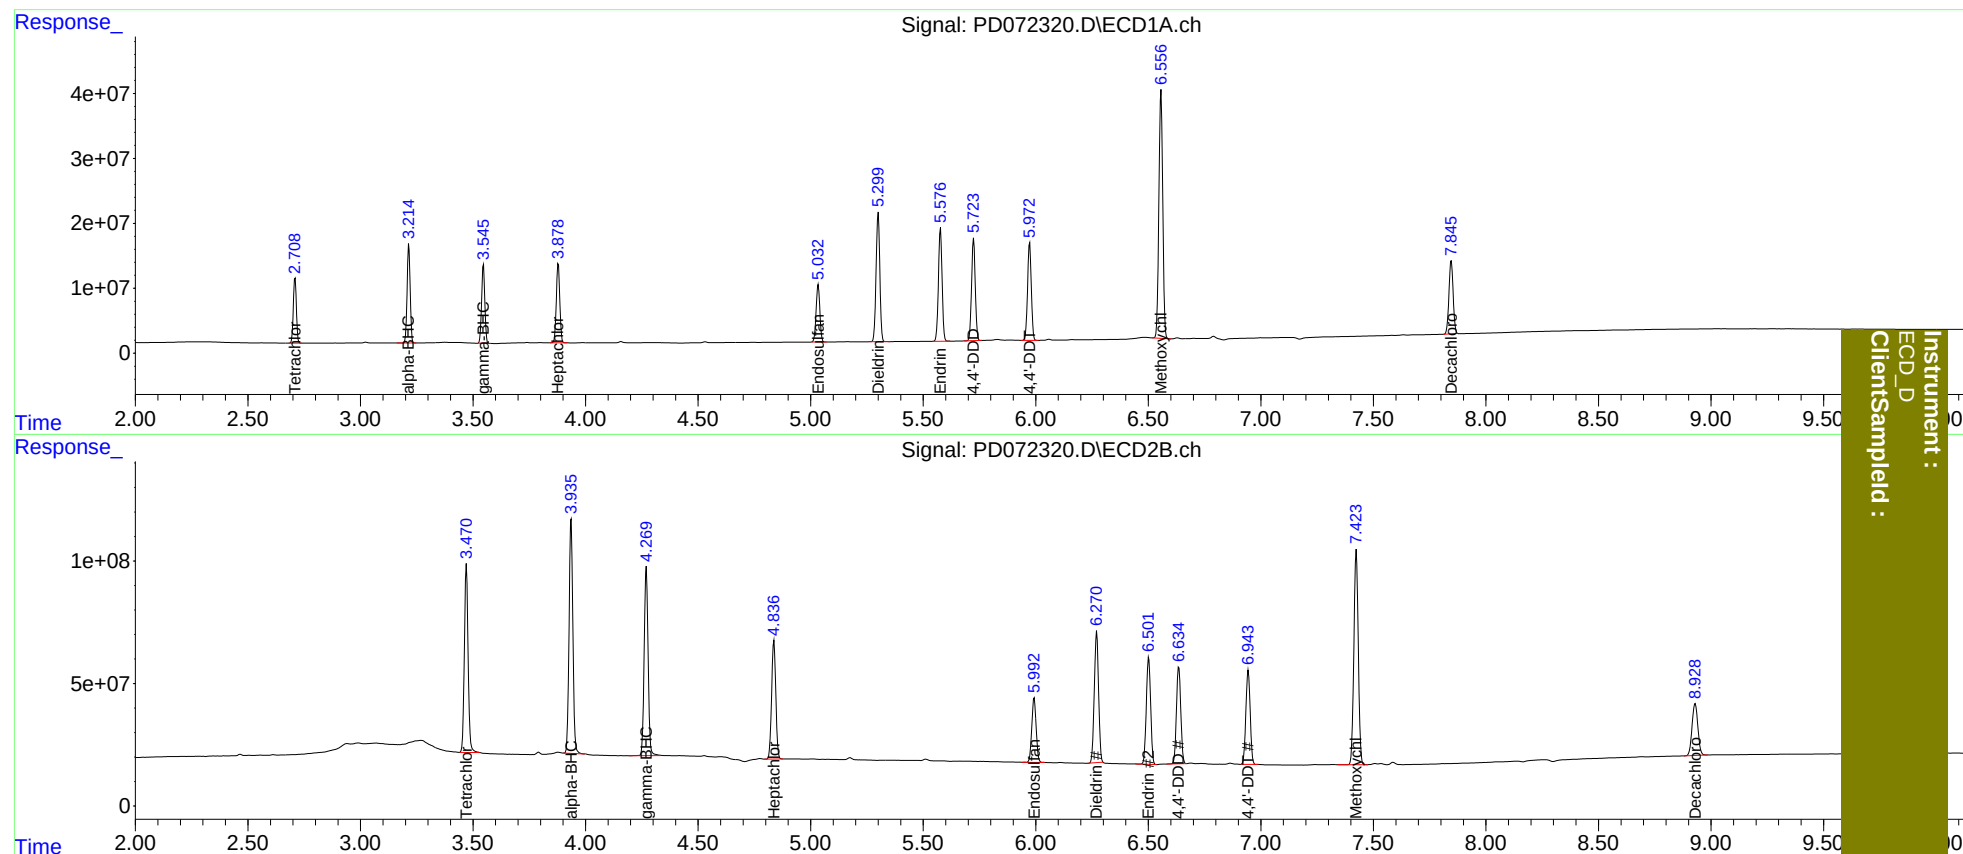


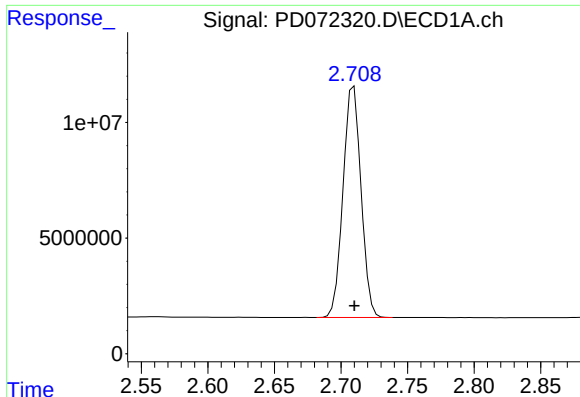

#1 Tetrachloro-m-xylene


R.T.: 2.710 min
Delta R.T.: 0.000 min
Response: 94122170
Conc: 38.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

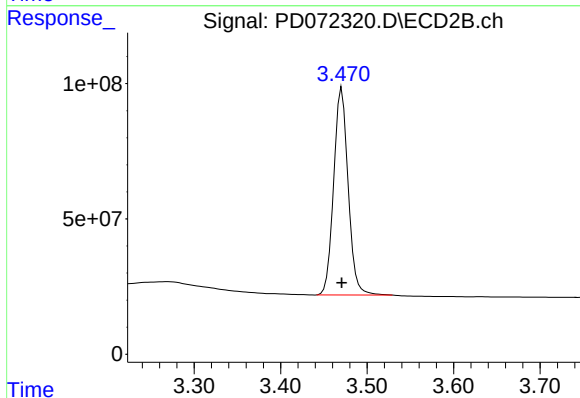


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: 0.000 min
Response: 886530038
Conc: 36.64 ng/ml

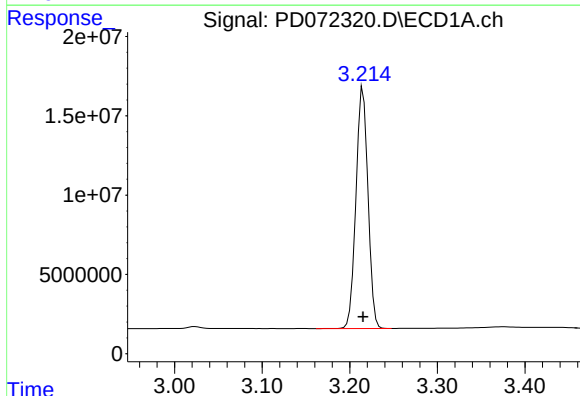


#2 alpha-BHC

R.T.: 3.215 min
Delta R.T.: 0.000 min
Response: 144826998
Conc: 40.28 ng/ml

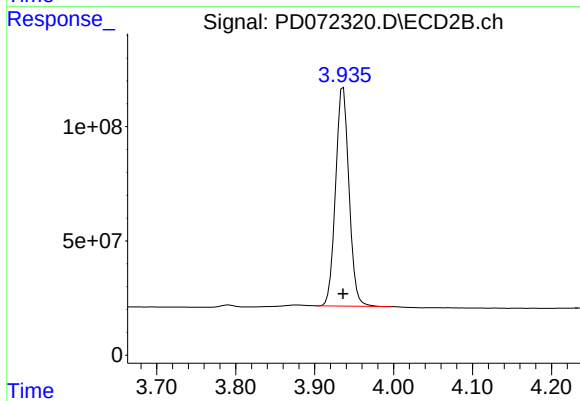

#2 alpha-BHC


R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 1128423339
Conc: 36.87 ng/ml

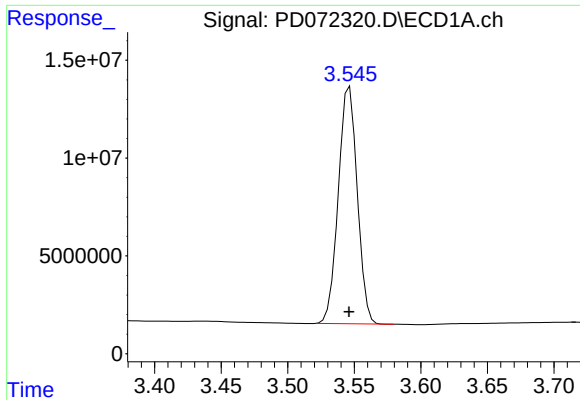

#3 gamma-BHC (Lindane)


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 120105095
Conc: 40.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

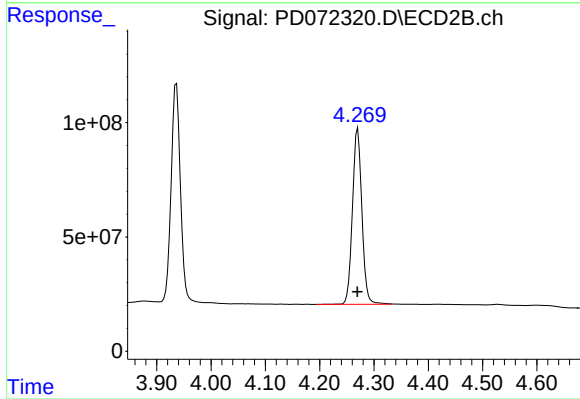


#3 gamma-BHC (Lindane)

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 935047866
Conc: 36.34 ng/ml

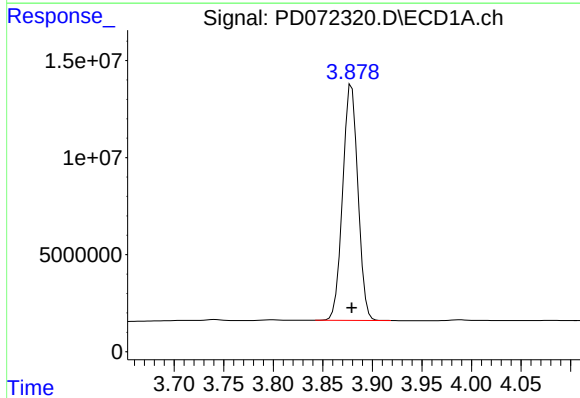


#4 Heptachlor

R.T.: 3.879 min
Delta R.T.: 0.000 min
Response: 130105408
Conc: 39.41 ng/ml

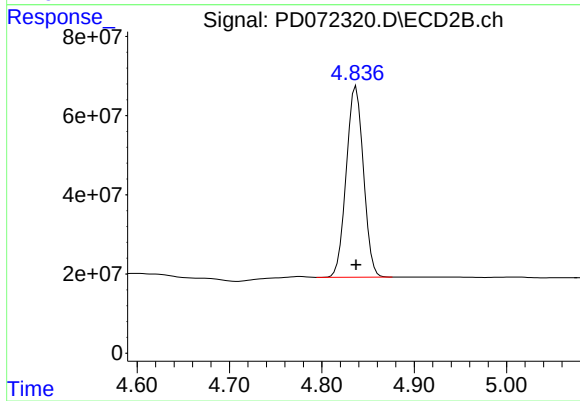

#4 Heptachlor


R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 623518348
Conc: 36.05 ng/ml

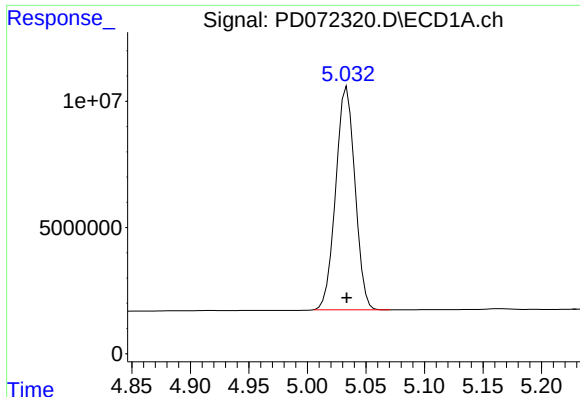

#9 Endosulfan I


R.T.: 5.034 min
Delta R.T.: 0.000 min
Response: 101223127
Conc: 38.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

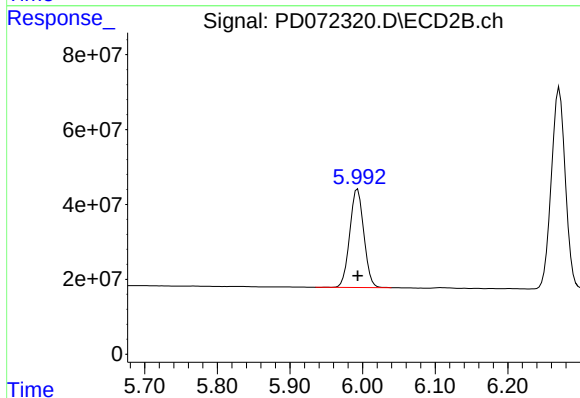


#9 Endosulfan I

R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 354589680
Conc: 36.47 ng/ml

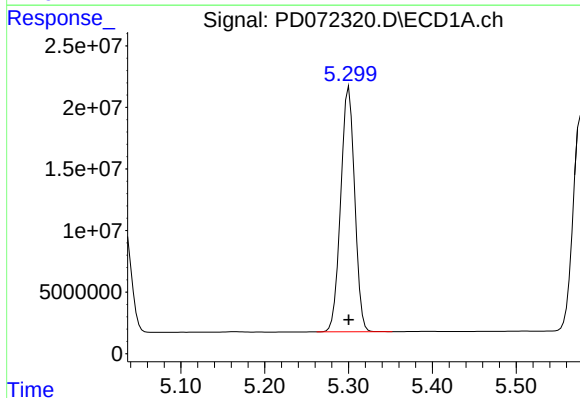


#13 Dieldrin

R.T.: 5.300 min
Delta R.T.: 0.000 min
Response: 230009707
Conc: 79.35 ng/ml

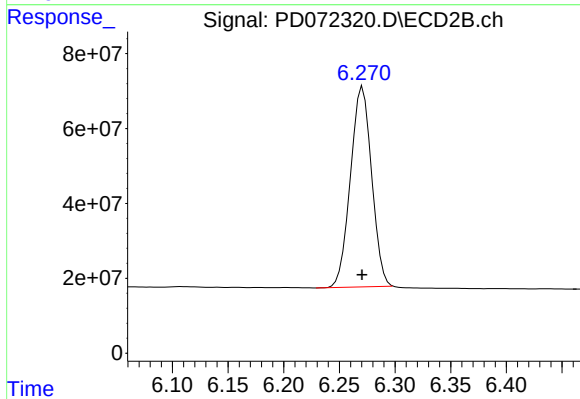

#13 Dieldrin


R.T.: 6.271 min
Delta R.T.: 0.000 min
Response: 708156546
Conc: 73.09 ng/ml

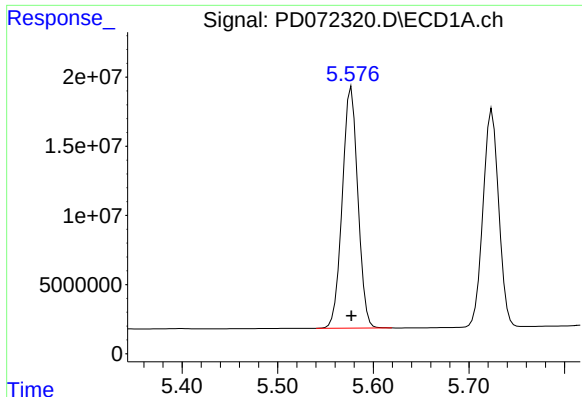

#14 Endrin


R.T.: 5.577 min
Delta R.T.: 0.000 min
Response: 197910421
Conc: 78.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

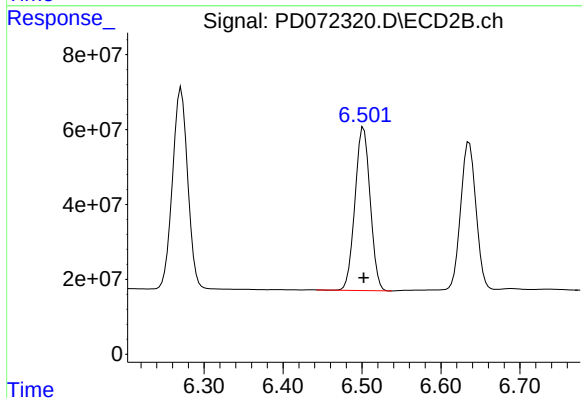


#14 Endrin

R.T.: 6.502 min
Delta R.T.: 0.000 min
Response: 583284924
Conc: 72.82 ng/ml

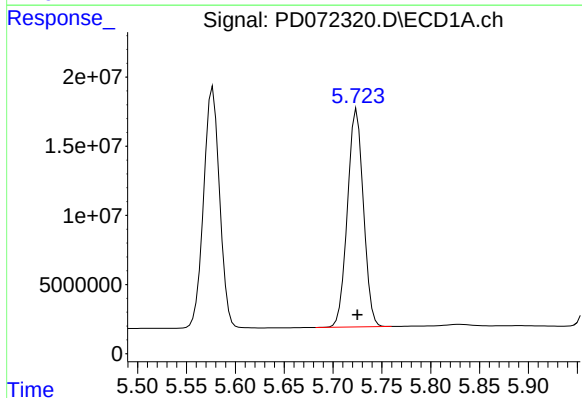


#16 4,4'-DDD

R.T.: 5.724 min
Delta R.T.: 0.000 min
Response: 179221344
Conc: 79.09 ng/ml

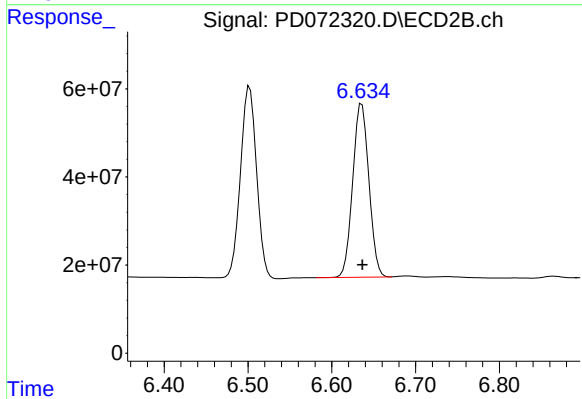

#16 4,4'-DDD


R.T.: 6.636 min
Delta R.T.: 0.000 min
Response: 529411872
Conc: 74.19 ng/ml

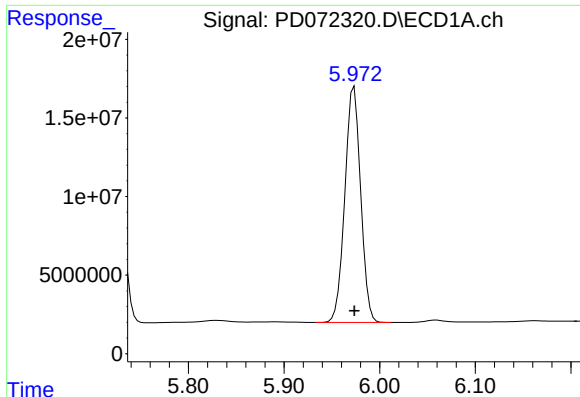

#17 4,4'-DDT


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 173300557
Conc: 79.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

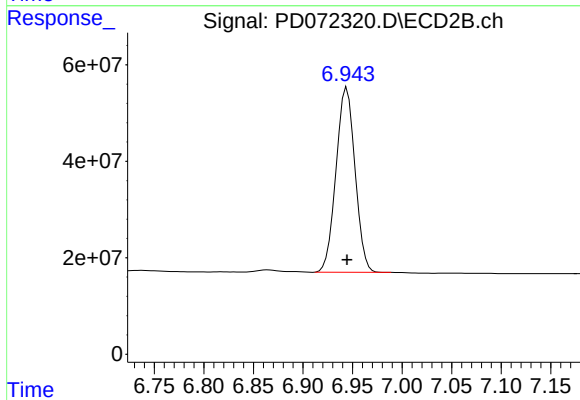


#17 4,4'-DDT

R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 511016905
Conc: 74.85 ng/ml

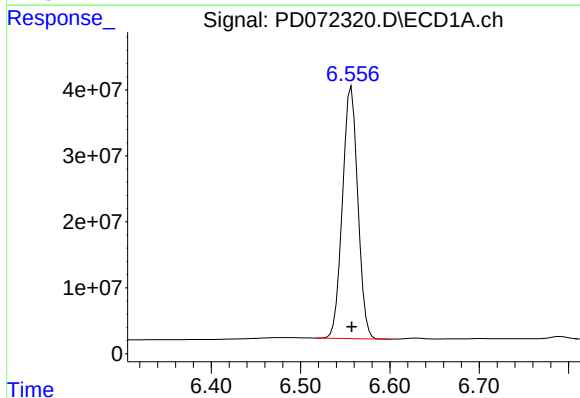


#20 Methoxychlor

R.T.: 6.557 min
Delta R.T.: 0.000 min
Response: 455678414
Conc: 384.49 ng/ml

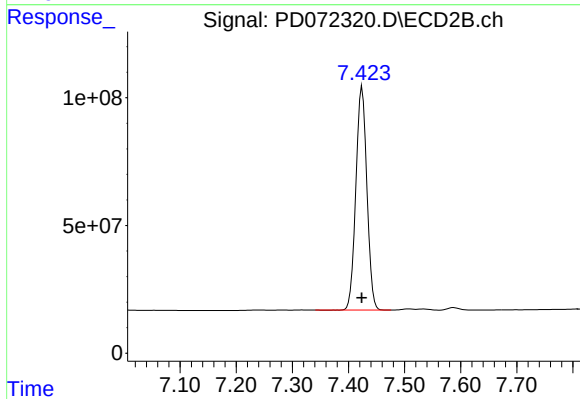

#20 Methoxychlor


R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 1194490670
Conc: 371.36 ng/ml

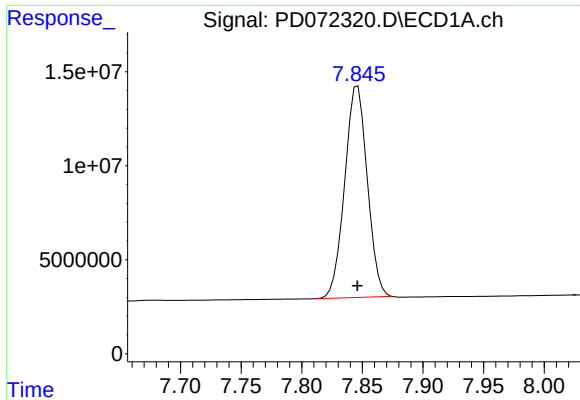

#27 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: 0.000 min
Response: 145728491
Conc: 74.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

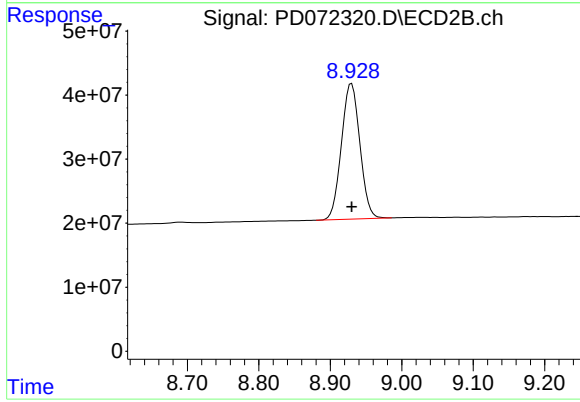

#27 Decachlorobiphenyl

R.T.: 8.930 min
Delta R.T.: 0.000 min
Response: 379714756
Conc: 74.13 ng/ml