

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2022 14:54
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 15:21:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 11 14:59:36 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.710	3.471	182.4E6	1625.8E6	74.392	67.188
27)	SA Decachlor...	7.847	8.930	286.5E6	744.8E6	146.839	145.402
Target Compounds							
2)	A alpha-BHC	3.215	3.937	293.1E6	2148.3E6	81.527	70.201
3)	MA gamma-BHC...	3.546	4.271	248.9E6	1744.0E6	83.225	67.788
4)	MA Heptachlor	3.879	4.838	264.7E6	1159.9E6	80.172	67.054
9)	A Endosulfan I	5.034	5.994	202.8E6	674.5E6	77.765	69.366
13)	MA Dieldrin	5.301	6.271	468.5E6	1380.5E6	161.623	142.475
14)	MA Endrin	5.577	6.503	406.5E6	1136.5E6	161.963	141.882
16)	A 4,4'-DDD	5.724	6.637	364.3E6	1033.4E6	160.766	144.821
17)	MA 4,4'-DDT	5.974	6.944	357.8E6	1010.7E6	164.953	148.032
20)	A Methoxychlor	6.558	7.424	912.3E6	2352.5E6	769.782	731.385


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2022 14:54
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 15:21:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 11 14:59:36 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

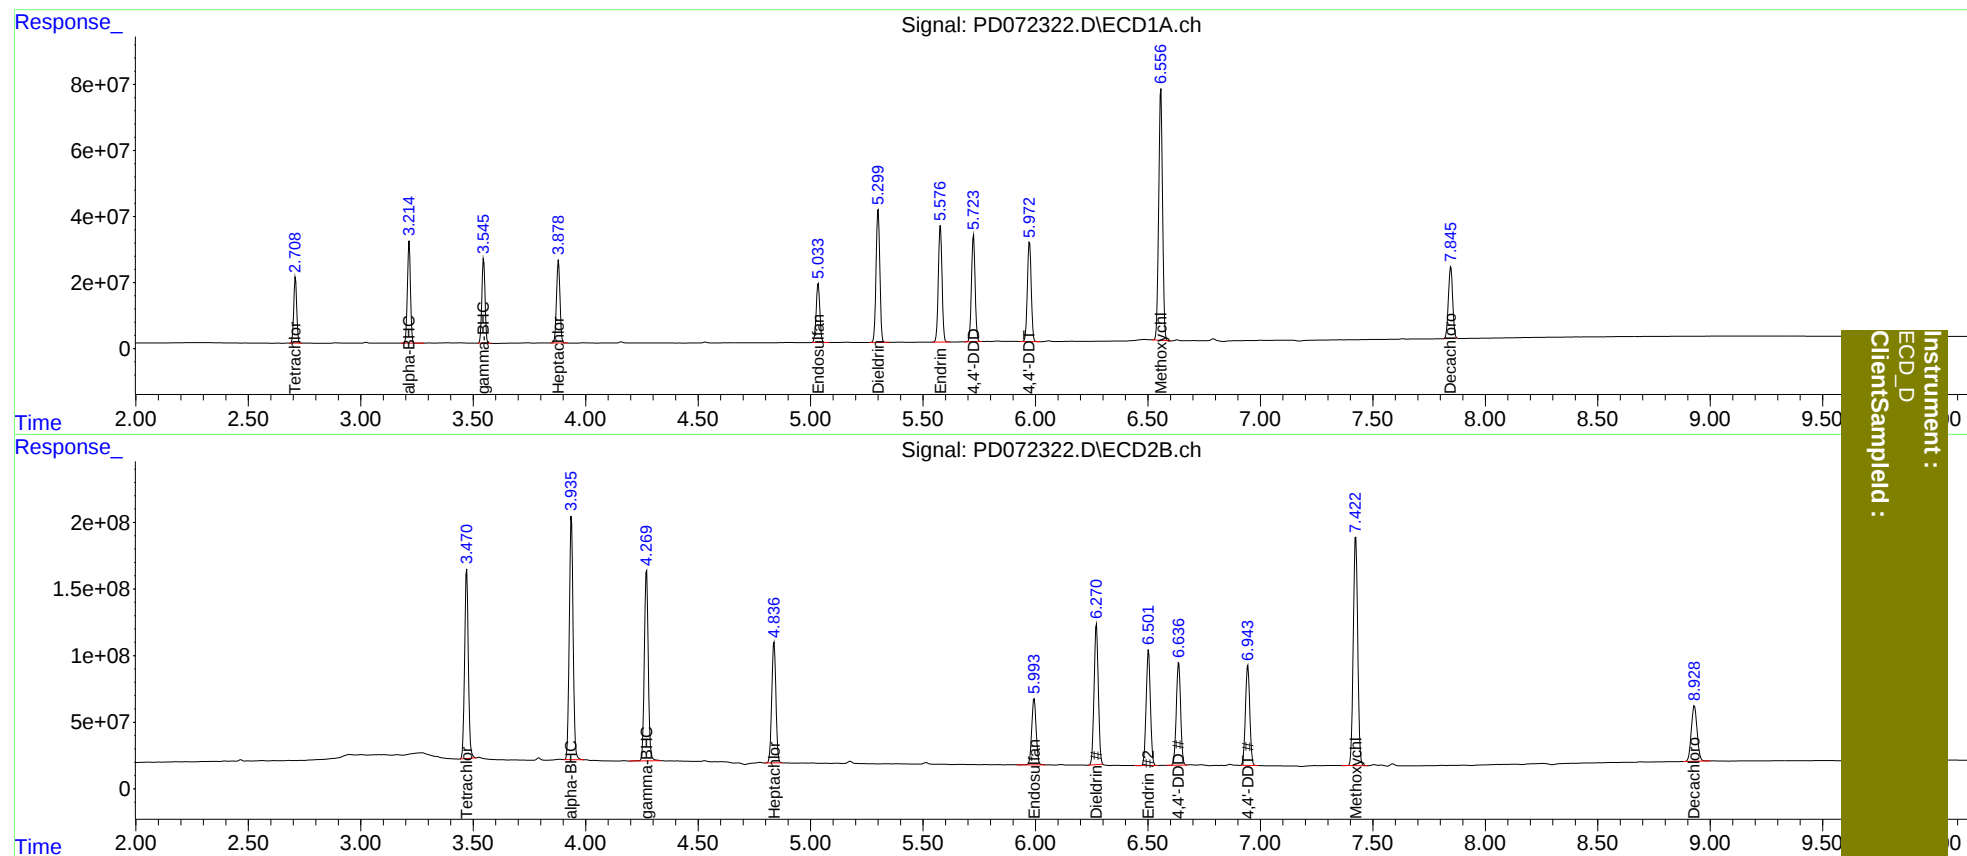


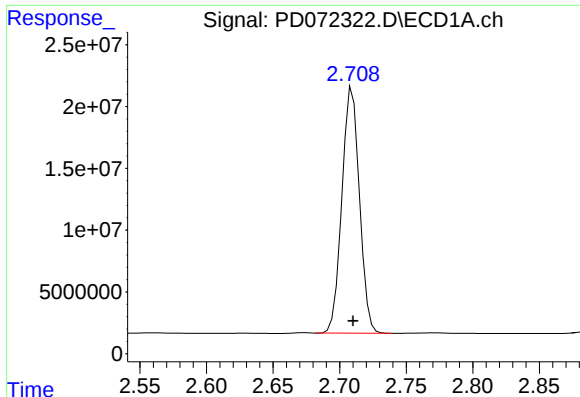

#1 Tetrachloro-m-xylene


R.T.: 2.710 min
Delta R.T.: 0.000 min
Response: 182421523
Conc: 74.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

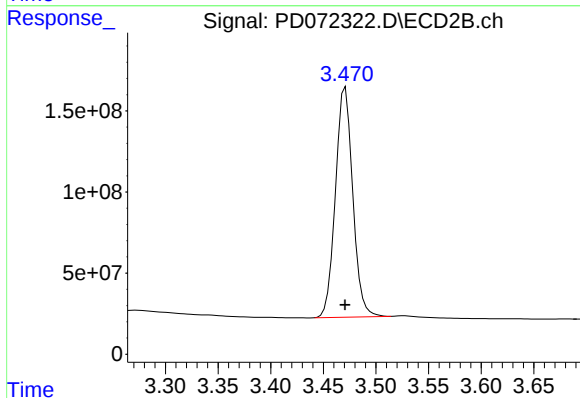


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: 0.000 min
Response: 1625751320
Conc: 67.19 ng/ml

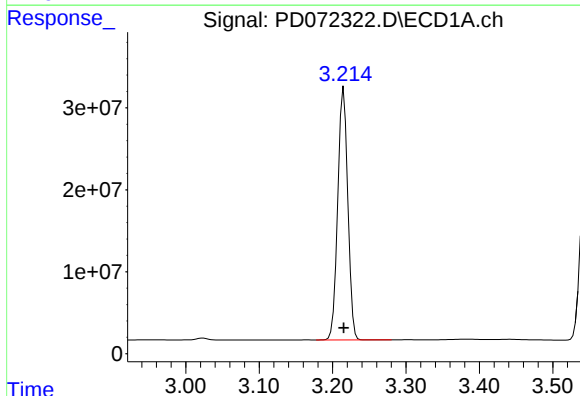


#2 alpha-BHC

R.T.: 3.215 min
Delta R.T.: 0.000 min
Response: 293144127
Conc: 81.53 ng/ml

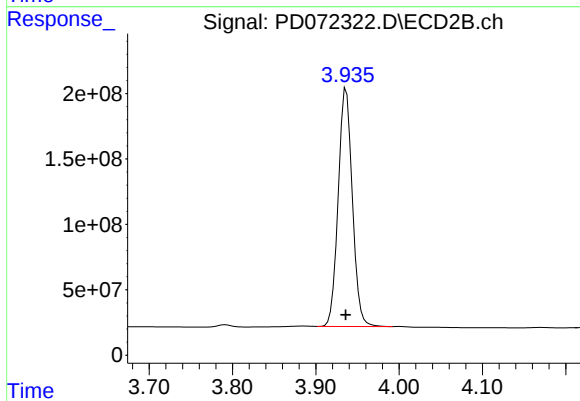

#2 alpha-BHC


R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 2148330306
Conc: 70.20 ng/ml

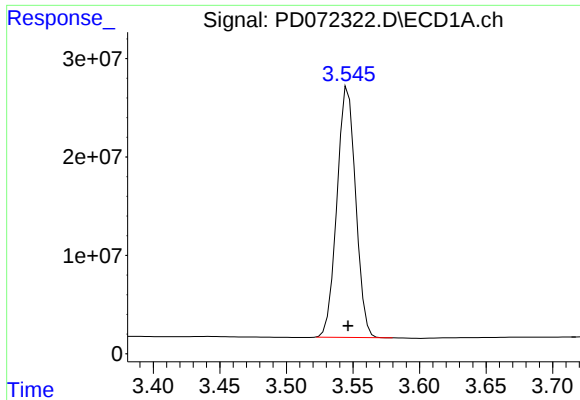

#3 gamma-BHC (Lindane)


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 248863288
Conc: 83.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

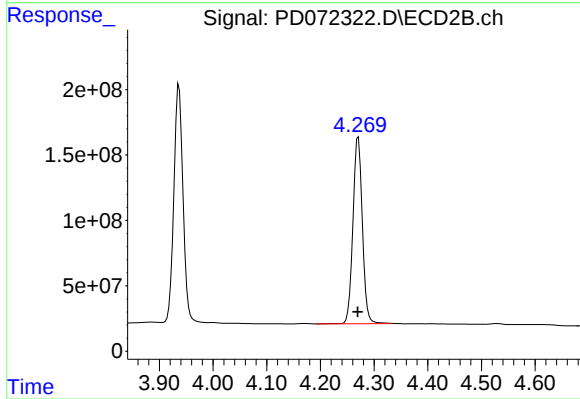


#3 gamma-BHC (Lindane)

R.T.: 4.271 min
Delta R.T.: 0.000 min
Response: 1744038913
Conc: 67.79 ng/ml

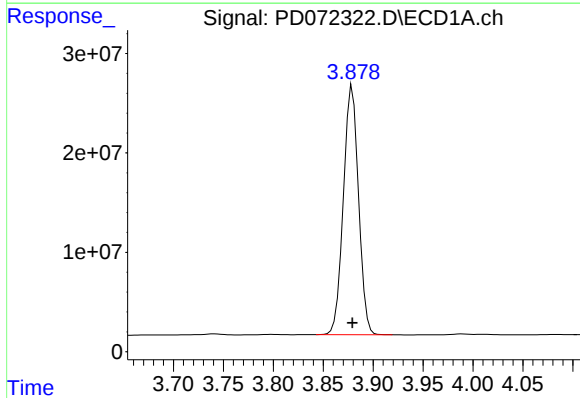


#4 Heptachlor

R.T.: 3.879 min
Delta R.T.: 0.000 min
Response: 264697102
Conc: 80.17 ng/ml

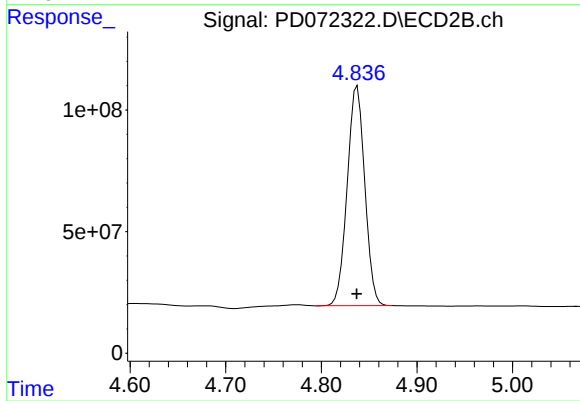

#4 Heptachlor


R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 1159909218
Conc: 67.05 ng/ml

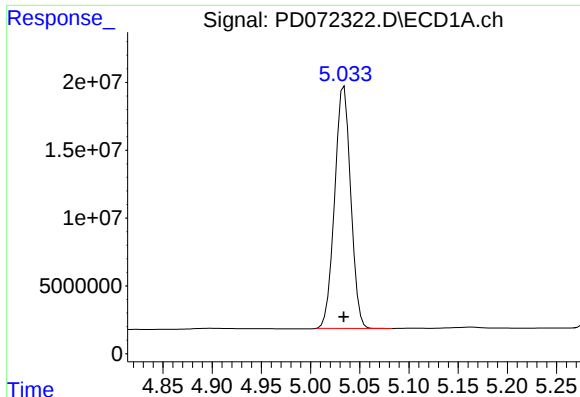

#9 Endosulfan I


R.T.: 5.034 min
Delta R.T.: 0.000 min
Response: 202788577
Conc: 77.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

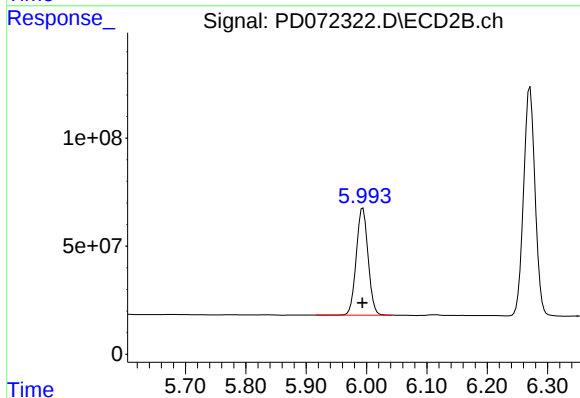


#9 Endosulfan I

R.T.: 5.994 min
Delta R.T.: 0.000 min
Response: 674500819
Conc: 69.37 ng/ml

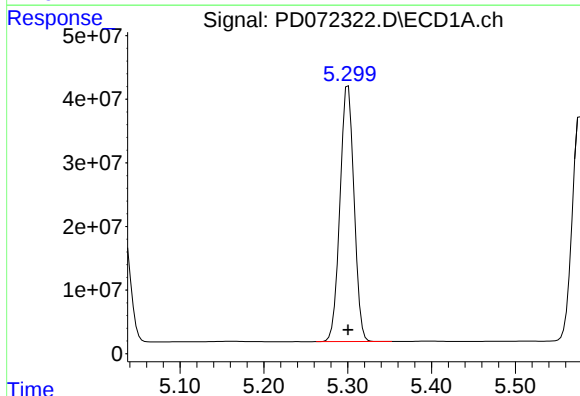


#13 Dieldrin

R.T.: 5.301 min
Delta R.T.: 0.000 min
Response: 468487150
Conc: 161.62 ng/ml

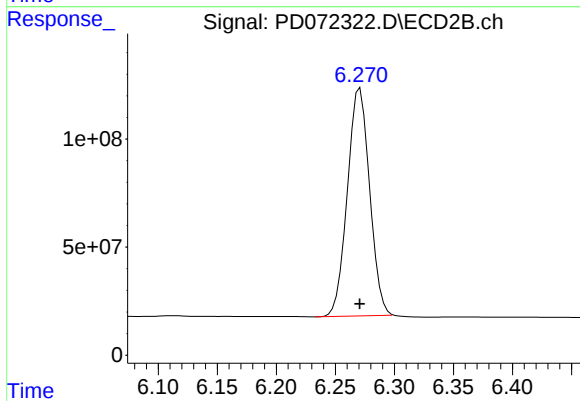

#13 Dieldrin


R.T.: 6.271 min
Delta R.T.: 0.000 min
Response: 1380498189
Conc: 142.47 ng/ml

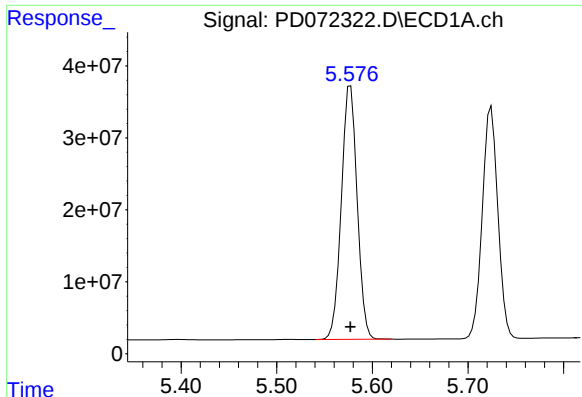

#14 Endrin


R.T.: 5.577 min
Delta R.T.: 0.000 min
Response: 406453686
Conc: 161.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

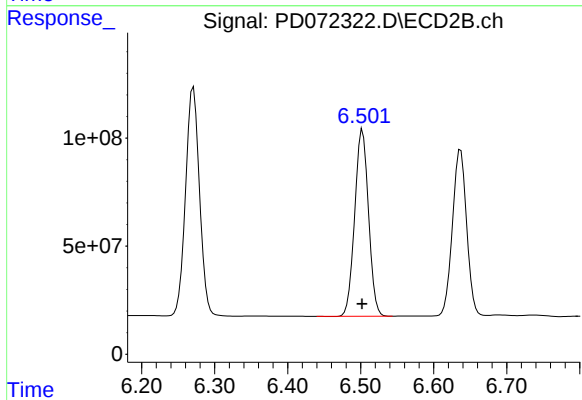


#14 Endrin

R.T.: 6.503 min
Delta R.T.: 0.000 min
Response: 1136535639
Conc: 141.88 ng/ml

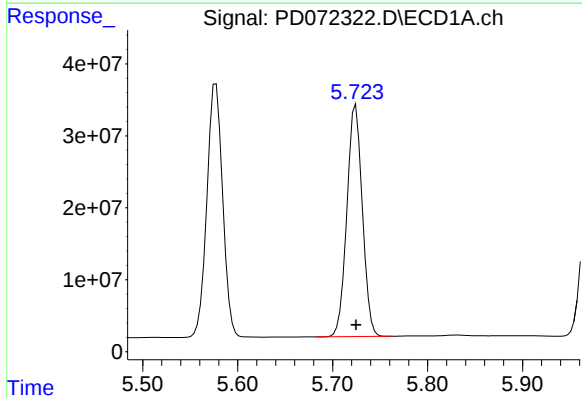


#16 4,4'-DDD

R.T.: 5.724 min
Delta R.T.: 0.000 min
Response: 364281046
Conc: 160.77 ng/ml

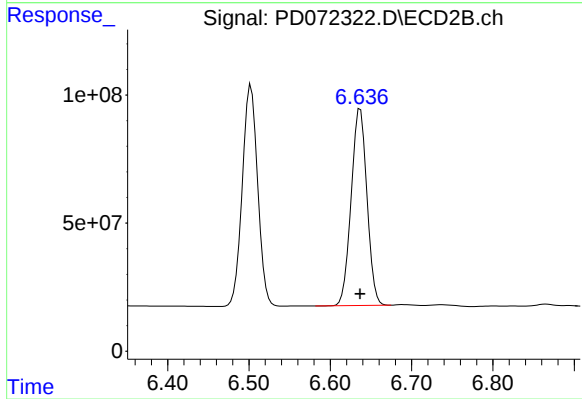

#16 4,4'-DDD


R.T.: 6.637 min
Delta R.T.: 0.000 min
Response: 1033359362
Conc: 144.82 ng/ml

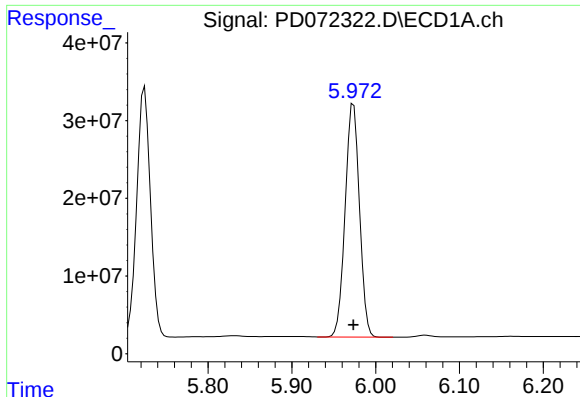

#17 4,4'-DDT


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 357773685
Conc: 164.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

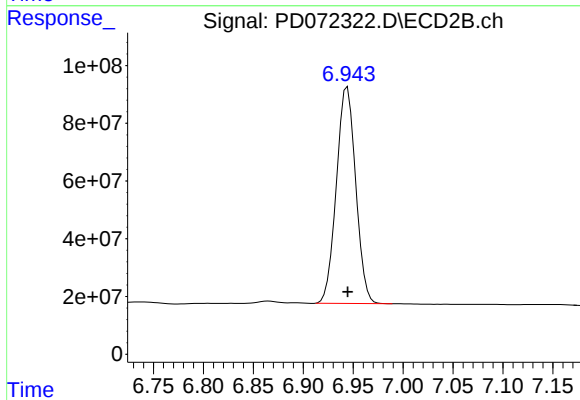


#17 4,4'-DDT

R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 1010686030
Conc: 148.03 ng/ml

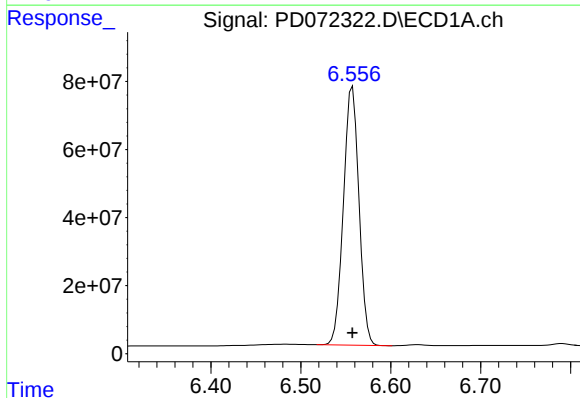


#20 Methoxychlor

R.T.: 6.558 min
Delta R.T.: 0.000 min
Response: 912311127
Conc: 769.78 ng/ml

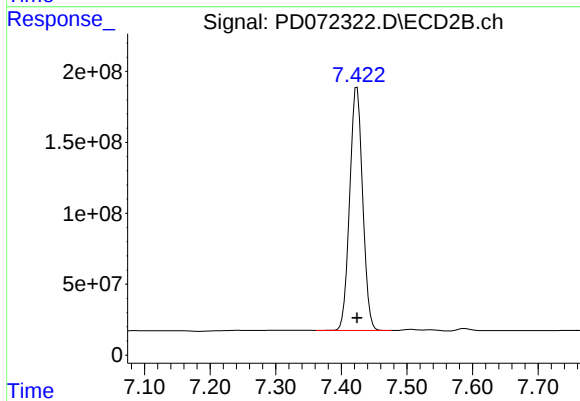

#20 Methoxychlor


R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 2352547467
Conc: 731.39 ng/ml

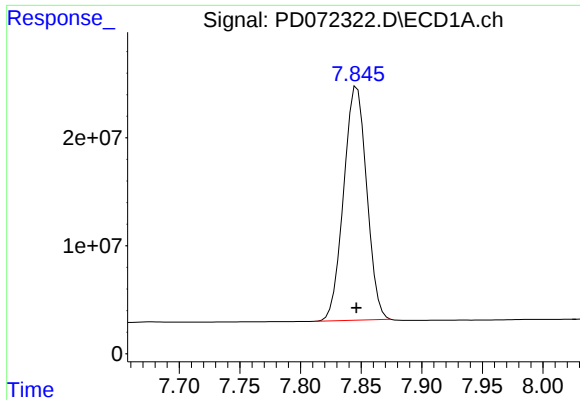

#27 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: 0.000 min
Response: 286453048
Conc: 146.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

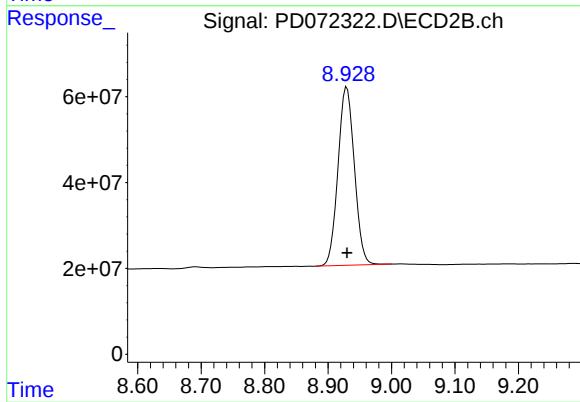

#27 Decachlorobiphenyl

R.T.: 8.930 min
Delta R.T.: 0.000 min
Response: 744818050
Conc: 145.40 ng/ml