

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2022 14:54
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5035

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 15:21:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 11 14:59:36 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.710	3.471	182.4E6	1625.8E6	74.392	67.188
27)	SA Decachlor...	7.847	8.930	286.5E6	744.8E6	146.839	145.402
Target Compounds							
2)	A alpha-BHC	3.215	3.937	293.1E6	2148.3E6	81.527	70.201
3)	MA gamma-BHC...	3.546	4.271	248.9E6	1744.0E6	83.225	67.788
4)	MA Heptachlor	3.879	4.838	264.7E6	1159.9E6	80.172	67.054
9)	A Endosulfan I	5.034	5.994	202.8E6	674.5E6	77.765	69.366
13)	MA Dieldrin	5.301	6.271	468.5E6	1380.5E6	161.623	142.475
14)	MA Endrin	5.577	6.503	406.5E6	1136.5E6	161.963	141.882
16)	A 4,4'-DDD	5.724	6.637	364.3E6	1033.4E6	160.766	144.821
17)	MA 4,4'-DDT	5.974	6.944	357.8E6	1010.7E6	164.953	148.032
20)	A Methoxychlor	6.558	7.424	912.3E6	2352.5E6	769.782	731.385

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2022 14:54
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 15:21:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 11 14:59:36 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

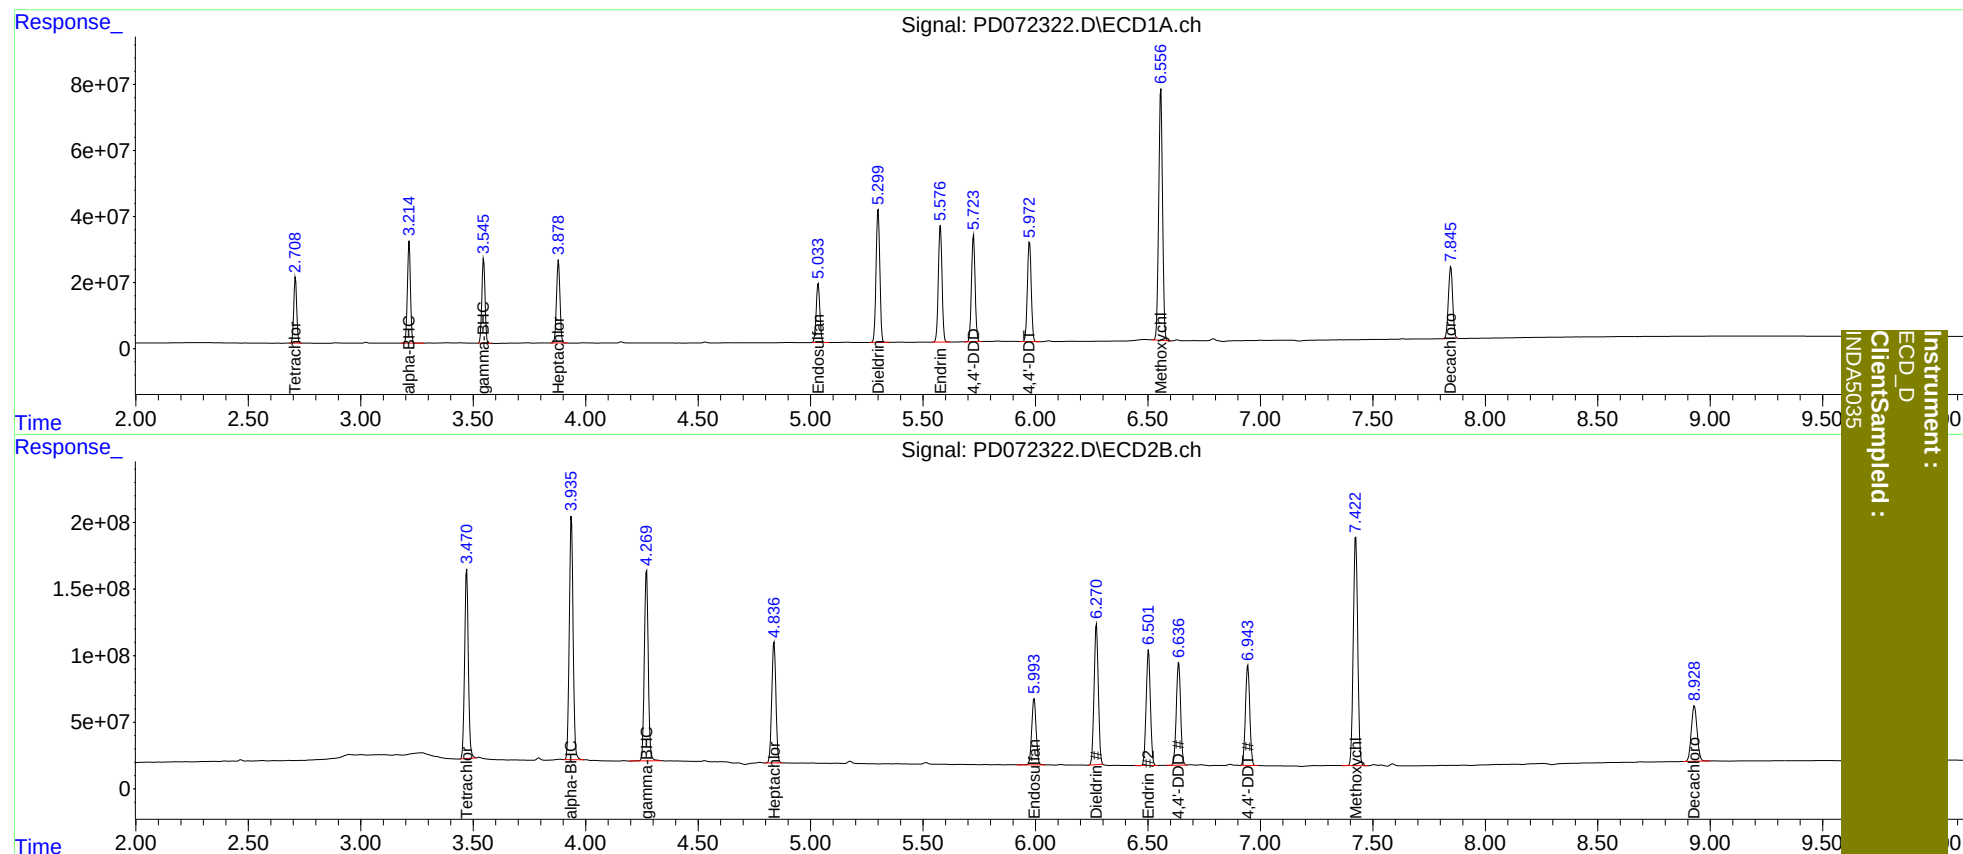

Instrument :
ECD_D
ClientSampled :
INDA5035