

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2022 16:55
 Operator : AR\AJ
 Sample : PB148220BS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS220

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/12/2022
 Supervised By :Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 06:18:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.710	3.470	47594773	495.9E6	19.499	20.738
27)	SA Decachlor...	7.848	8.929	74731962	204.6E6	38.258	40.501
Target Compounds							
2)	A alpha-BHC	3.215	3.935	15358799	157.0E6	4.303	5.187
3)	MA gamma-BHC...	3.547	4.269	13980509	136.8E6	4.723	5.259
4)	MA Heptachlor	3.878	4.837	15126127	92925312	4.617m	5.427
5)	MB Aldrin	4.158	5.175	14965650	79599394	4.551	5.508
6)	B beta-BHC	3.848	4.485	6537448	51600298	4.335m	5.114
7)	B delta-BHC	4.079	4.729	14042992	103.4E6	4.161	5.451 #
8)	B Heptachlo...	4.665	5.609	13522925	63697094	4.554	5.645
9)	A Endosulfan I	5.034	5.993	12316349	47641060	4.742	4.981
10)	B trans-Chl...	4.913	5.862	13191571	55159913	4.342	4.982
11)	B cis-Chlor...	4.977	5.938	13321181	53397123	4.533	5.059
12)	B 4,4'-DDE	5.166	6.111	24438746	94156793	8.471	10.013
13)	MA Dieldrin	5.301	6.270	25643349	102.4E6	8.938	10.743
14)	MA Endrin	5.578	6.502	21902367	86047021	8.784	10.724
15)	B Endosulfa...	5.876	6.732	21852075	74982242	9.322	10.382
16)	A 4,4'-DDD	5.725	6.636	20083690	74642493	8.946	10.481
17)	MA 4,4'-DDT	5.974	6.944	19286052	69706772	8.942	10.340
18)	B Endrin al...	6.059	6.864	18508887	63259076	9.203	10.256
19)	B Endosulfa...	6.282	7.096	20855745	67461941	8.802	9.876
20)	A Methoxychlor	6.559	7.424	56176239	168.9E6	47.729	52.621
21)	B Endrin ke...	6.793	7.587	27285589	78354753	9.800	10.668

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2022 16:55
Operator : AR\AJ
Sample : PB148220BS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 06:18:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

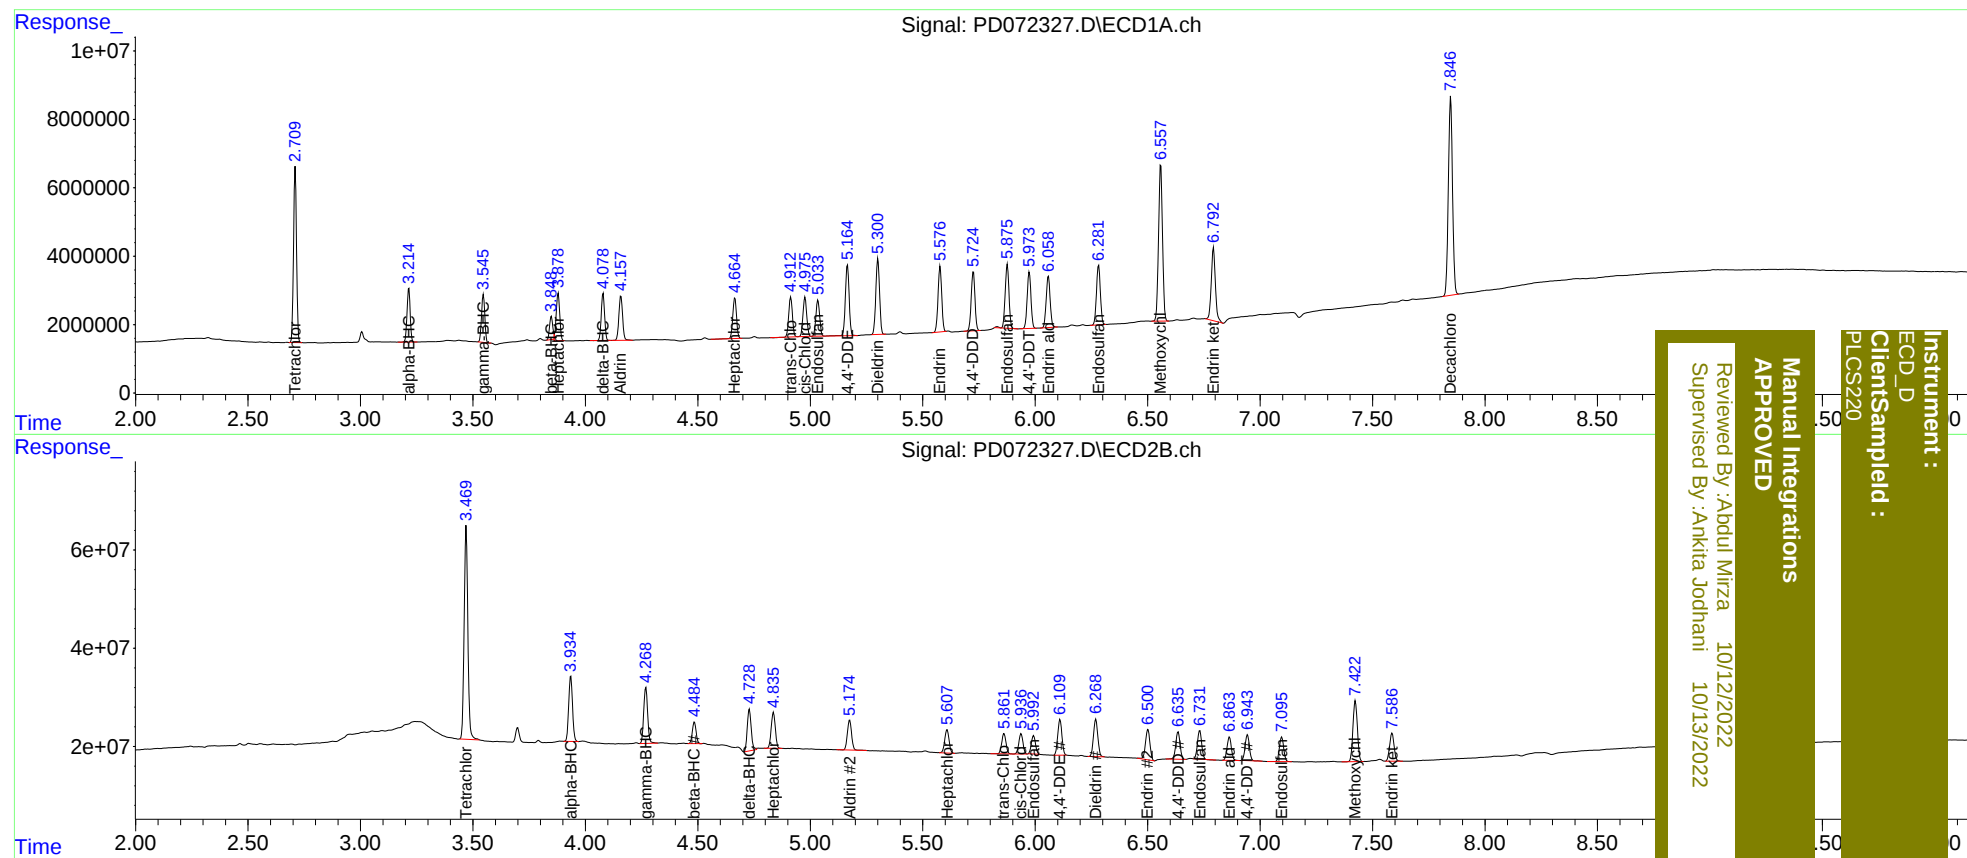

Reviewed By: Abdul Mirza 10/12/2022
Supervised By: Ankita Jodhani 10/13/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
PLCS220