

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2022 19:08
 Operator : AR\AJ
 Sample : N4976-10MSD
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8Y5MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/14/2022
 Supervised By : Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 06:41:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.710	3.472	30576881	358.4E6	12.527	14.987
27)	SA Decachlor...	7.845	8.929	31334144	89661646	16.041	17.751
Target Compounds							
2)	A alpha-BHC	3.215	3.936	134.3E6	962.5E6	37.630	31.798
3)	MA gamma-BHC...	3.544	4.270	137.8E6	923.8E6	46.547m	35.518
4)	MA Heptachlor	3.877	4.837	123.1E6	609.8E6	37.564m	35.614
5)	MB Aldrin	4.158	5.175	134.2E6	497.9E6	40.821	34.456
6)	B beta-BHC	3.847	4.486	47420808	366.7E6	31.446m	36.342
7)	B delta-BHC	4.079	4.730	43868863	263.3E6	12.999	13.882
8)	B Heptachlo...	4.664	5.606	111.5E6	651.2E6	37.555	57.705m#
9)	A Endosulfan I	5.034	5.993	104.4E6	366.5E6	40.206	38.314
10)	B trans-Chl...	4.912	5.861	111.6E6	399.3E6	36.729	36.071
11)	B cis-Chlor...	4.976	5.937	111.8E6	383.4E6	38.031	36.318
12)	B 4,4'-DDE	5.164	6.111	220.6E6	646.9E6	76.445	68.800
13)	MA Dieldrin	5.300	6.270	248.5E6	890.5E6	86.605	93.413
14)	MA Endrin	5.576	6.502	212.5E6	371.7E6	85.233	46.327 #
15)	B Endosulfa...	5.875	6.731	208.0E6	636.4E6	88.744	88.112
16)	A 4,4'-DDD	5.724	6.636	184.3E6	593.8E6	82.097	83.383
17)	MA 4,4'-DDT	5.972	6.944	167.3E6	550.7E6	77.564	81.685
18)	B Endrin al...	6.057	6.863	154.5E6	496.7E6	76.808	80.527
19)	B Endosulfa...	6.281	7.097	163.4E6	507.4E6	68.965	74.288
20)	A Methoxychlor	6.556	7.422	522.3E6	1475.3E6	443.736	459.635m
21)	B Endrin ke...	6.790	7.586	213.6E6	682.4E6	76.726m	92.911

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2022 19:08
Operator : AR\AJ
Sample : N4976-10MSD
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 06:41:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

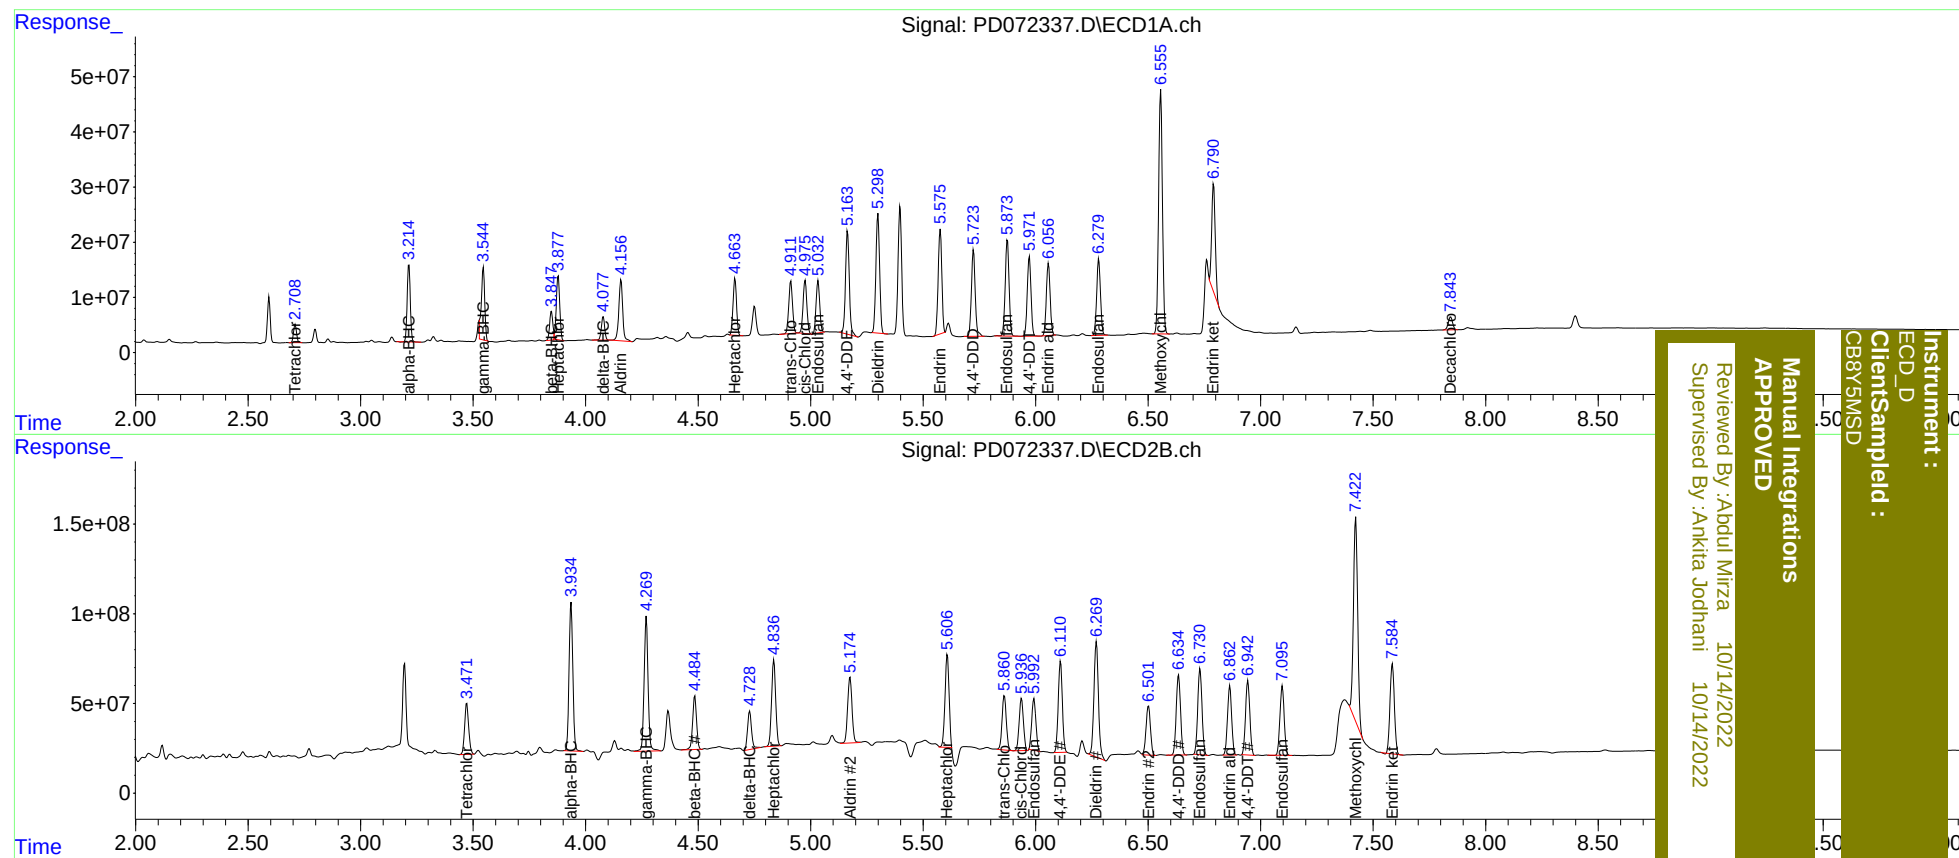

Instrument :
ECD_D
Client Sampled :
CB8Y5MSD

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/14/2022
Supervised By : Ankita Jodhani 10/14/2022