

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 01:49
 Operator : AR\AJ
 Sample : N5041-03MS
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGS19MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/12/2022
 Supervised By : Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 07:39:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.709	3.471	50384404	598.8E6	20.642	25.042
27)	SA Decachlor...	7.844	8.926	72644115	216.8E6	37.189	42.921
Target Compounds							
2)	A alpha-BHC	3.214	3.935	204.2E6	1557.0E6	57.200	51.440
3)	MA gamma-BHC...	3.545	4.269	188.1E6	1310.7E6	63.551	50.393
4)	MA Heptachlor	3.878	4.836	196.8E6	917.2E6	60.057	53.570
5)	MB Aldrin	4.157	5.175	193.8E6	756.8E6	58.923	52.366
6)	B beta-BHC	3.847	4.484	80681529	511.2E6	53.502	50.661
7)	B delta-BHC	4.078	4.729	64144701	389.0E6	19.007	20.512
8)	B Heptachlo...	4.663	5.607	175.0E6	679.8E6	58.953	60.247
9)	A Endosulfan I	5.032	5.990	156.8E6	546.9E6	60.383	57.172m
10)	B trans-Chl...	4.911	5.860	168.2E6	598.7E6	55.354	54.080
11)	B cis-Chlor...	4.975	5.936	165.0E6	563.9E6	56.138	53.419
12)	B 4,4'-DDE	5.163	6.109	337.0E6	1049.7E6	116.788	111.632
13)	MA Dieldrin	5.298	6.268	356.4E6	1149.9E6	124.219	120.617
14)	MA Endrin	5.575	6.500	311.2E6	894.7E6	124.802	111.513
15)	B Endosulfa...	5.873	6.730	286.1E6	894.8E6	122.029	123.888
16)	A 4,4'-DDD	5.722	6.634	274.3E6	851.0E6	122.195	119.490
17)	MA 4,4'-DDT	5.971	6.940	267.2E6	837.6E6	123.907	124.240m
18)	B Endrin al...	6.056	6.861	223.9E6	711.7E6	111.320	115.387
19)	B Endosulfa...	6.279	7.094	223.4E6	684.3E6	94.288	100.182
20)	A Methoxychlor	6.554	7.421	705.5E6	1987.4E6	599.388	619.164
21)	B Endrin ke...	6.789	7.583	322.6E6	919.1E6	115.851	125.143

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 01:49
Operator : AR\AJ
Sample : N5041-03MS
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 07:39:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

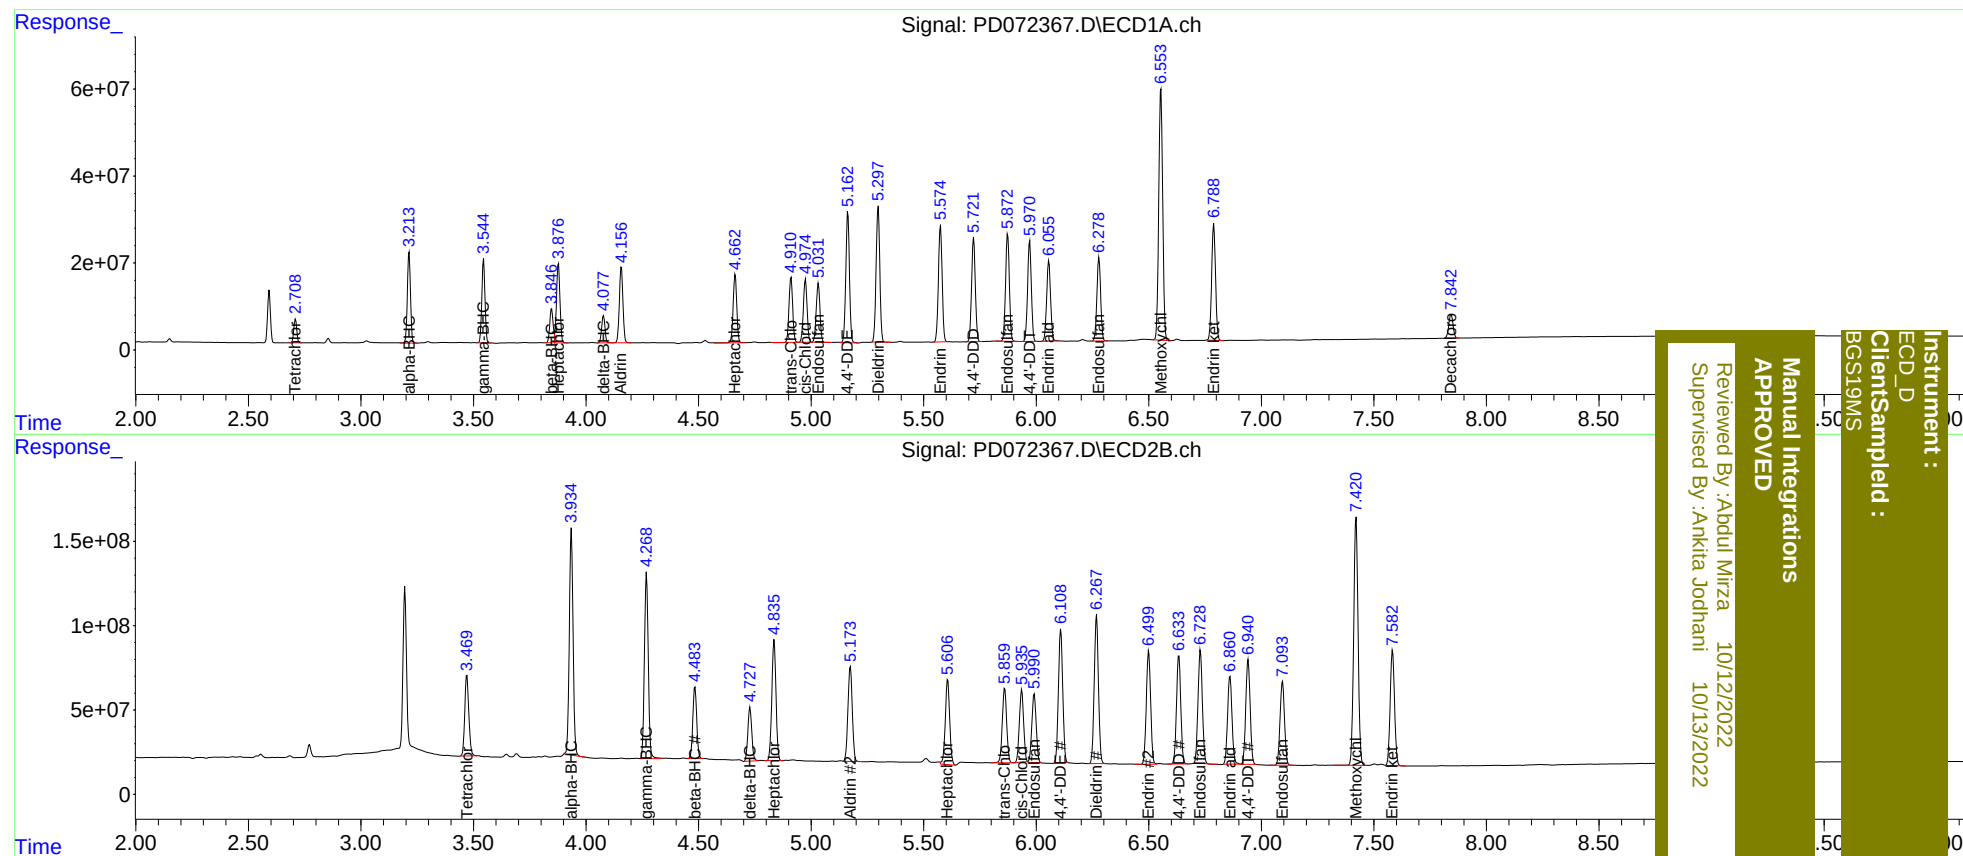

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/12/2022
Supervised By: Ankita Jodhani 10/13/2022

Instrument :
ECD_D
Client Sampled :
BGS19MS