

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2022 02:02
 Operator : AR\AJ
 Sample : N5041-04MSD
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGS19MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/12/2022
 Supervised By : Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 07:41:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.709	3.471	50976090	609.5E6	20.884	25.489
27)	SA Decachlor...	7.843	8.926	72808817	217.2E6	37.273	42.991
Target Compounds							
2)	A alpha-BHC	3.214	3.935	205.9E6	1587.8E6	57.680	52.458
3)	MA gamma-BHC...	3.545	4.269	188.1E6	1333.6E6	63.554	51.273
4)	MA Heptachlor	3.877	4.836	196.7E6	929.4E6	60.020	54.284
5)	MB Aldrin	4.157	5.174	192.7E6	765.4E6	58.585	52.962
6)	B beta-BHC	3.847	4.484	81107459	517.5E6	53.784	51.285
7)	B delta-BHC	4.077	4.728	64523874	421.8E6	19.119	22.243
8)	B Heptachlo...	4.663	5.607	173.1E6	648.9E6	58.286	57.501
9)	A Endosulfan I	5.031	5.990	156.3E6	565.8E6	60.193	59.150m
10)	B trans-Chl...	4.911	5.860	168.3E6	606.7E6	55.392	54.799
11)	B cis-Chlor...	4.975	5.936	165.4E6	571.6E6	56.280	54.148
12)	B 4,4'-DDE	5.163	6.109	332.7E6	1060.1E6	115.303	112.739
13)	MA Dieldrin	5.298	6.268	357.0E6	1161.6E6	124.442	121.848
14)	MA Endrin	5.574	6.500	312.5E6	957.8E6	125.311	119.379
15)	B Endosulfa...	5.873	6.730	285.8E6	905.3E6	121.905	125.344
16)	A 4,4'-DDD	5.722	6.634	271.0E6	856.0E6	120.700	120.197
17)	MA 4,4'-DDT	5.970	6.940	268.2E6	853.8E6	124.357	126.647m
18)	B Endrin al...	6.056	6.861	224.1E6	715.4E6	111.417	115.994
19)	B Endosulfa...	6.279	7.095	223.9E6	689.3E6	94.492	100.910
20)	A Methoxychlor	6.554	7.421	707.5E6	2003.6E6	601.080	624.204
21)	B Endrin ke...	6.789	7.584	322.0E6	924.5E6	115.656	125.878

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2022 02:02
Operator : AR\AJ
Sample : N5041-04MSD
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 07:41:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

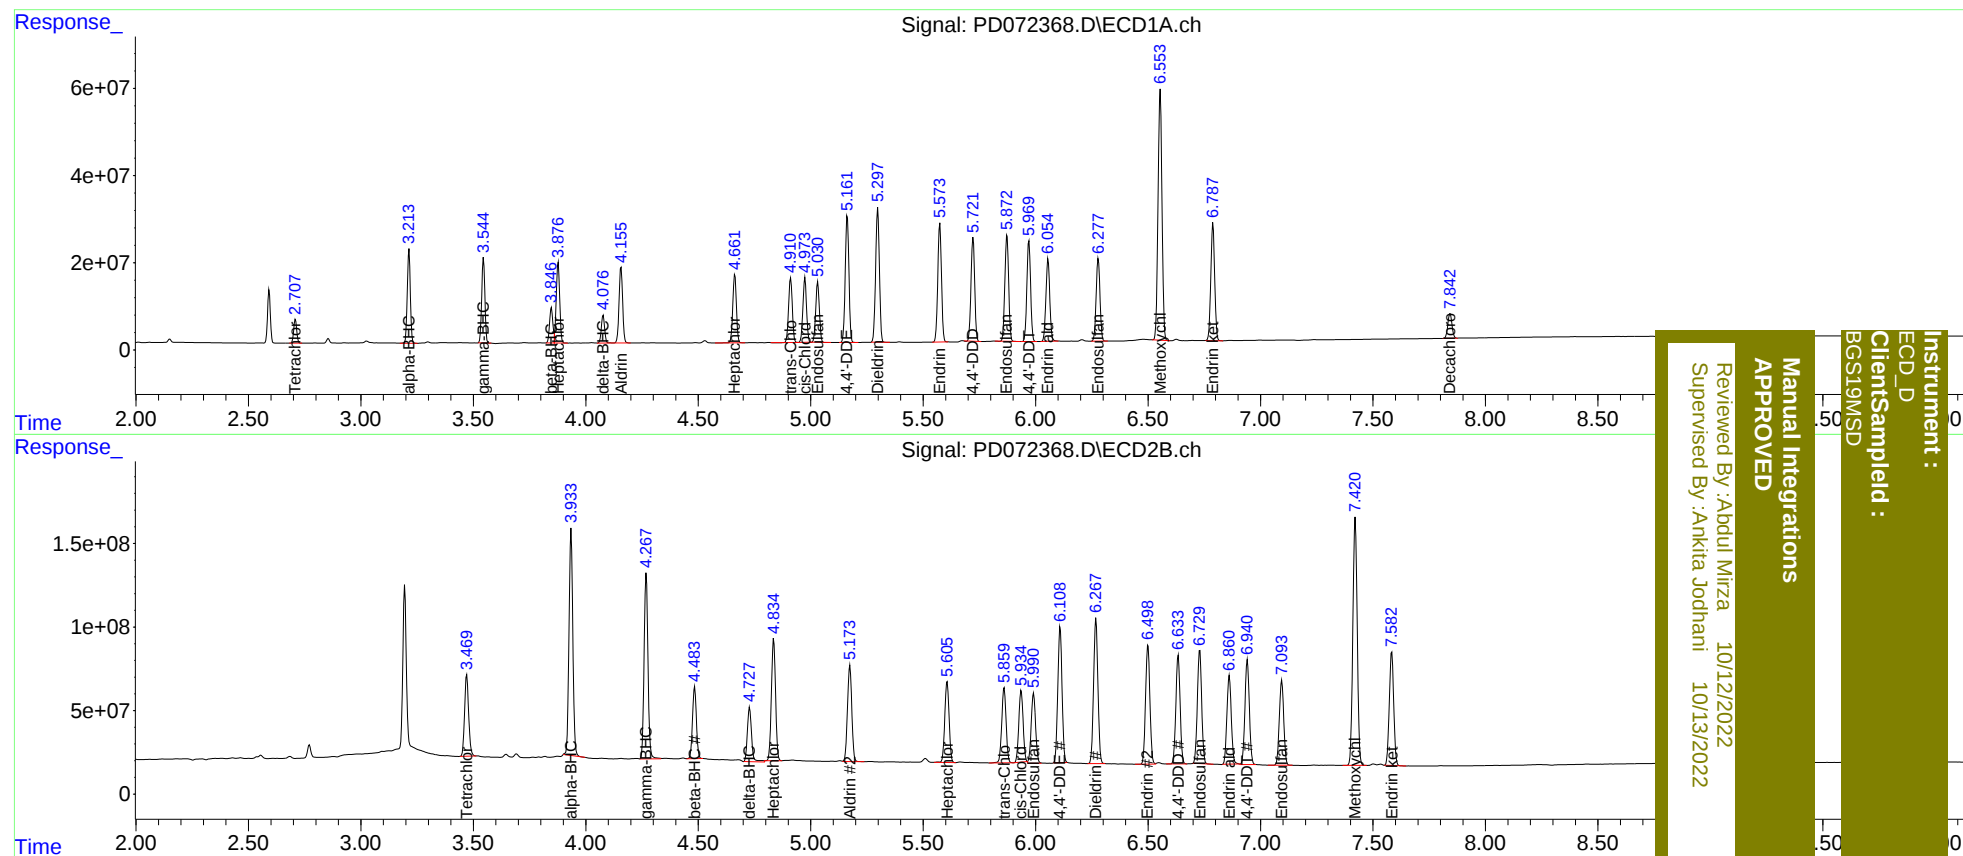

Reviewed By: Abdul Mirza 10/12/2022
Supervised By: Ankita Jodhani 10/13/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BGS19MSD