

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2022 18:55
 Operator : AR\AJ
 Sample : N4976-09MS
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB8Y5MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/14/2022
 Supervised By :Ankita Jodhani 10/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 06:36:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.709	3.471	30769235	362.1E6	12.606	15.142
27)	SA Decachlor...	7.844	8.928	31246800	88061973	15.996	17.434
Target Compounds							
2)	A alpha-BHC	3.215	3.935	135.2E6	965.7E6	37.866	31.905
3)	MA gamma-BHC...	3.544	4.270	146.3E6	918.2E6	49.435m	35.301 #
4)	MA Heptachlor	3.877	4.836	125.0E6	614.4E6	38.149m	35.883
5)	MB Aldrin	4.157	5.175	127.6E6	506.1E6	38.788	35.022
6)	B beta-BHC	3.846	4.485	49519171	362.6E6	32.837m	35.935
7)	B delta-BHC	4.078	4.729	44565163	259.0E6	13.205	13.659
8)	B Heptachlo...	4.663	5.606	111.2E6	559.5E6	37.460	49.585m#
9)	A Endosulfan I	5.032	5.991	107.3E6	393.5E6	41.329	41.142m
10)	B trans-Chl...	4.911	5.861	111.3E6	410.6E6	36.648	37.092
11)	B cis-Chlor...	4.975	5.935	109.5E6	390.5E6	37.248	36.989m
12)	B 4,4'-DDE	5.163	6.110	213.2E6	669.8E6	73.911	71.228
13)	MA Dieldrin	5.298	6.269	250.5E6	860.7E6	87.301	90.285
14)	MA Endrin	5.576	6.501	222.1E6	552.3E6	89.055	68.839
15)	B Endosulfa...	5.874	6.731	207.9E6	640.7E6	88.701	88.714
16)	A 4,4'-DDD	5.723	6.635	184.6E6	596.7E6	82.230	83.777
17)	MA 4,4'-DDT	5.972	6.943	169.1E6	559.5E6	78.396	82.987
18)	B Endrin al...	6.057	6.863	157.1E6	506.9E6	78.092	82.177
19)	B Endosulfa...	6.280	7.095	164.2E6	506.7E6	69.295	74.172
20)	A Methoxychlor	6.555	7.422	524.7E6	1609.2E6	445.771	501.323
21)	B Endrin ke...	6.790	7.585	229.8E6	696.7E6	82.545	94.855

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2022 18:55
Operator : AR\AJ
Sample : N4976-09MS
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 06:36:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

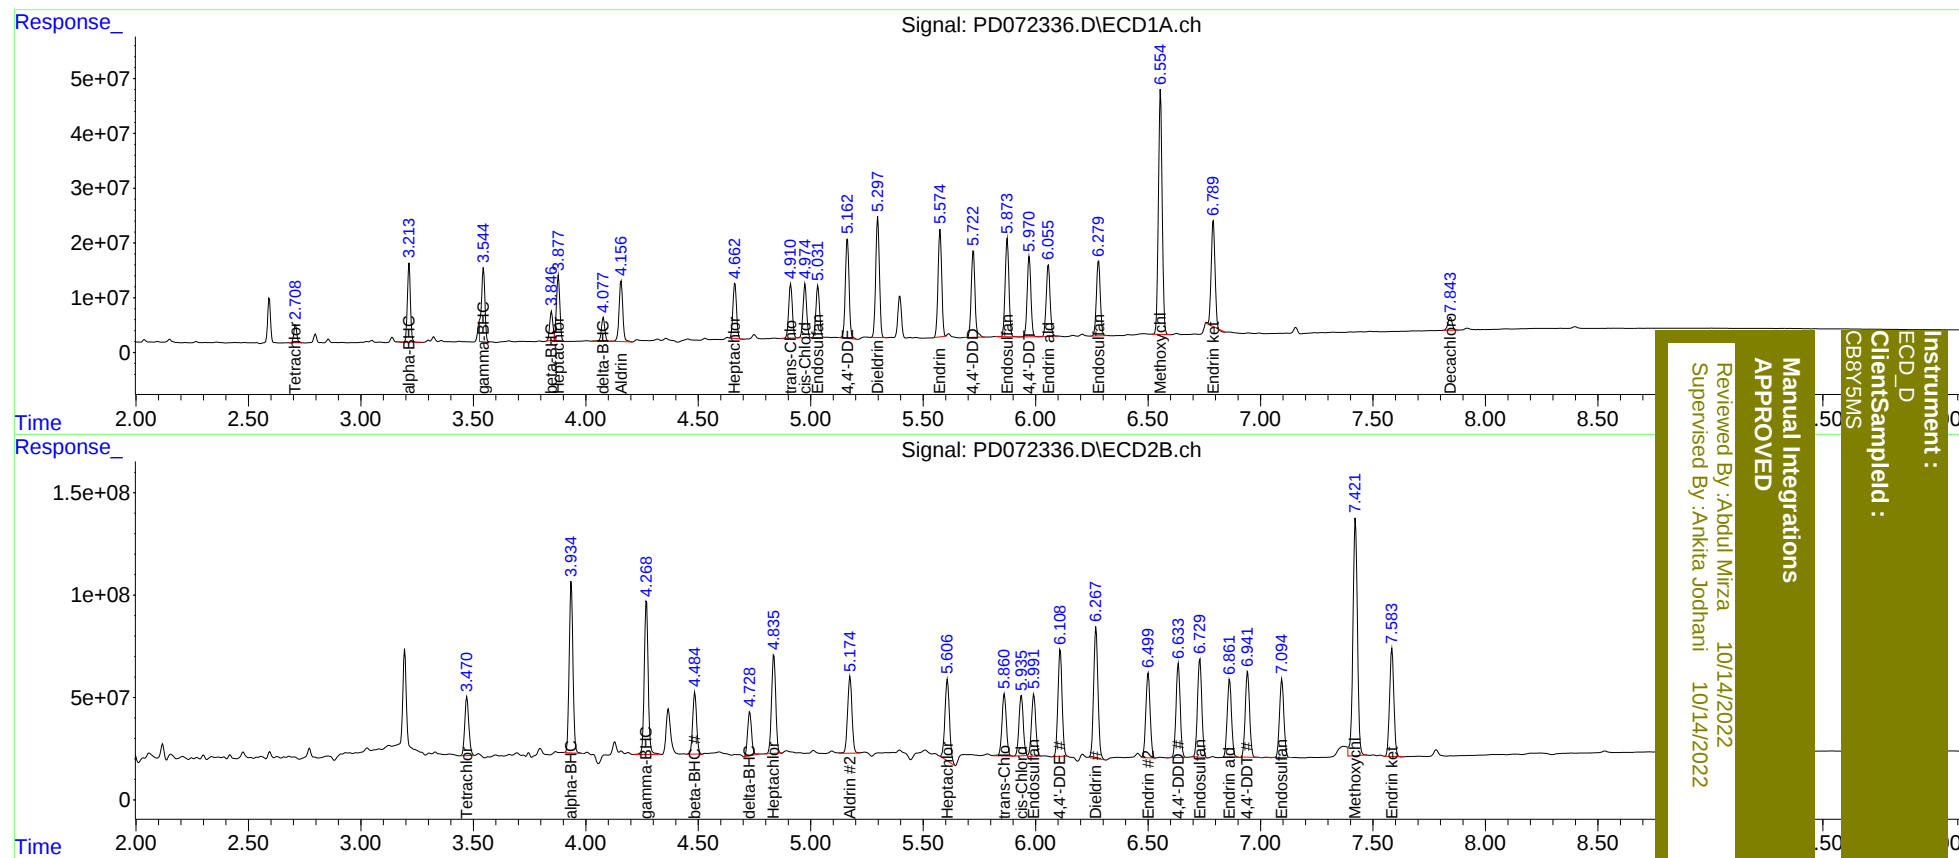

Reviewed By: Abdul Mirza 10/14/2022
Supervised By: Ankita Jodhani 10/14/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
CB8Y5MS