

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2022 20:02
 Operator : AR\AJ
 Sample : PB148222BS
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS222

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/12/2022
 Supervised By :Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 06:54:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.728	3.470	45451642	469.1E6	18.621m	19.615
27)	SA Decachlor...	7.862	8.928	69625882	199.1E6	35.644m	39.421
Target Compounds							
2)	A alpha-BHC	3.235	3.935	14521767	148.1E6	4.068	4.894
3)	MA gamma-BHC...	3.564	4.269	13578374	136.8E6	4.587m	5.259
4)	MA Heptachlor	3.896	4.836	14467817	89026632	4.416m	5.200
5)	MB Aldrin	4.177	5.175	14793506	74764113	4.499	5.173
6)	B beta-BHC	3.866	4.485	6395699	48318484	4.241m	4.788
7)	B delta-BHC	4.098	4.729	13498971	101.3E6	4.000	5.343 #
8)	B Heptachlo...	4.683	5.607	12857091	68216151	4.330	6.045 #
9)	A Endosulfan I	5.051	5.991	11894347	45855543	4.580m	4.794m
10)	B trans-Chl...	4.931	5.861	12229762	52591358	4.025	4.750
11)	B cis-Chlor...	4.994	5.937	13123528	50488149	4.466m	4.783
12)	B 4,4'-DDE	5.183	6.109	23560156	89191664	8.166	9.485
13)	MA Dieldrin	5.318	6.269	24200328	99044626	8.435	10.389
14)	MA Endrin	5.594	6.501	20720185	80187298	8.310m	9.994
15)	B Endosulfa...	5.893	6.731	20282424	72828972	8.652	10.083
16)	A 4,4'-DDD	5.742	6.635	18568231	71691057	8.271	10.066
17)	MA 4,4'-DDT	5.991	6.942	17788984	67218950	8.248	9.971
18)	B Endrin al...	6.076	6.862	16523739	60597596	8.216	9.825
19)	B Endosulfa...	6.300	7.095	18692027	64952423	7.889	9.509
20)	A Methoxychlor	6.575	7.421	53055228	165.5E6	45.077	51.574m
21)	B Endrin ke...	6.810	7.585	29133032	75845480	10.463	10.327

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2022 20:02
Operator : AR\AJ
Sample : PB148222BS
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 06:54:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

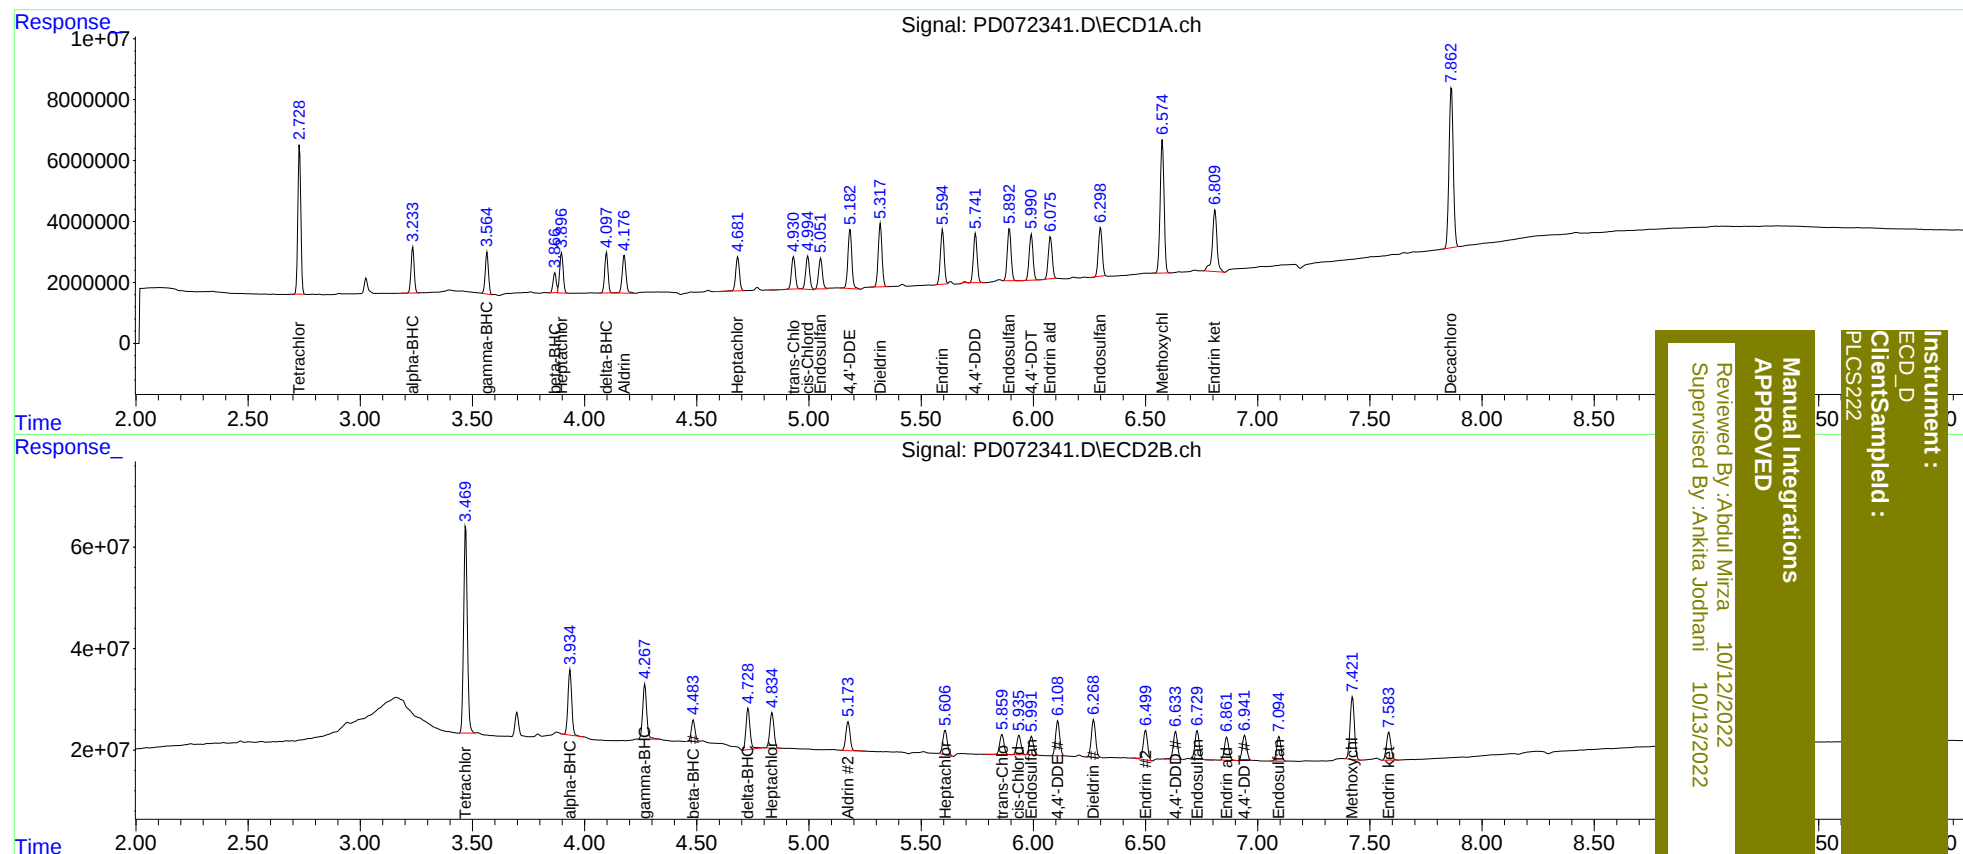

Instrument :
ECD_D
Client: Sampled :
PLCS222

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 10/12/2022
Supervised By: Ankita Jodhani 10/13/2022