

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
 Data File : PD072344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2022 20:42
 Operator : AR\AJ
 Sample : N4982-04MS
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C1BB2MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/12/2022
 Supervised By : Ankita Jodhani 10/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 07:09:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 12 06:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.710	3.472	43815541	530.9E6	17.950	22.203
27)	SA Decachlor...	7.844	8.927	60818073	178.3E6	31.135	35.290
Target Compounds							
2)	A alpha-BHC	3.215	3.936	172.2E6	1386.9E6	48.247	45.819
3)	MA gamma-BHC...	3.546	4.270	159.2E6	1190.5E6	53.784	45.769
4)	MA Heptachlor	3.878	4.836	164.7E6	797.8E6	50.261	46.594
5)	MB Aldrin	4.158	5.175	177.9E6	664.7E6	54.099	45.998
6)	B beta-BHC	3.848	4.485	68923892	476.3E6	45.705	47.205
7)	B delta-BHC	4.077	4.729	51611080	329.9E6	15.293m	17.394
8)	B Heptachlo...	4.663	5.606	151.8E6	642.3E6	51.110	56.923m
9)	A Endosulfan I	5.032	5.991	126.4E6	467.7E6	48.687m	48.893m
10)	B trans-Chl...	4.912	5.861	149.6E6	517.7E6	49.255	46.760
11)	B cis-Chlor...	4.976	5.937	145.3E6	485.7E6	49.426	46.017
12)	B 4,4'-DDE	5.164	6.110	305.6E6	884.3E6	105.934	94.043
13)	MA Dieldrin	5.299	6.269	300.3E6	1046.5E6	104.651	109.778
14)	MA Endrin	5.575	6.500	251.0E6	484.7E6	100.674m	60.410 #
15)	B Endosulfa...	5.874	6.731	244.0E6	762.4E6	104.085	105.562
16)	A 4,4'-DDD	5.723	6.635	228.0E6	720.6E6	101.574	101.179
17)	MA 4,4'-DDT	5.972	6.943	223.5E6	698.1E6	103.642	103.556
18)	B Endrin al...	6.057	6.862	188.7E6	597.4E6	93.844	96.858
19)	B Endosulfa...	6.280	7.095	187.4E6	578.6E6	79.095	84.699
20)	A Methoxychlor	6.555	7.420	601.2E6	1654.0E6	510.798	515.295m
21)	B Endrin ke...	6.789	7.584	238.7E6	751.5E6	85.734m	102.317

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101122\
Data File : PD072344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2022 20:42
Operator : AR\AJ
Sample : N4982-04MS
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 07:09:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101122CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 12 06:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

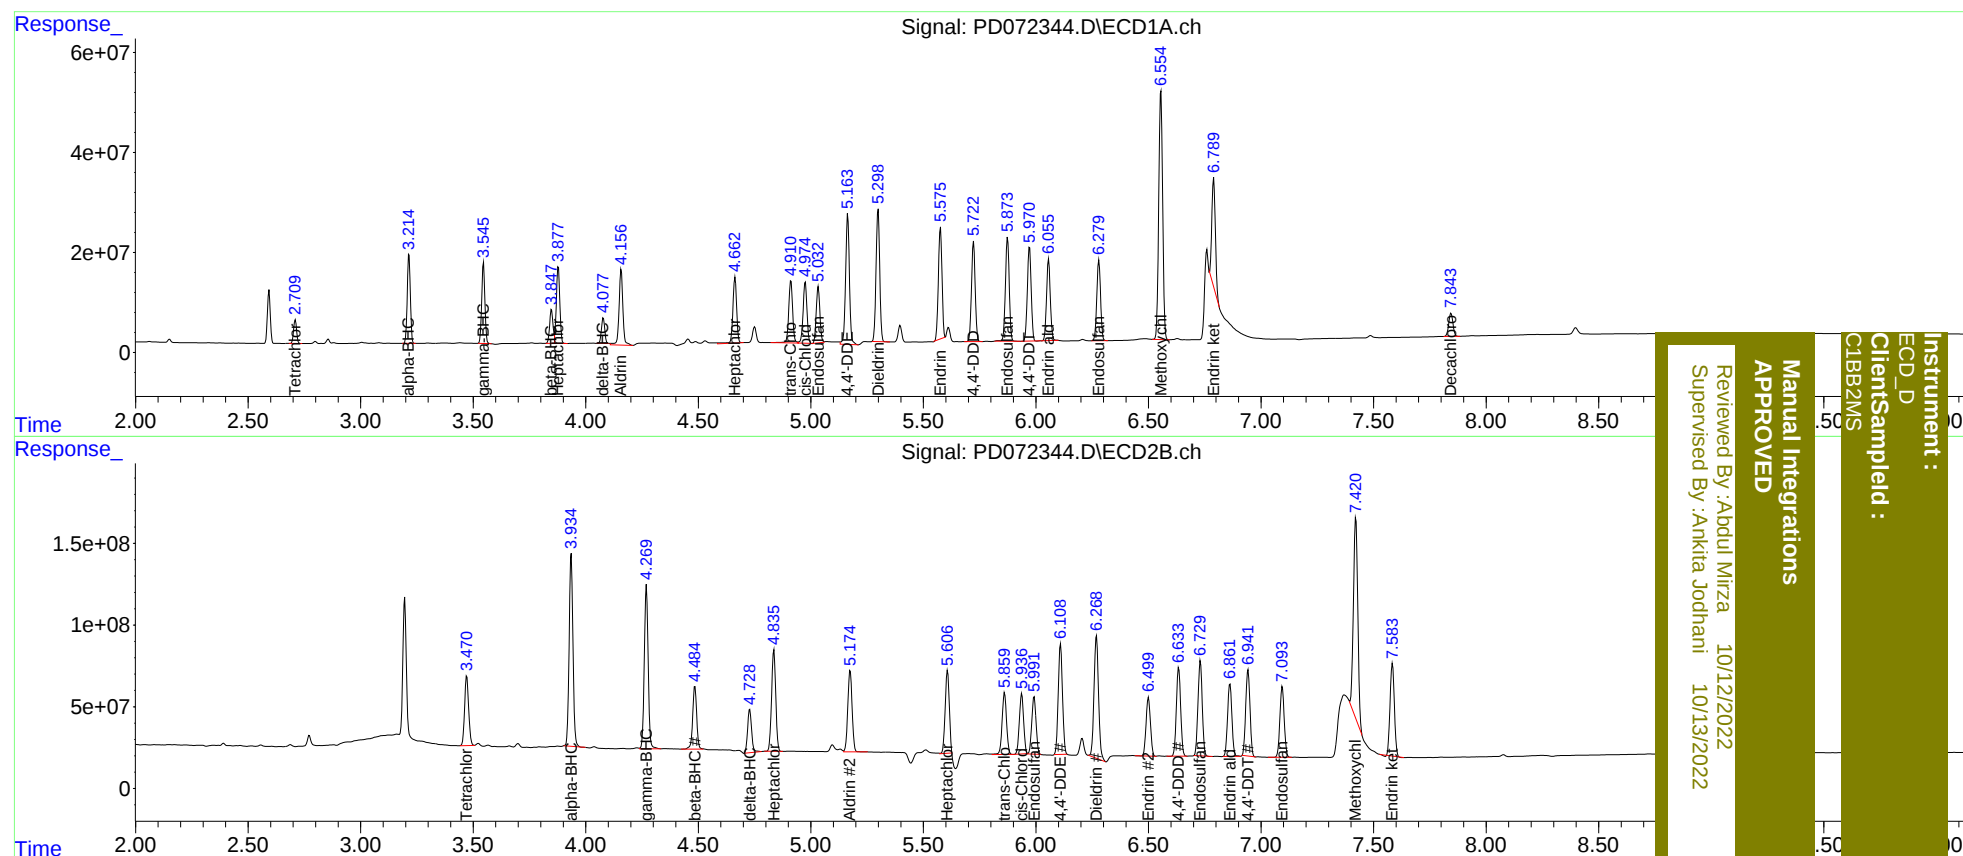

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/12/2022
Supervised By: Ankita Jodhani 10/13/2022

Instrument :
ECD_D
Client Sampled :
C1BB2MS