

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
 Data File : PD078800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2023 23:35
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 05:35:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 05:31:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.807	8012349	10106966	5.273	5.248
27)	SA Decachlor...	9.118	7.959	18944024	15455451	10.994	11.176
Target Compounds							
2)	A alpha-BHC	4.027	3.311	12553963	13004612	4.915	4.821
3)	MA gamma-BHC...	4.360	3.641	12172487	11962896	4.993	4.790
4)	MA Heptachlor	4.954	3.985	13444344	11966991	5.092	4.939
9)	A Endosulfan I	6.110	5.139	11127572	10053293	5.330	5.097
13)	MA Dieldrin	6.386	5.404	22330770	20433401	10.052	9.735
14)	MA Endrin	6.616	5.679	18137039	17136499	10.034	9.890
16)	A 4,4'-DDD	6.747	5.826	16007216	14696240	9.847	9.946
17)	MA 4,4'-DDT	7.062	6.078	16926955	14494939	9.786	10.180
20)	A Methoxychlor	7.537	6.654	49794446	43624093	53.366	55.896


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 23:35
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 05:35:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:31:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

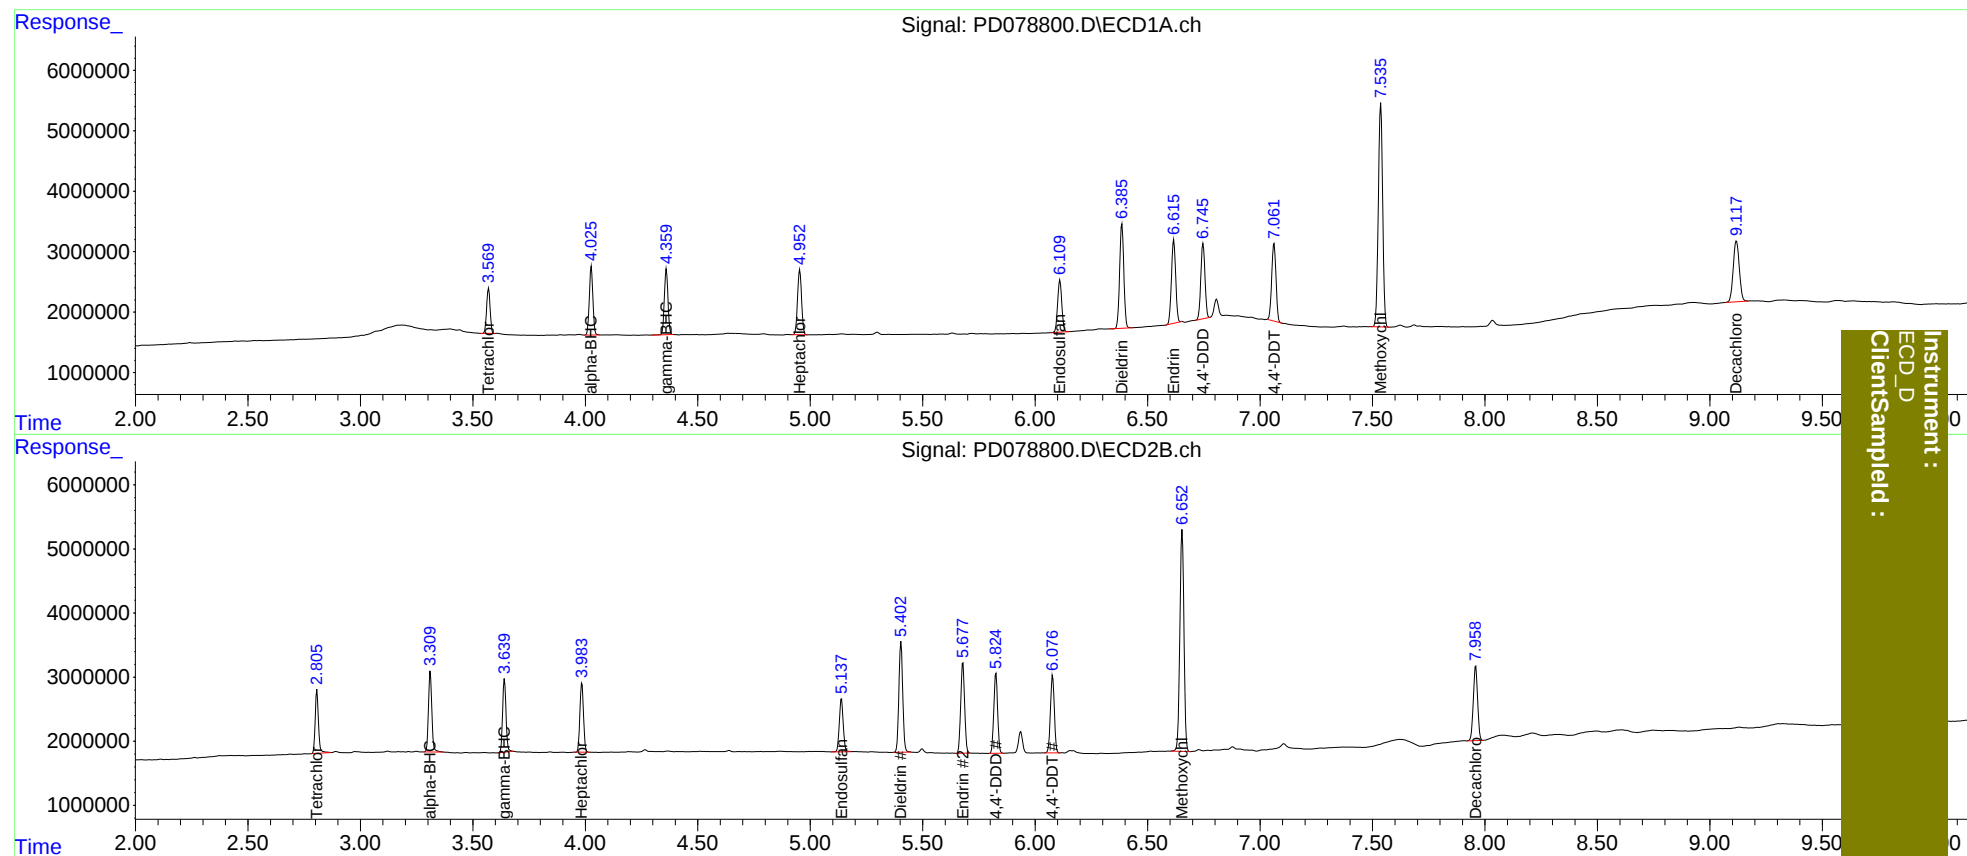


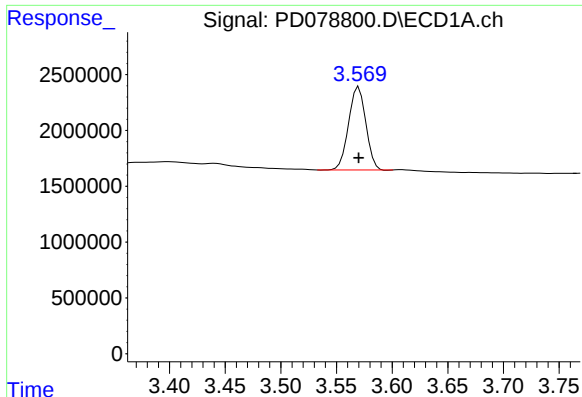

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 8012349
Conc: 5.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

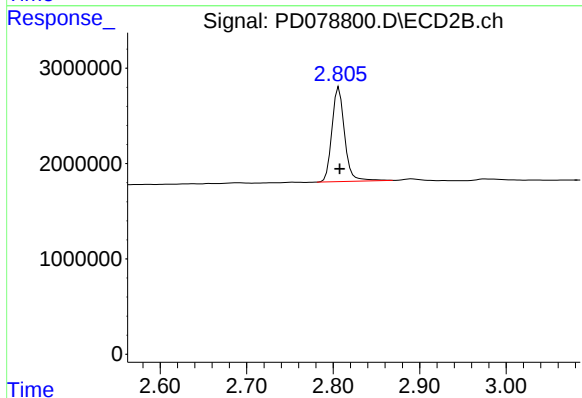


#1 Tetrachloro-m-xylene

R.T.: 2.807 min
Delta R.T.: 0.000 min
Response: 10106966
Conc: 5.25 ng/ml

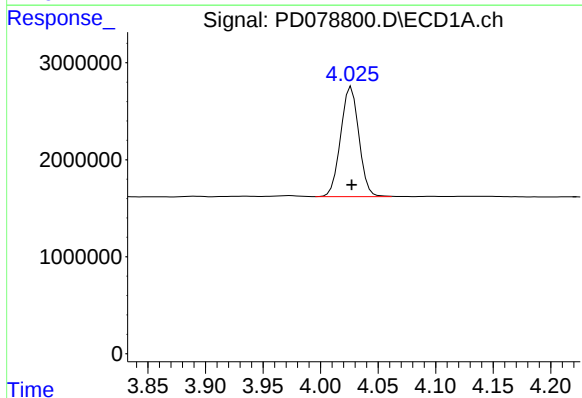


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 12553963
Conc: 4.92 ng/ml

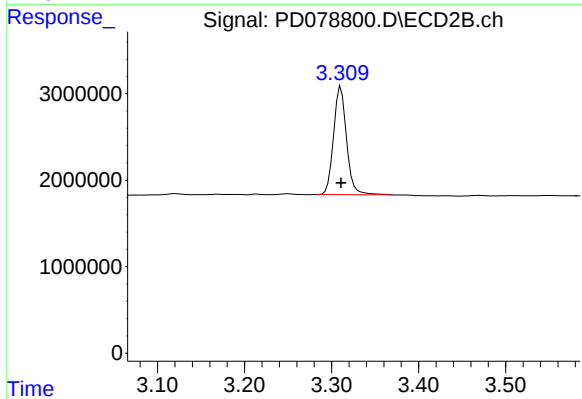

#2 alpha-BHC


R.T.: 3.311 min
Delta R.T.: 0.000 min
Response: 13004612
Conc: 4.82 ng/ml

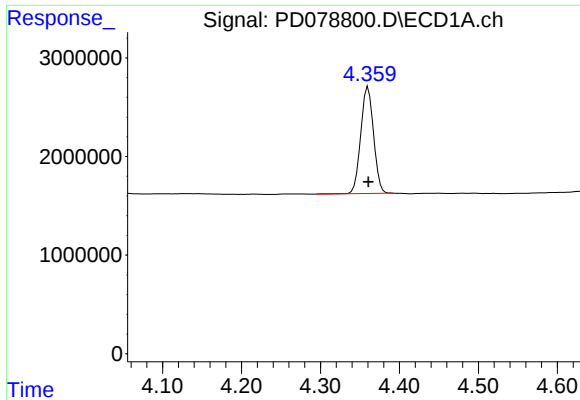

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 12172487
Conc: 4.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

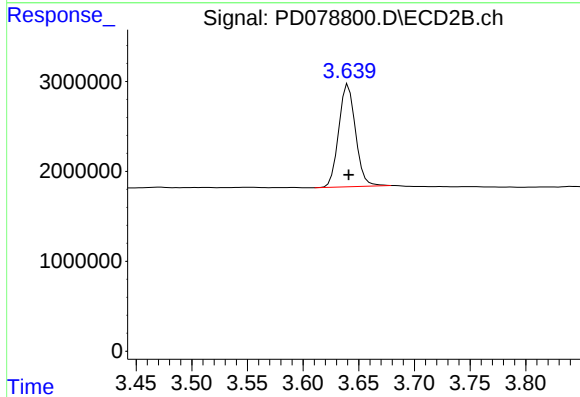


#3 gamma-BHC (Lindane)

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 11962896
Conc: 4.79 ng/ml

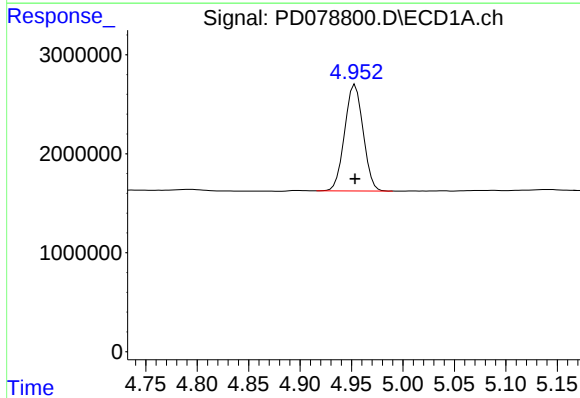


#4 Heptachlor

R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 13444344
Conc: 5.09 ng/ml

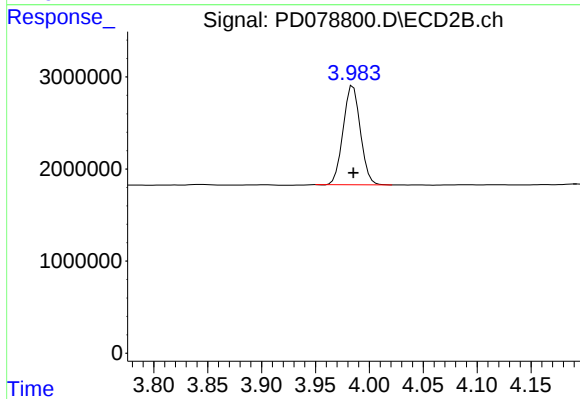

#4 Heptachlor


R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 11966991
Conc: 4.94 ng/ml

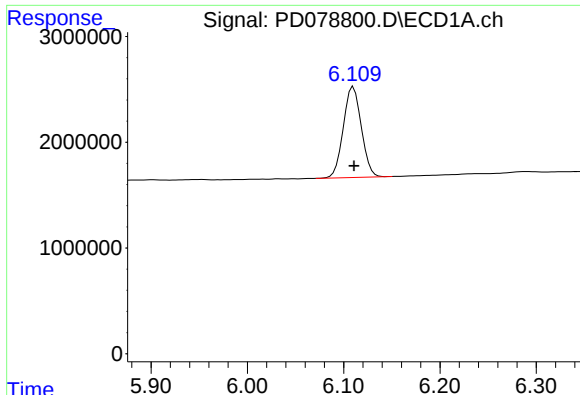

#9 Endosulfan I


R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 11127572
Conc: 5.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

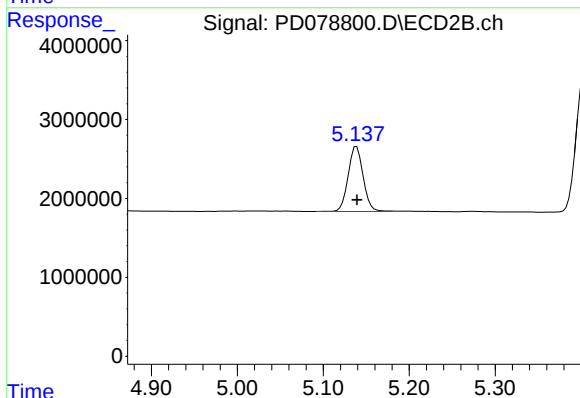


#9 Endosulfan I

R.T.: 5.139 min
Delta R.T.: 0.000 min
Response: 10053293
Conc: 5.10 ng/ml

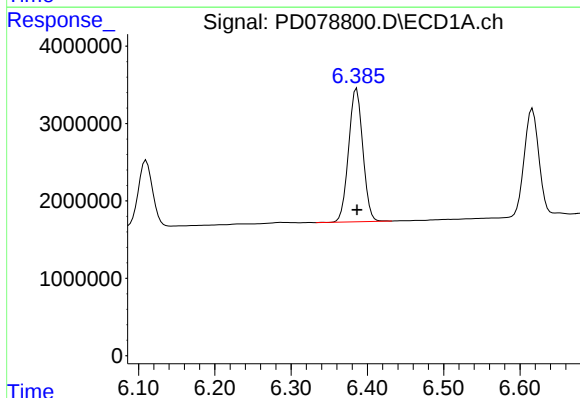


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 22330770
Conc: 10.05 ng/ml

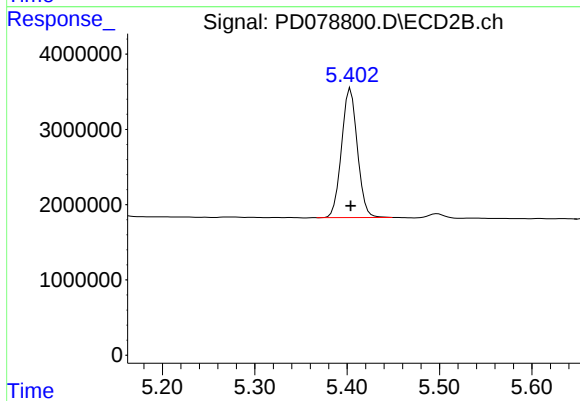

#13 Dieldrin


R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 20433401
Conc: 9.73 ng/ml

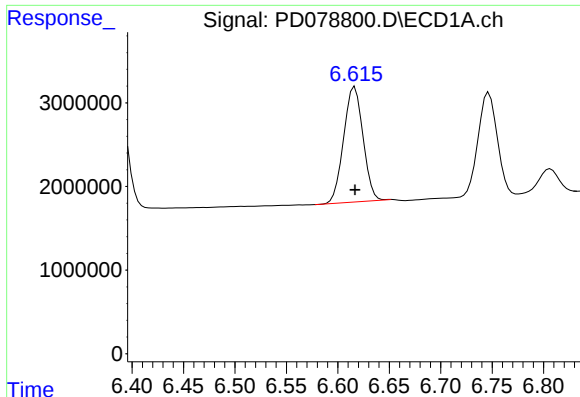

#14 Endrin


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 18137039
Conc: 10.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

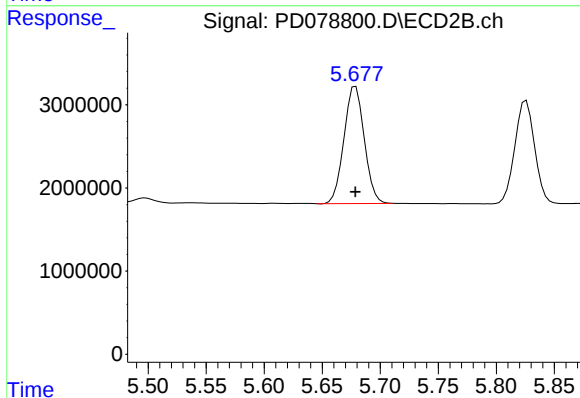


#14 Endrin

R.T.: 5.679 min
Delta R.T.: 0.000 min
Response: 17136499
Conc: 9.89 ng/ml

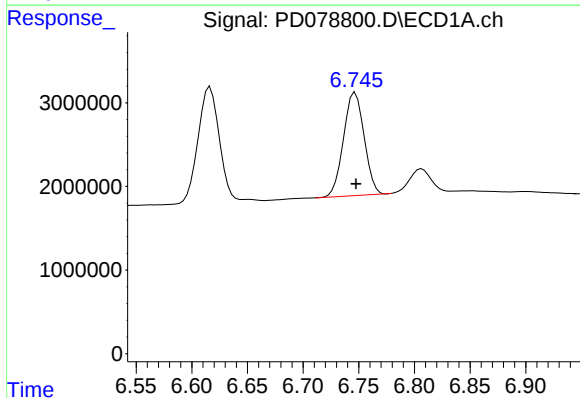


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 16007216
Conc: 9.85 ng/ml

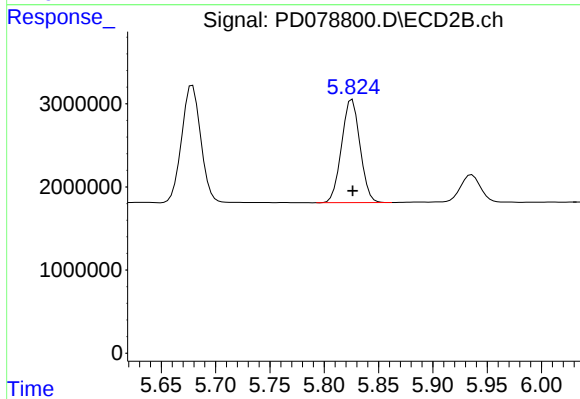

#16 4,4'-DDD


R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 14696240
Conc: 9.95 ng/ml

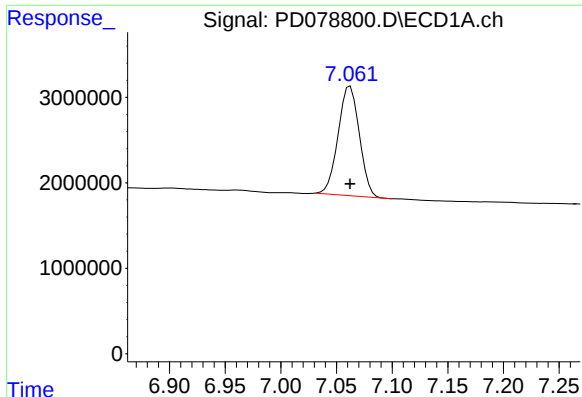

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 16926955
Conc: 9.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

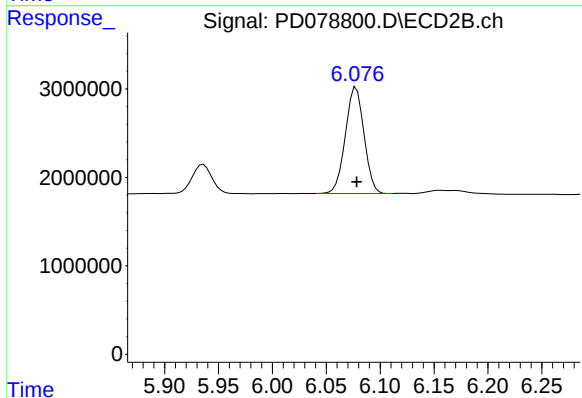


#17 4,4'-DDT

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 14494939
Conc: 10.18 ng/ml

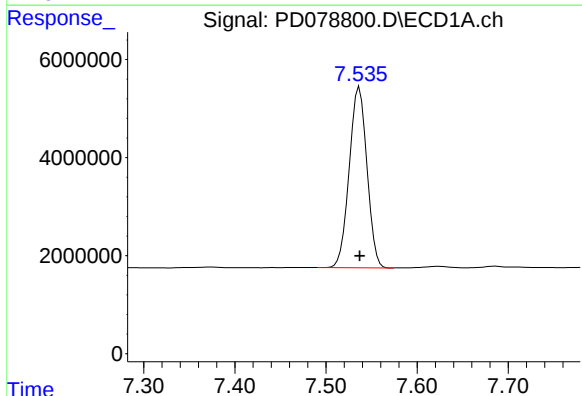


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 49794446
Conc: 53.37 ng/ml

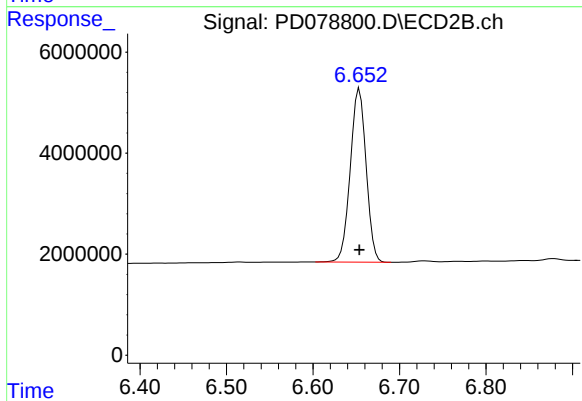

#20 Methoxychlor


R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 43624093
Conc: 55.90 ng/ml

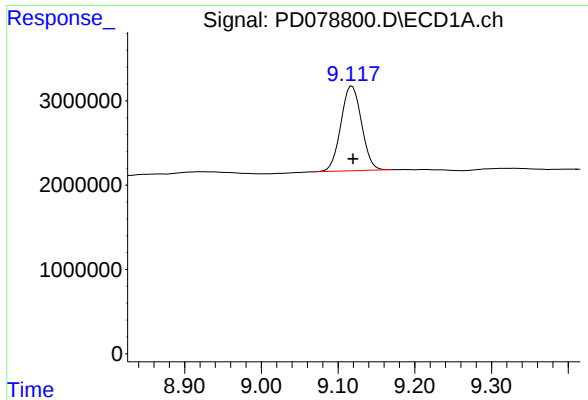

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.001 min
Response: 18944024
Conc: 10.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

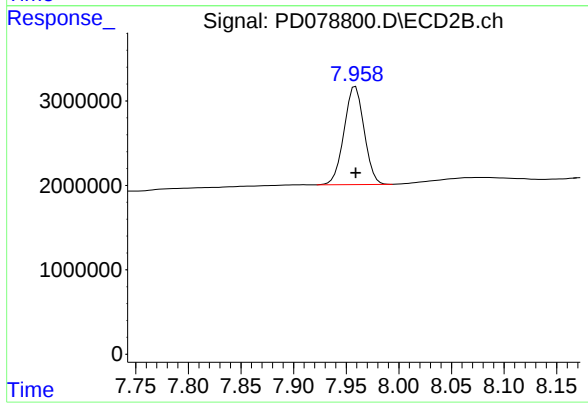

#27 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: 0.000 min
Response: 15455451
Conc: 11.18 ng/ml