

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
 Data File : PD078802.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 00:01
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 05:36:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 05:31:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.807	15970876	20381300	10.510	10.582
27)	SA Decachlor...	9.119	7.959	36696337	29187115	21.295	21.105
Target Compounds							
2)	A alpha-BHC	4.027	3.311	25878304	27206019	10.132	10.086
3)	MA gamma-BHC...	4.361	3.641	24856097	25038320	10.195	10.026
4)	MA Heptachlor	4.954	3.985	26971382	24695462	10.216	10.192
9)	A Endosulfan I	6.111	5.139	22111581	20545836	10.591	10.416
13)	MA Dieldrin	6.386	5.404	45662445	43024872	20.555	20.498
14)	MA Endrin	6.617	5.679	36995211	35664252	20.468	20.583
16)	A 4,4'-DDD	6.747	5.826	33380204	30258713	20.534	20.479
17)	MA 4,4'-DDT	7.063	6.078	35408138	29396812	20.471	20.646
20)	A Methoxychlor	7.536	6.654	98146869	84462640	105.187	108.223


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078802.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 00:01
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 05:36:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:31:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

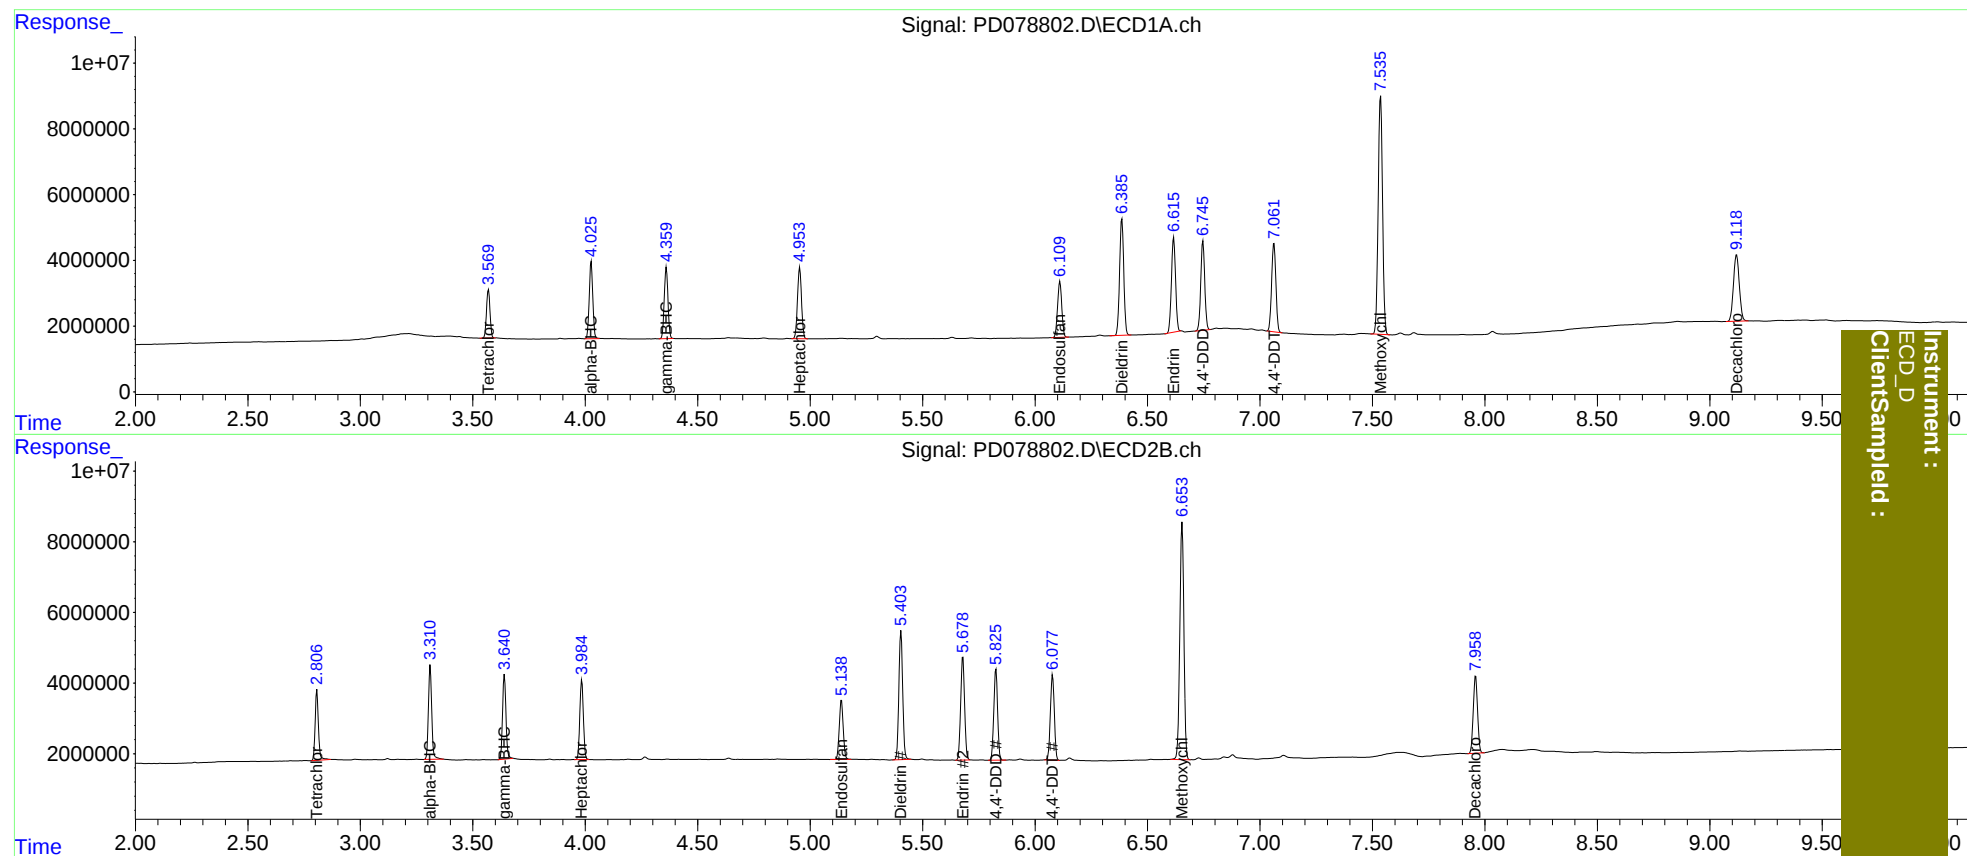


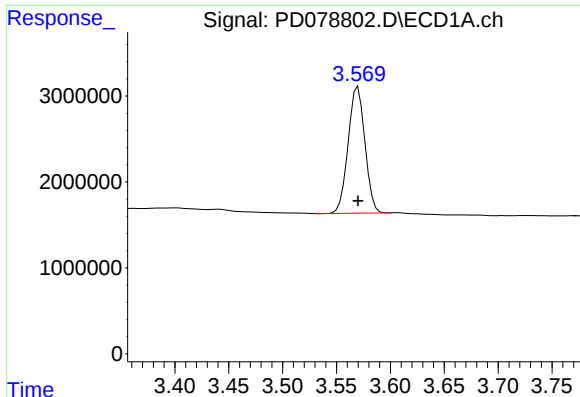

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 15970876
Conc: 10.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

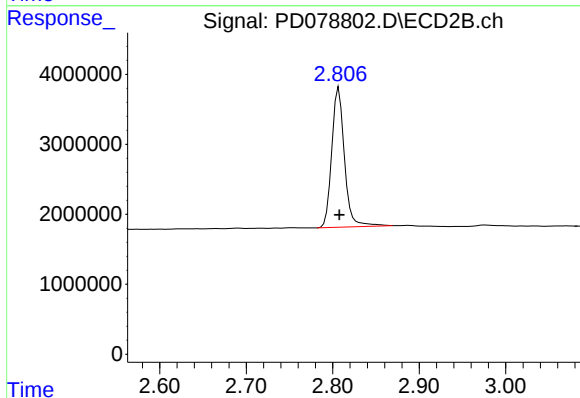


#1 Tetrachloro-m-xylene

R.T.: 2.807 min
Delta R.T.: 0.000 min
Response: 20381300
Conc: 10.58 ng/ml

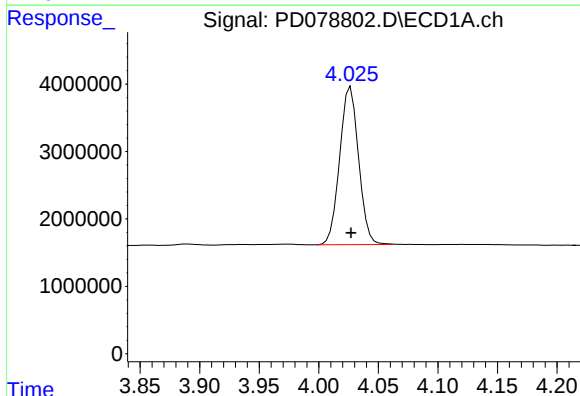


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 25878304
Conc: 10.13 ng/ml

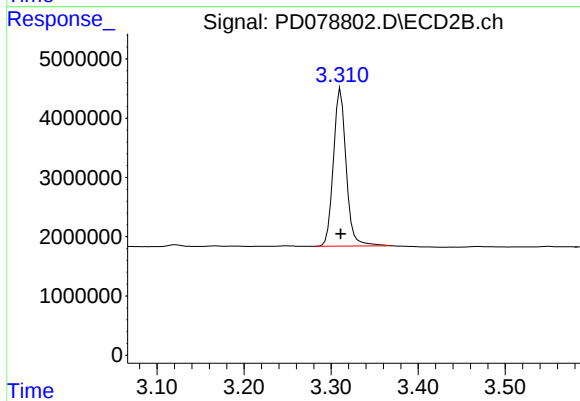

#2 alpha-BHC


R.T.: 3.311 min
Delta R.T.: 0.000 min
Response: 27206019
Conc: 10.09 ng/ml

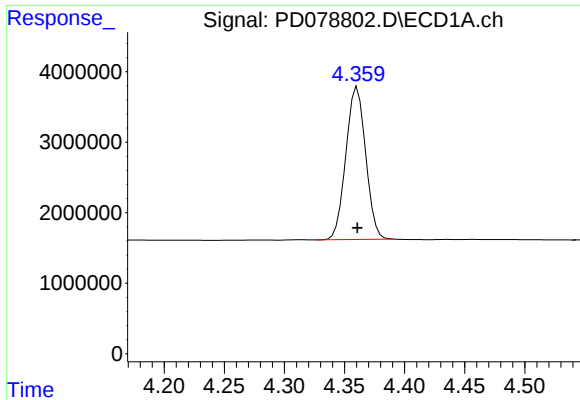

#3 gamma-BHC (Lindane)


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 24856097
Conc: 10.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

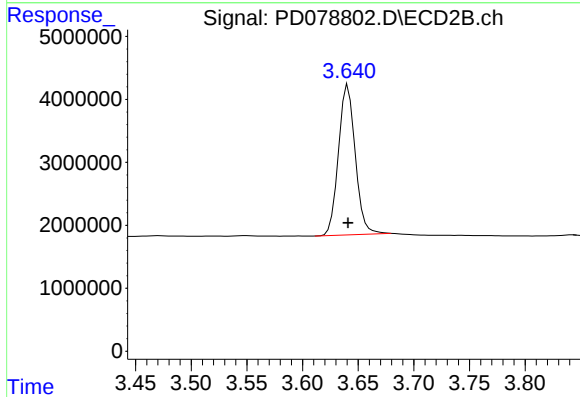


#3 gamma-BHC (Lindane)

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 25038320
Conc: 10.03 ng/ml

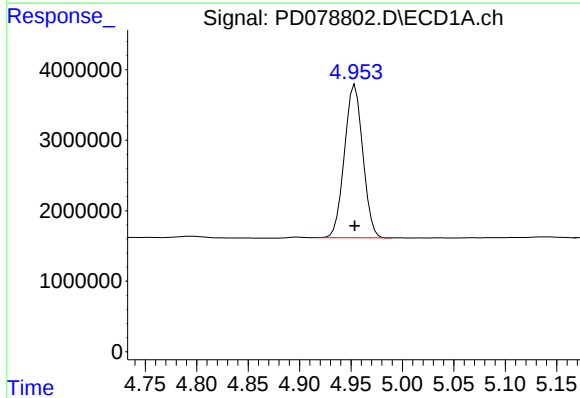


#4 Heptachlor

R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 26971382
Conc: 10.22 ng/ml

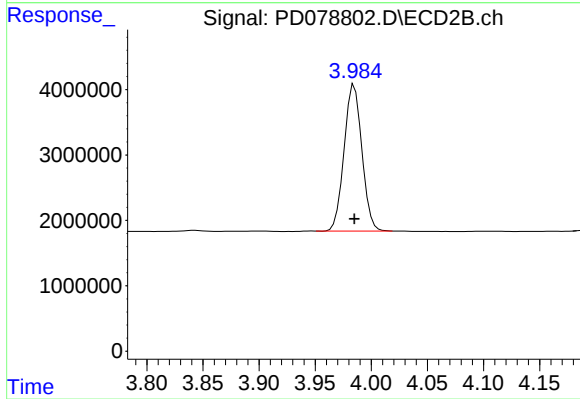

#4 Heptachlor


R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 24695462
Conc: 10.19 ng/ml

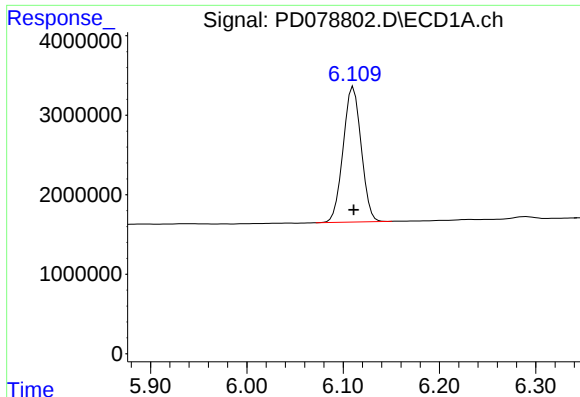

#9 Endosulfan I


R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 22111581
Conc: 10.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

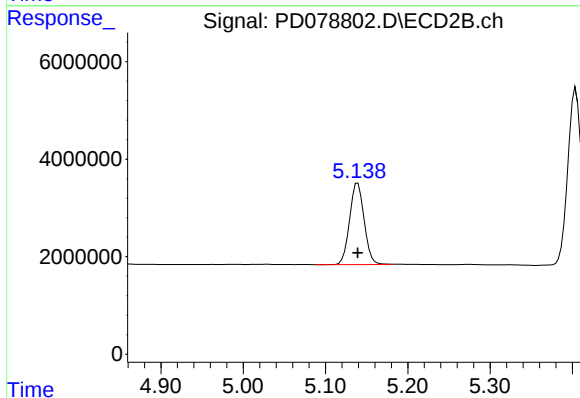


#9 Endosulfan I

R.T.: 5.139 min
Delta R.T.: 0.000 min
Response: 20545836
Conc: 10.42 ng/ml

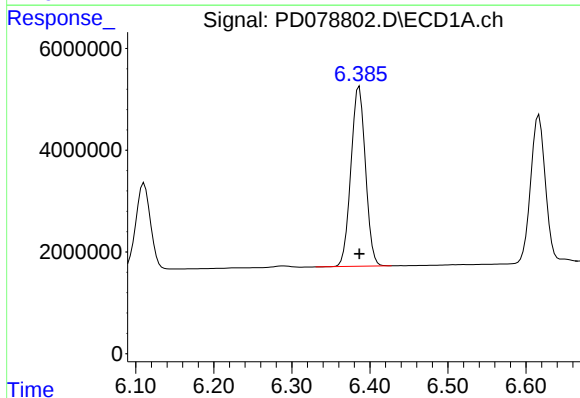


#13 Dieldrin

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 45662445
Conc: 20.56 ng/ml

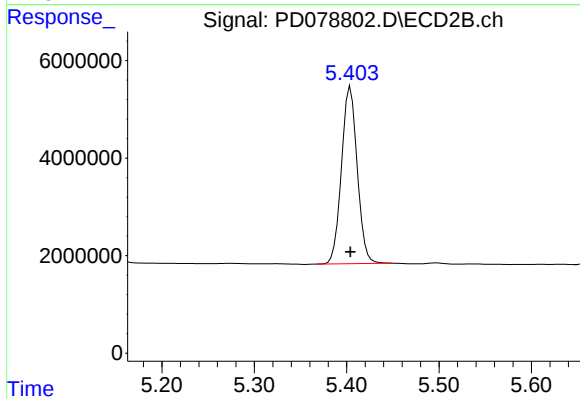

#13 Dieldrin


R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 43024872
Conc: 20.50 ng/ml

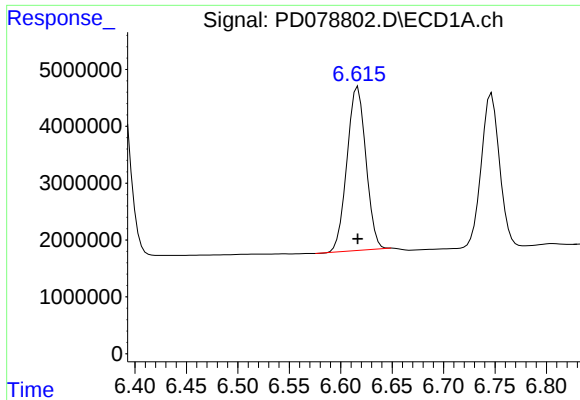

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 36995211
Conc: 20.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

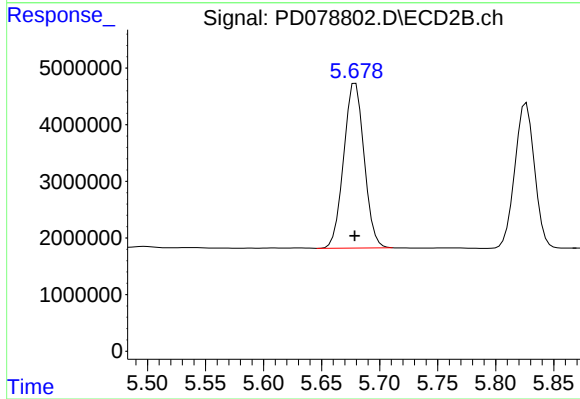


#14 Endrin

R.T.: 5.679 min
Delta R.T.: 0.000 min
Response: 35664252
Conc: 20.58 ng/ml

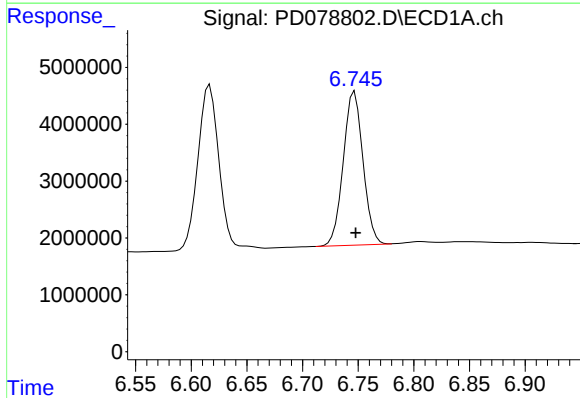


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 33380204
Conc: 20.53 ng/ml

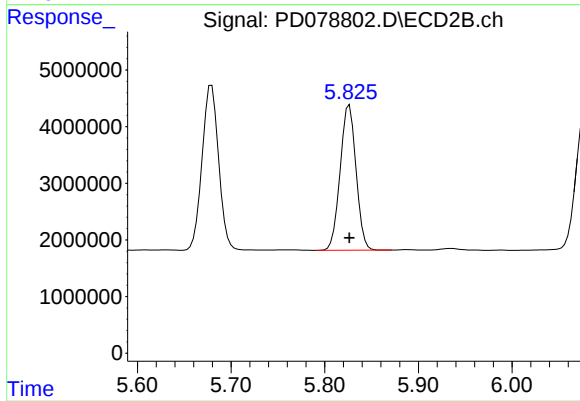

#16 4,4'-DDD


R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 30258713
Conc: 20.48 ng/ml

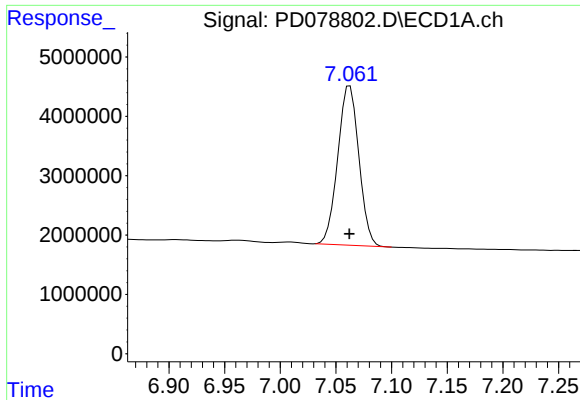

#17 4,4'-DDT


R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 35408138
Conc: 20.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

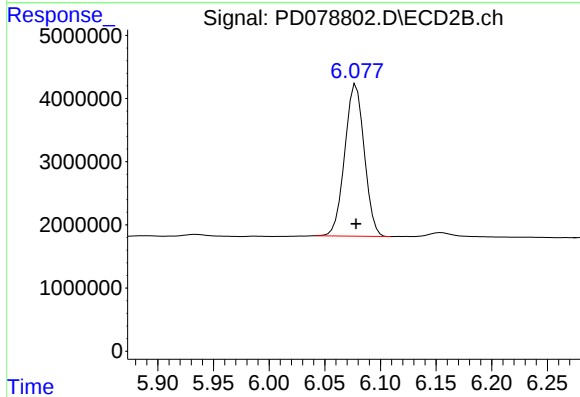


#17 4,4'-DDT

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 29396812
Conc: 20.65 ng/ml

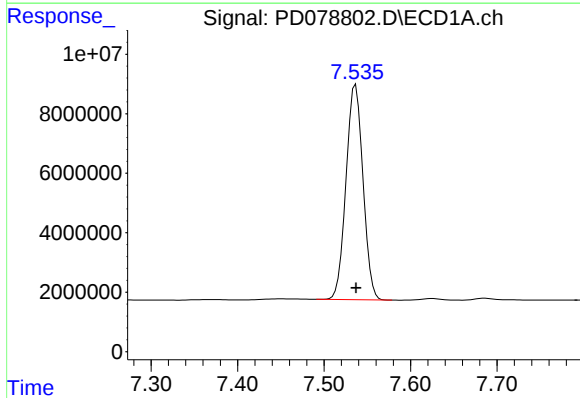


#20 Methoxychlor

R.T.: 7.536 min
Delta R.T.: 0.000 min
Response: 98146869
Conc: 105.19 ng/ml

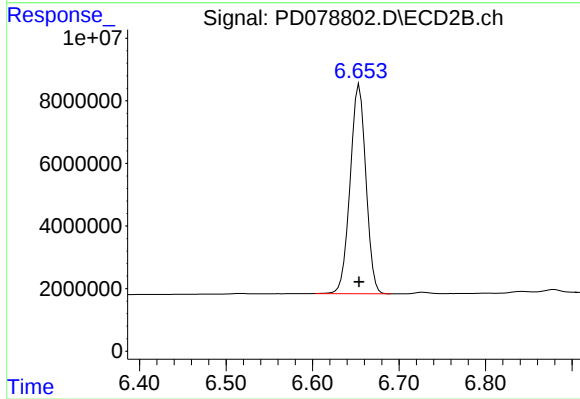

#20 Methoxychlor


R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 84462640
Conc: 108.22 ng/ml

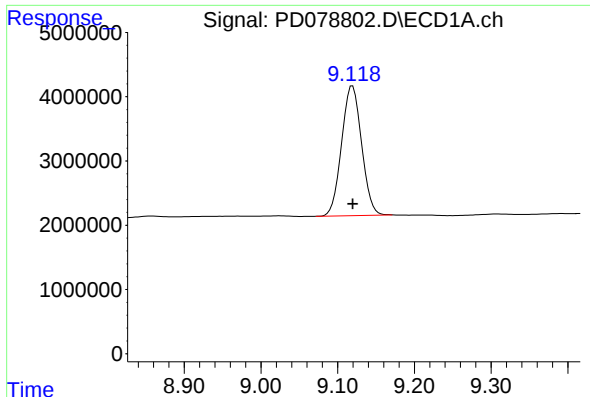

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 36696337
Conc: 21.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

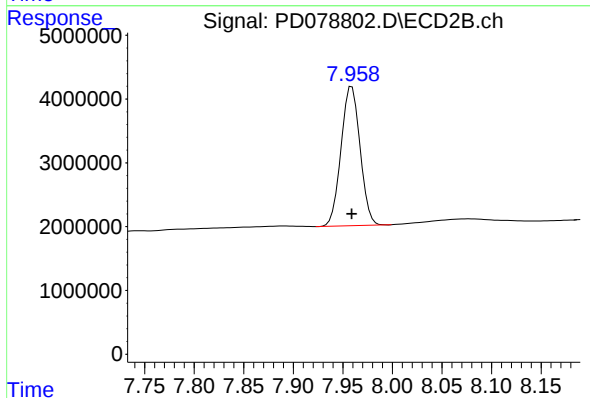

#27 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: 0.000 min
Response: 29187115
Conc: 21.11 ng/ml