

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
 Data File : PD078804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 00:28
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 05:36:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 05:31:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.808	30390813	38519022	20.000	20.000
27)	SA Decachlor...	9.119	7.959	68928043	55317392	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.027	3.311	51082876	53947848	20.000	20.000
3)	MA gamma-BHC...	4.361	3.641	48761987	49948168	20.000	20.000
4)	MA Heptachlor	4.954	3.985	52801565	48462253	20.000	20.000
9)	A Endosulfan I	6.111	5.139	41755589	39449435	20.000	20.000
13)	MA Dieldrin	6.387	5.404	88858068	83959948	40.000	40.000
14)	MA Endrin	6.617	5.679	72298788	69308238	40.000	40.000
16)	A 4,4'-DDD	6.748	5.826	65023148	59103293	40.000	40.000
17)	MA 4,4'-DDT	7.062	6.078	69185326	56955054	40.000	40.000
20)	A Methoxychlor	7.537	6.654	186.6E6	156.1E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 00:28
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 05:36:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:31:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

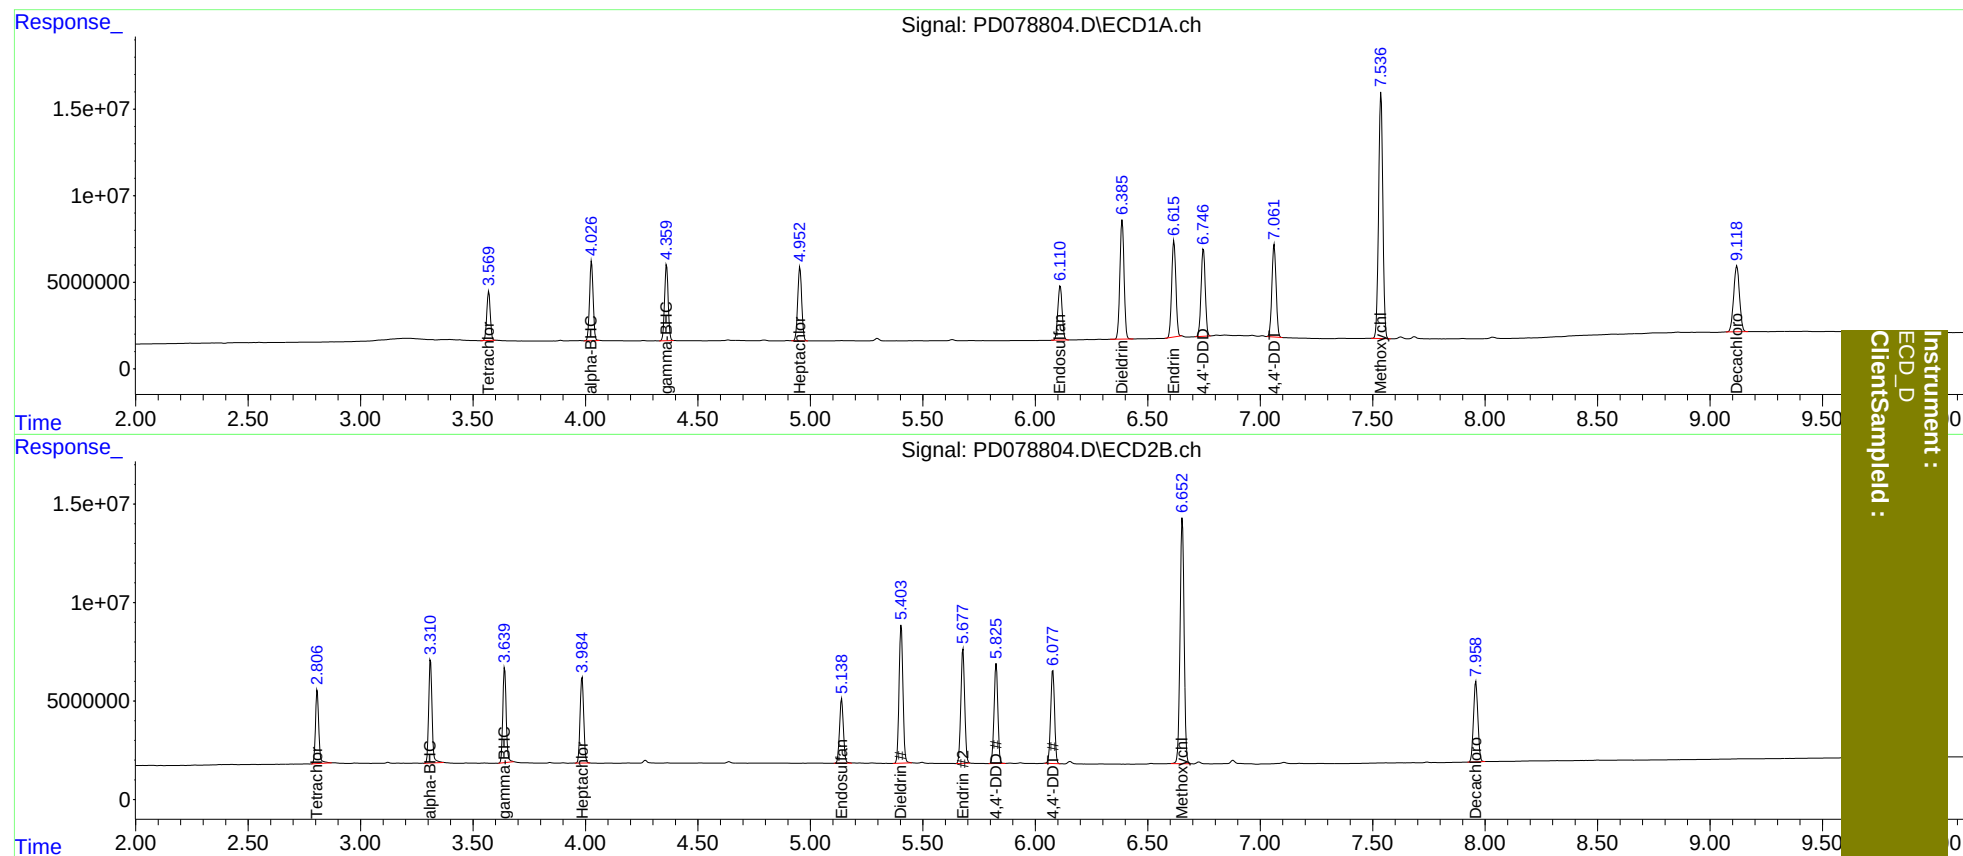


Instrument :
ECD_D
ClientSampled :
0

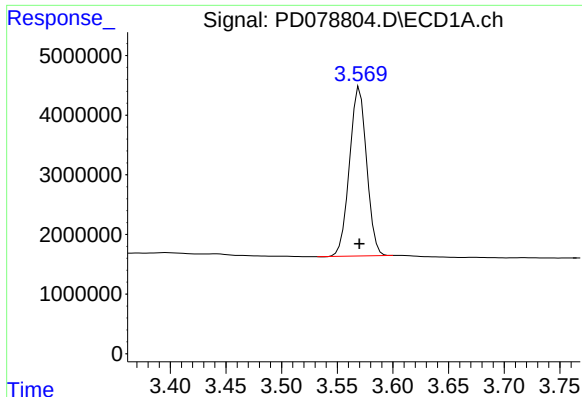

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 30390813
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

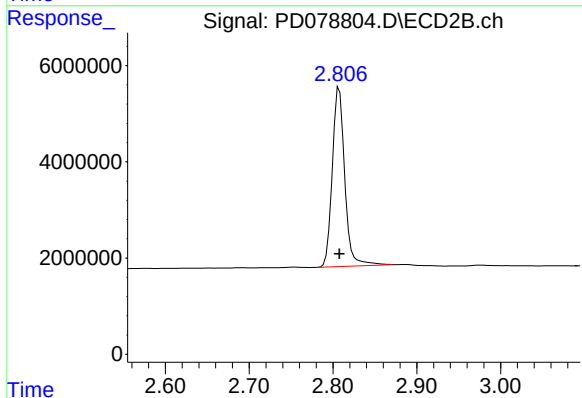


#1 Tetrachloro-m-xylene

R.T.: 2.808 min
Delta R.T.: 0.000 min
Response: 38519022
Conc: 20.00 ng/ml

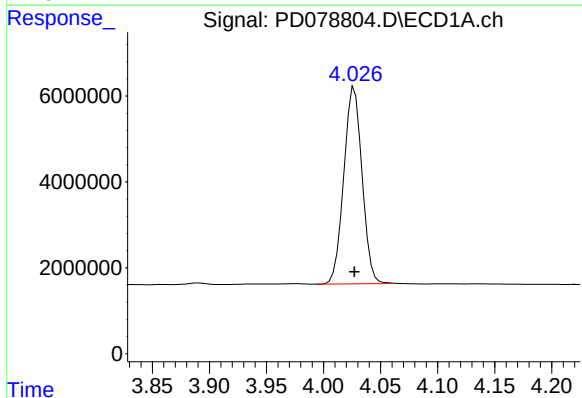


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 51082876
Conc: 20.00 ng/ml

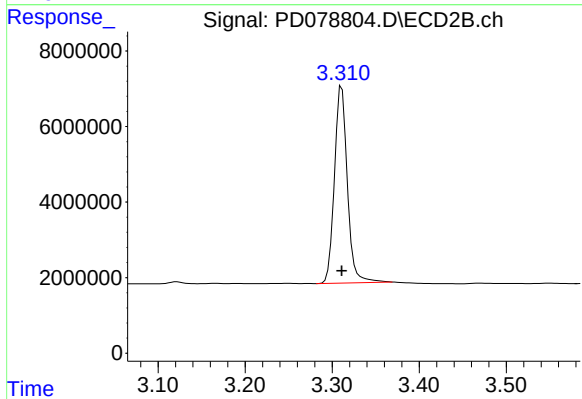

#2 alpha-BHC


R.T.: 3.311 min
Delta R.T.: 0.000 min
Response: 53947848
Conc: 20.00 ng/ml

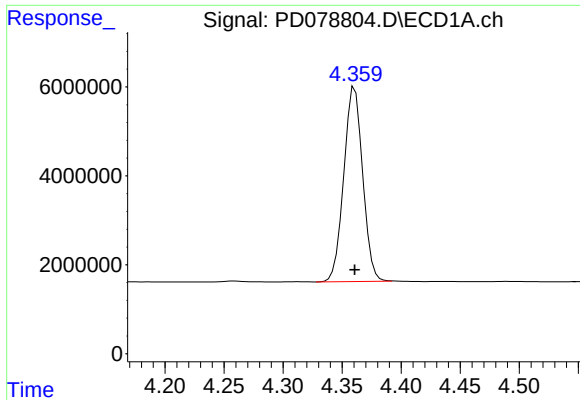

#3 gamma-BHC (Lindane)


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 48761987
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

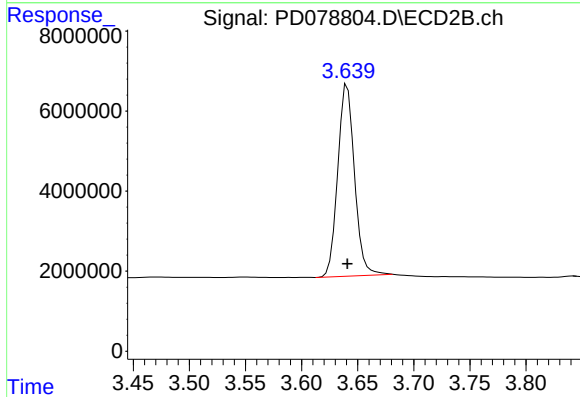


#3 gamma-BHC (Lindane)

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 49948168
Conc: 20.00 ng/ml

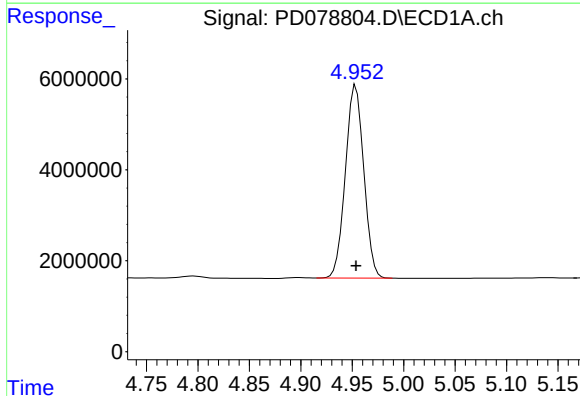


#4 Heptachlor

R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 52801565
Conc: 20.00 ng/ml

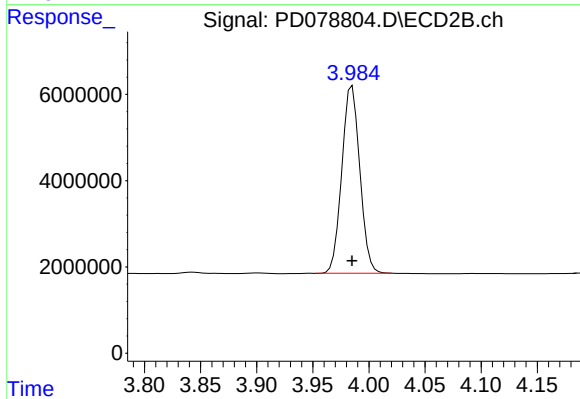

#4 Heptachlor


R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 48462253
Conc: 20.00 ng/ml

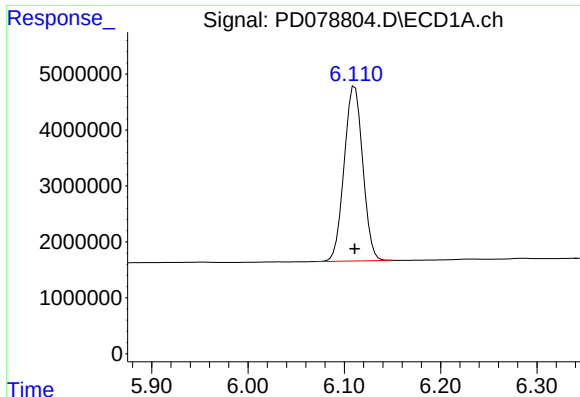

#9 Endosulfan I


R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 41755589
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

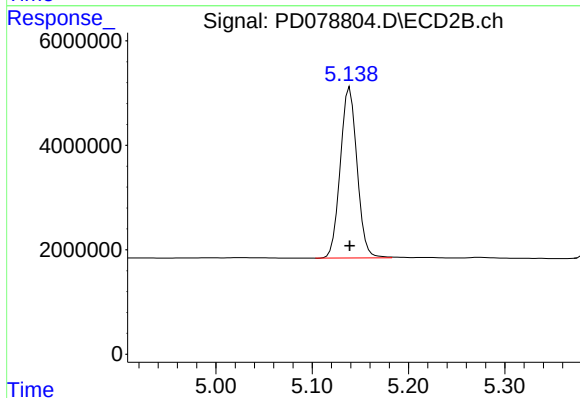


#9 Endosulfan I

R.T.: 5.139 min
Delta R.T.: 0.000 min
Response: 39449435
Conc: 20.00 ng/ml

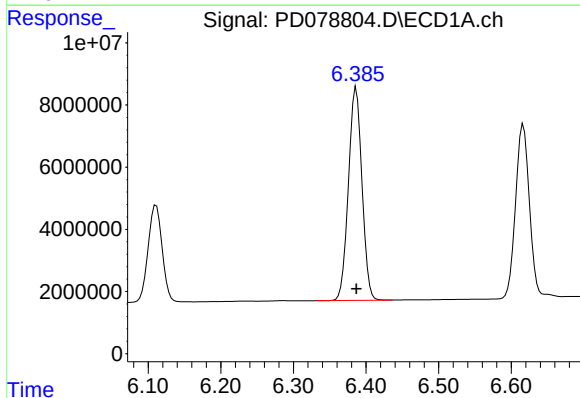


#13 Dieldrin

R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 88858068
Conc: 40.00 ng/ml

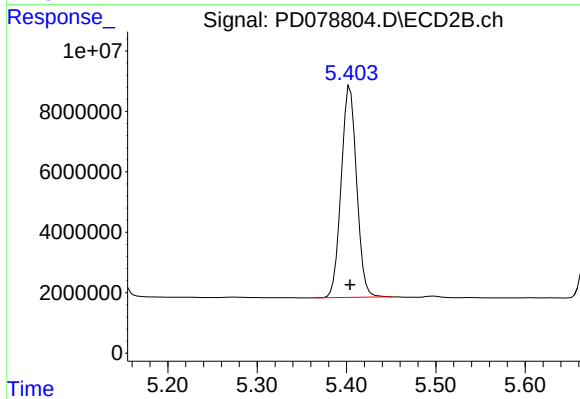

#13 Dieldrin


R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 83959948
Conc: 40.00 ng/ml

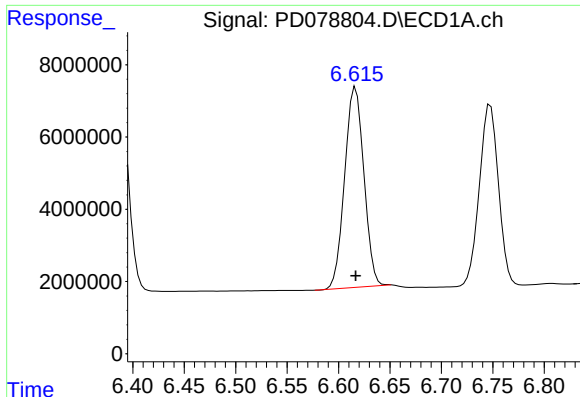

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 72298788
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

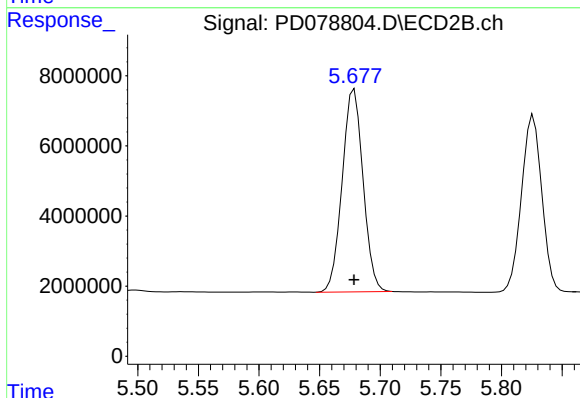


#14 Endrin

R.T.: 5.679 min
Delta R.T.: 0.000 min
Response: 69308238
Conc: 40.00 ng/ml

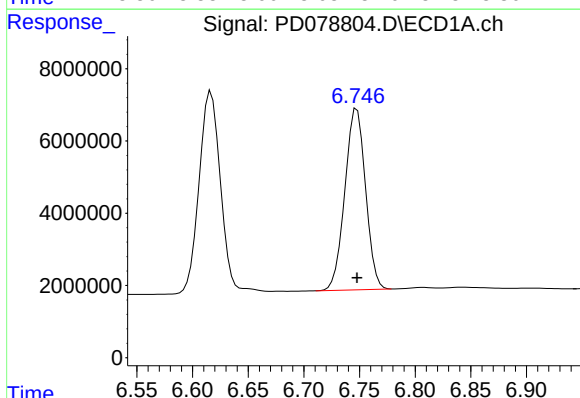


#16 4,4'-DDD

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 65023148
Conc: 40.00 ng/ml

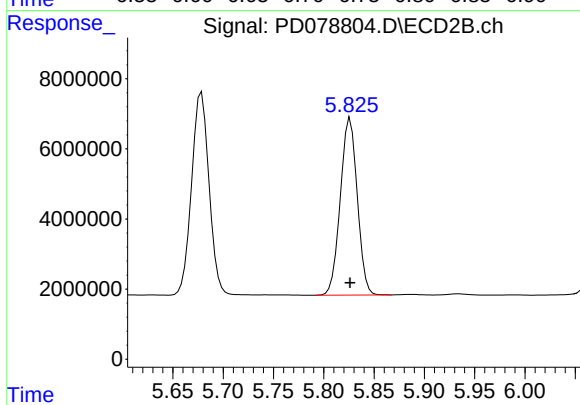

#16 4,4'-DDD


R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 59103293
Conc: 40.00 ng/ml

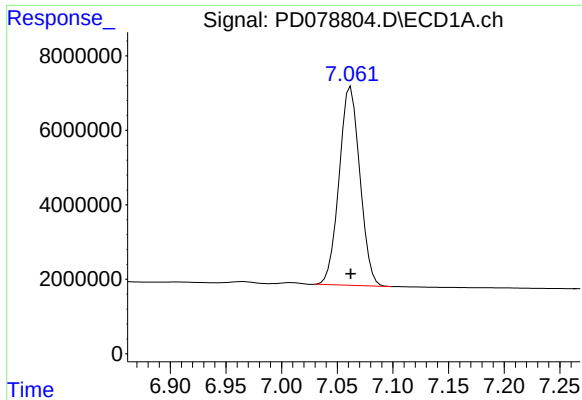

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 69185326
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

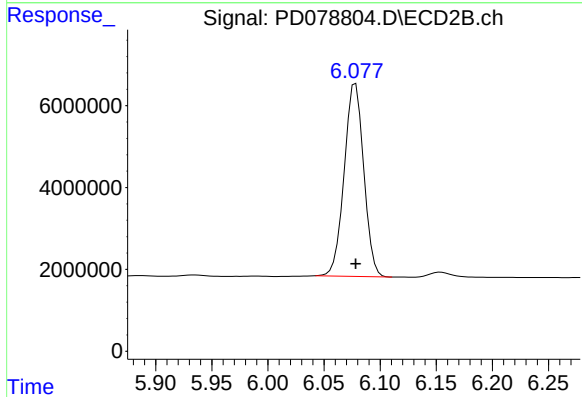


#17 4,4'-DDT

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 56955054
Conc: 40.00 ng/ml

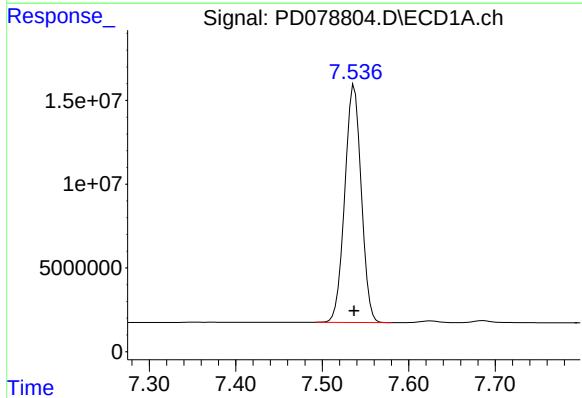


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 186614596
Conc: 200.00 ng/ml

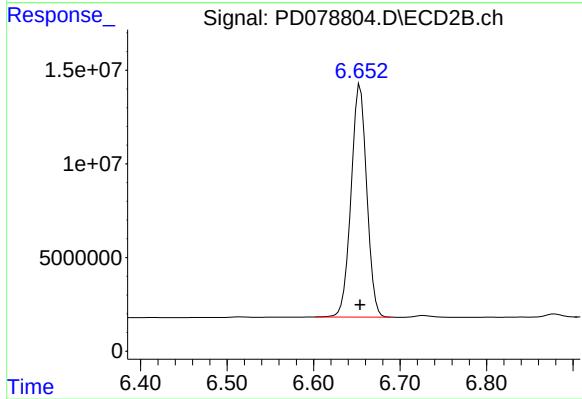

#20 Methoxychlor


R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 156089752
Conc: 200.00 ng/ml

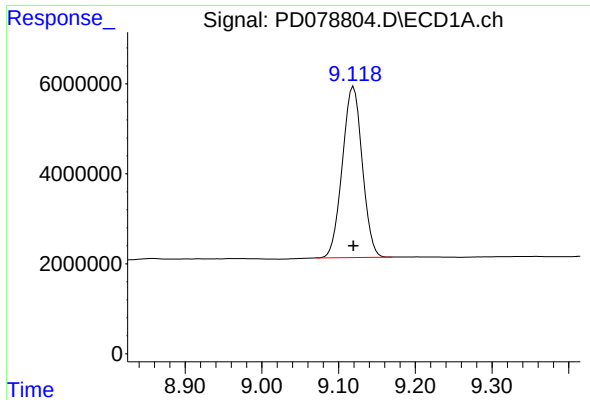

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 68928043
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

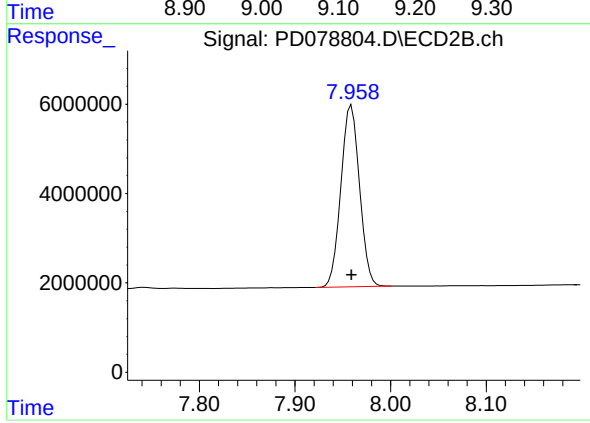

#27 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: 0.000 min
Response: 55317392
Conc: 40.00 ng/ml