

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
 Data File : PD078806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 00:55
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 05:36:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 05:31:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.808	59143979	76675209	38.922	39.812
27)	SA Decachlor...	9.120	7.960	130.3E6	104.7E6	75.610	75.734
Target Compounds							
2)	A alpha-BHC	4.027	3.312	104.9E6	113.5E6	41.075	42.080
3)	MA gamma-BHC...	4.361	3.641	97607418	103.3E6	40.034	41.366
4)	MA Heptachlor	4.954	3.985	102.1E6	98918134	38.678	40.823
9)	A Endosulfan I	6.111	5.140	80747934	77278376	38.676	39.178
13)	MA Dieldrin	6.387	5.404	178.0E6	170.3E6	80.122	81.151
14)	MA Endrin	6.617	5.679	143.8E6	138.6E6	79.579	79.996
16)	A 4,4'-DDD	6.747	5.827	130.7E6	118.8E6	80.380	80.378
17)	MA 4,4'-DDT	7.063	6.078	138.5E6	113.6E6	80.104	79.799
20)	A Methoxychlor	7.537	6.654	363.4E6	292.3E6	389.412	374.517


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 00:55
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 05:36:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:31:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

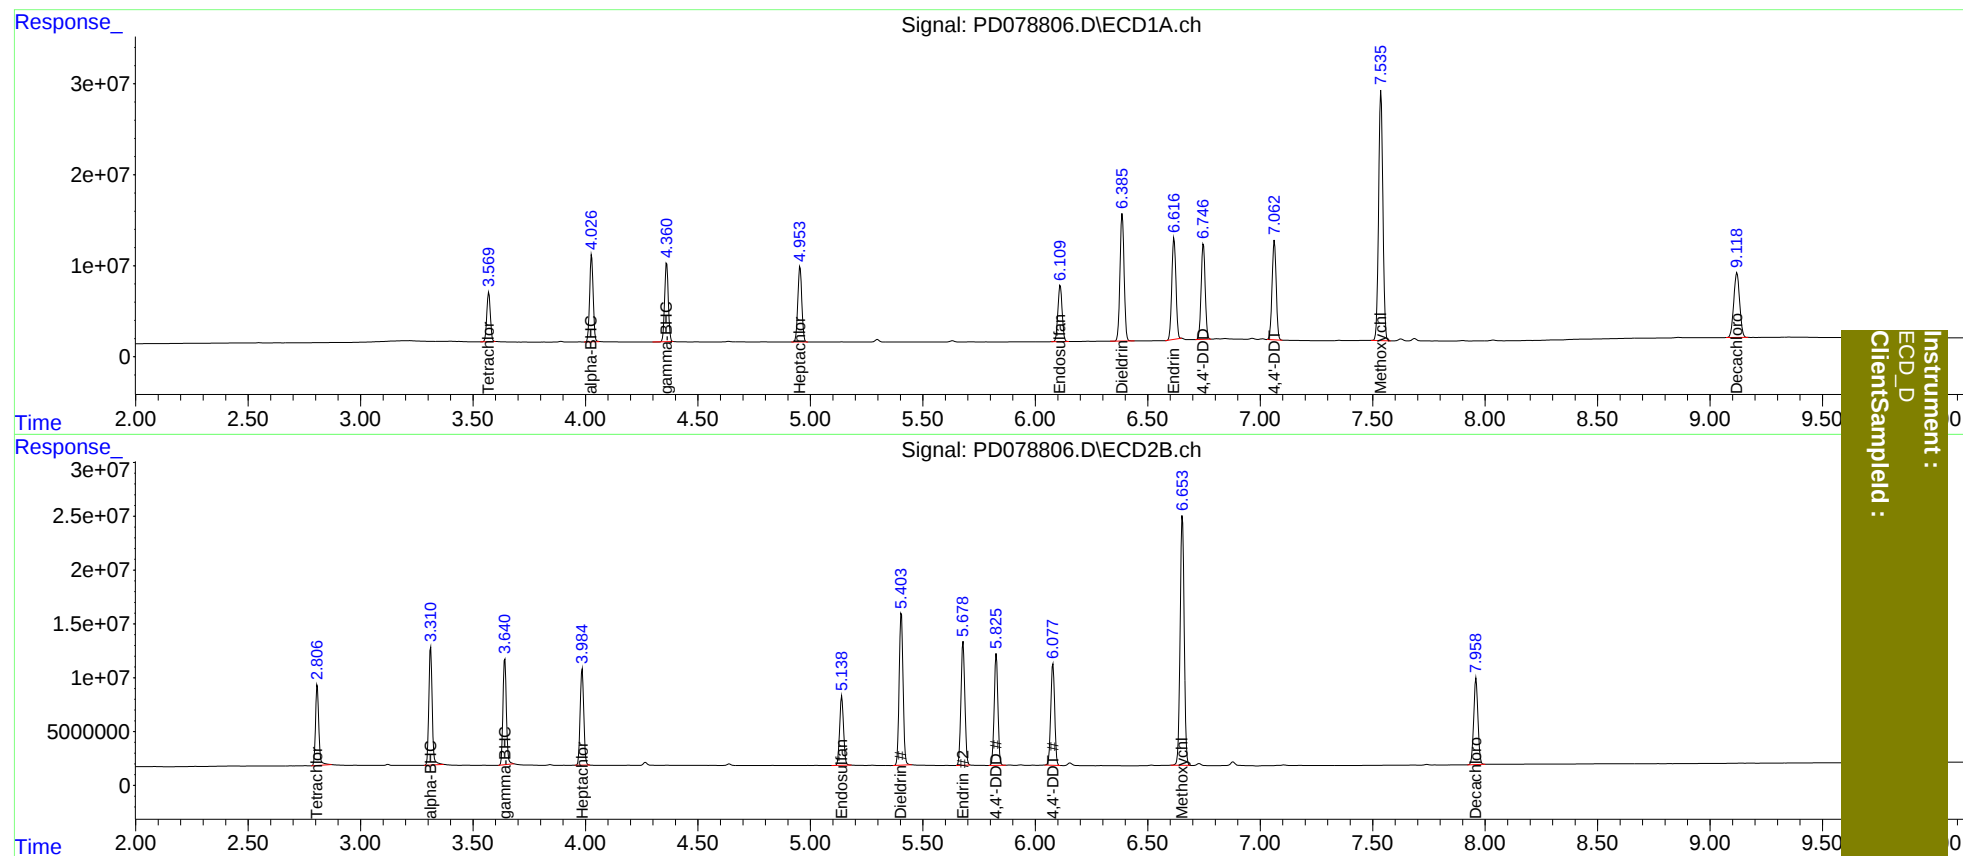


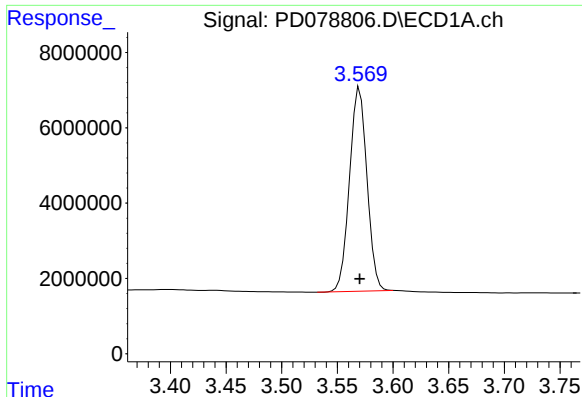

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 59143979
Conc: 38.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

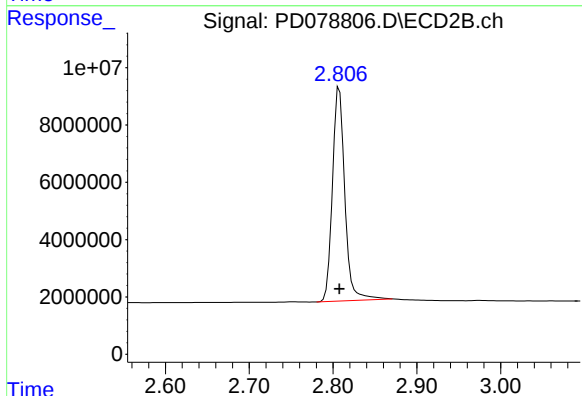


#1 Tetrachloro-m-xylene

R.T.: 2.808 min
Delta R.T.: 0.000 min
Response: 76675209
Conc: 39.81 ng/ml

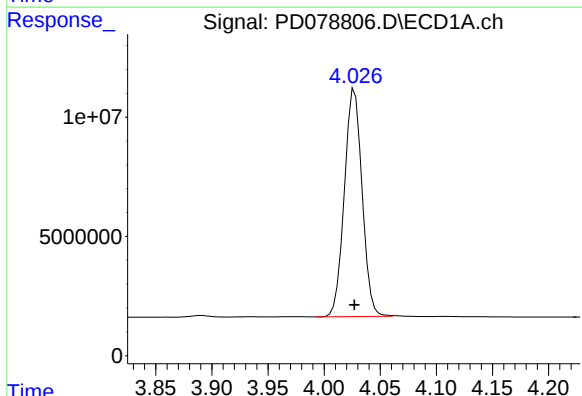


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 104912061
Conc: 41.08 ng/ml

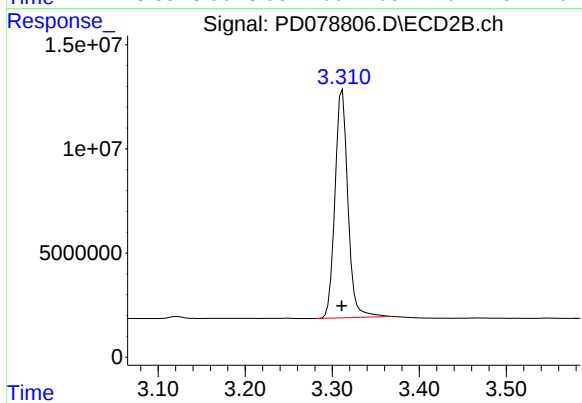

#2 alpha-BHC


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 113506638
Conc: 42.08 ng/ml

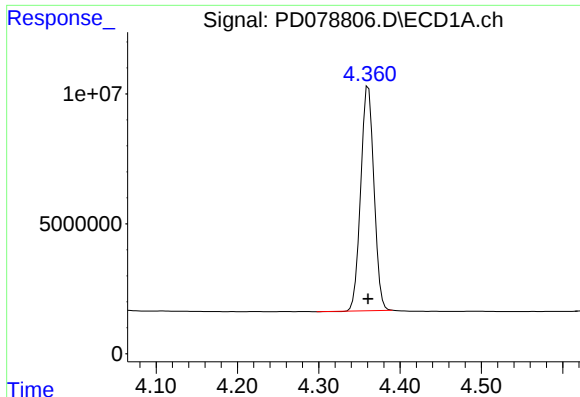

#3 gamma-BHC (Lindane)


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 97607418
Conc: 40.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

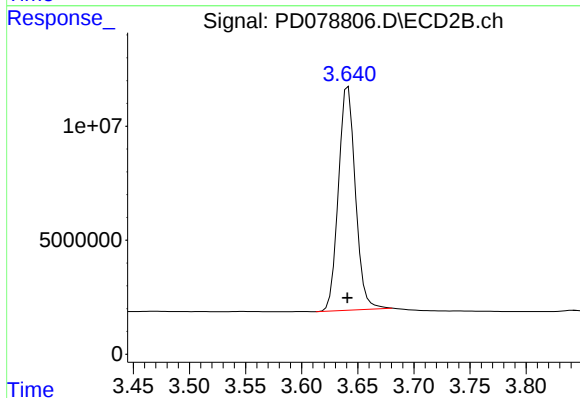


#3 gamma-BHC (Lindane)

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 103308437
Conc: 41.37 ng/ml

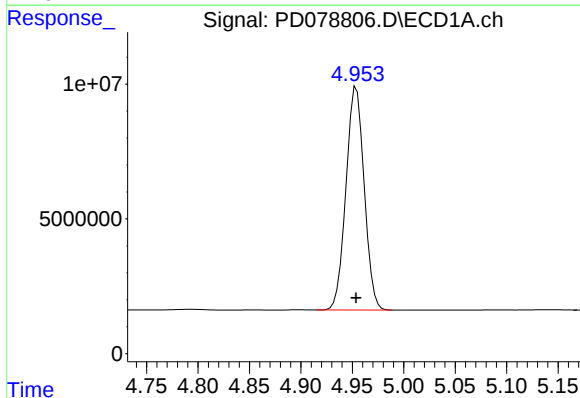


#4 Heptachlor

R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 102113376
Conc: 38.68 ng/ml

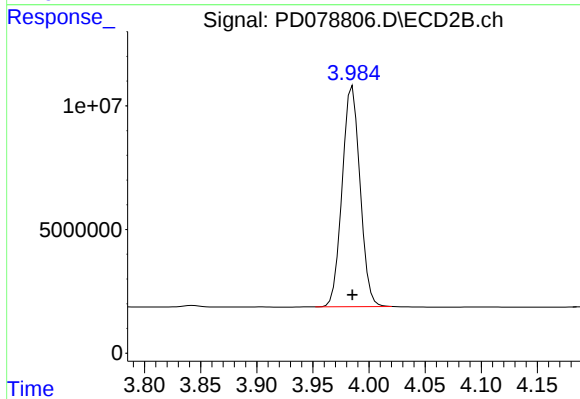

#4 Heptachlor


R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 98918134
Conc: 40.82 ng/ml

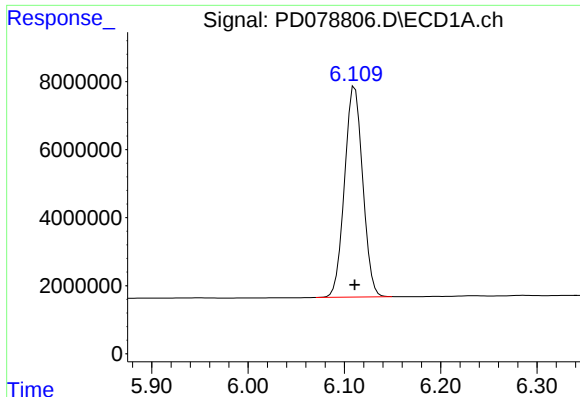

#9 Endosulfan I


R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 80747934
Conc: 38.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

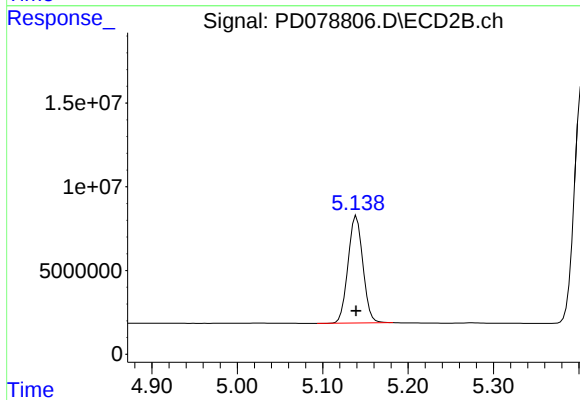


#9 Endosulfan I

R.T.: 5.140 min
Delta R.T.: 0.000 min
Response: 77278376
Conc: 39.18 ng/ml

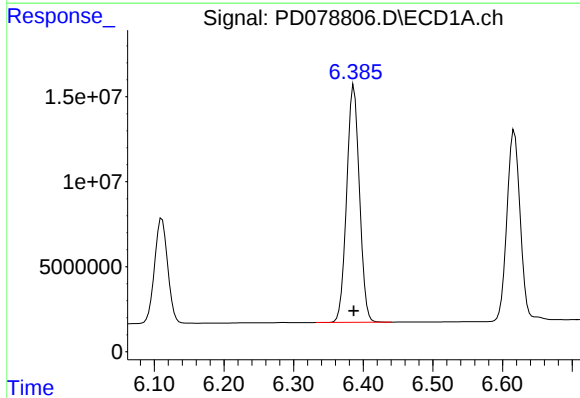


#13 Dieldrin

R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 177987151
Conc: 80.12 ng/ml

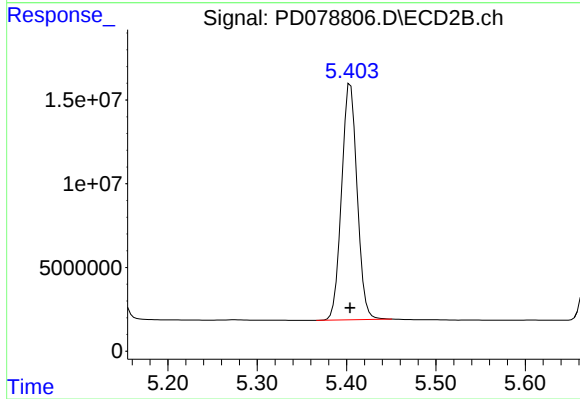

#13 Dieldrin


R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 170336288
Conc: 81.15 ng/ml

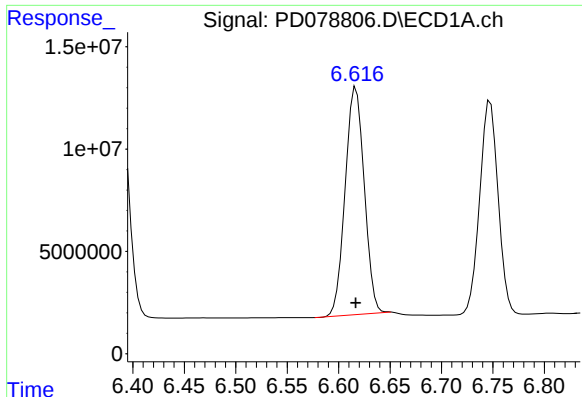

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 143836403
Conc: 79.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

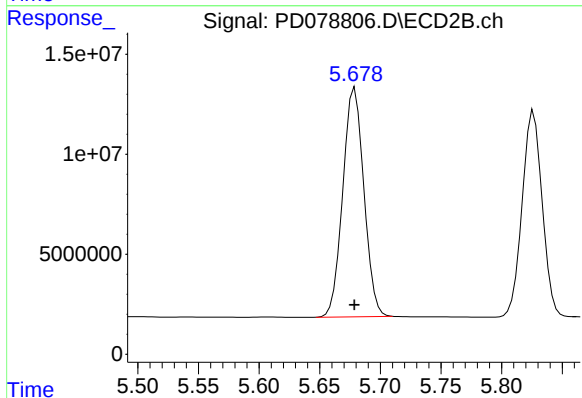


#14 Endrin

R.T.: 5.679 min
Delta R.T.: 0.000 min
Response: 138609882
Conc: 80.00 ng/ml

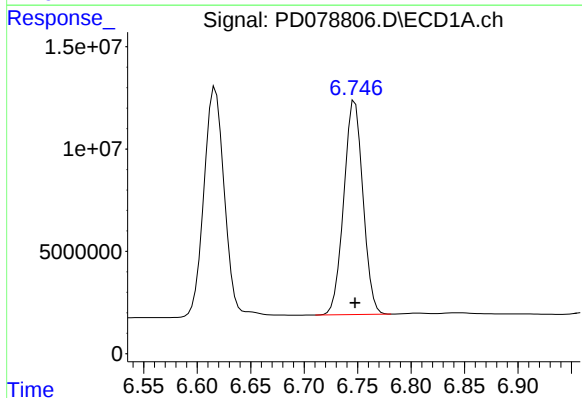


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 130664253
Conc: 80.38 ng/ml

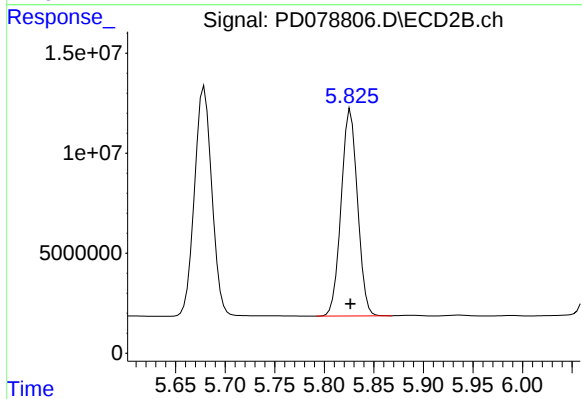

#16 4,4'-DDD


R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 118765302
Conc: 80.38 ng/ml

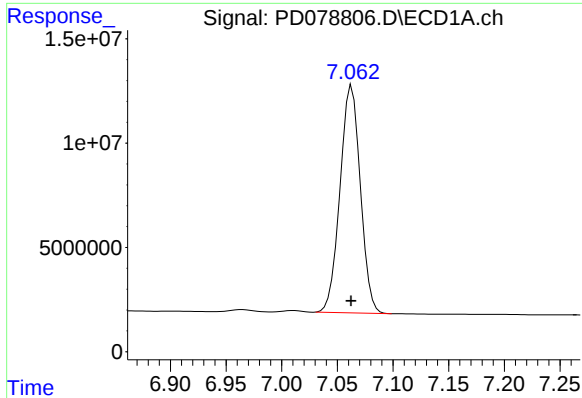

#17 4,4'-DDT


R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 138549756
Conc: 80.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

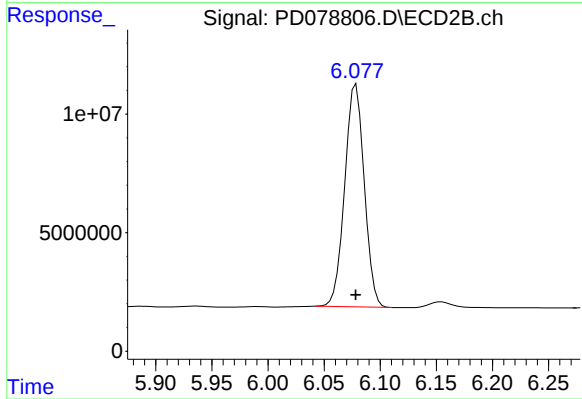


#17 4,4'-DDT

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 113623384
Conc: 79.80 ng/ml

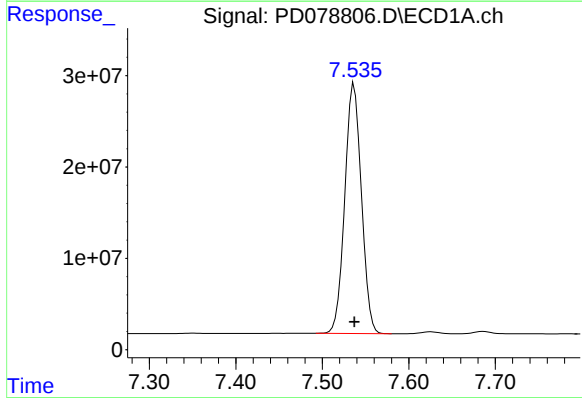


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 363350211
Conc: 389.41 ng/ml

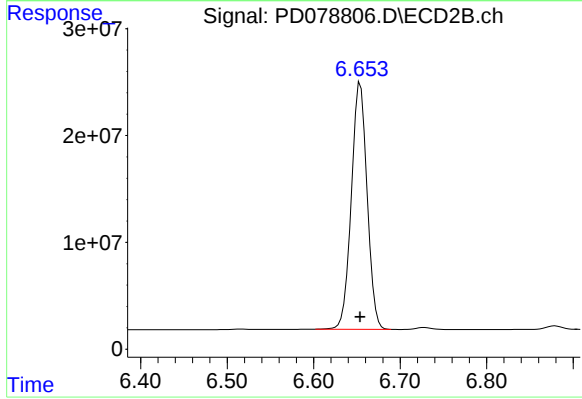

#20 Methoxychlor


R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 292291229
Conc: 374.52 ng/ml

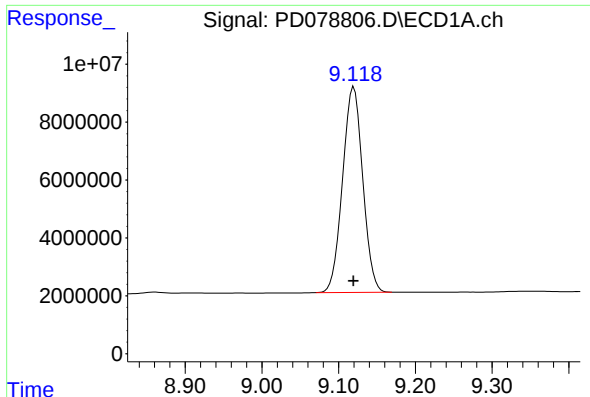

#27 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 130291870
Conc: 75.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

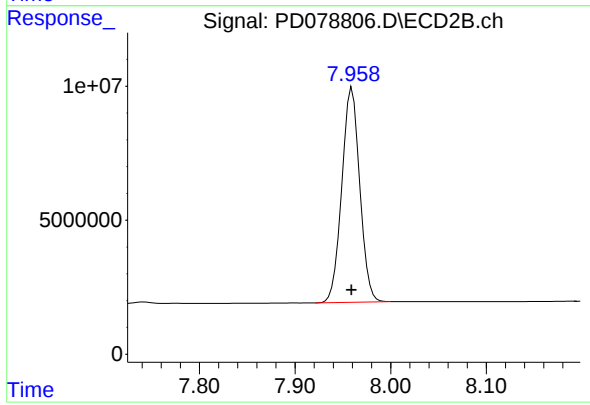

#27 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: 0.000 min
Response: 104734870
Conc: 75.73 ng/ml