

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
 Data File : PD078808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 01:21
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 05:36:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 05:31:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.807	117.3E6	153.5E6	77.205	79.712
27)	SA Decachlor...	9.119	7.959	255.1E6	197.5E6	148.028	142.796
Target Compounds							
2)	A alpha-BHC	4.027	3.311	218.7E6	238.9E6	85.641	88.563
3)	MA gamma-BHC...	4.360	3.641	201.7E6	215.7E6	82.721	86.353
4)	MA Heptachlor	4.953	3.985	215.5E6	202.9E6	81.617	83.720
9)	A Endosulfan I	6.110	5.139	159.7E6	155.8E6	76.470	78.970
13)	MA Dieldrin	6.387	5.404	363.8E6	348.1E6	163.748	165.841
14)	MA Endrin	6.617	5.679	292.0E6	279.5E6	161.573	161.281
16)	A 4,4'-DDD	6.747	5.826	267.0E6	240.3E6	164.220	162.650
17)	MA 4,4'-DDT	7.063	6.078	281.9E6	229.1E6	162.983	160.901
20)	A Methoxychlor	7.537	6.654	710.8E6	535.5E6	761.792	686.105

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 01:21
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 05:36:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:31:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

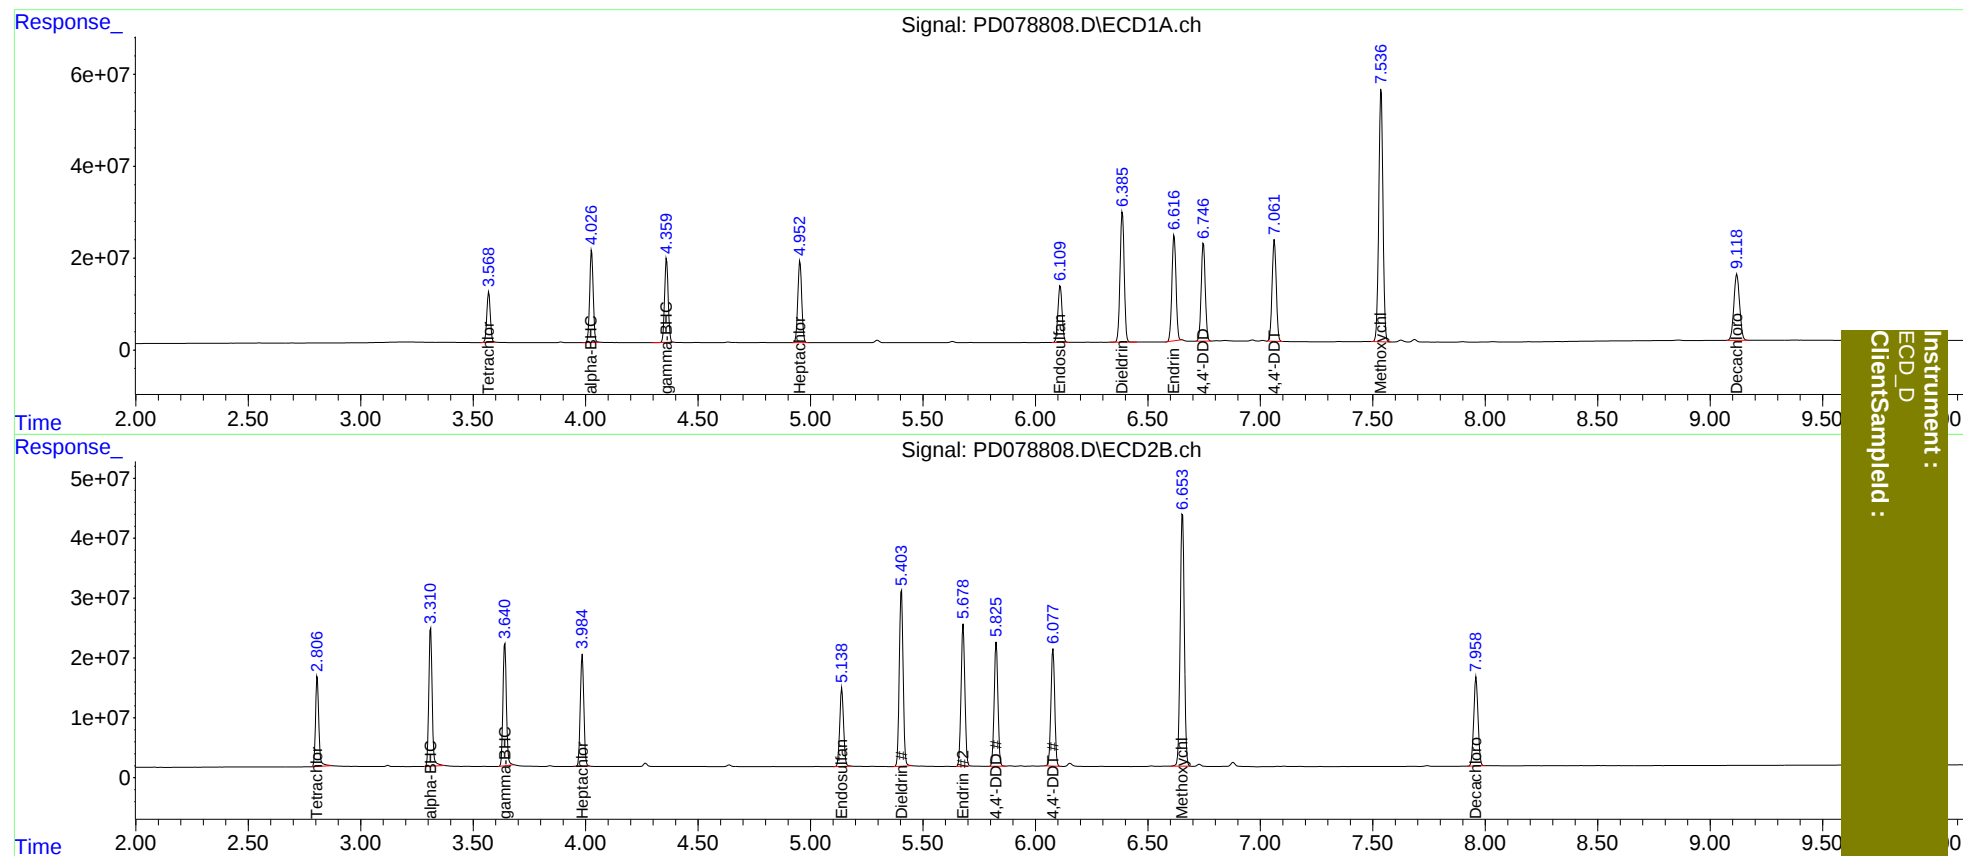


Instrument :
ECD_D
ClientSampled :
0

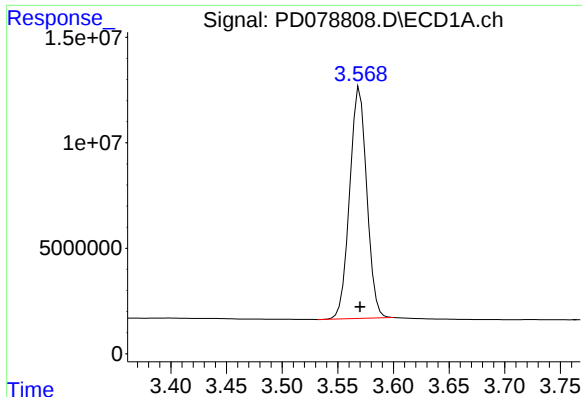

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 117316074
Conc: 77.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

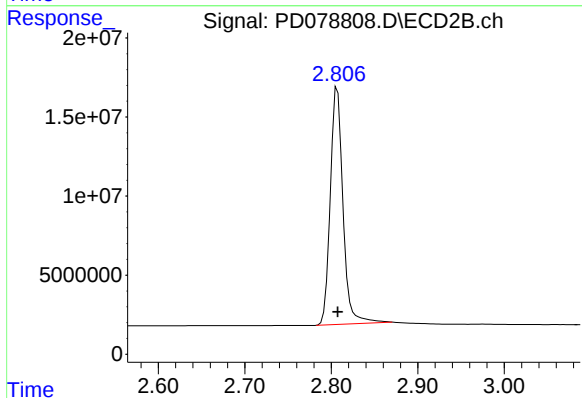


#1 Tetrachloro-m-xylene

R.T.: 2.807 min
Delta R.T.: 0.000 min
Response: 153521040
Conc: 79.71 ng/ml

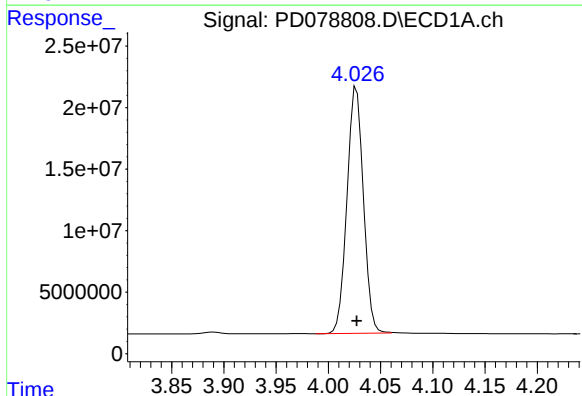


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 218738589
Conc: 85.64 ng/ml

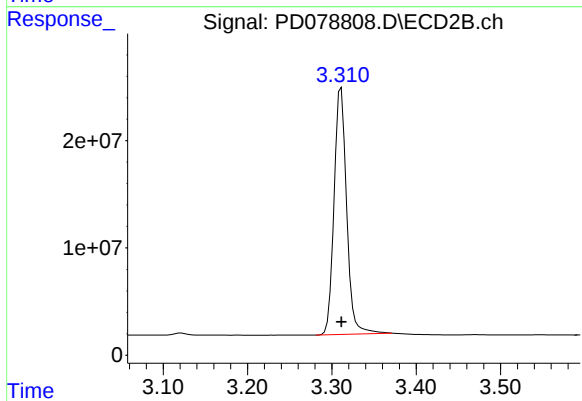

#2 alpha-BHC


R.T.: 3.311 min
Delta R.T.: 0.000 min
Response: 238889171
Conc: 88.56 ng/ml

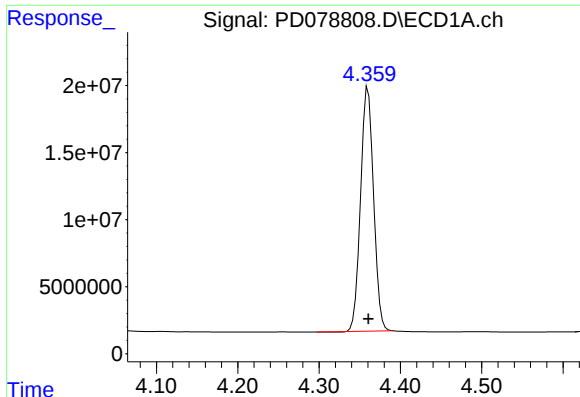

#3 gamma-BHC (Lindane)


R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 201681402
Conc: 82.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

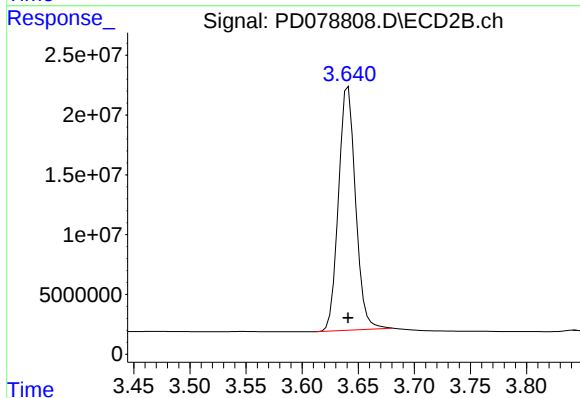


#3 gamma-BHC (Lindane)

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 215659246
Conc: 86.35 ng/ml

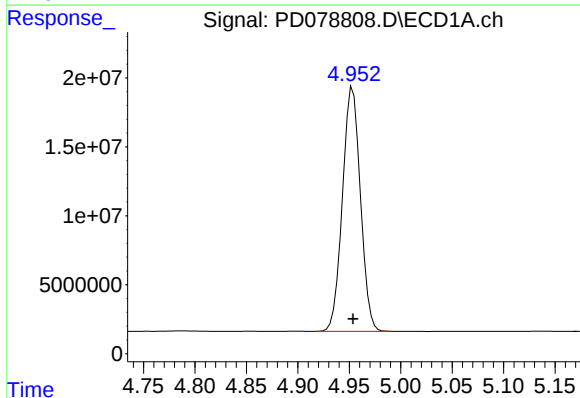


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 215474487
Conc: 81.62 ng/ml

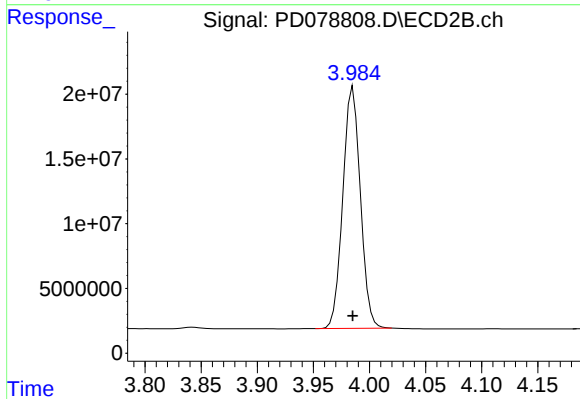

#4 Heptachlor


R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 202863858
Conc: 83.72 ng/ml

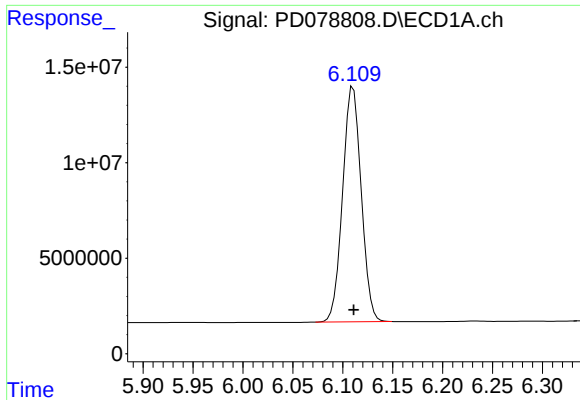

#9 Endosulfan I


R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 159653405
Conc: 76.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

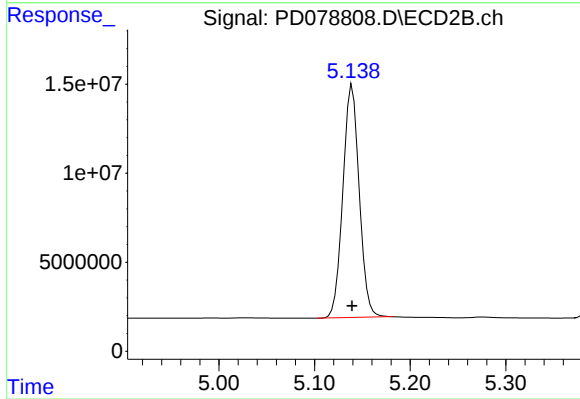


#9 Endosulfan I

R.T.: 5.139 min
Delta R.T.: 0.000 min
Response: 155765528
Conc: 78.97 ng/ml

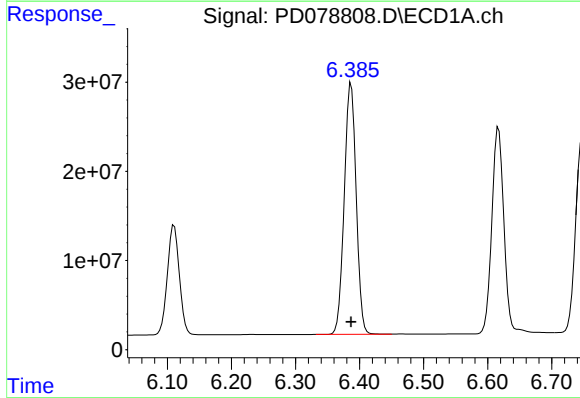


#13 Dieldrin

R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 363757411
Conc: 163.75 ng/ml

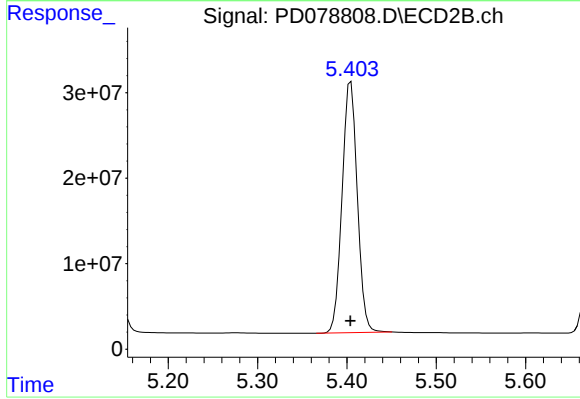

#13 Dieldrin


R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 348099959
Conc: 165.84 ng/ml

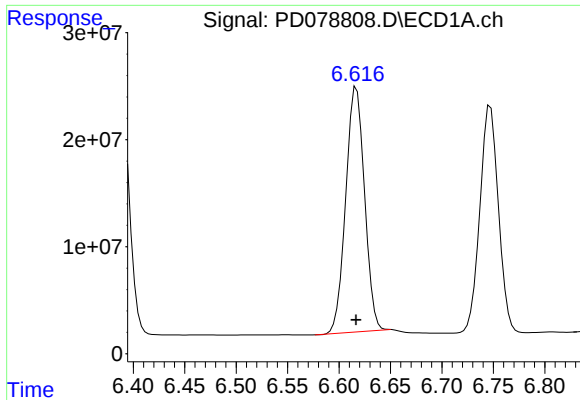

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 292037751
Conc: 161.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

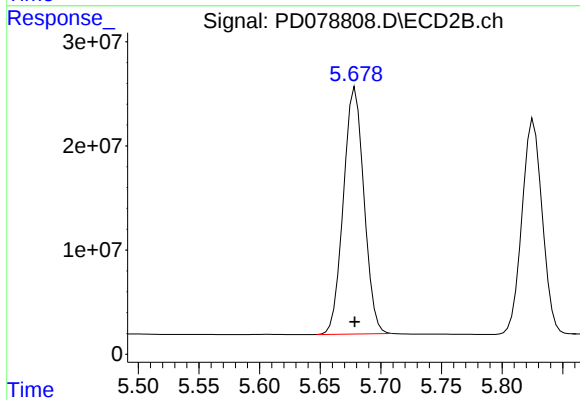


#14 Endrin

R.T.: 5.679 min
Delta R.T.: 0.000 min
Response: 279452005
Conc: 161.28 ng/ml

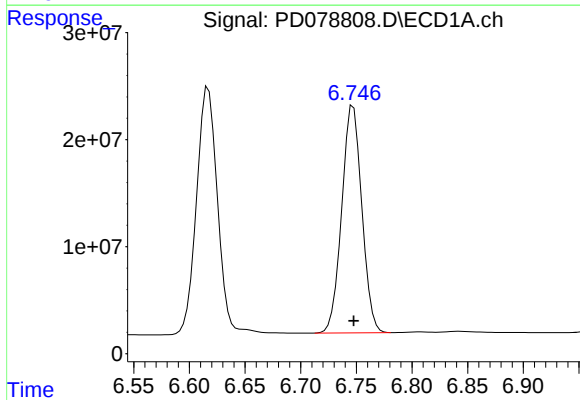


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 266951764
Conc: 164.22 ng/ml

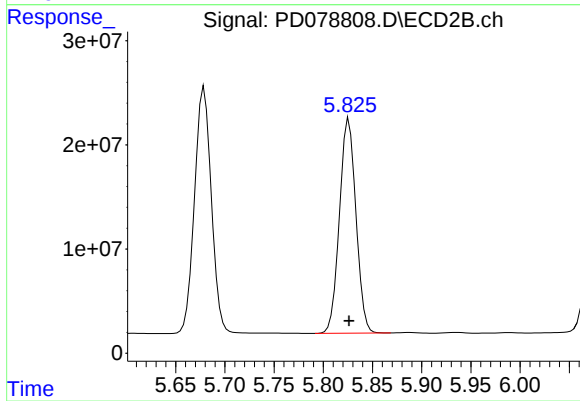

#16 4,4'-DDD


R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 240328613
Conc: 162.65 ng/ml

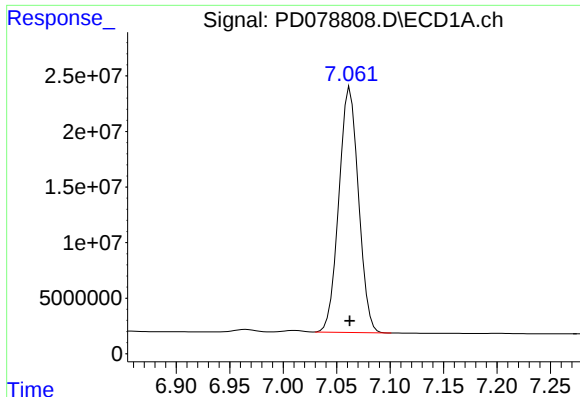

#17 4,4'-DDT


R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 281900402
Conc: 162.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

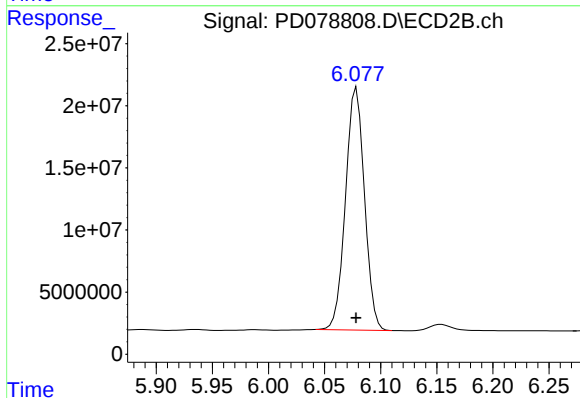


#17 4,4'-DDT

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 229102784
Conc: 160.90 ng/ml

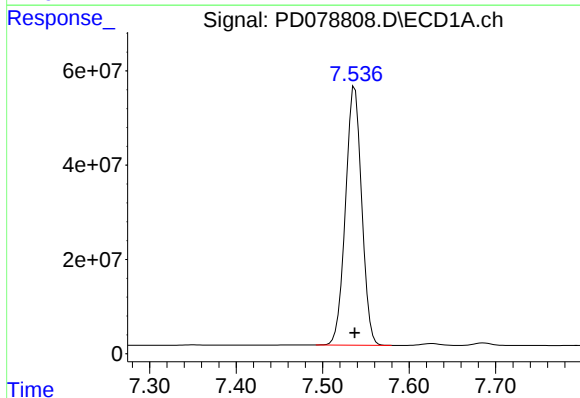


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 710807324
Conc: 761.79 ng/ml

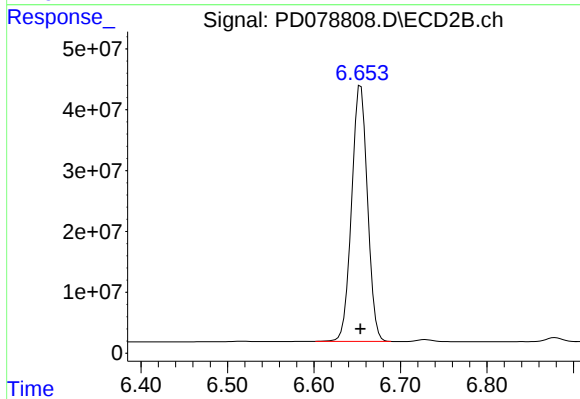

#20 Methoxychlor

R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 535469894
Conc: 686.11 ng/ml

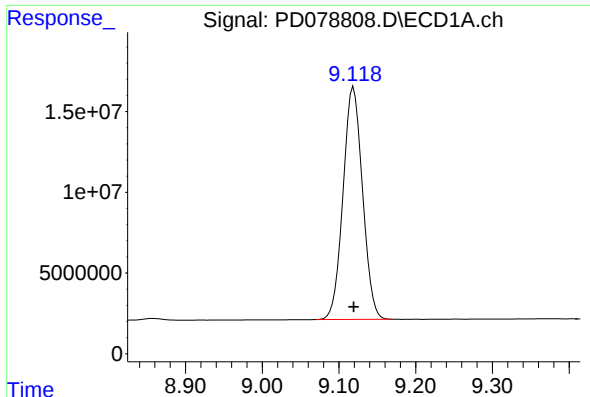

#27 Decachlorobiphenyl


R.T.: 9.119 min

Delta R.T.: 0.000 min

Response: 255081920

Conc: 148.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

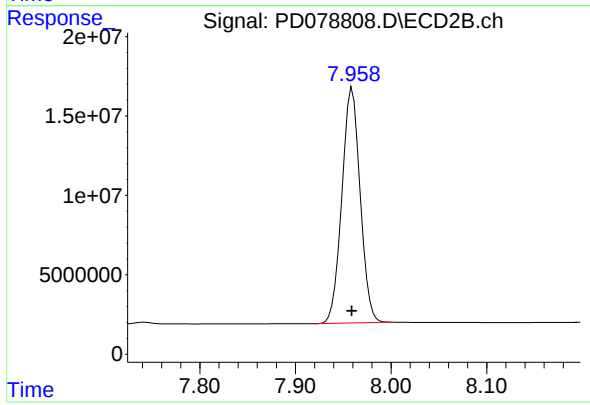

#27 Decachlorobiphenyl

R.T.: 7.959 min

Delta R.T.: 0.000 min

Response: 197477257

Conc: 142.80 ng/ml