

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
 Data File : PD078810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 01:48
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 05:36:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 05:31:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.808	227.8E6	301.9E6	149.931	156.749
27)	SA Decachlor...	9.119	7.960	501.1E6	378.0E6	290.780	273.297
Target Compounds							
2)	A alpha-BHC	4.027	3.312	439.8E6	480.6E6	172.192	178.169
3)	MA gamma-BHC...	4.361	3.642	401.7E6	434.5E6	164.776	173.977
4)	MA Heptachlor	4.954	3.986	399.3E6	403.6E6	151.234	166.549
9)	A Endosulfan I	6.111	5.140	307.1E6	307.6E6	147.110	155.969
13)	MA Dieldrin	6.387	5.405	710.1E6	684.4E6	319.670	326.058
14)	MA Endrin	6.617	5.679	577.0E6	551.4E6	319.240	318.252
16)	A 4,4'-DDD	6.748	5.827	527.5E6	477.8E6	324.507	323.335
17)	MA 4,4'-DDT	7.063	6.079	558.3E6	458.1E6	322.762	321.710
20)	A Methoxychlor	7.537	6.654	1359.1E6	974.5E6	1456.592	1248.673

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 01:48
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 05:36:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:31:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

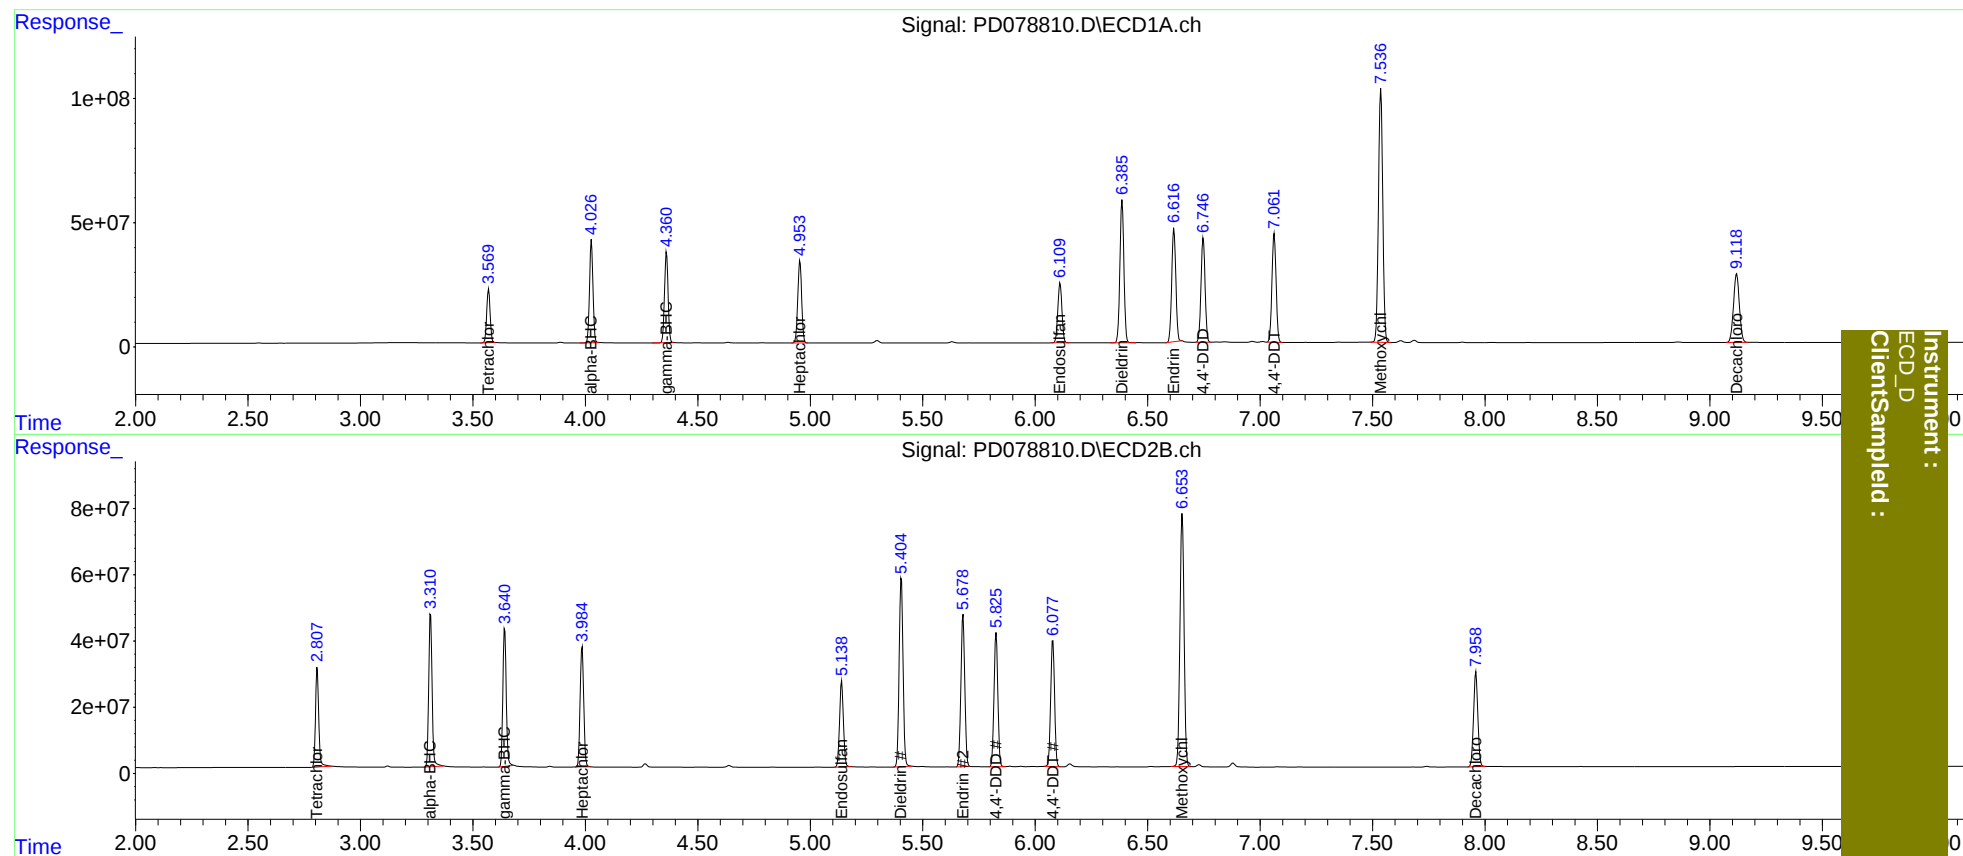


Instrument :
ECD_D
ClientSampled :
0

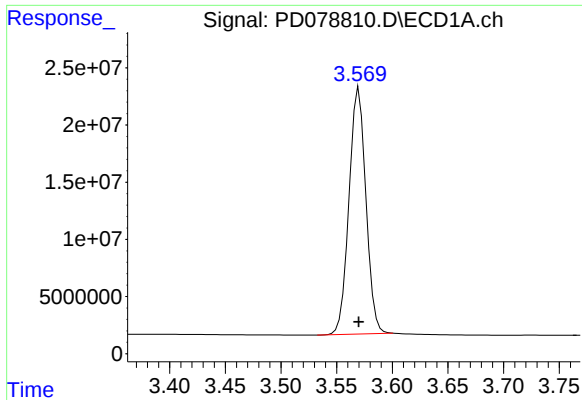

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 227826939
Conc: 149.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

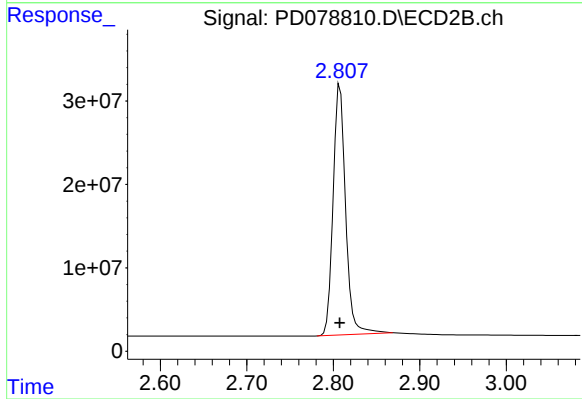


#1 Tetrachloro-m-xylene

R.T.: 2.808 min
Delta R.T.: 0.000 min
Response: 301890710
Conc: 156.75 ng/ml

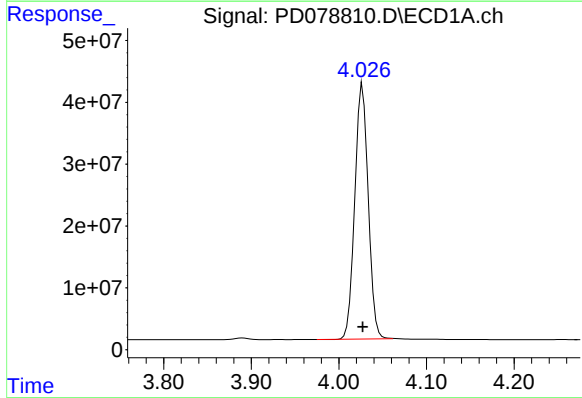


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.000 min
Response: 439802042
Conc: 172.19 ng/ml

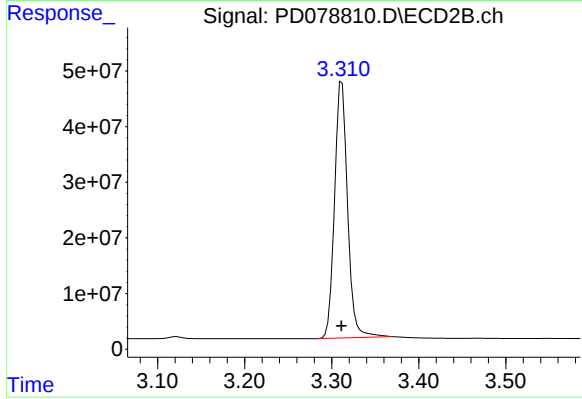

#2 alpha-BHC


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 480591541
Conc: 178.17 ng/ml

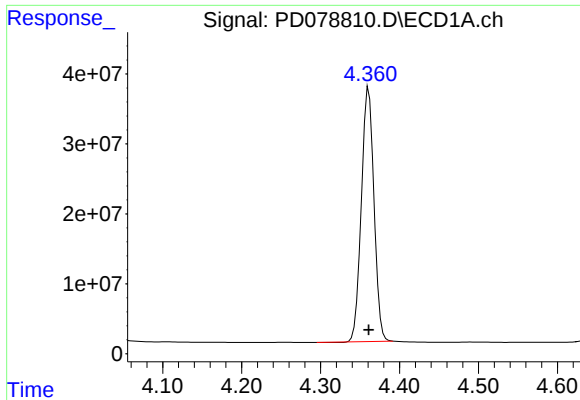

#3 gamma-BHC (Lindane)


R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 401741398
Conc: 164.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

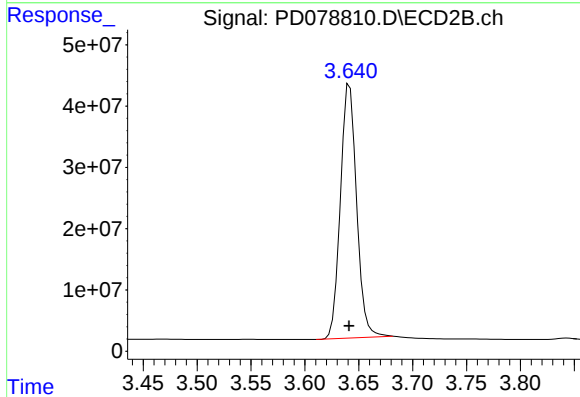


#3 gamma-BHC (Lindane)

R.T.: 3.642 min
Delta R.T.: 0.000 min
Response: 434491303
Conc: 173.98 ng/ml

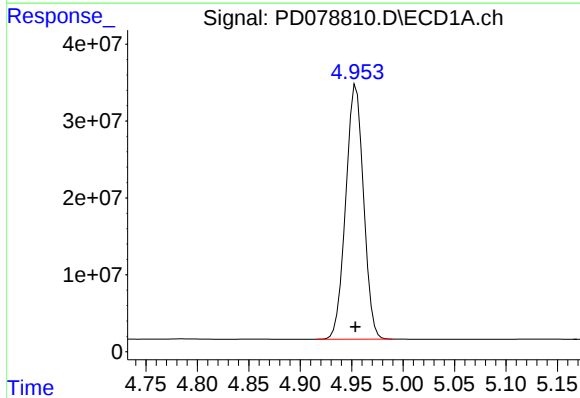


#4 Heptachlor

R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 399268344
Conc: 151.23 ng/ml

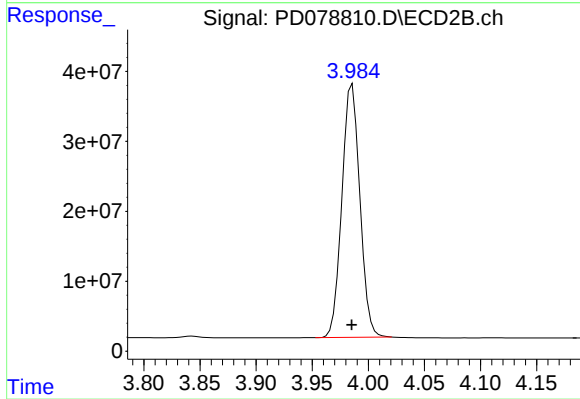

#4 Heptachlor


R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 403566806
Conc: 166.55 ng/ml

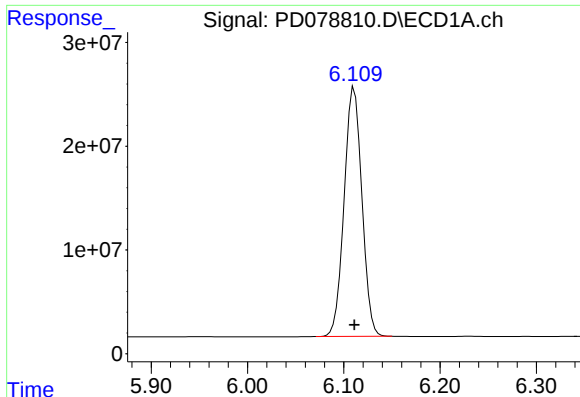

#9 Endosulfan I


R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 307133663
Conc: 147.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

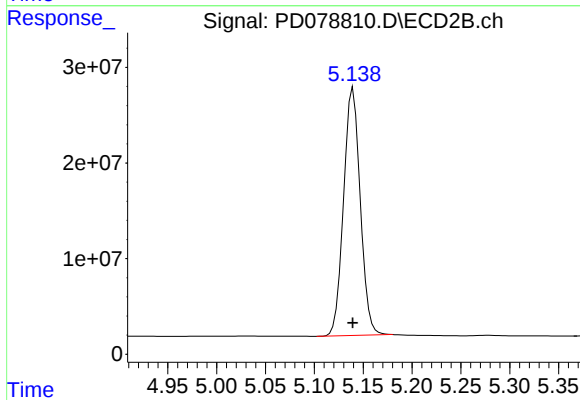


#9 Endosulfan I

R.T.: 5.140 min
Delta R.T.: 0.000 min
Response: 307643650
Conc: 155.97 ng/ml

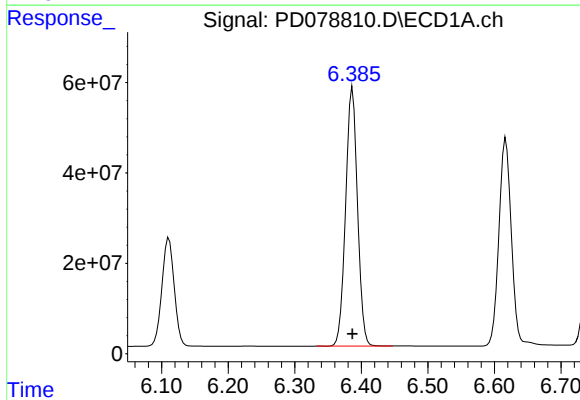


#13 Dieldrin

R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 710131632
Conc: 319.67 ng/ml

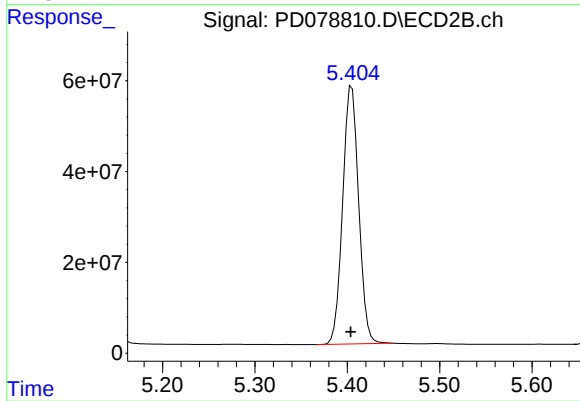

#13 Dieldrin


R.T.: 5.405 min
Delta R.T.: 0.001 min
Response: 684394468
Conc: 326.06 ng/ml

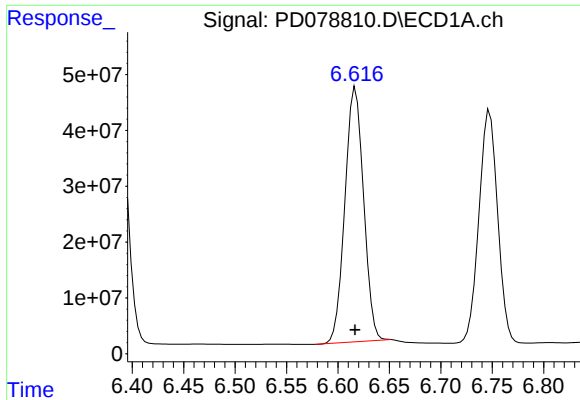

#14 Endrin


R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 577016926
Conc: 319.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

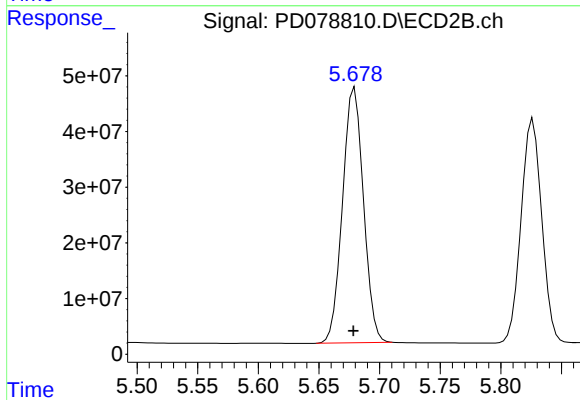


#14 Endrin

R.T.: 5.679 min
Delta R.T.: 0.000 min
Response: 551437844
Conc: 318.25 ng/ml

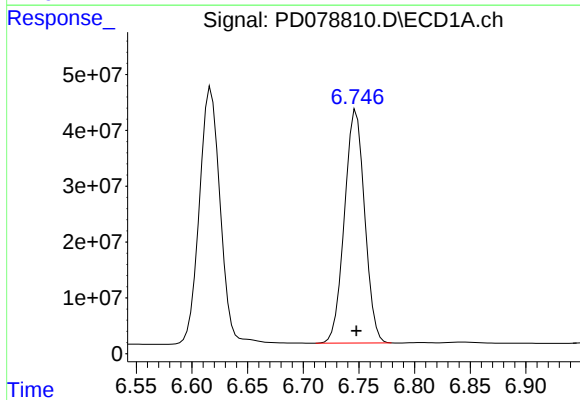


#16 4,4'-DDD

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 527511644
Conc: 324.51 ng/ml

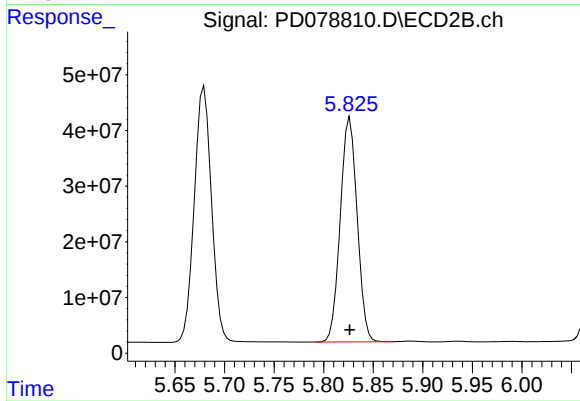

#16 4,4'-DDD


R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 477753985
Conc: 323.33 ng/ml

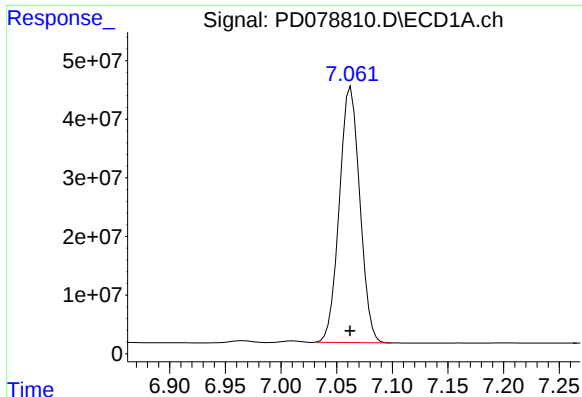

#17 4,4'-DDT


R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 558260181
Conc: 322.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

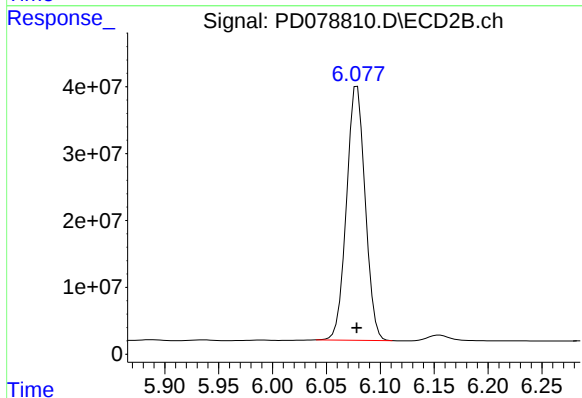


#17 4,4'-DDT

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 458075121
Conc: 321.71 ng/ml

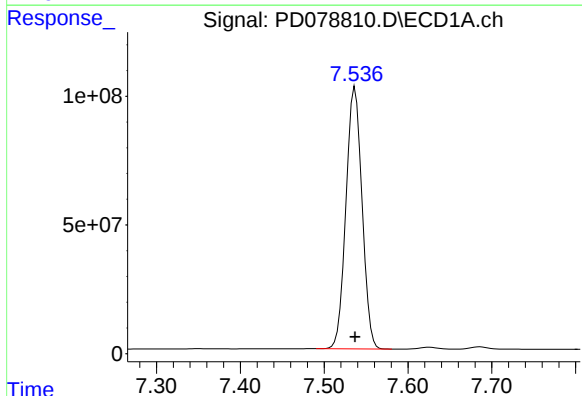


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 1359106758
Conc: 1456.59 ng/ml

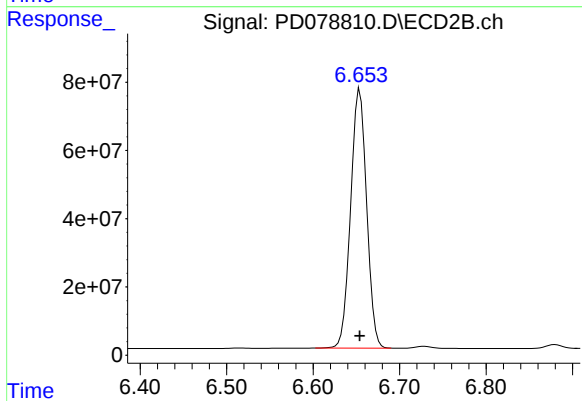

#20 Methoxychlor

R.T.: 6.654 min
Delta R.T.: 0.000 min
Response: 974525660
Conc: 1248.67 ng/ml

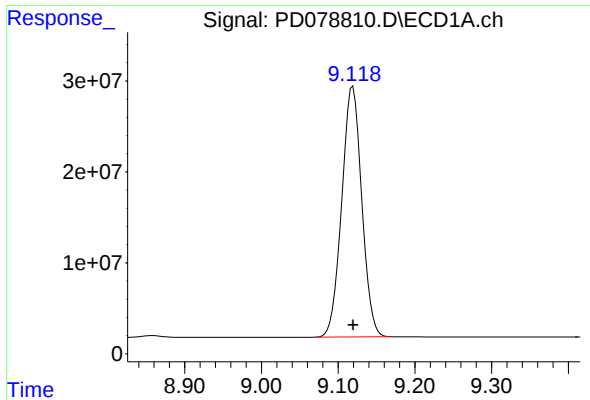

#27 Decachlorobiphenyl


R.T.: 9.119 min

Delta R.T.: 0.000 min

Response: 501072071

Conc: 290.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

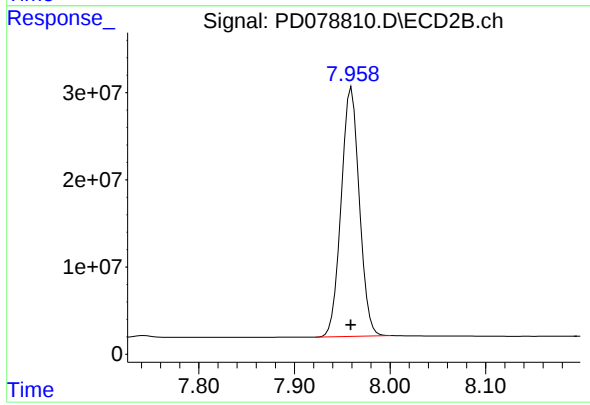

#27 Decachlorobiphenyl

R.T.: 7.960 min

Delta R.T.: 0.000 min

Response: 377951516

Conc: 273.30 ng/ml