

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
 Data File : PD078811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 02:01
 Operator : AR\AJ
 Sample : INDB601
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 04:57:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 04:54:10 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.808	238.9E6	314.3E6	151.730	155.364
27)	SA Decachlor...	9.121	7.959	523.4E6	389.2E6	289.406	267.358
Target Compounds							
5)	MB Aldrin	5.298	4.267	390.6E6	415.8E6	157.606	165.342
6)	B beta-BHC	4.553	3.936	161.0E6	185.8E6	142.533	147.958
7)	B delta-BHC	4.803	4.167	469.4E6	467.6E6	179.068	173.476
8)	B Heptachlo...	5.724	4.769	349.3E6	367.3E6	150.604	156.301
10)	B trans-Chl...	5.980	5.019	346.7E6	356.1E6	156.495	162.284
11)	B cis-Chlor...	6.060	5.084	344.9E6	359.8E6	152.332	158.291
12)	B 4,4'-DDE	6.231	5.273	687.0E6	657.5E6	331.337	335.434
15)	B Endosulfa...	6.834	5.972	619.3E6	477.3E6	320.241	282.703
18)	B Endrin al...	6.965	6.151	448.1E6	373.1E6	314.091	300.055
19)	B Endosulfa...	7.199	6.373	574.0E6	446.4E6	302.795	286.701
21)	B Endrin ke...	7.686	6.879	618.0E6	500.0E6	301.299	276.986


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 02:01
Operator : AR\AJ
Sample : INDB601
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 04:57:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 04:54:10 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

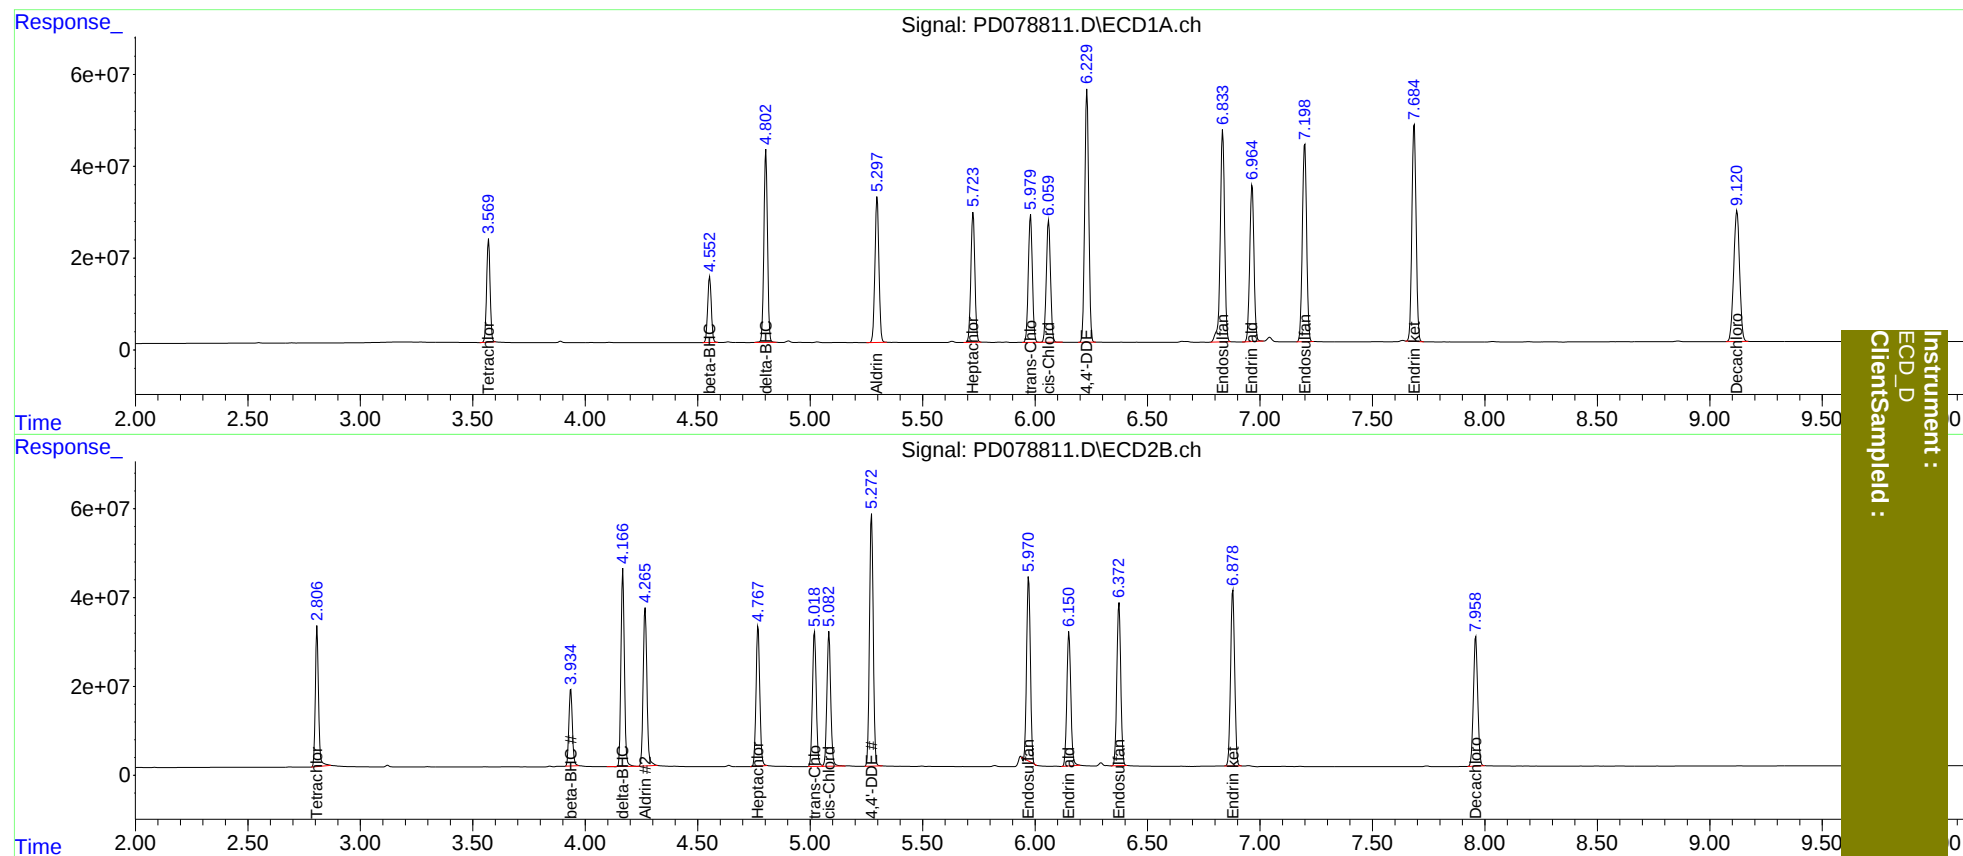


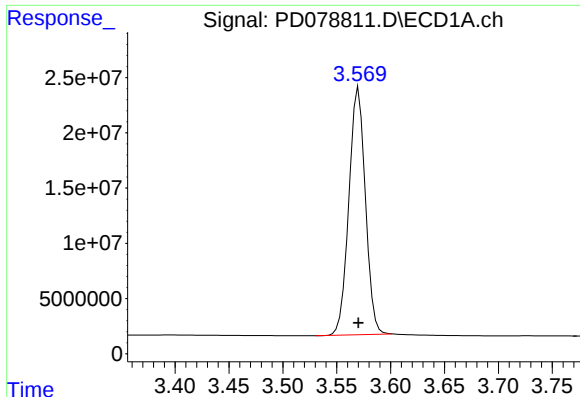

#1 Tetrachloro-m-xylene


R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 238909263
Conc: 151.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

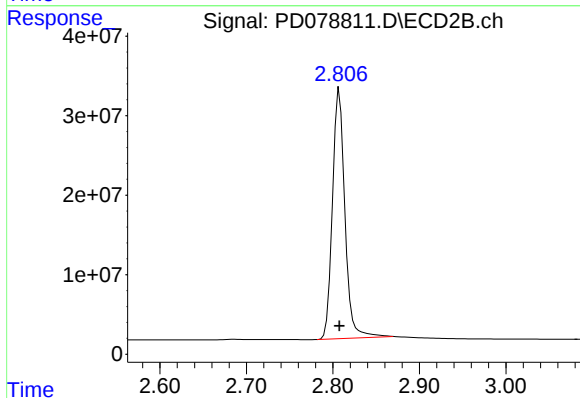


#1 Tetrachloro-m-xylene

R.T.: 2.808 min
Delta R.T.: 0.000 min
Response: 314267584
Conc: 155.36 ng/ml

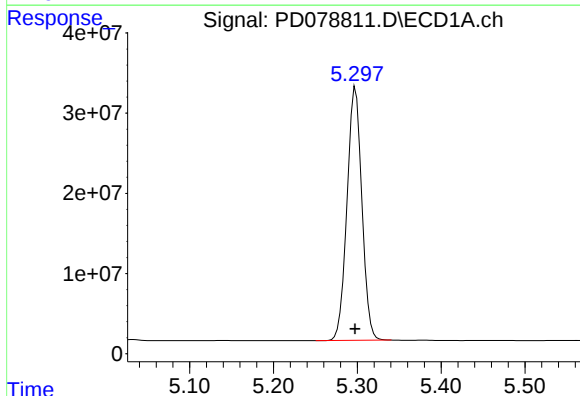


#5 Aldrin

R.T.: 5.298 min
Delta R.T.: 0.000 min
Response: 390575343
Conc: 157.61 ng/ml

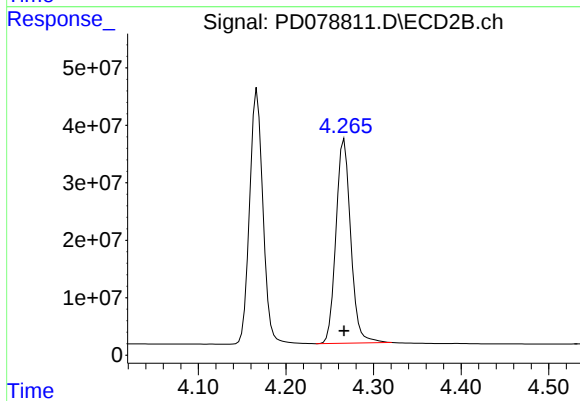

#5 Aldrin


R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 415770365
Conc: 165.34 ng/ml

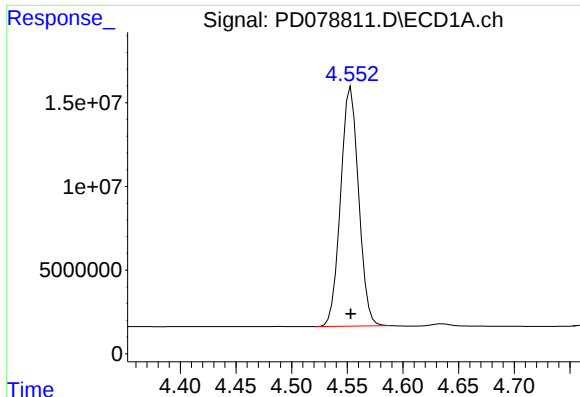

#6 beta-BHC


R.T.: 4.553 min
Delta R.T.: 0.000 min
Response: 161013686
Conc: 142.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

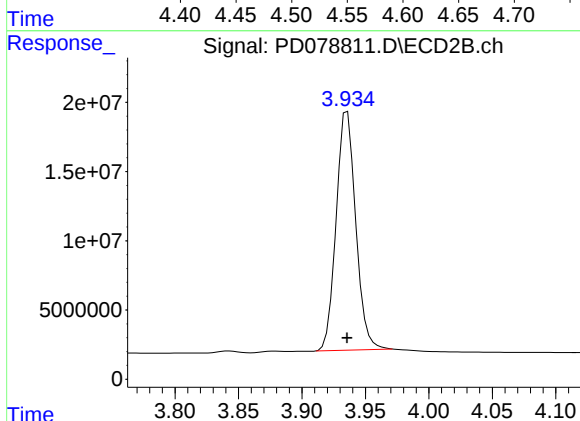


#6 beta-BHC

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 185769200
Conc: 147.96 ng/ml

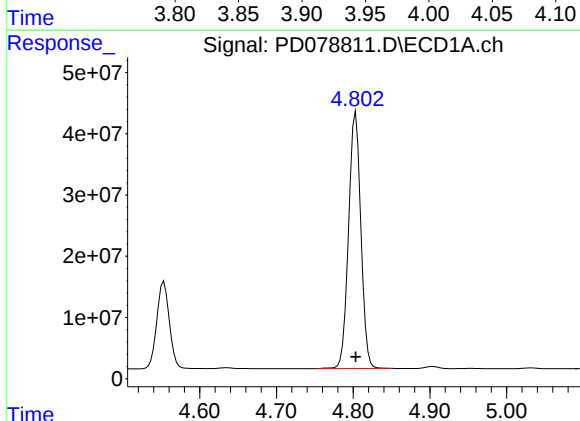


#7 delta-BHC

R.T.: 4.803 min
Delta R.T.: 0.000 min
Response: 469429697
Conc: 179.07 ng/ml

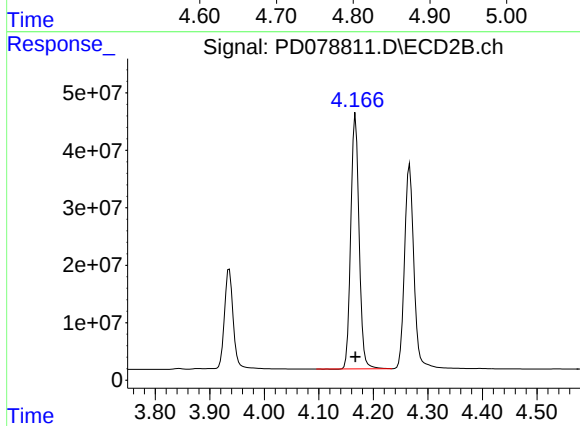

#7 delta-BHC


R.T.: 4.167 min
Delta R.T.: 0.000 min
Response: 467607028
Conc: 173.48 ng/ml

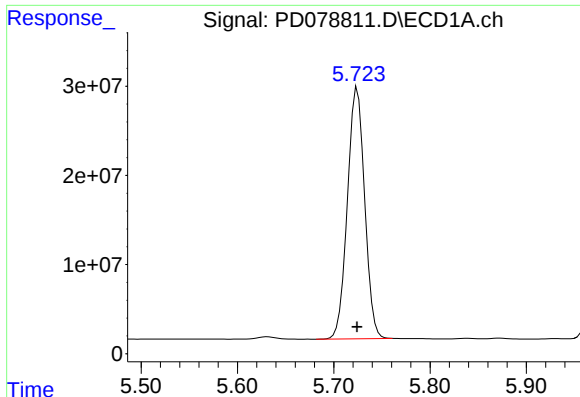

#8 Heptachlor epoxide


R.T.: 5.724 min
Delta R.T.: 0.000 min
Response: 349277167
Conc: 150.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

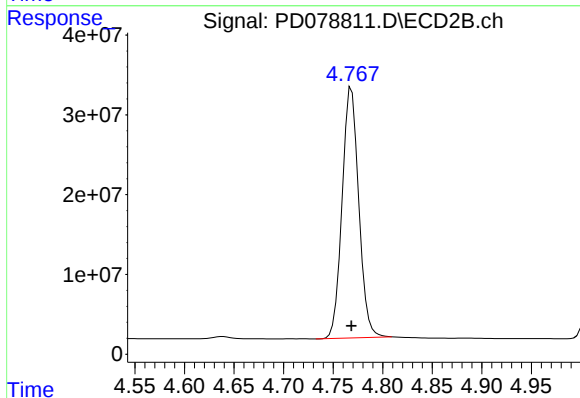


#8 Heptachlor epoxide

R.T.: 4.769 min
Delta R.T.: 0.000 min
Response: 367306005
Conc: 156.30 ng/ml

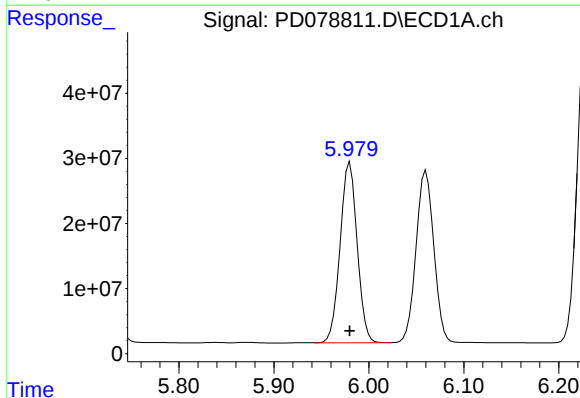


#10 trans-Chlordane

R.T.: 5.980 min
Delta R.T.: 0.000 min
Response: 346703596
Conc: 156.50 ng/ml

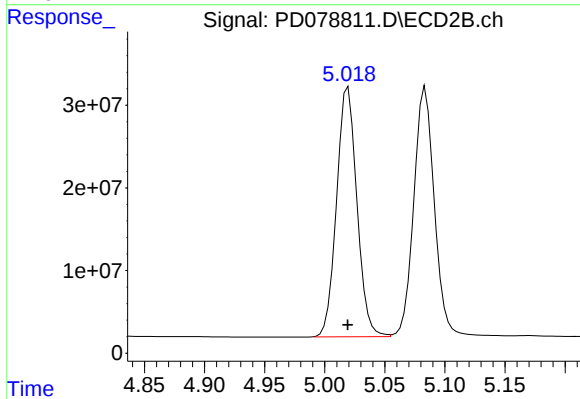

#10 trans-Chlordane


R.T.: 5.019 min
Delta R.T.: 0.000 min
Response: 356093443
Conc: 162.28 ng/ml

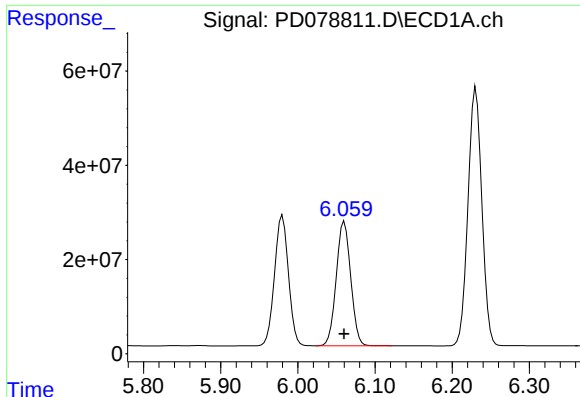

#11 cis-Chlordane


R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 344868896
Conc: 152.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

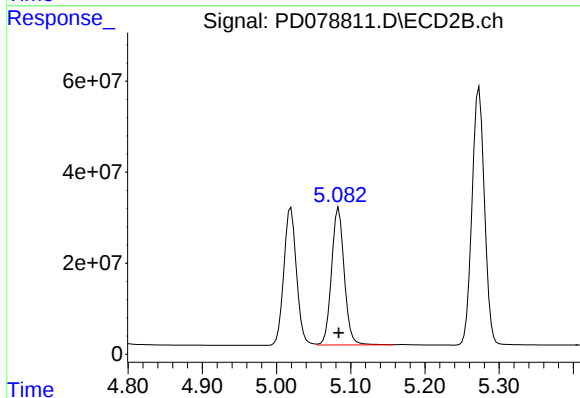


#11 cis-Chlordane

R.T.: 5.084 min
Delta R.T.: 0.000 min
Response: 359773024
Conc: 158.29 ng/ml

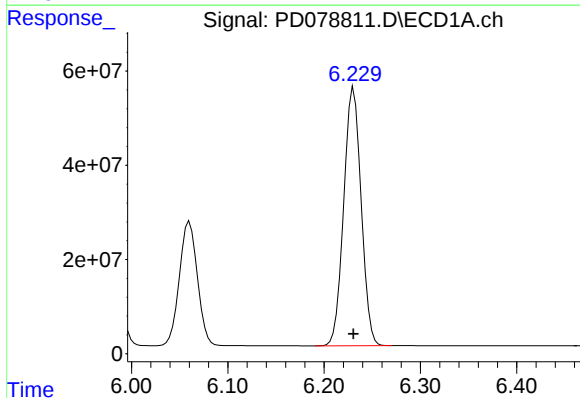


#12 4,4'-DDE

R.T.: 6.231 min
Delta R.T.: 0.000 min
Response: 687001192
Conc: 331.34 ng/ml

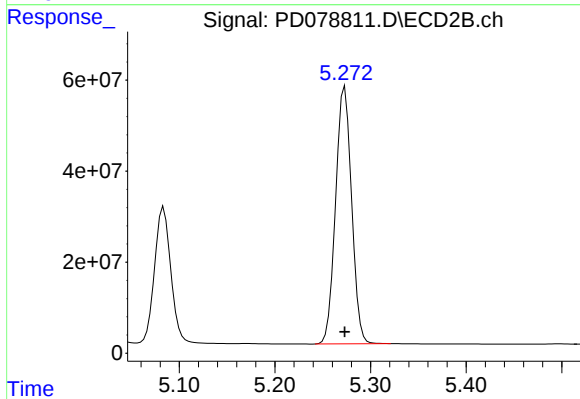

#12 4,4'-DDE


R.T.: 5.273 min
Delta R.T.: 0.000 min
Response: 657481743
Conc: 335.43 ng/ml

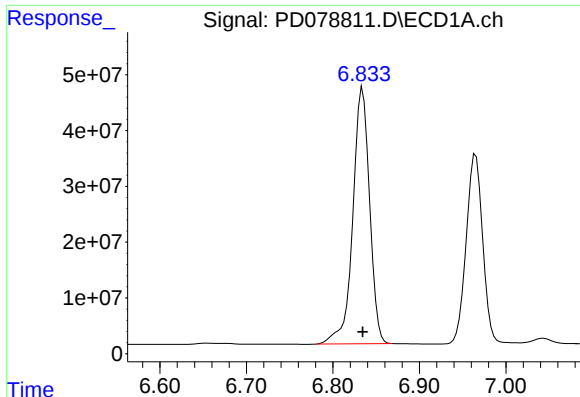

#15 Endosulfan II


R.T.: 6.834 min
Delta R.T.: 0.000 min
Response: 619278287
Conc: 320.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

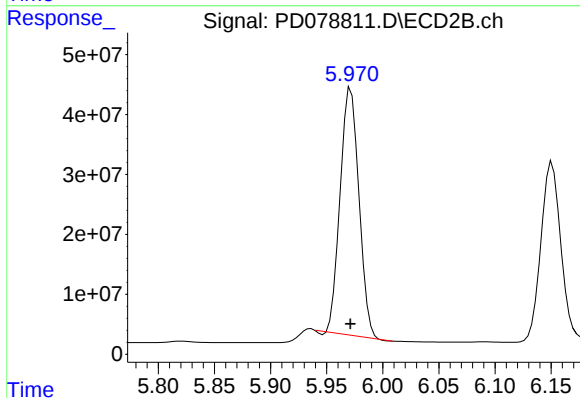


#15 Endosulfan II

R.T.: 5.972 min
Delta R.T.: 0.000 min
Response: 477345401
Conc: 282.70 ng/ml

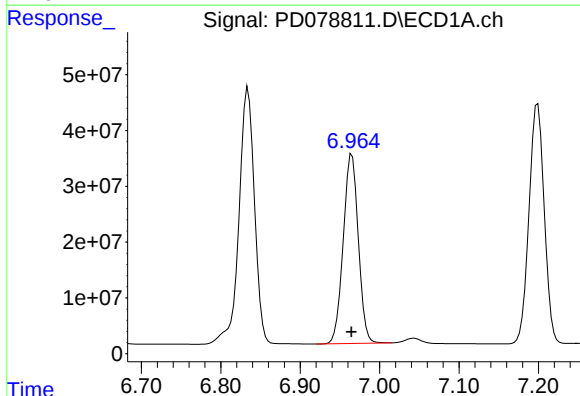


#18 Endrin aldehyde

R.T.: 6.965 min
Delta R.T.: 0.000 min
Response: 448119841
Conc: 314.09 ng/ml

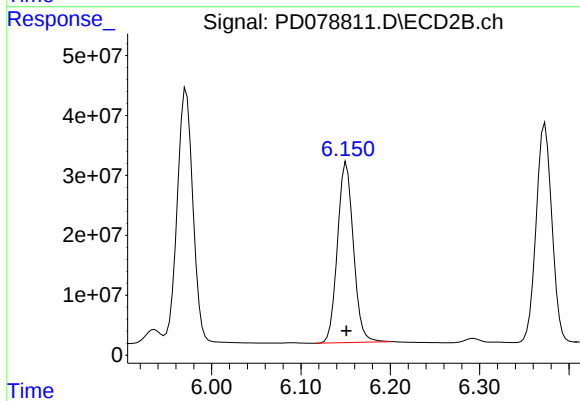

#18 Endrin aldehyde


R.T.: 6.151 min
Delta R.T.: 0.000 min
Response: 373064470
Conc: 300.06 ng/ml

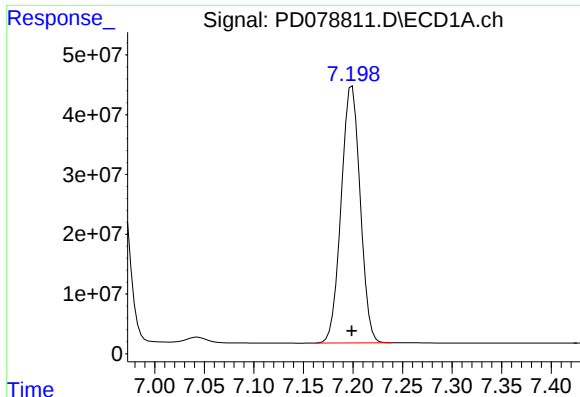

#19 Endosulfan Sulfate


R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 574026113
Conc: 302.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

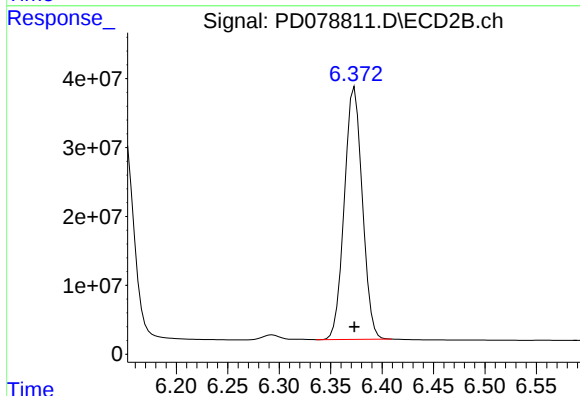


#19 Endosulfan Sulfate

R.T.: 6.373 min
Delta R.T.: 0.000 min
Response: 446414986
Conc: 286.70 ng/ml

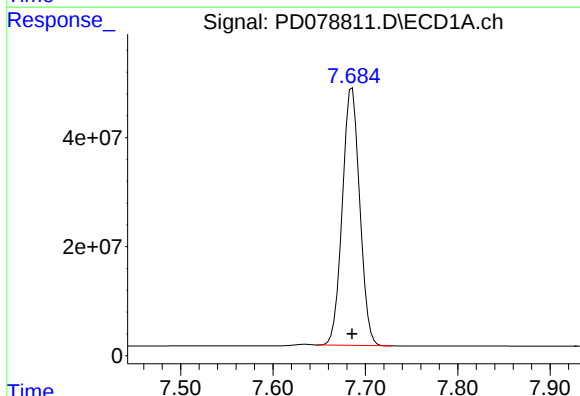


#21 Endrin ketone

R.T.: 7.686 min
Delta R.T.: 0.000 min
Response: 618009482
Conc: 301.30 ng/ml

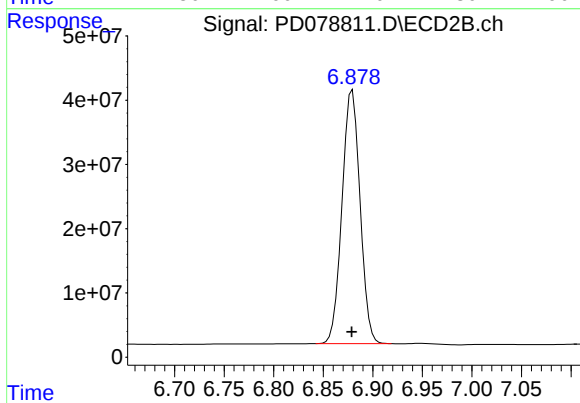

#21 Endrin ketone

R.T.: 6.879 min
Delta R.T.: 0.000 min
Response: 500012968
Conc: 276.99 ng/ml

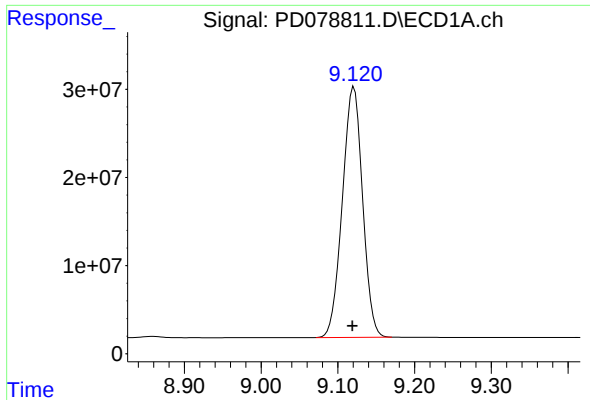

#27 Decachlorobiphenyl


R.T.: 9.121 min

Delta R.T.: 0.002 min

Response: 523414981

Conc: 289.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

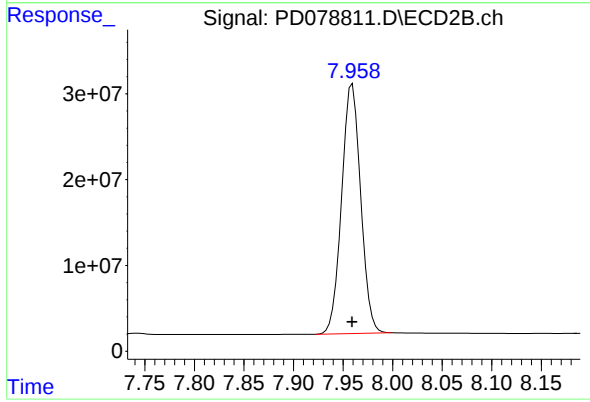

#27 Decachlorobiphenyl

R.T.: 7.959 min

Delta R.T.: 0.000 min

Response: 389243397

Conc: 267.36 ng/ml