

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
 Data File : PD078792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2023 21:48
 Operator : AR\AJ
 Sample : RESC010
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC010

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 06:08:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 05:55:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.807	30575718	37068613	20.186	18.996
27)	SA Decachlor...	9.120	7.959	67302103	54007125	39.430	39.944
Target Compounds							
2)	A alpha-BHC	4.027	3.310	24588706	24620166	9.362	8.769
3)	MA gamma-BHC...	4.361	3.640	23543784	22976372	9.525	8.959
4)	MA Heptachlor	4.954	3.984	25319450	22303996	9.635	9.032
5)	MB Aldrin	5.298	4.266	25385924	23948009	10.117	9.392
6)	B beta-BHC	4.553	3.935	11757192	12120098	10.419	9.733
7)	B delta-BHC	4.803	4.166	25959046	24667884	9.556	8.941
8)	B Heptachlo...	5.724	4.768	23397558	22123559	10.034	9.342
9)	A Endosulfan I	6.110	5.138	20730562	18424918	9.984	9.337
10)	B trans-Chl...	5.980	5.019	22281687	20659241	9.909	9.228
11)	B cis-Chlor...	6.060	5.083	22741580	21101120	9.980	9.157
12)	B 4,4'-DDE	6.230	5.273	39347883	36269936	18.659	18.128
13)	MA Dieldrin	6.387	5.404	42728287	38993494	19.054	18.368
14)	MA Endrin	6.616	5.678	34917116	33150764	19.225	19.067
15)	B Endosulfa...	6.834	5.971	38823708	33537798	19.912	19.944
16)	A 4,4'-DDD	6.747	5.826	31079292	28901797	18.940	19.398
17)	MA 4,4'-DDT	7.063	6.078	32939876	28266638	18.947	19.659
18)	B Endrin al...	6.964	6.151	28029529	26380851	19.281	21.141
19)	B Endosulfa...	7.198	6.373	38017476	32502238	19.964	21.125
20)	A Methoxychlor	7.537	6.653	91513308	79671057	98.813	106.070
21)	B Endrin ke...	7.686	6.879	41037053	36426737	19.989	20.636

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 21:48
Operator : AR\AJ
Sample : RESC010
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 06:08:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:55:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

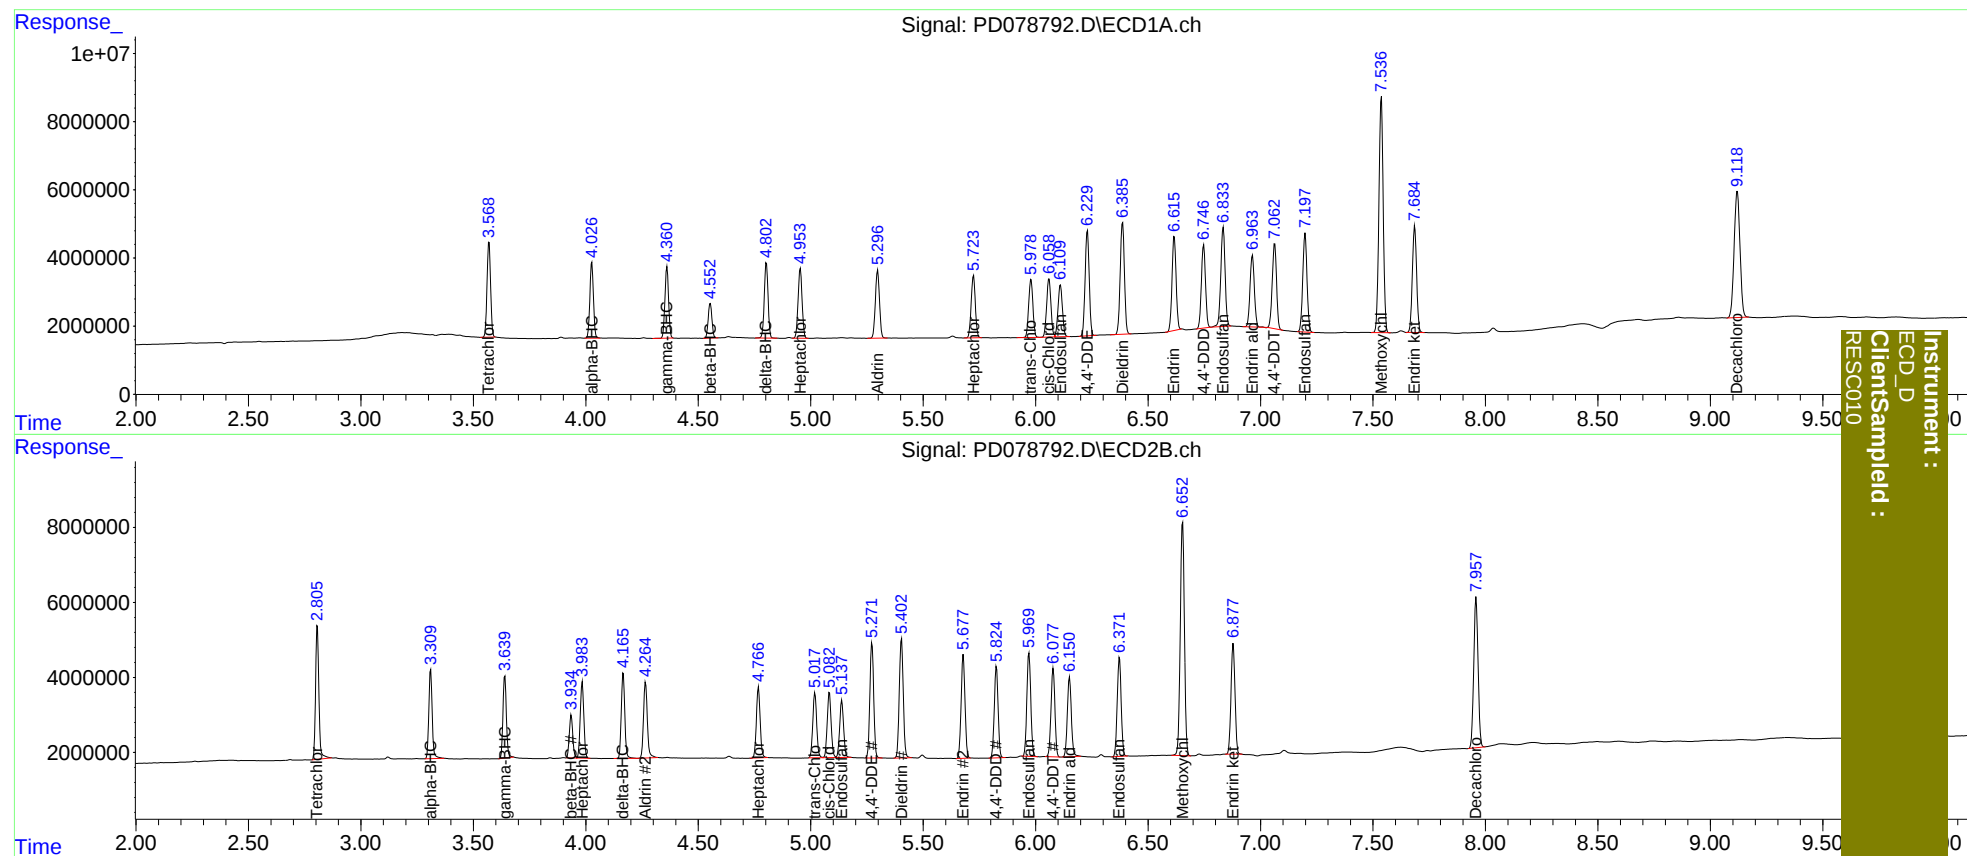

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078792.D
Acq On : 10 Oct 2023 21:48
Operator : AR\AJ
Sample : RESC010
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Title : GC Extractables
Last Update : Wed Oct 11 05:55:02 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.570	4.027	100.00%
4.027	4.361	100.00%
4.361	4.553	100.00%
4.553	4.803	100.00%
4.803	4.954	100.00%
4.954	5.298	100.00%
5.298	5.724	100.00%
5.724	5.980	100.00%
5.980	6.060	99.73%
6.060	6.110	97.13%
6.110	6.230	100.00%
6.230	6.387	100.00%
6.387	6.616	100.00%
6.616	6.747	100.00%
6.747	6.834	100.00%
6.834	6.964	100.00%
6.964	7.063	100.00%
7.063	7.198	100.00%
7.198	7.537	100.00%
7.537	7.686	100.00%
7.686	9.120	100.00%

Signal #2


2.807	3.310	100.00%
3.310	3.640	100.00%
3.640	3.935	100.00%
3.935	3.984	99.65%
3.984	4.166	100.00%
4.166	4.266	100.00%
4.266	4.768	100.00%
4.768	5.019	100.00%
5.019	5.083	100.00%
5.083	5.138	100.00%
5.138	5.273	100.00%
5.273	5.404	100.00%
5.404	5.678	100.00%
5.678	5.826	100.00%
5.826	5.971	100.00%
5.971	6.078	100.00%
6.078	6.151	100.00%
6.151	6.373	100.00%
6.373	6.653	100.00%
6.653	6.879	100.00%
6.879	7.959	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 21:48
Operator : AR\AJ
Sample : RESC010
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 06:08:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:55:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

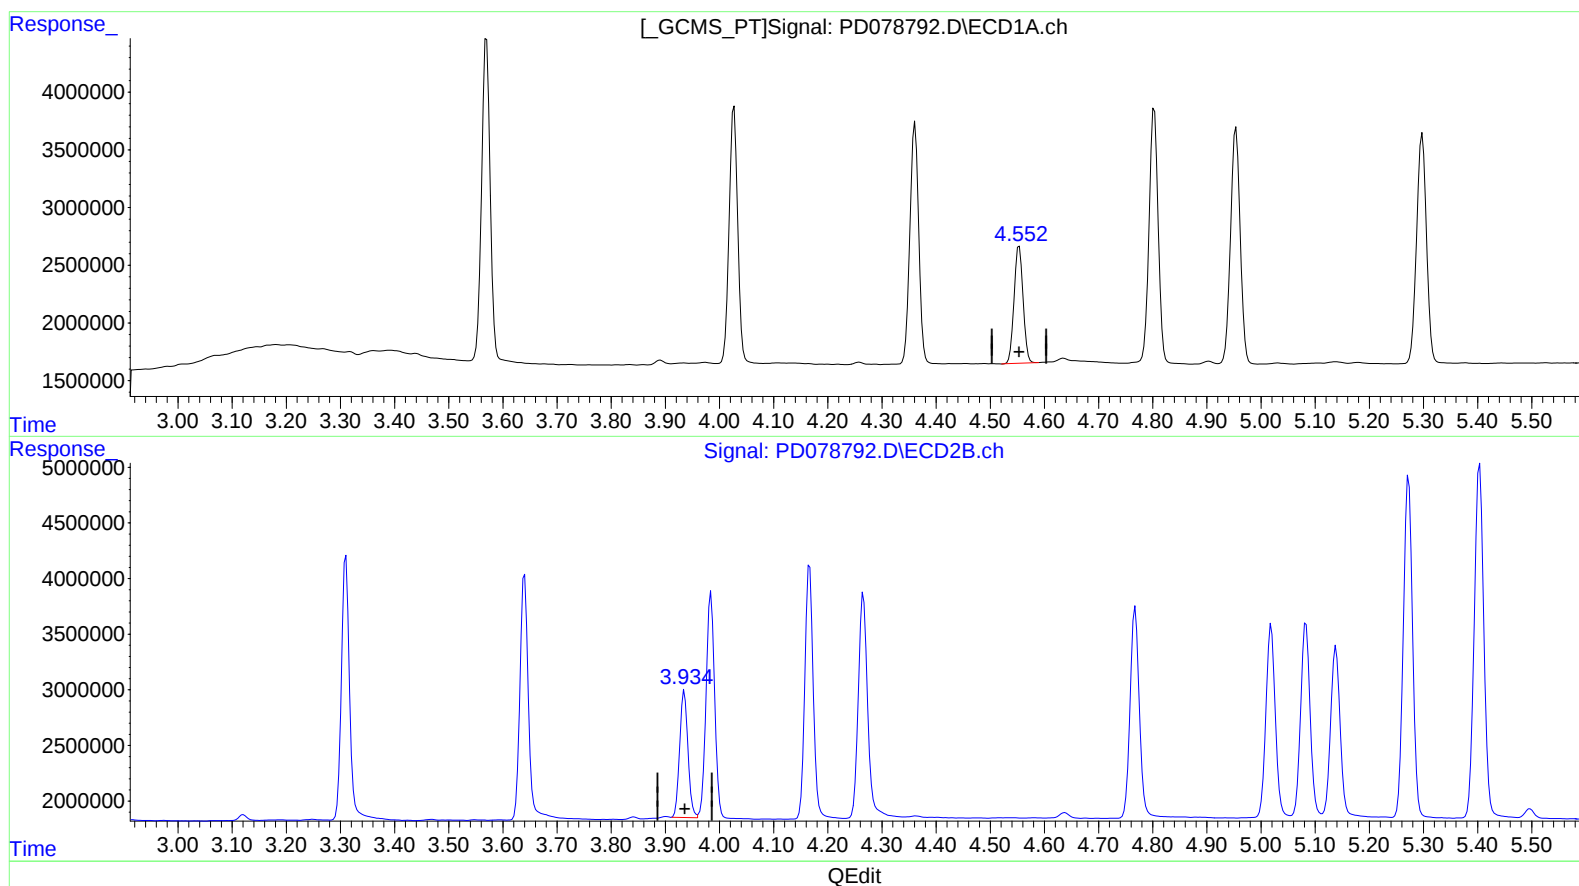

(6) beta-BHC (B)

4.553min 10.419 ng/ml

response 11757192

(6) beta-BHC #2 (B)

3.935min 9.733 ng/ml


response 12120098

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 21:48
Operator : AR\AJ
Sample : RESC010
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 06:08:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:55:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

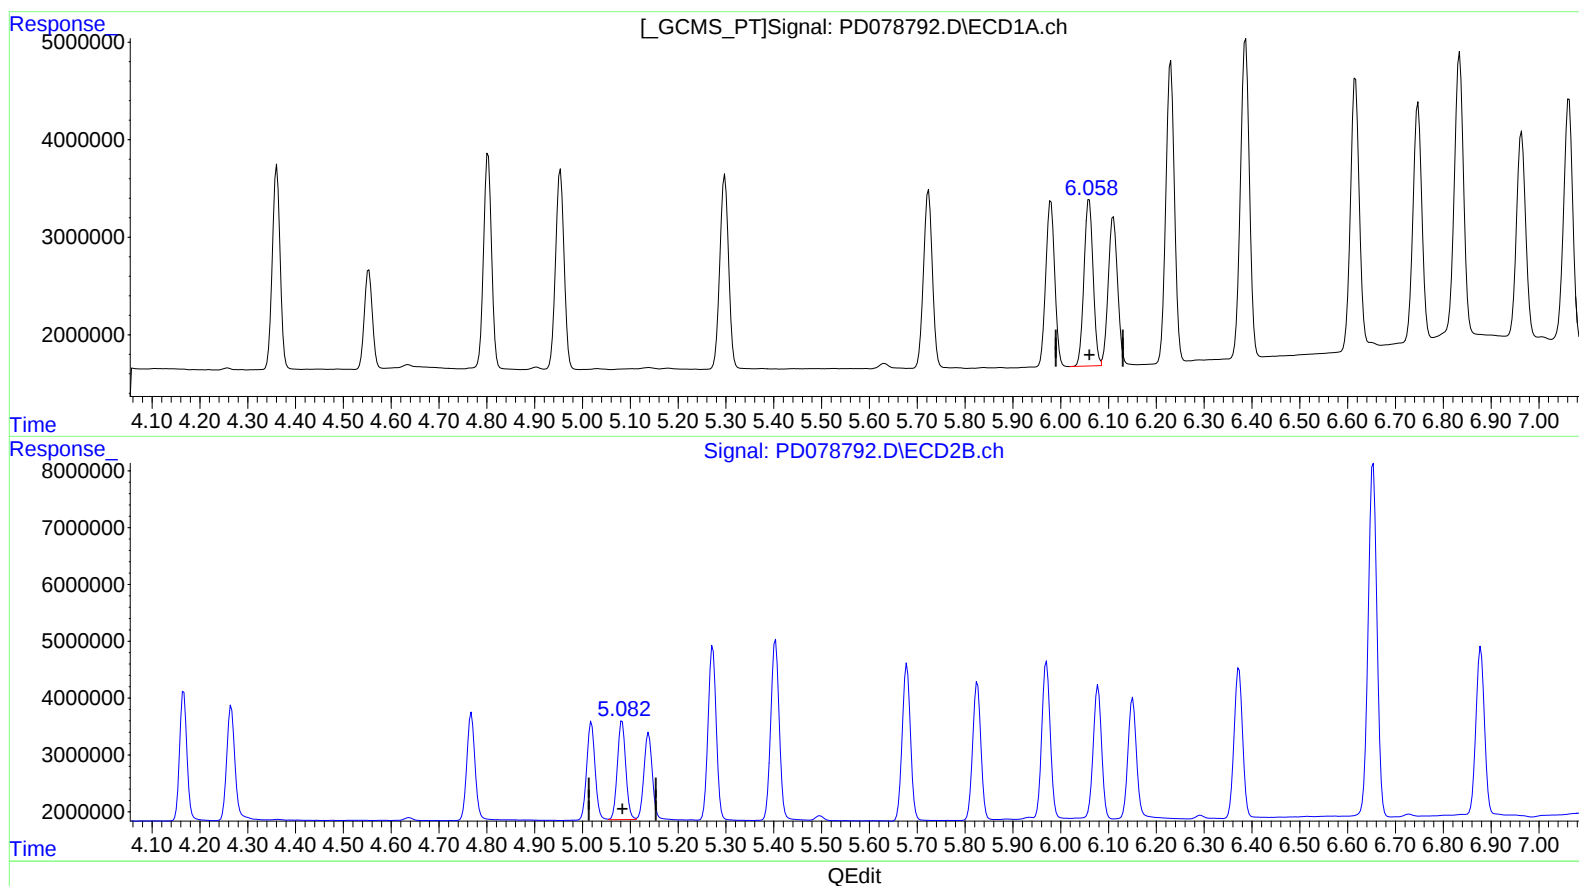

(11) cis-Chlordane (B)

6.060min 9.980 ng/ml

response 22741580

(11) cis-Chlordane #2 (B)

5.083min 9.157 ng/ml


response 21101120

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 21:48
Operator : AR\AJ
Sample : RESC010
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 06:08:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:55:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

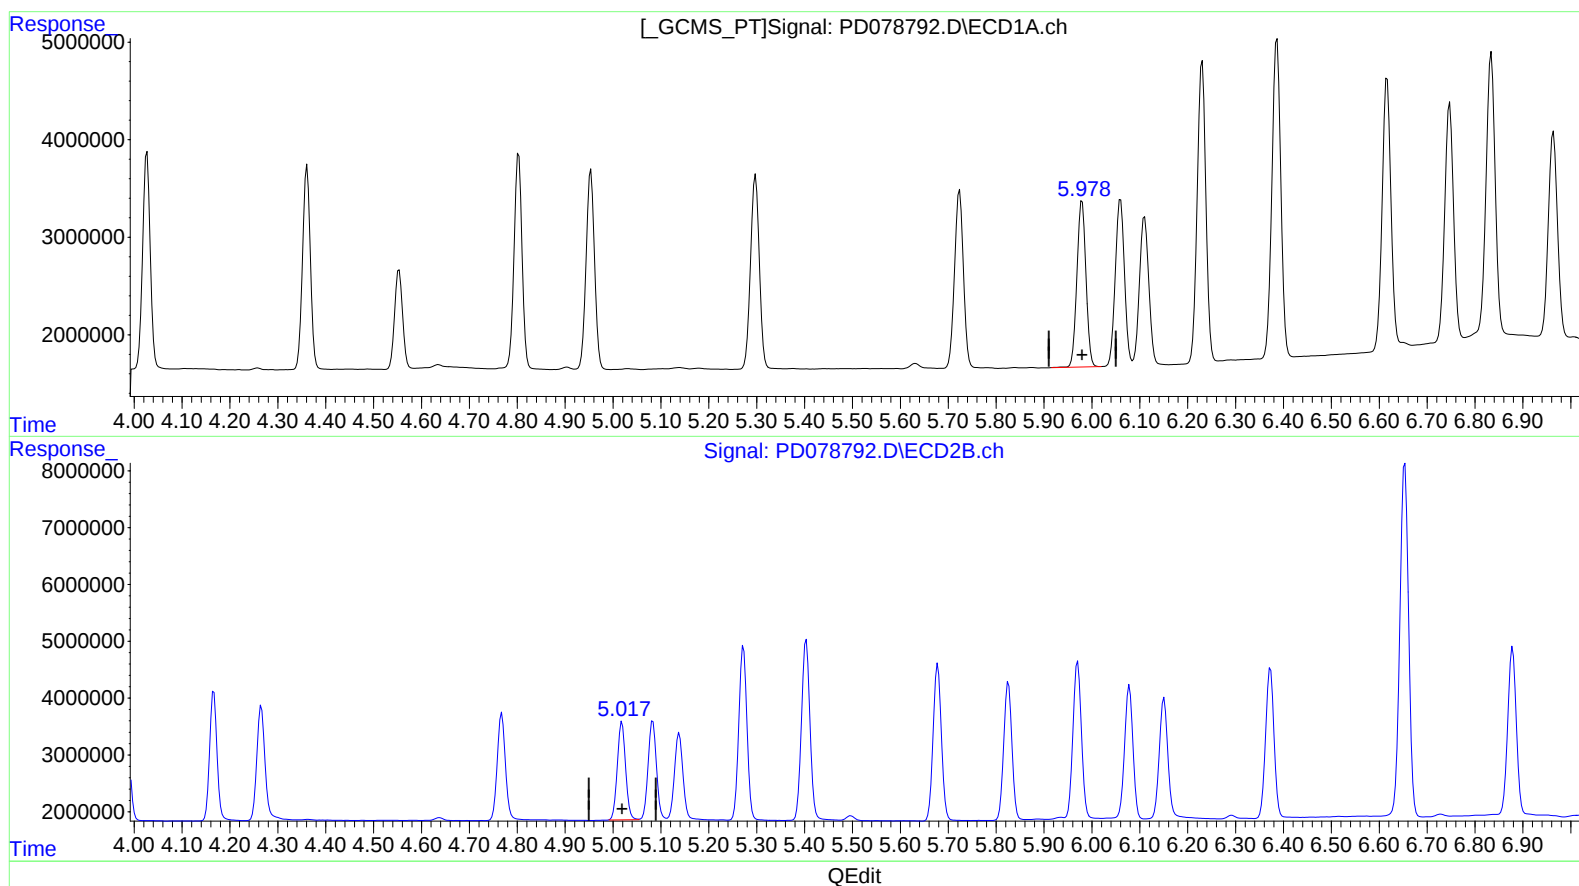

(10) trans-Chlordane (B)

5.980min 9.909 ng/ml

response 22281687

(10) trans-Chlordane #2 (B)

5.019min 9.228 ng/ml

response 20659241