

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
 Data File : PD078808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 01:21
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5028

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 05:45:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 05:45:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.807	117.3E6	153.5E6	76.536	78.157
27)	SA Decachlor...	9.119	7.959	255.1E6	197.5E6	147.016	142.454
Target Compounds							
2)	A alpha-BHC	4.027	3.311	218.7E6	238.9E6	84.067	86.287
3)	MA gamma-BHC...	4.360	3.641	201.7E6	215.7E6	81.855	85.091
4)	MA Heptachlor	4.953	3.985	215.5E6	202.9E6	81.174	82.500
9)	A Endosulfan I	6.110	5.139	159.7E6	155.8E6	75.745	78.537
13)	MA Dieldrin	6.387	5.404	363.8E6	348.1E6	161.872	164.223
14)	MA Endrin	6.617	5.679	292.0E6	279.5E6	160.564	160.443
16)	A 4,4'-DDD	6.747	5.826	267.0E6	240.3E6	162.834	161.365
17)	MA 4,4'-DDT	7.063	6.078	281.9E6	229.1E6	162.264	159.201
20)	A Methoxychlor	7.537	6.654	710.8E6	535.5E6	755.003	686.919

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 01:21
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 05:45:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:45:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

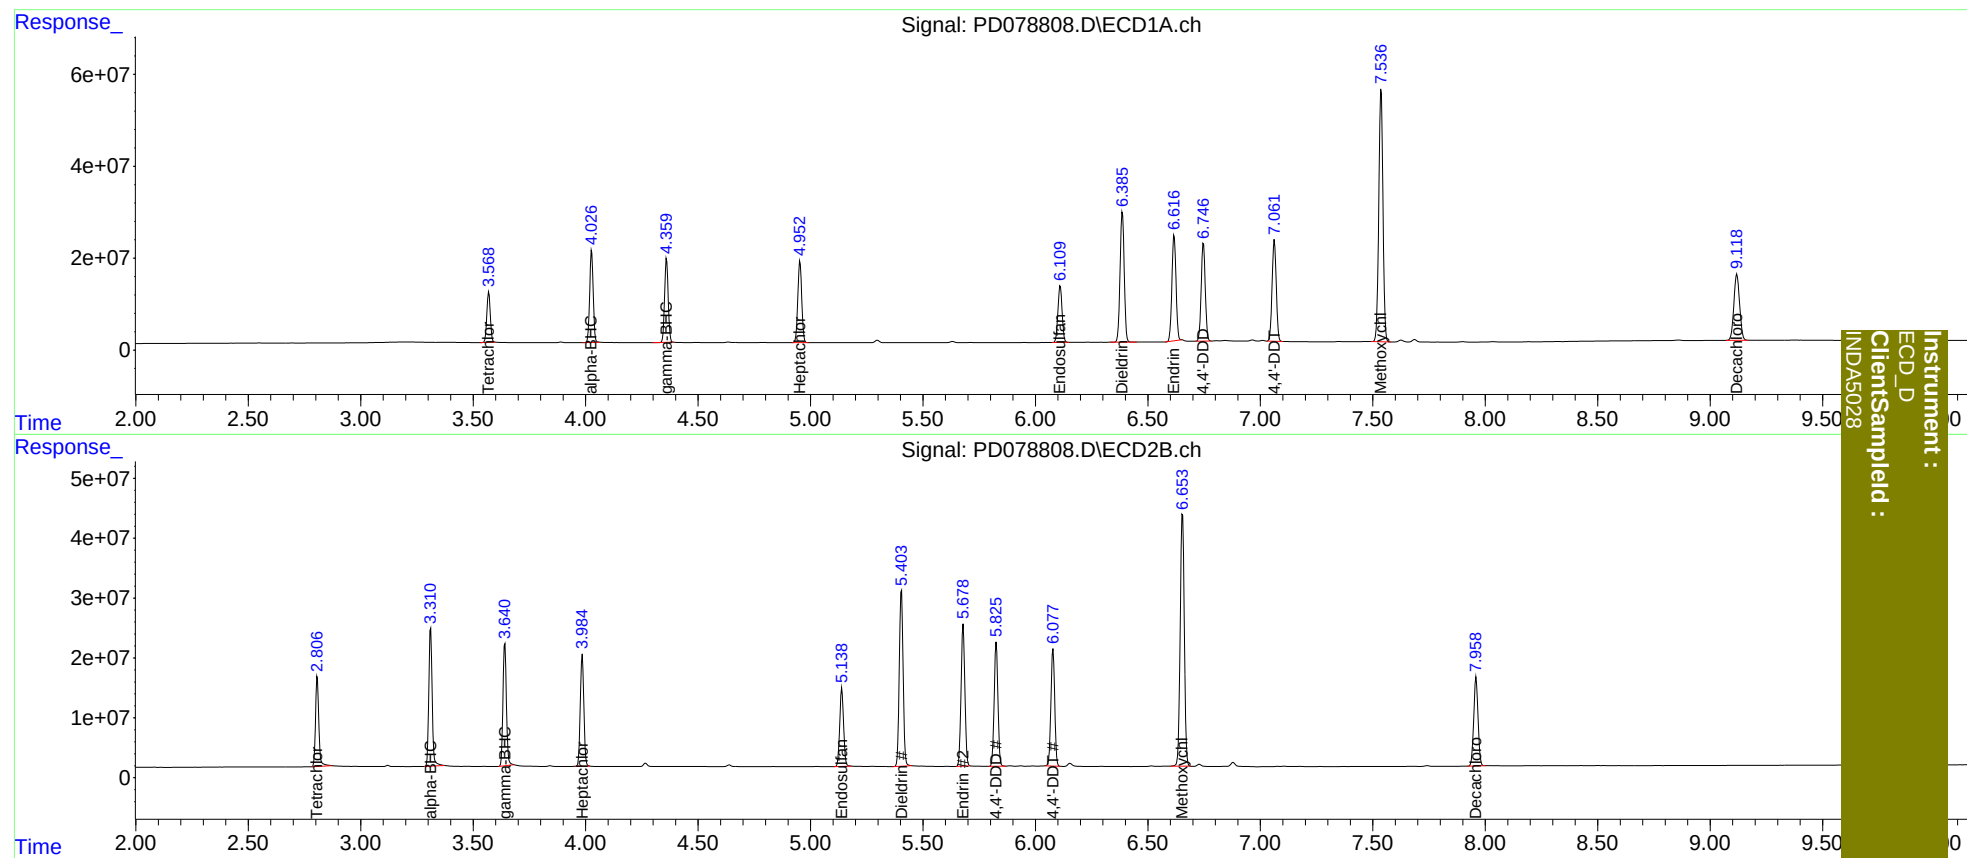

Instrument :
ECD_D
ClientSampled :
INDA5028