

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
 Data File : PD078810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2023 01:48
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA6030

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 05:47:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 11 05:47:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.808	227.8E6	301.9E6	150.413	154.708
27)	SA Decachlor...	9.119	7.960	501.1E6	378.0E6	293.563	279.538
Target Compounds							
2)	A alpha-BHC	4.027	3.312	439.8E6	480.6E6	167.453	171.167
3)	MA gamma-BHC...	4.361	3.642	401.7E6	434.5E6	162.535	169.416
4)	MA Heptachlor	4.954	3.986	399.3E6	403.6E6	151.931	163.419
9)	A Endosulfan I	6.111	5.140	307.1E6	307.6E6	147.916	155.907
13)	MA Dieldrin	6.387	5.405	710.1E6	684.4E6	316.666	322.393
14)	MA Endrin	6.617	5.679	577.0E6	551.4E6	317.703	317.161
16)	A 4,4'-DDD	6.748	5.827	527.5E6	477.8E6	321.473	320.649
17)	MA 4,4'-DDT	7.063	6.079	558.3E6	458.1E6	321.115	318.591
20)	A Methoxychlor	7.537	6.654	1359.1E6	974.5E6	1467.518	1297.436

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101123\
Data File : PD078810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2023 01:48
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 05:47:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101123CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 11 05:47:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

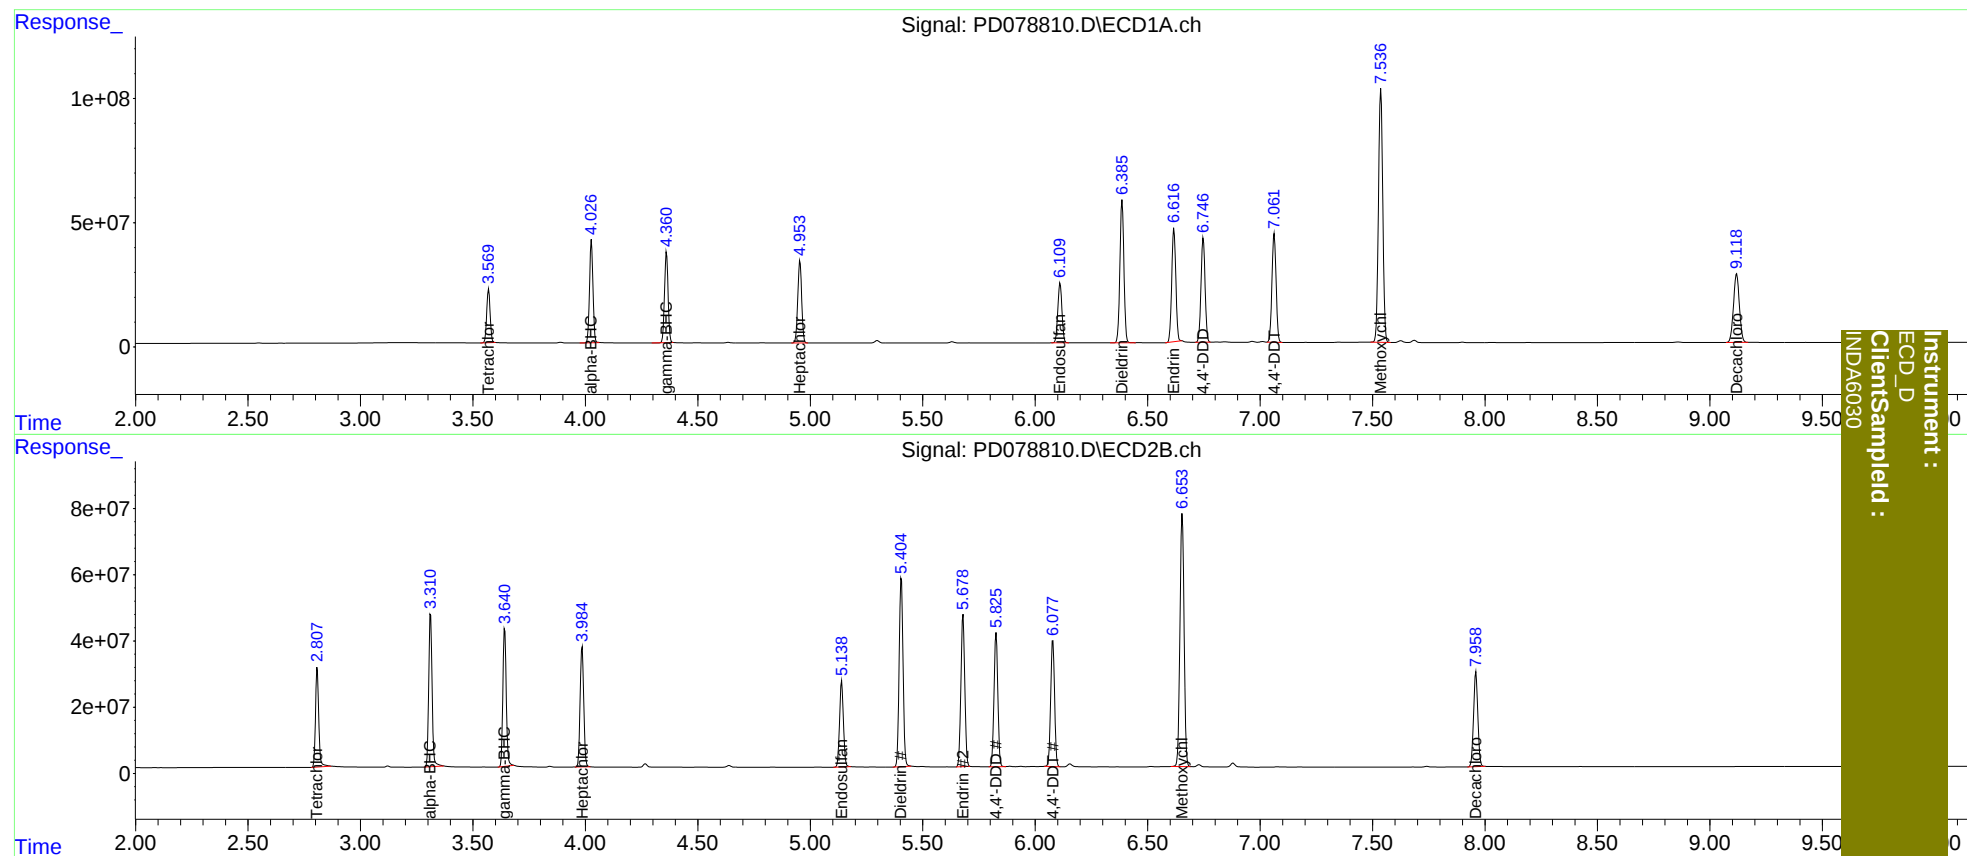

Instrument :
ECD_D
ClientSampled :
INDA6030