

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101124\
 Data File : PD085974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2024 12:36
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 13:51:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101124.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 11 13:43:09 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	2.876	84907420	497.8E6	74.085	74.080
28)	SA Decachlor...	8.897	8.057	149.0E6	369.5E6	74.184	73.971
Target Compounds							
23)	Chlordane-1	4.593	3.895	53535153	190.2E6	747.098	739.386
24)	Chlordane-2	5.117	4.475	57605356	205.7E6	741.003	741.139
25)	Chlordane-3	5.819	5.112	237.7E6	554.0E6	746.311	740.326
26)	Chlordane-4	5.904	5.176	288.8E6	494.2E6	746.217	739.799
27)	Chlordane-5	6.739	6.077	49883218	209.3E6	743.998	737.890



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101124\
Data File : PD085974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2024 12:36
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 13:51:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101124.M
Quant Title : GC Extractables
QLast Update : Fri Oct 11 13:43:09 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

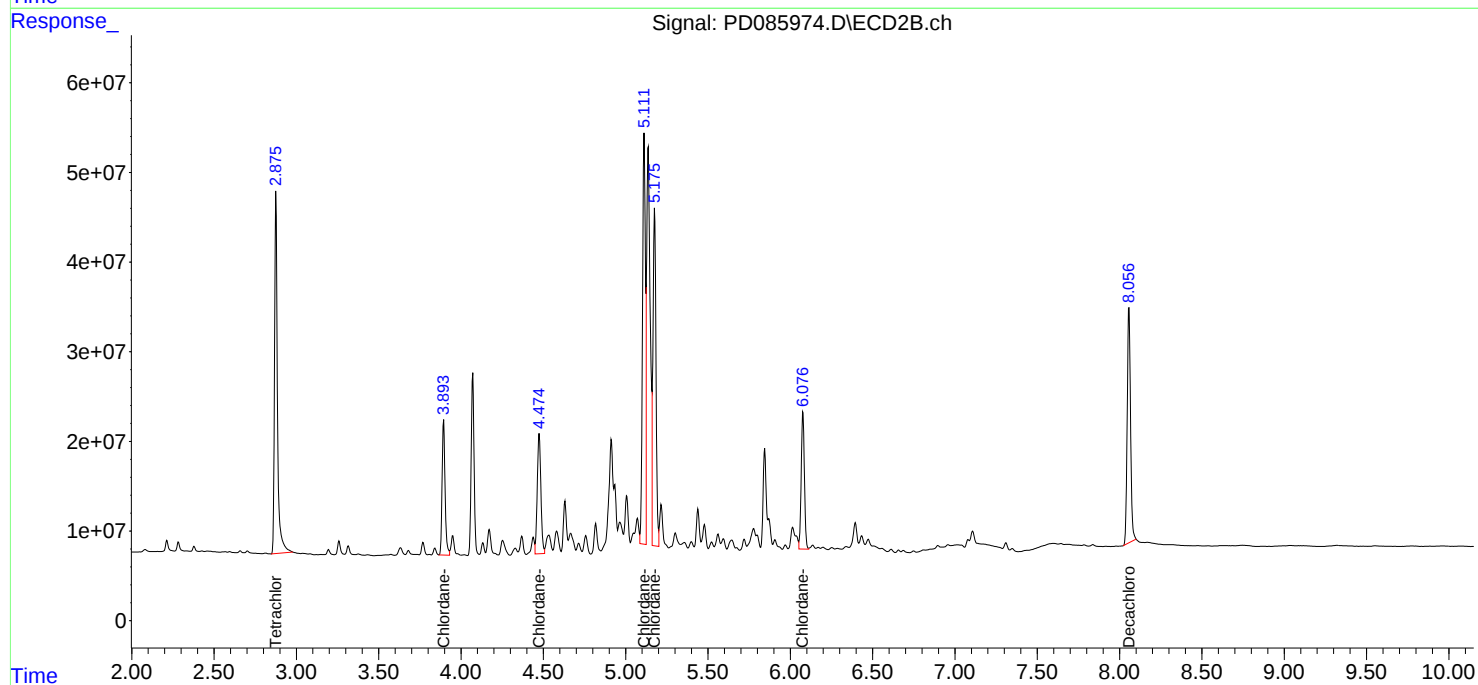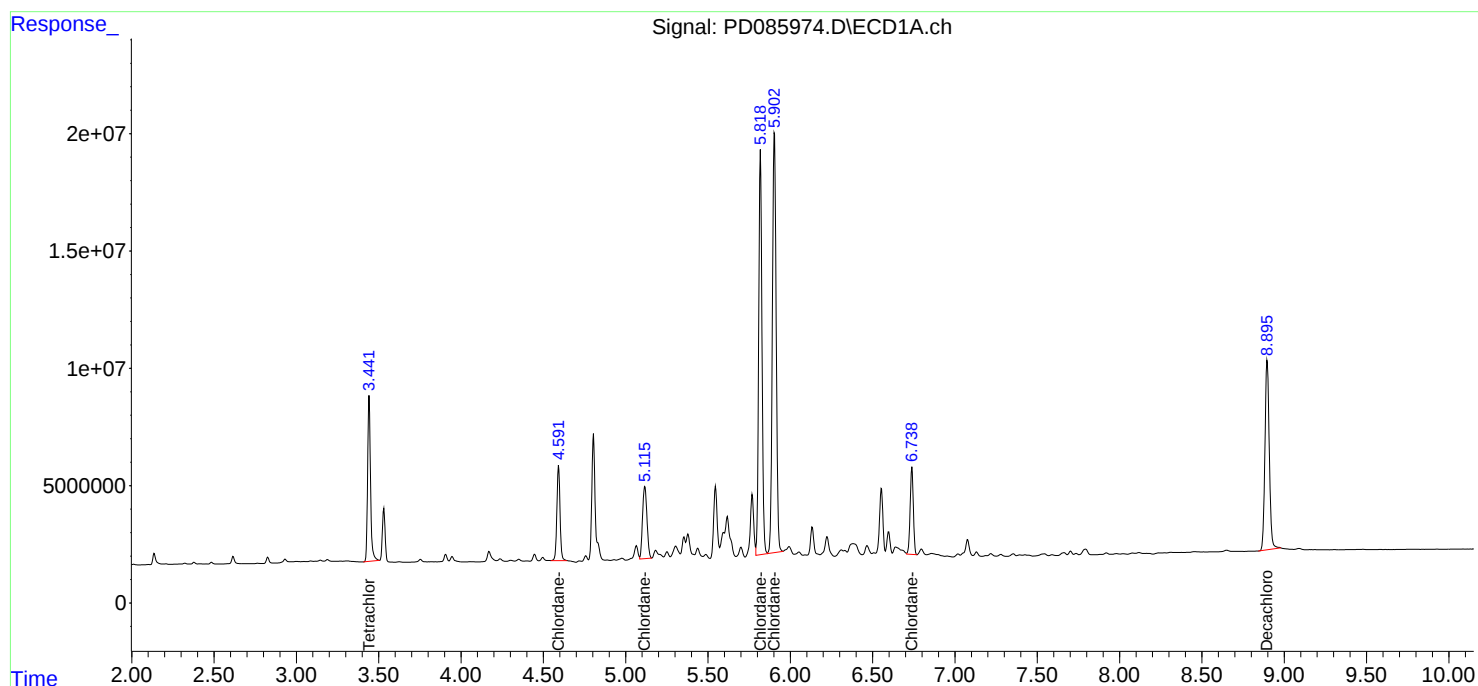


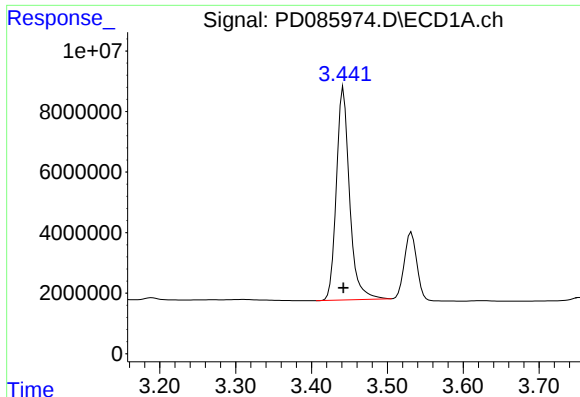

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 84907420
Conc: 74.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

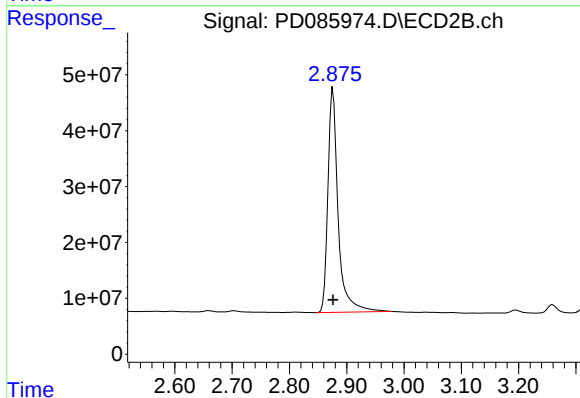


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.000 min
Response: 497849143
Conc: 74.08 ng/ml

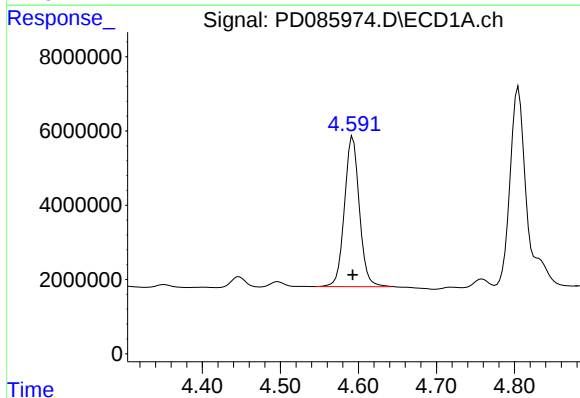


#23 Chlordane-1

R.T.: 4.593 min
Delta R.T.: 0.000 min
Response: 53535153
Conc: 747.10 ng/ml

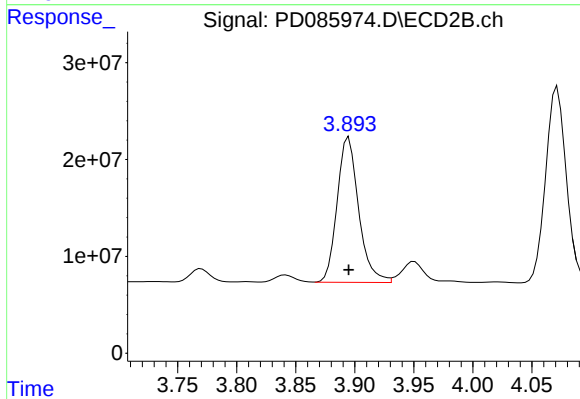

#23 Chlordane-1


R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 190171594
Conc: 739.39 ng/ml

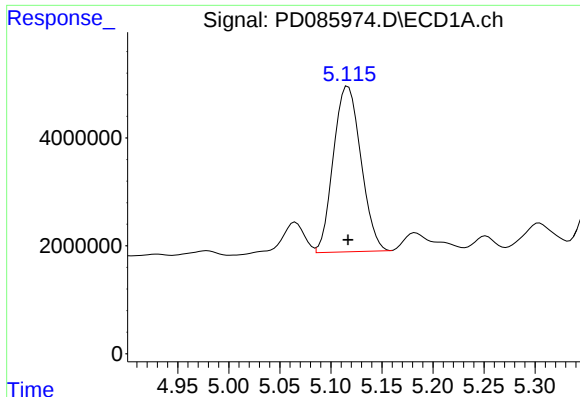

#24 Chlordane-2


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 57605356
Conc: 741.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

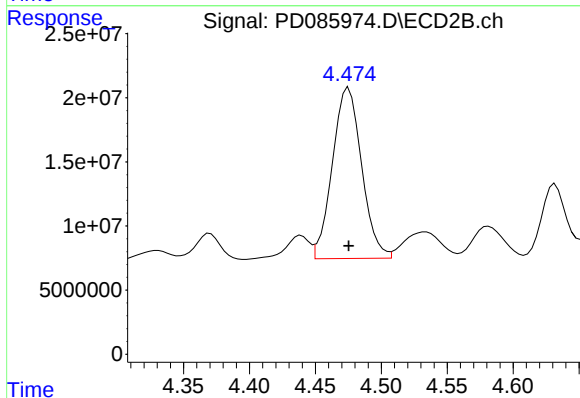


#24 Chlordane-2

R.T.: 4.475 min
Delta R.T.: 0.000 min
Response: 205665389
Conc: 741.14 ng/ml

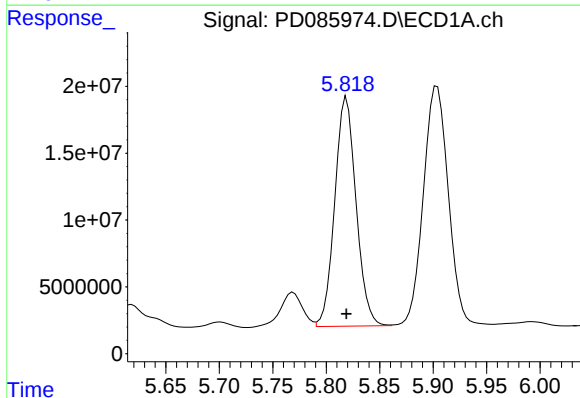


#25 Chlordane-3

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 237748229
Conc: 746.31 ng/ml

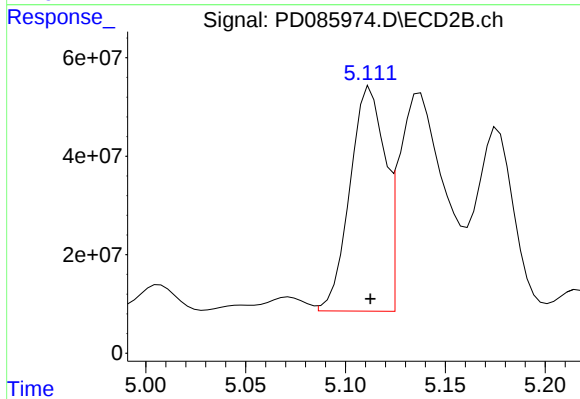

#25 Chlordane-3


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 553952830
Conc: 740.33 ng/ml

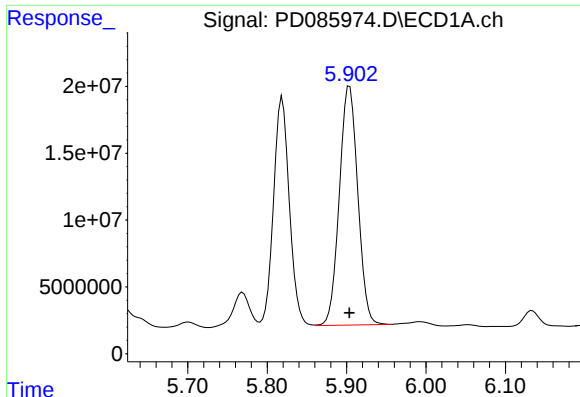

#26 Chlordane-4


R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 288847359
Conc: 746.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

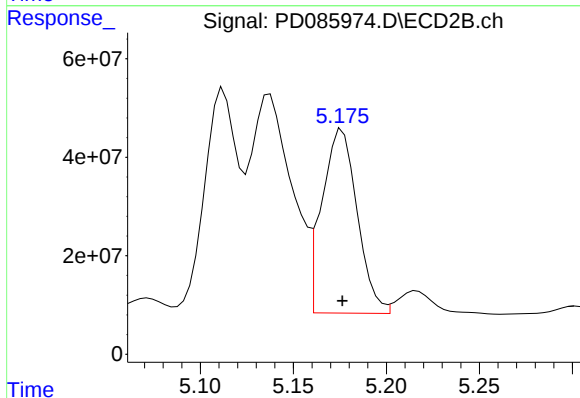


#26 Chlordane-4

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 494196343
Conc: 739.80 ng/ml

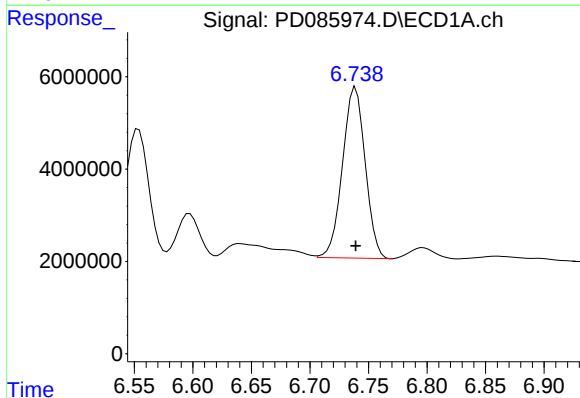


#27 Chlordane-5

R.T.: 6.739 min
Delta R.T.: 0.000 min
Response: 49883218
Conc: 744.00 ng/ml

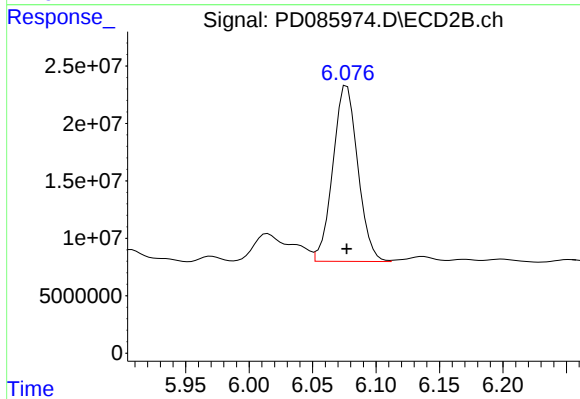

#27 Chlordane-5

R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 209295932
Conc: 737.89 ng/ml

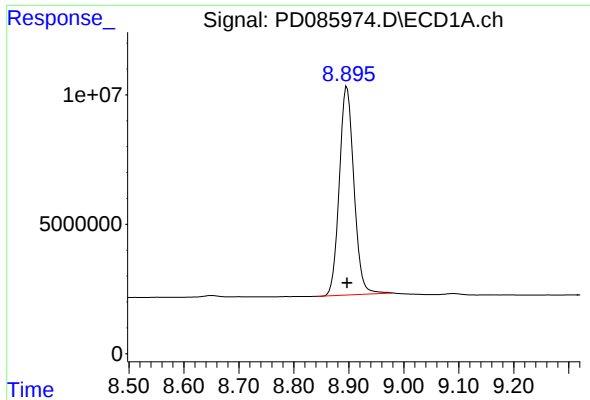

#28 Decachlorobiphenyl


R.T.: 8.897 min

Delta R.T.: 0.000 min

Response: 149003615

Conc: 74.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

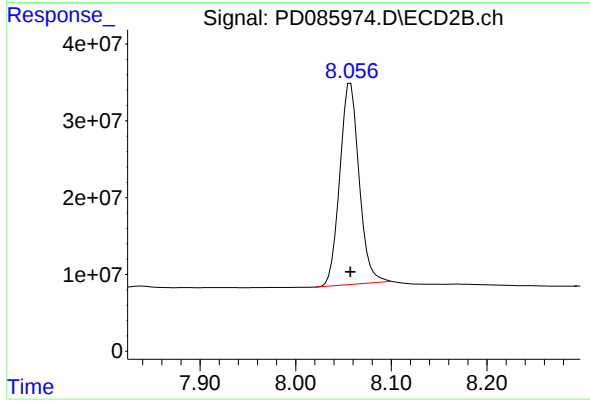

#28 Decachlorobiphenyl

R.T.: 8.057 min

Delta R.T.: 0.000 min

Response: 369485230

Conc: 73.97 ng/ml