

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101124\
 Data File : PD085976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2024 13:02
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 13:53:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101124.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 11 13:43:09 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.443	2.876	28815196	178.6E6	25.107	26.169
28)	SA Decachlor...	8.898	8.058	54107499	135.7E6	26.426	26.592
Target Compounds							
23)	Chlordane-1	4.592	3.895	17791764	69737237	248.715	265.525
24)	Chlordane-2	5.117	4.475	20745237	77449490	262.432	271.207
25)	Chlordane-3	5.819	5.112	74576458	198.3E6	237.884	261.057
26)	Chlordane-4	5.904	5.176	93346760	179.5E6	243.307	263.719
27)	Chlordane-5	6.738	6.076	16481857	75520108	246.855	261.994



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101124\
Data File : PD085976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2024 13:02
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 13:53:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101124.M
Quant Title : GC Extractables
QLast Update : Fri Oct 11 13:43:09 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

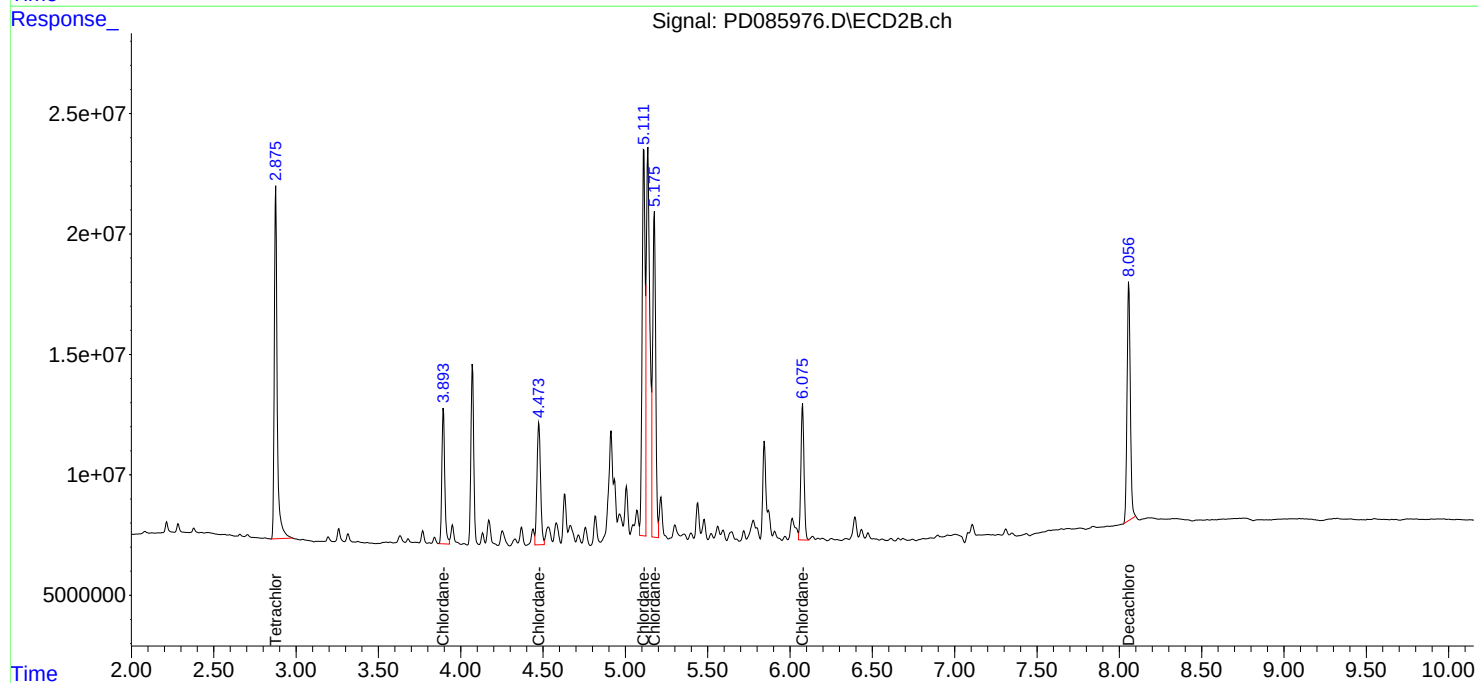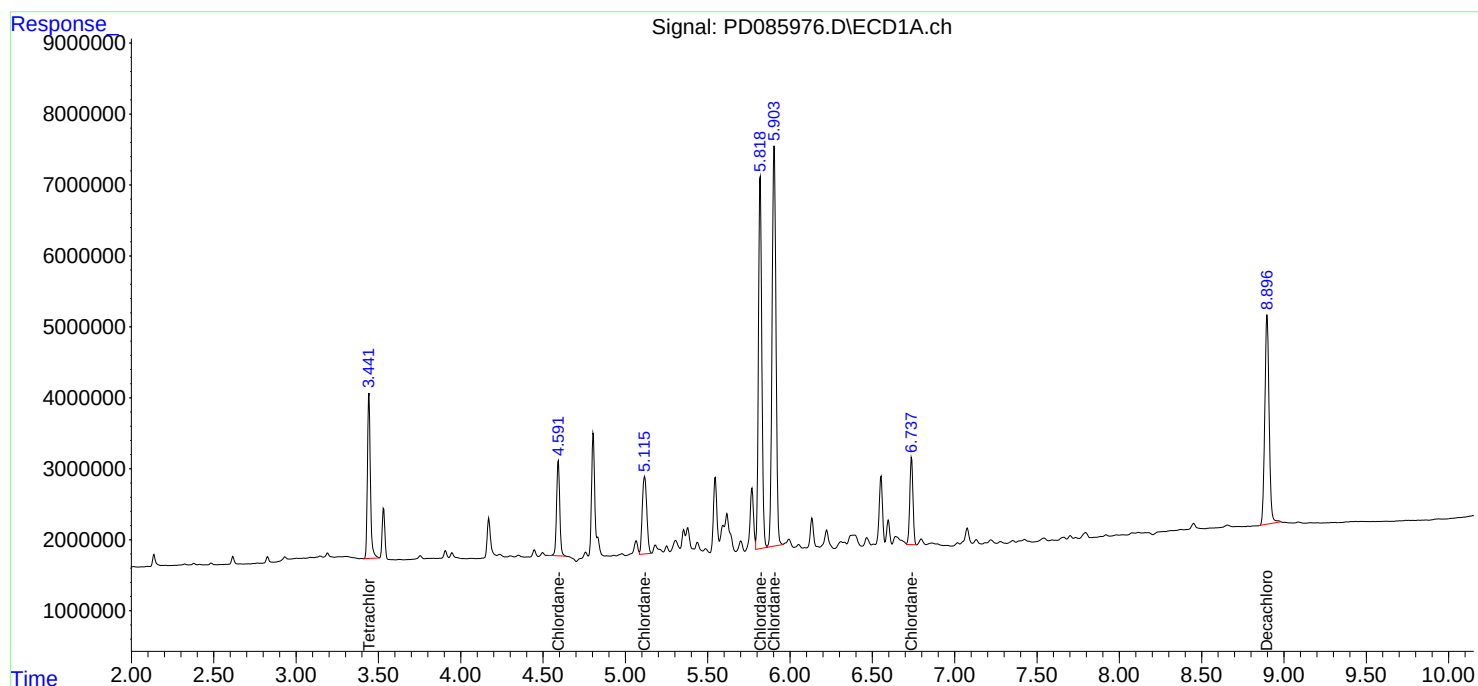


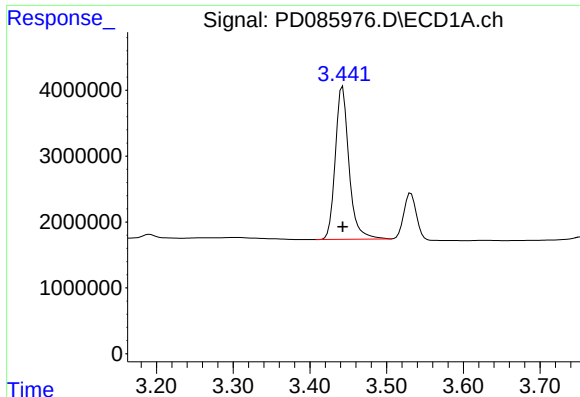

#1 Tetrachloro-m-xylene


R.T.: 3.443 min
Delta R.T.: 0.000 min
Response: 28815196
Conc: 25.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

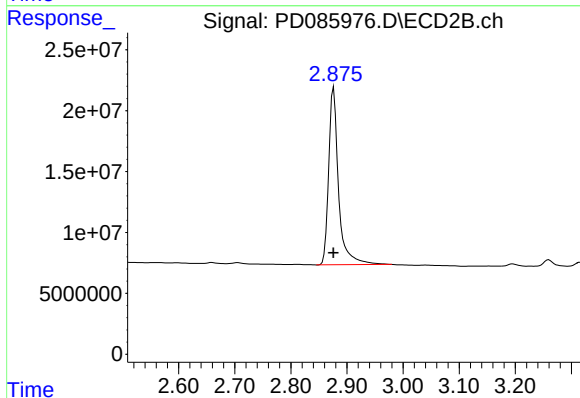


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.000 min
Response: 178648507
Conc: 26.17 ng/ml

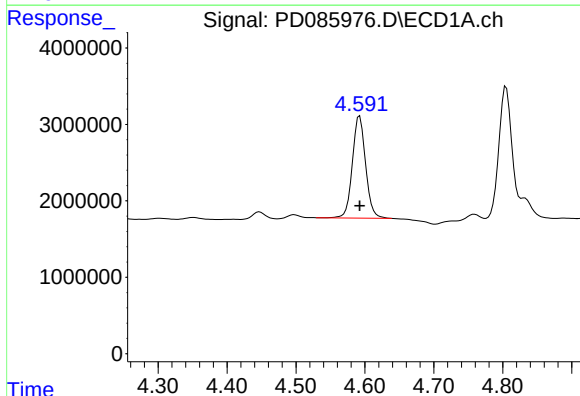


#23 Chlordane-1

R.T.: 4.592 min
Delta R.T.: 0.000 min
Response: 17791764
Conc: 248.71 ng/ml

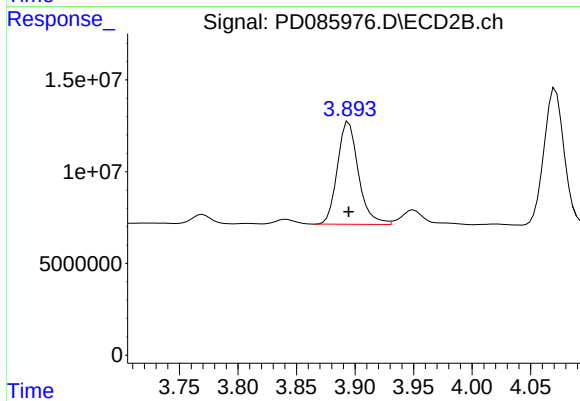

#23 Chlordane-1


R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 69737237
Conc: 265.53 ng/ml

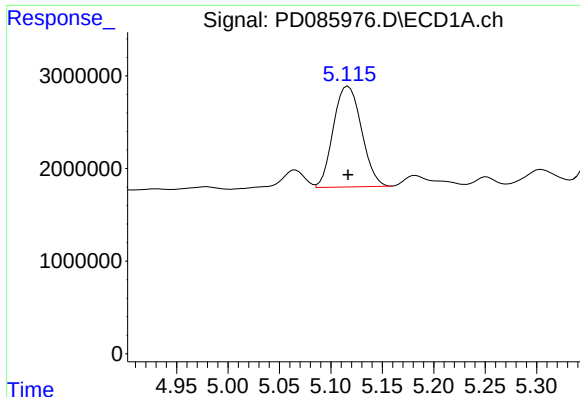

#24 Chlordane-2


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 20745237
Conc: 262.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

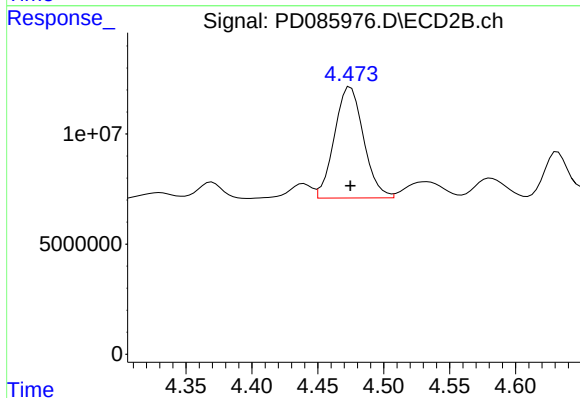


#24 Chlordane-2

R.T.: 4.475 min
Delta R.T.: 0.000 min
Response: 77449490
Conc: 271.21 ng/ml

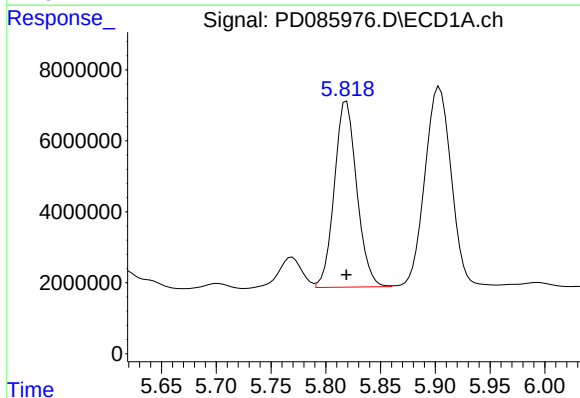


#25 Chlordane-3

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 74576458
Conc: 237.88 ng/ml

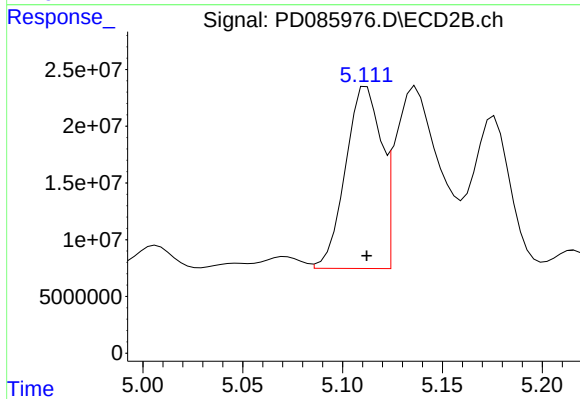

#25 Chlordane-3


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 198260693
Conc: 261.06 ng/ml

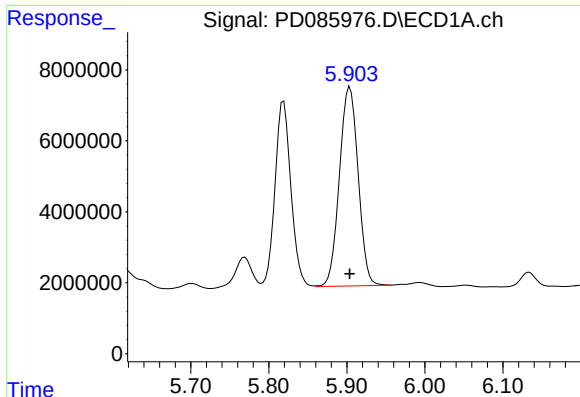

#26 Chlordane-4


R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 93346760
Conc: 243.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

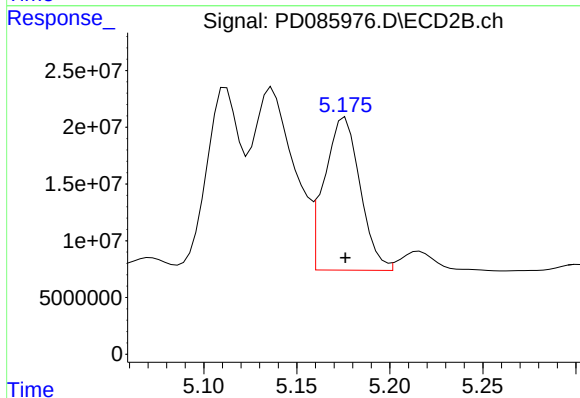


#26 Chlordane-4

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 179450991
Conc: 263.72 ng/ml

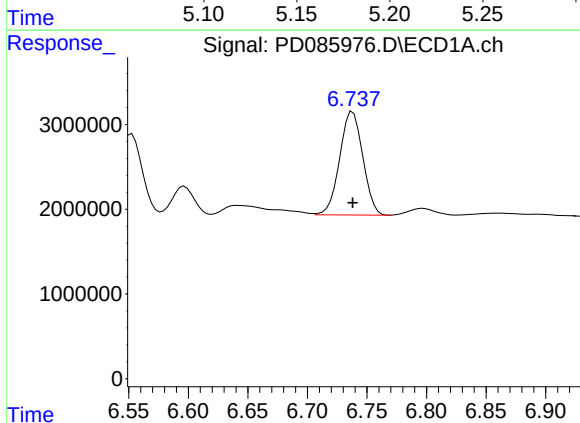


#27 Chlordane-5

R.T.: 6.738 min
Delta R.T.: 0.000 min
Response: 16481857
Conc: 246.85 ng/ml

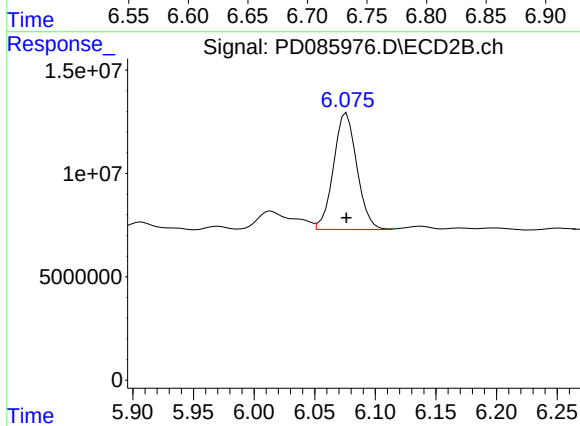

#27 Chlordane-5


R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 75520108
Conc: 261.99 ng/ml

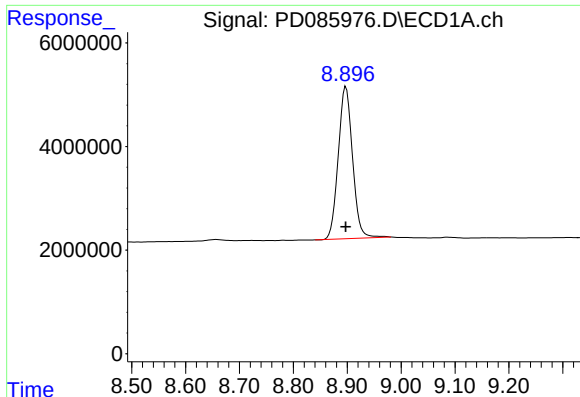

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 54107499
Conc: 26.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

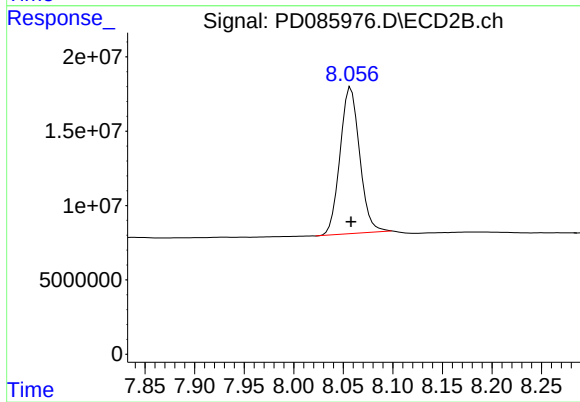

#28 Decachlorobiphenyl

R.T.: 8.058 min
Delta R.T.: 0.000 min
Response: 135705925
Conc: 26.59 ng/ml