

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101124\
 Data File : PD085975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Oct 2024 12:49
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 13:48:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101124.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 11 13:43:09 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.442	2.876	58242996	349.5E6	50.000	50.000
28) SA Decachlor...	8.898	8.058	104.1E6	260.4E6	50.000	50.000
Target Compounds						
23) Chlordane-1	4.593	3.895	36151448	134.4E6	500.000	500.000
24) Chlordane-2	5.117	4.475	40380938	146.6E6	500.000	500.000
25) Chlordane-3	5.818	5.112	157.6E6	389.4E6	500.000	500.000
26) Chlordane-4	5.904	5.176	193.2E6	345.3E6	500.000	500.000
27) Chlordane-5	6.738	6.077	33965071	147.8E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101124\
Data File : PD085975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Oct 2024 12:49
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 13:48:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101124.M
Quant Title : GC Extractables
QLast Update : Fri Oct 11 13:43:09 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

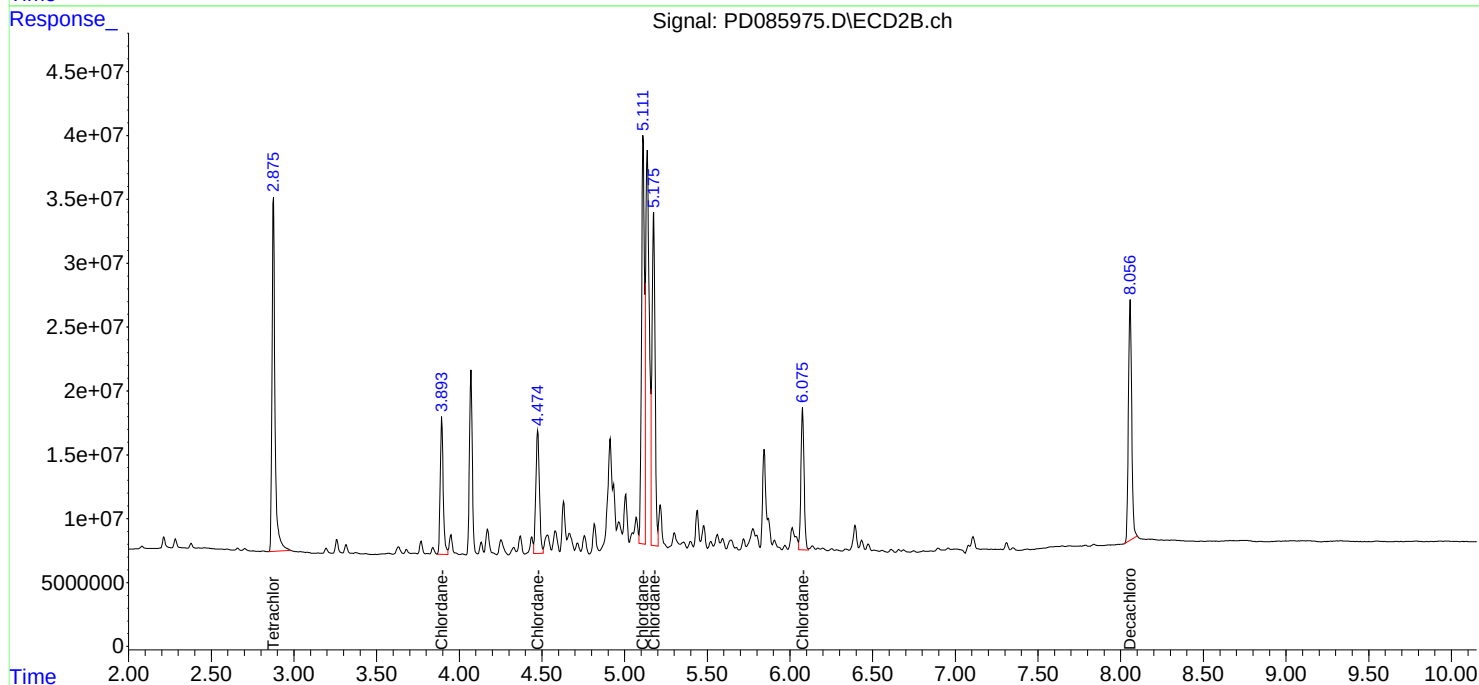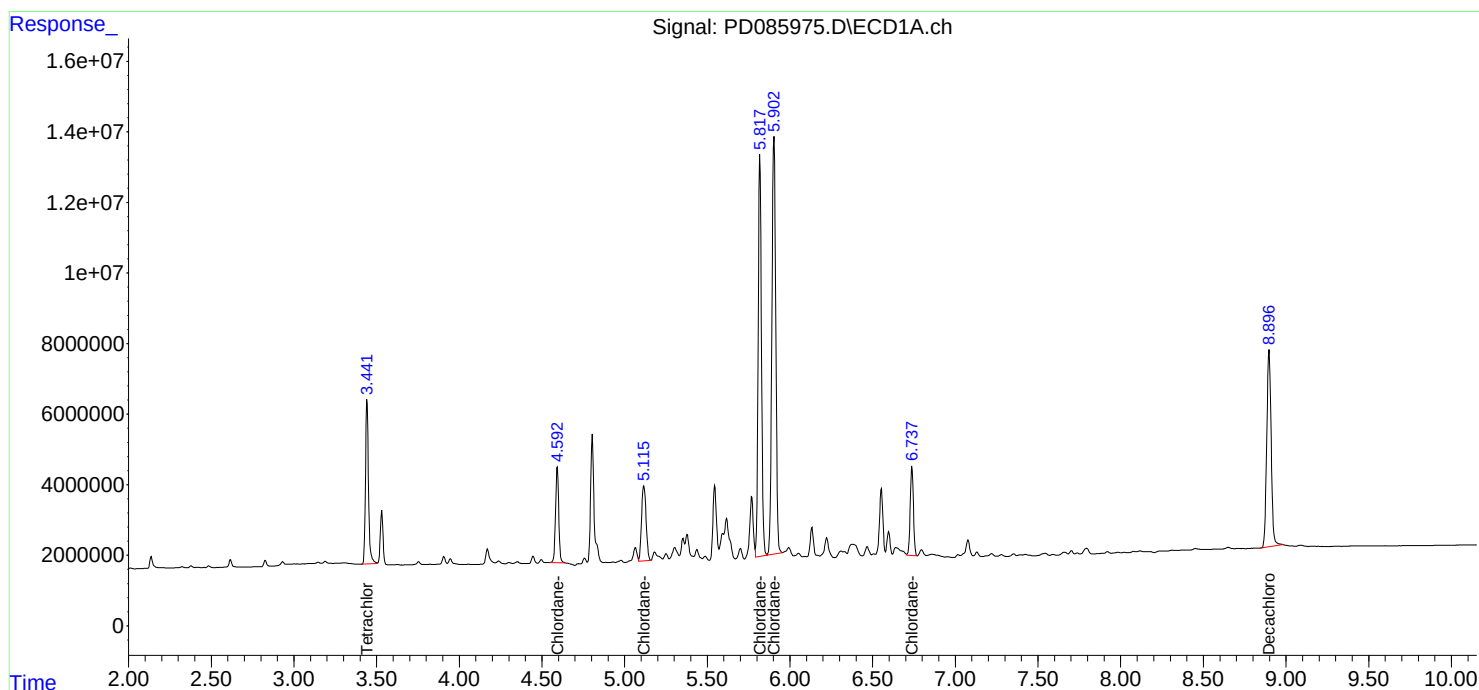


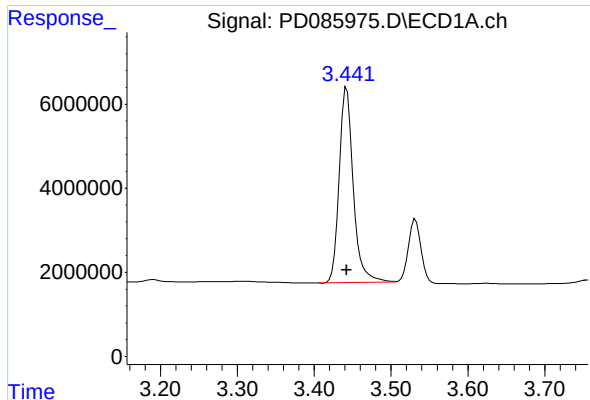

#1 Tetrachloro-m-xylene


R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 58242996
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

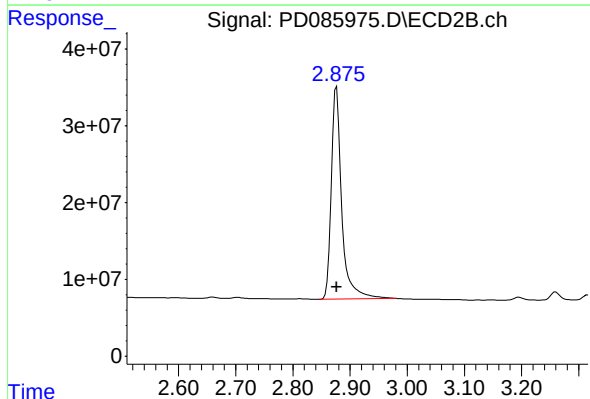


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.000 min
Response: 349475419
Conc: 50.00 ng/ml

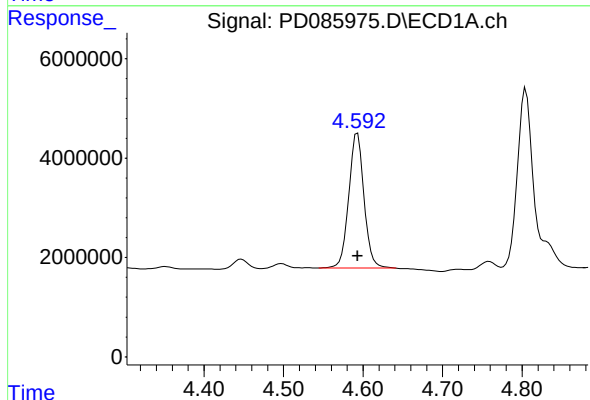


#23 Chlordane-1

R.T.: 4.593 min
Delta R.T.: 0.000 min
Response: 36151448
Conc: 500.00 ng/ml

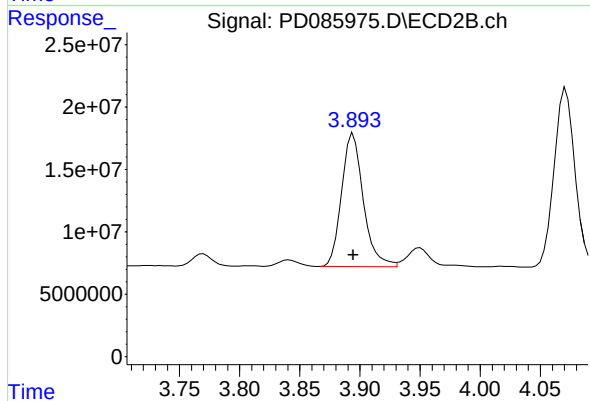

#23 Chlordane-1


R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 134400318
Conc: 500.00 ng/ml

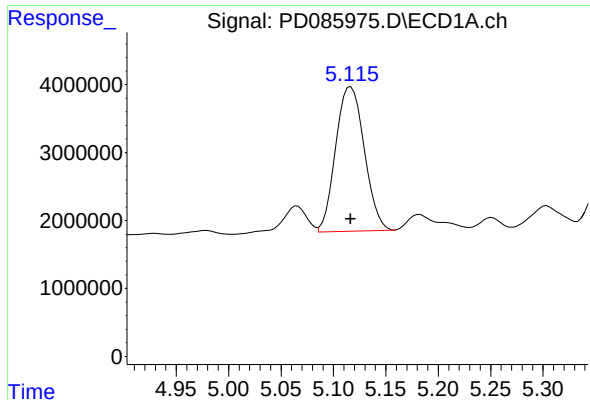

#24 Chlordane-2


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 40380938
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

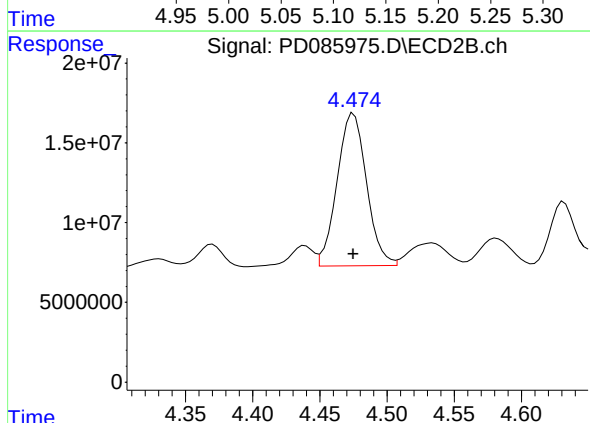


#24 Chlordane-2

R.T.: 4.475 min
Delta R.T.: 0.000 min
Response: 146555241
Conc: 500.00 ng/ml

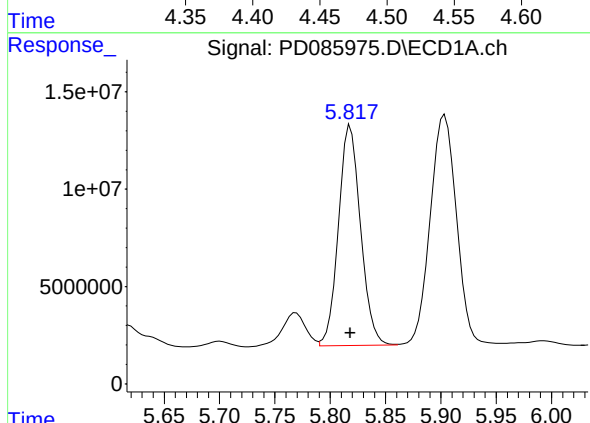


#25 Chlordane-3

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 157629040
Conc: 500.00 ng/ml

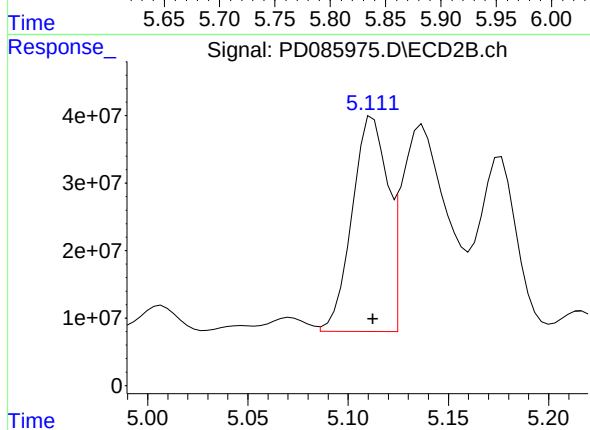

#25 Chlordane-3


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 389405605
Conc: 500.00 ng/ml

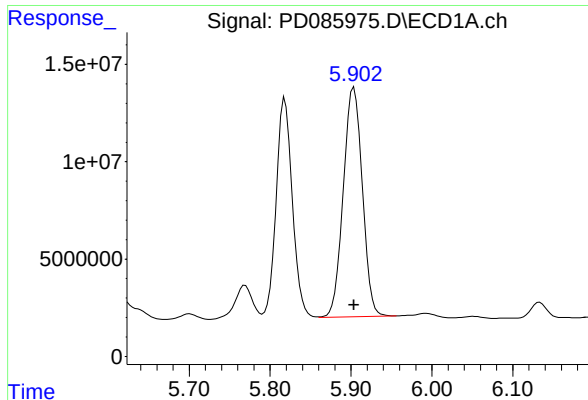

#26 Chlordane-4


R.T.: 5.904 min
Delta R.T.: 0.000 min
Response: 193178691
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

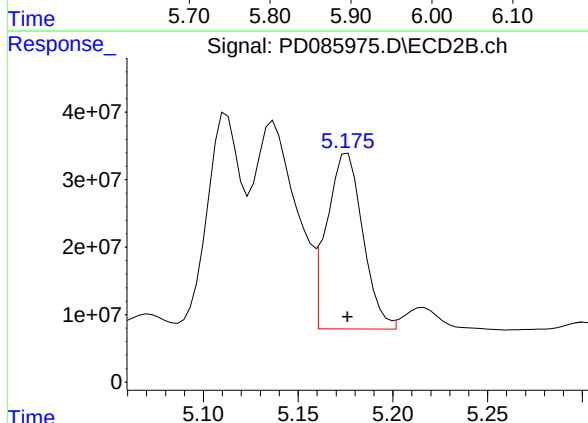


#26 Chlordane-4

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 345309195
Conc: 500.00 ng/ml

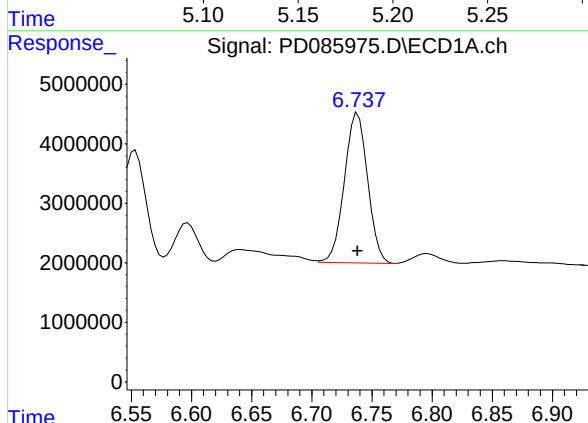


#27 Chlordane-5

R.T.: 6.738 min
Delta R.T.: 0.000 min
Response: 33965071
Conc: 500.00 ng/ml

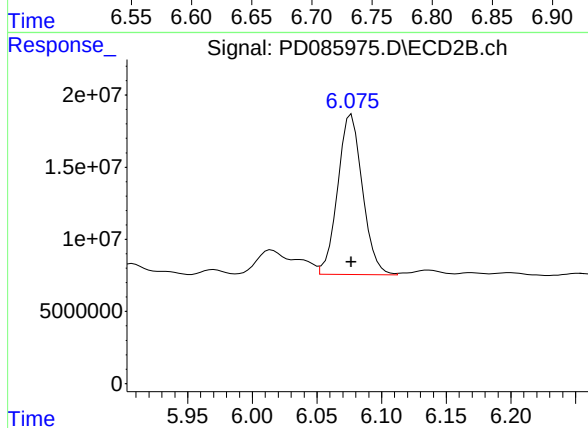

#27 Chlordane-5


R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 147777056
Conc: 500.00 ng/ml

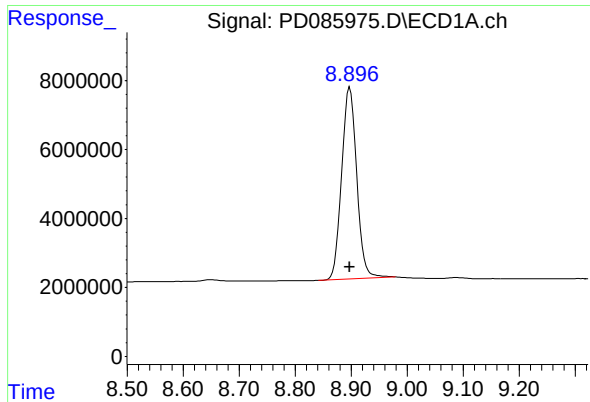

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.000 min
Response: 104117574
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

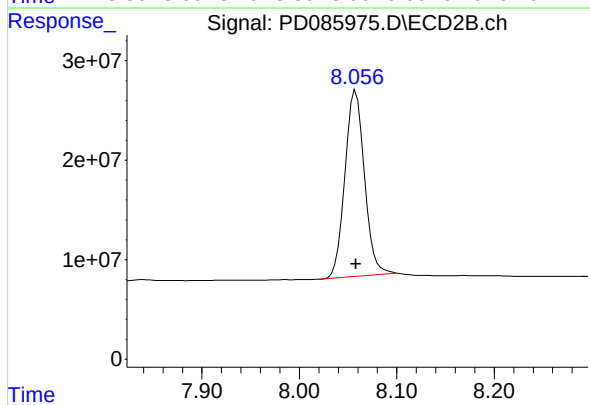

#28 Decachlorobiphenyl

R.T.: 8.058 min
Delta R.T.: 0.000 min
Response: 260403388
Conc: 50.00 ng/ml