

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101220\
 Data File : PD059685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2020 10:52
 Operator : DD\AJ
 Sample : L4358-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 13:27:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.509	4.025	27907866	40985849	19.356	18.853
28)	SA Decachlor...	8.312	9.110	21951436	27567543	19.761	17.109
Target Compounds							
6)	B beta-BHC	4.461f	0.000	1917431	0	2.251	N.D. #
15)	B Endosulfa...	0.000	6.953	0	2189391	N.D.	1.020 #
18)	B Endrin al...	0.000	7.055f	0	4137817	N.D.	2.348 #
20)	A Methoxychlor	0.000	7.638f	0	447982	N.D.	0.427 #
23)	Chlordane-1	4.419f	0.000	3483762	0	67.054	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101220\
Data File : PD059685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2020 10:52
Operator : DD\AJ
Sample : L4358-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 13:27:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

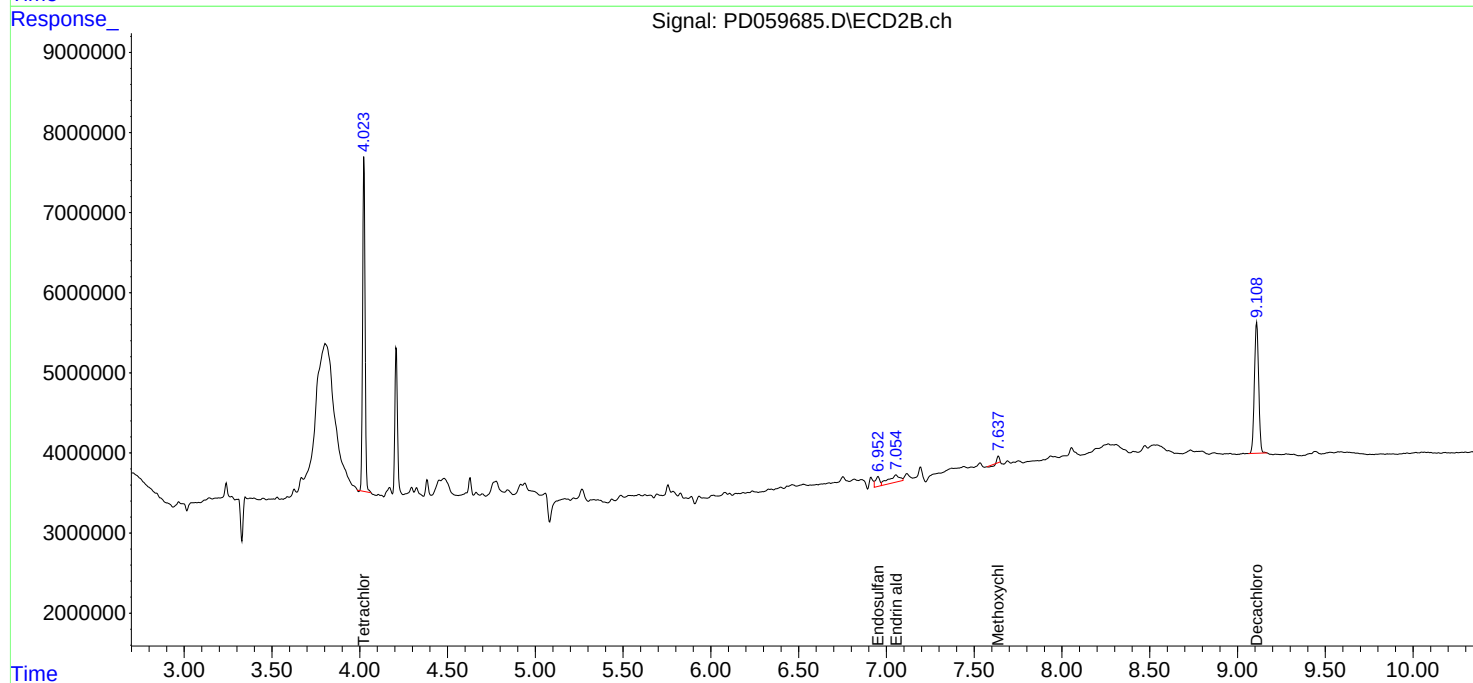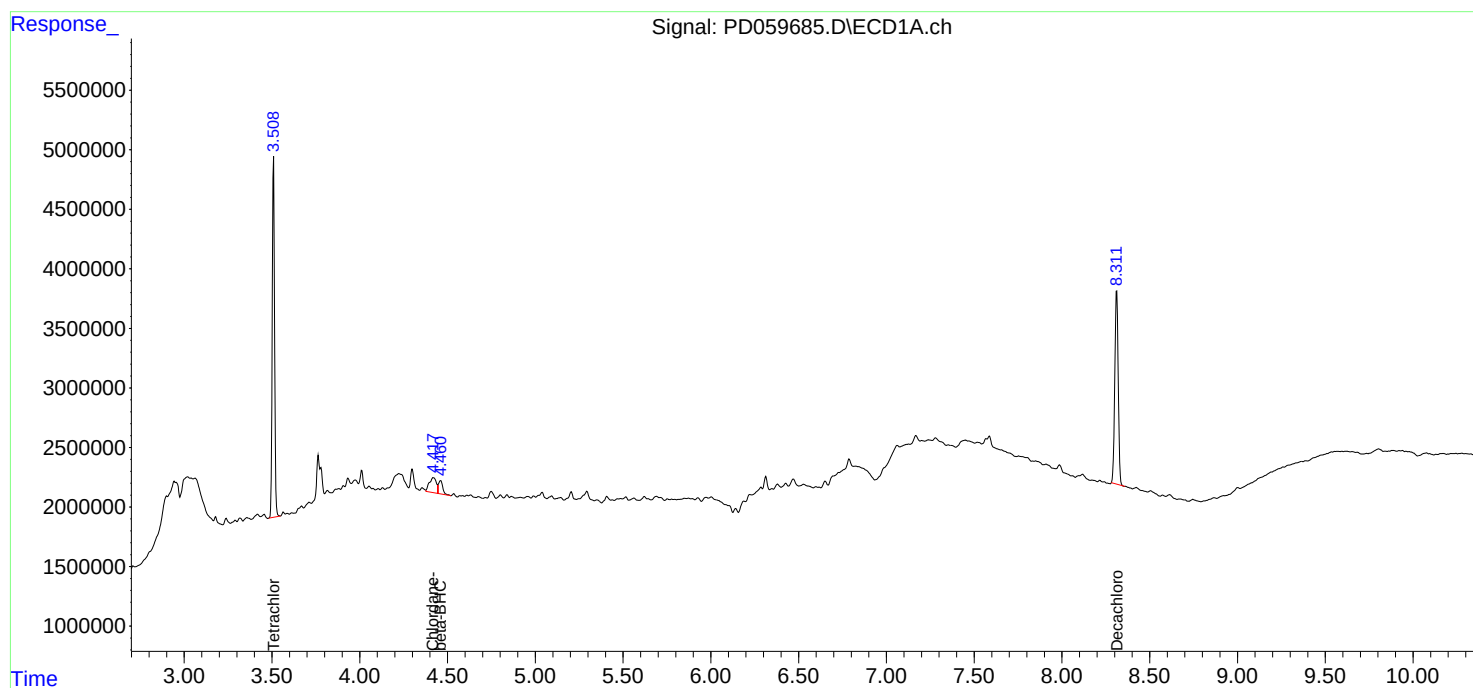


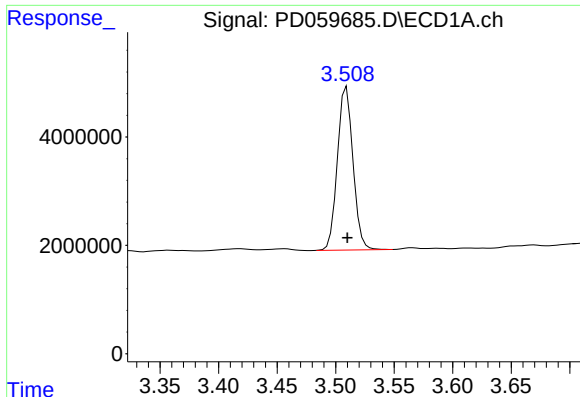

#1 Tetrachloro-m-xylene


R.T.: 3.509 min
Delta R.T.: 0.000 min
Response: 27907866
Conc: 19.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

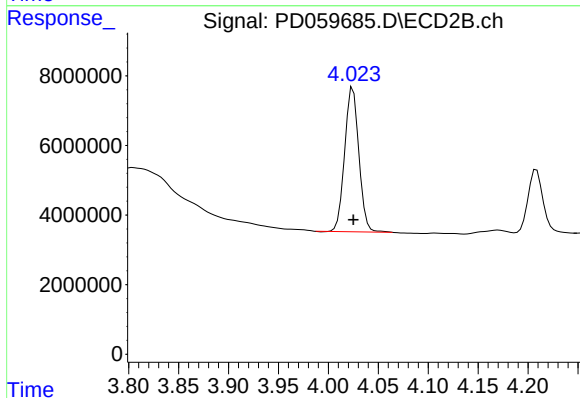


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 40985849
Conc: 18.85 ng/ml

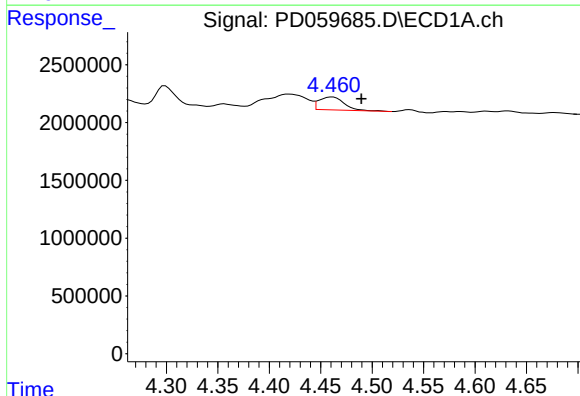


#6 beta-BHC

R.T.: 4.461 min
Delta R.T.: -0.028 min
Response: 1917431
Conc: 2.25 ng/ml

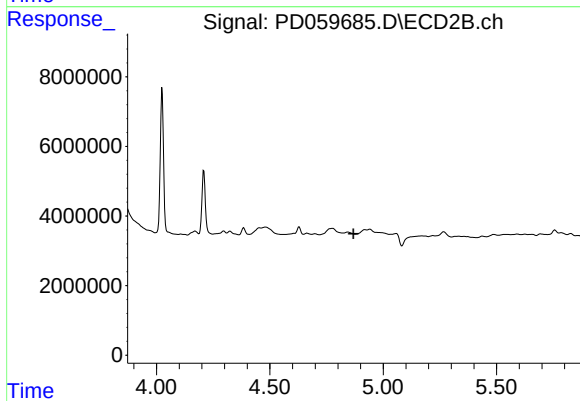

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.869 min
Response: 0
Conc: N.D.

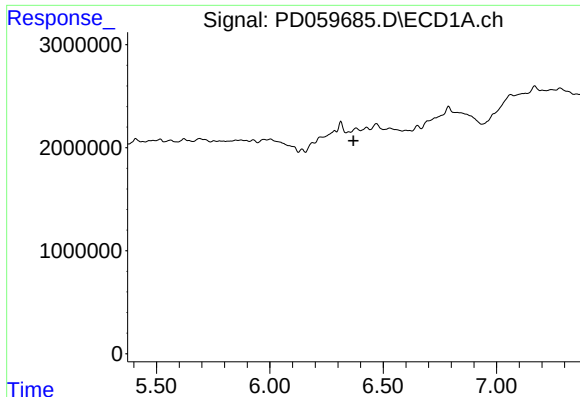

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

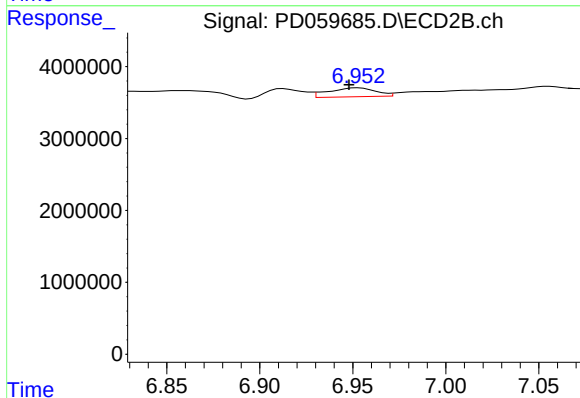


#15 Endosulfan II

R.T.: 6.953 min
Delta R.T.: 0.005 min
Response: 2189391
Conc: 1.02 ng/ml

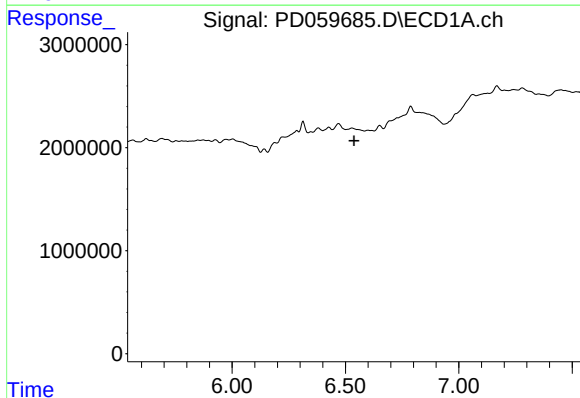


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.538 min
Response: 0
Conc: N.D.

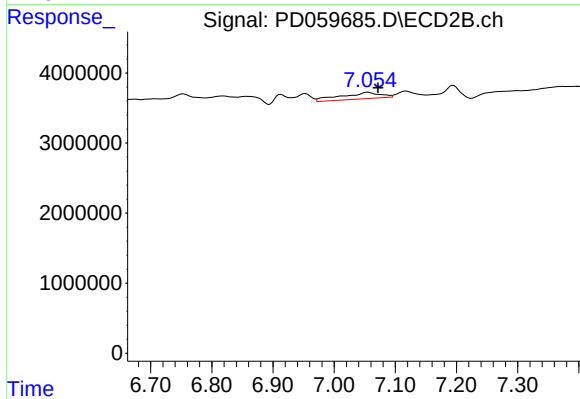

#18 Endrin aldehyde


R.T.: 7.055 min
Delta R.T.: -0.017 min
Response: 4137817
Conc: 2.35 ng/ml

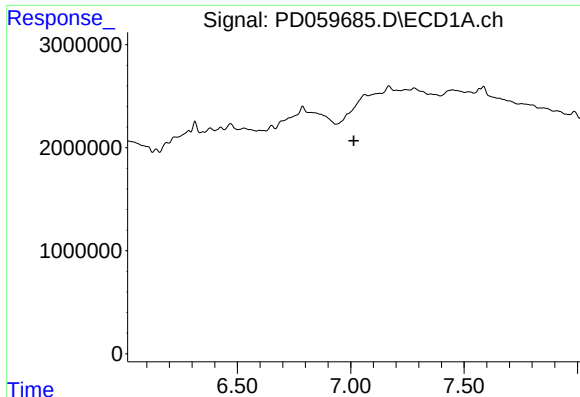

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.014 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

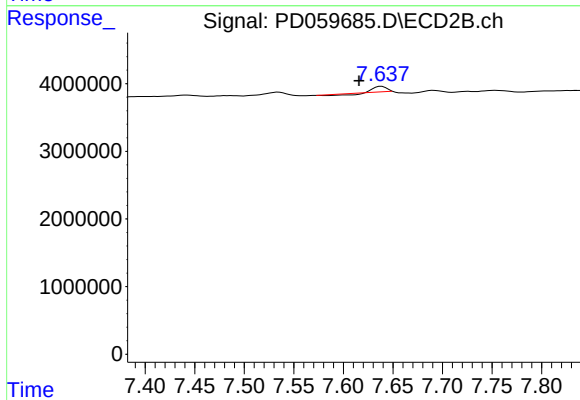


#20 Methoxychlor

R.T.: 7.638 min
Delta R.T.: 0.023 min
Response: 447982
Conc: 0.43 ng/ml

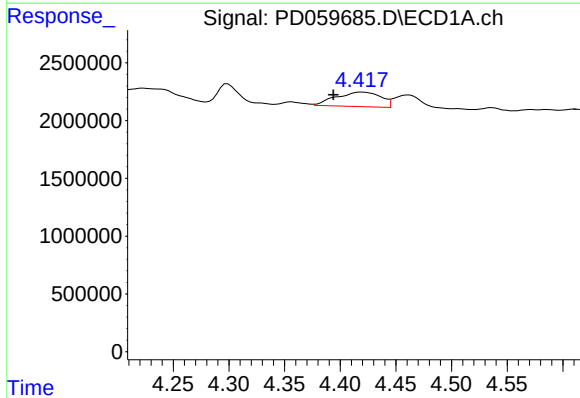


#23 Chlordane-1

R.T.: 4.419 min
Delta R.T.: 0.025 min
Response: 3483762
Conc: 67.05 ng/ml

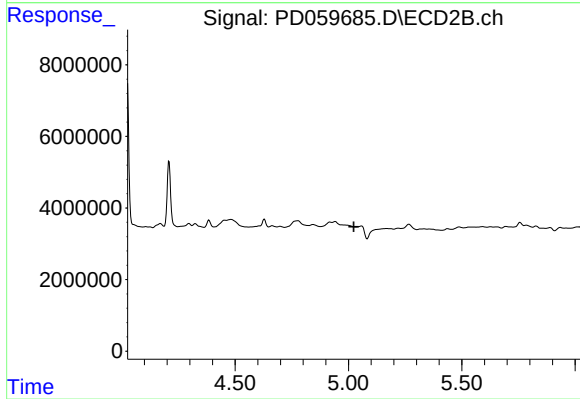

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.024 min
Response: 0
Conc: N.D.

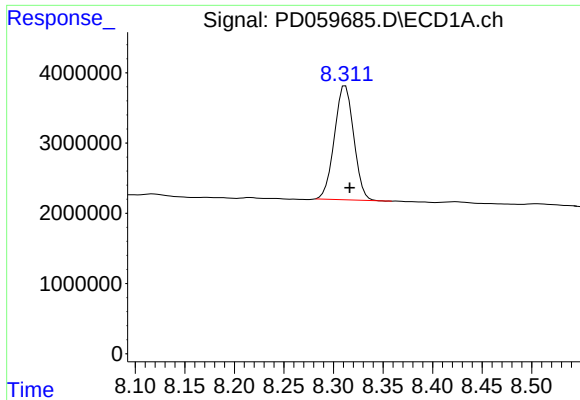

#28 Decachlorobiphenyl

R.T.: 8.312 min
Delta R.T.: -0.004 min
Response: 21951436
Conc: 19.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

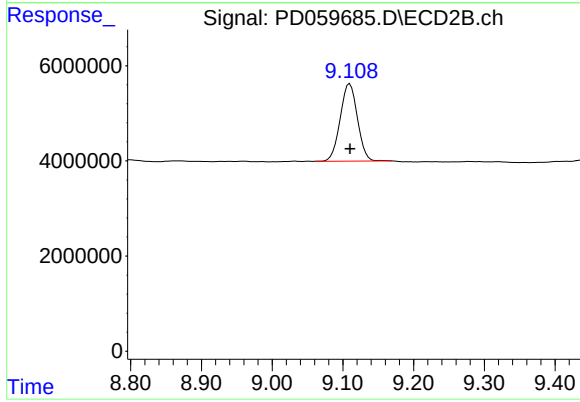

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 27567543
Conc: 17.11 ng/ml