

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101220\
 Data File : PD059697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2020 14:49
 Operator : DD\AJ
 Sample : L4341-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 16:14:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.509	4.025	19547248	28863300	13.557	13.277
28)	SA Decachlor...	8.311	9.110	15375941	19336311	13.841	12.000
Target Compounds							
10)	B gamma-Chl...	5.469	0.000	632289	0	0.356	N.D. #
12)	B 4,4'-DDE	5.698	6.368	13386072	18040312	7.894	7.598
13)	MA Dieldrin	5.849	0.000	1609003	0	0.934	N.D. #
16)	A 4,4'-DDD	6.217	6.859	10040222	14518504	7.186	7.168
17)	MA 4,4'-DDT	6.460	7.159	2819256	3903588	1.850	1.991
19)	B Endosulfa...	6.767	0.000	2248239	0	1.746	N.D. #
23)	Chlordane-1	4.418f	0.000	3718540	0	71.573	N.D. #
25)	Chlordane-3	5.469	0.000	632289	0	3.999	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101220\
Data File : PD059697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2020 14:49
Operator : DD\AJ
Sample : L4341-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 16:14:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

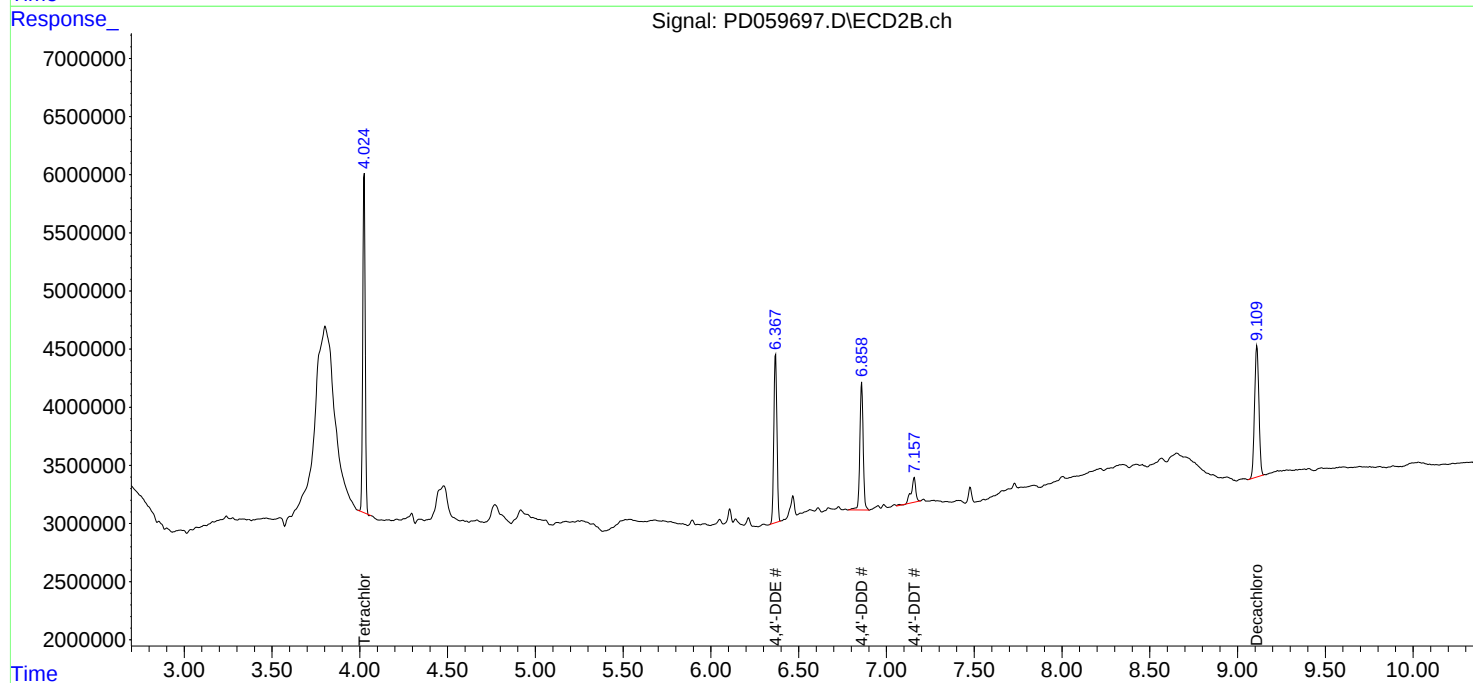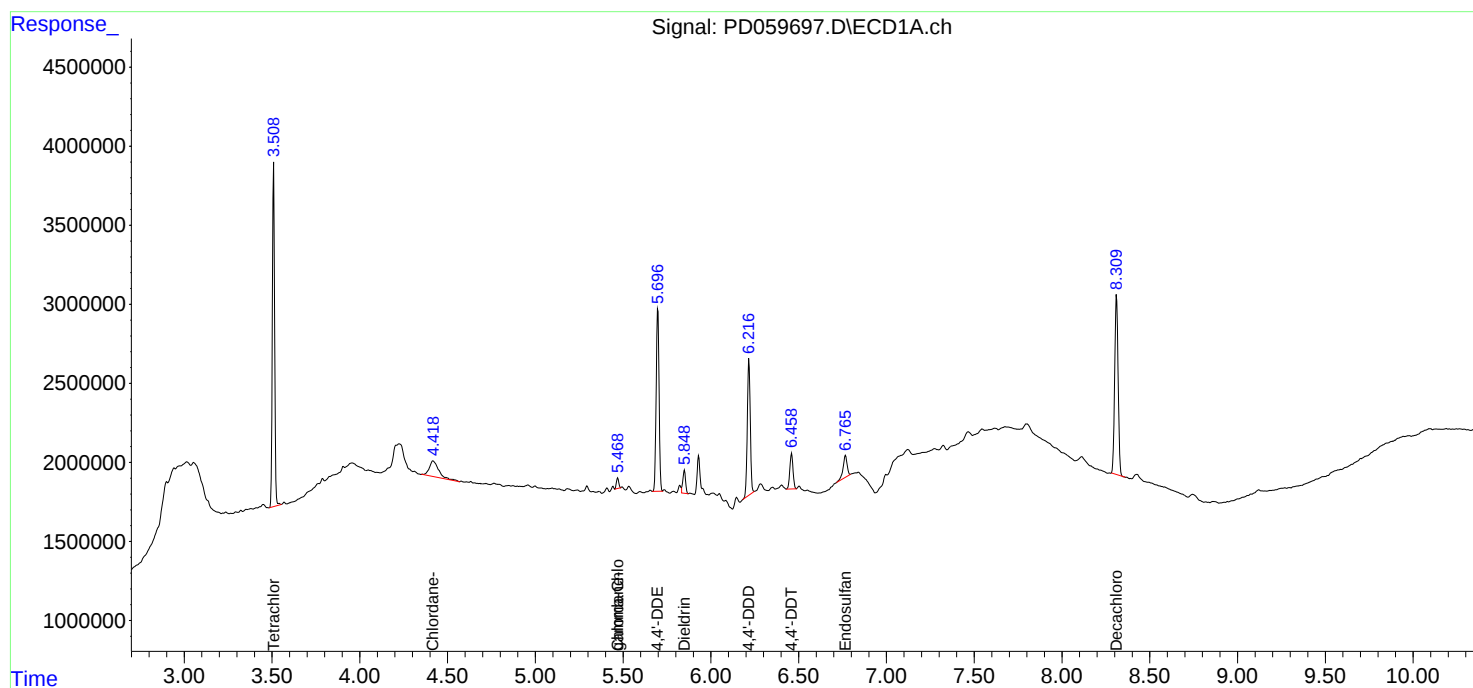


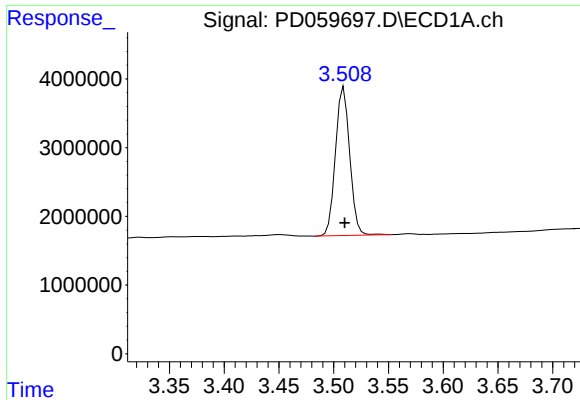

#1 Tetrachloro-m-xylene


R.T.: 3.509 min
Delta R.T.: 0.000 min
Response: 19547248
Conc: 13.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

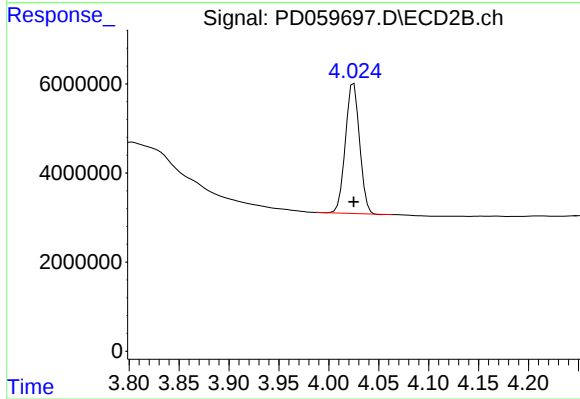


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 28863300
Conc: 13.28 ng/ml

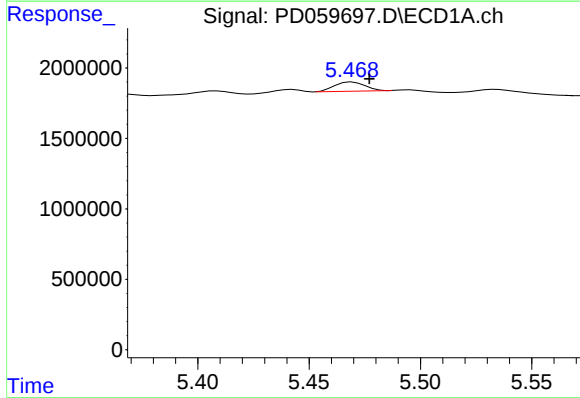


#10 gamma-Chlordane

R.T.: 5.469 min
Delta R.T.: -0.008 min
Response: 632289
Conc: 0.36 ng/ml

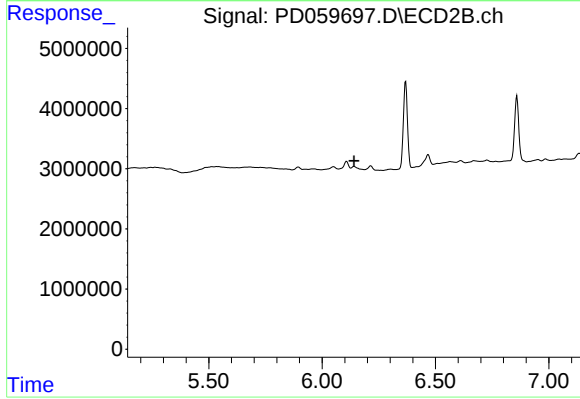

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.141 min
Response: 0
Conc: N.D.

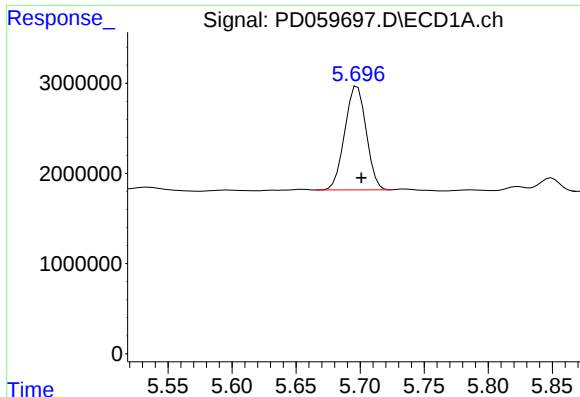

#12 4,4'-DDE


R.T.: 5.698 min
Delta R.T.: -0.003 min
Response: 13386072
Conc: 7.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

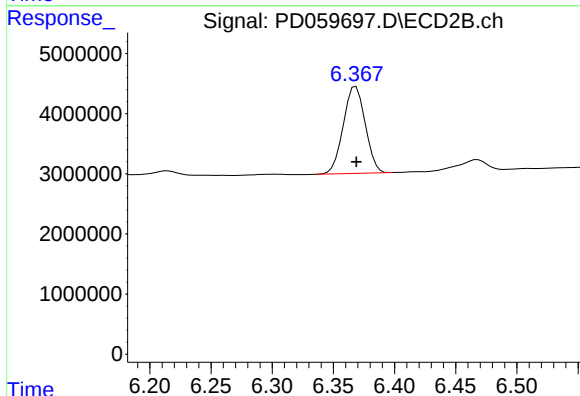


#12 4,4'-DDE

R.T.: 6.368 min
Delta R.T.: 0.000 min
Response: 18040312
Conc: 7.60 ng/ml

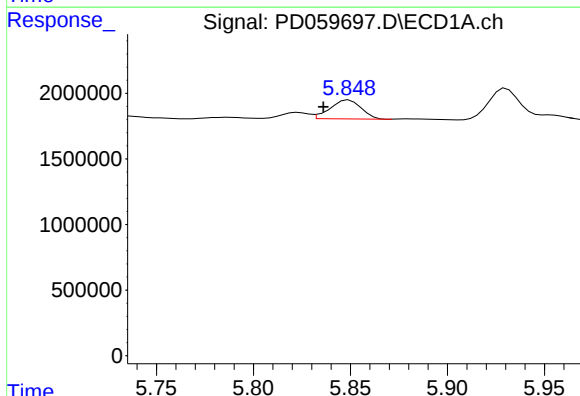


#13 Dieldrin

R.T.: 5.849 min
Delta R.T.: 0.013 min
Response: 1609003
Conc: 0.93 ng/ml

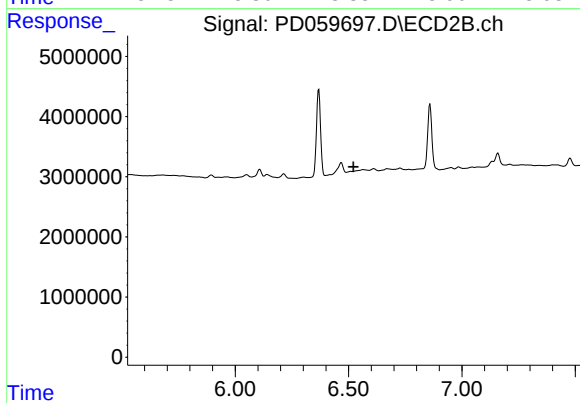

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

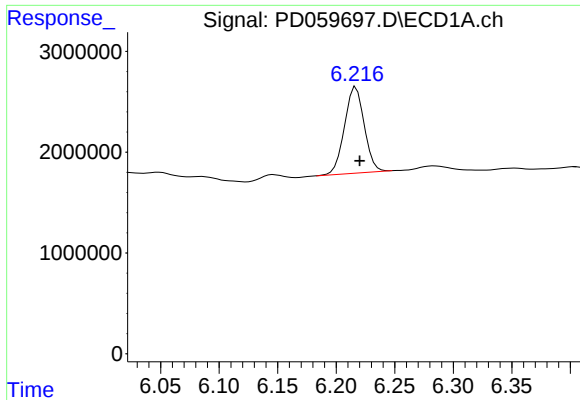

#16 4,4'-DDD


R.T.: 6.217 min
Delta R.T.: -0.003 min
Response: 10040222
Conc: 7.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

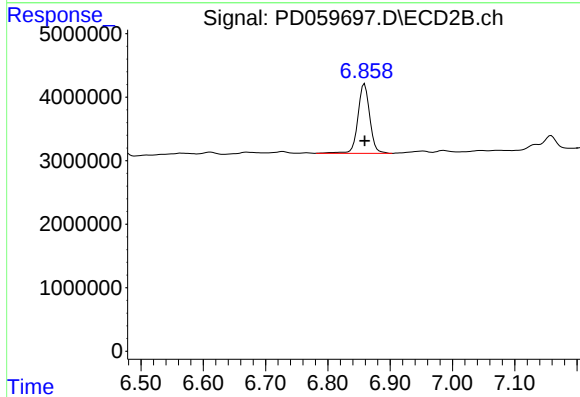


#16 4,4'-DDD

R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 14518504
Conc: 7.17 ng/ml

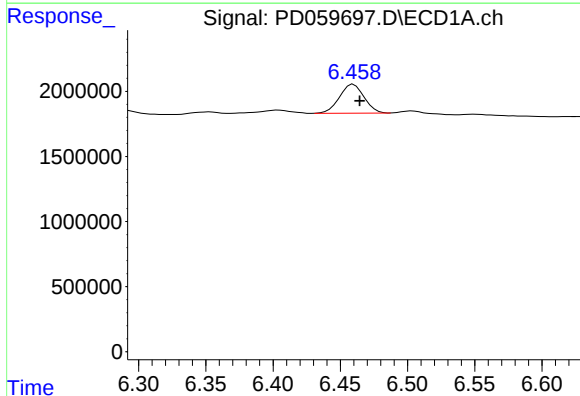


#17 4,4'-DDT

R.T.: 6.460 min
Delta R.T.: -0.005 min
Response: 2819256
Conc: 1.85 ng/ml

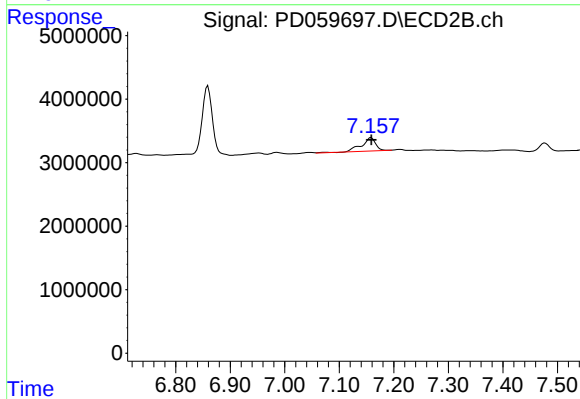

#17 4,4'-DDT


R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 3903588
Conc: 1.99 ng/ml

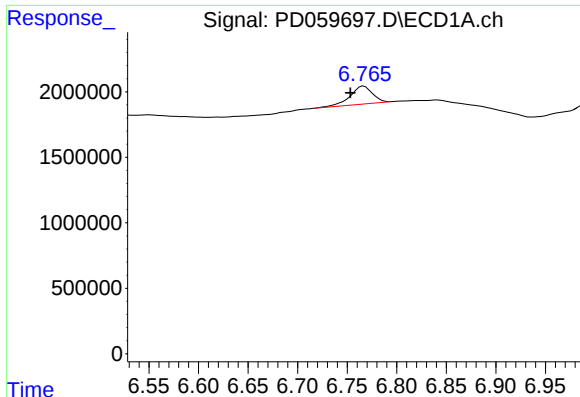

#19 Endosulfan Sulfate


R.T.: 6.767 min
Delta R.T.: 0.014 min
Response: 2248239
Conc: 1.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

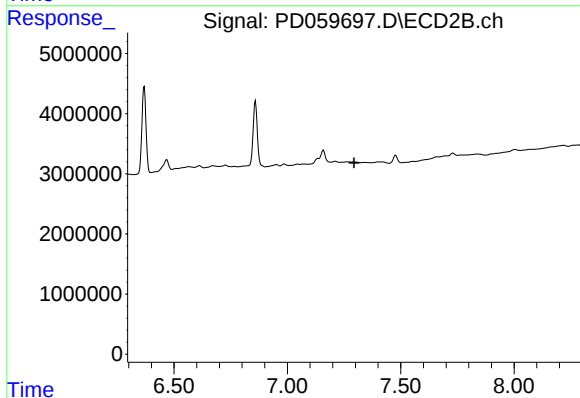


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.295 min
Response: 0
Conc: N.D.

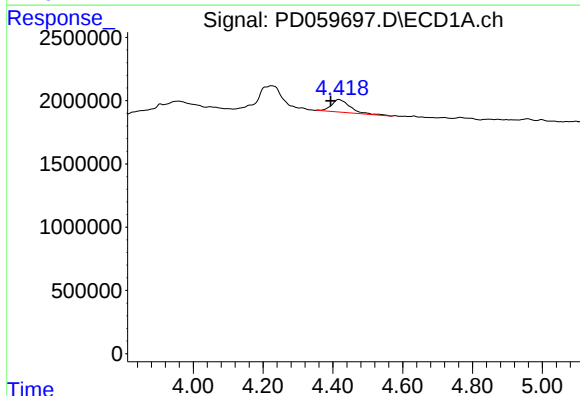


#23 Chlordane-1

R.T.: 4.418 min
Delta R.T.: 0.023 min
Response: 3718540
Conc: 71.57 ng/ml

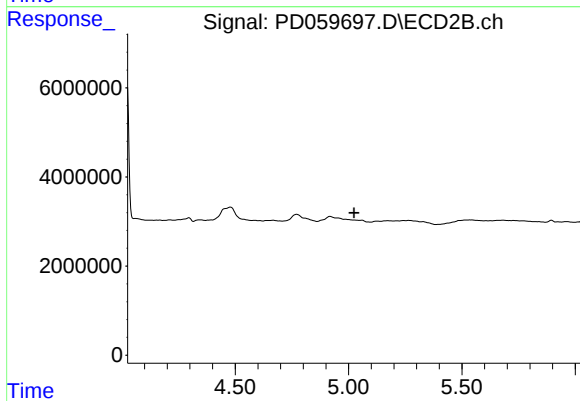

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.024 min
Response: 0
Conc: N.D.

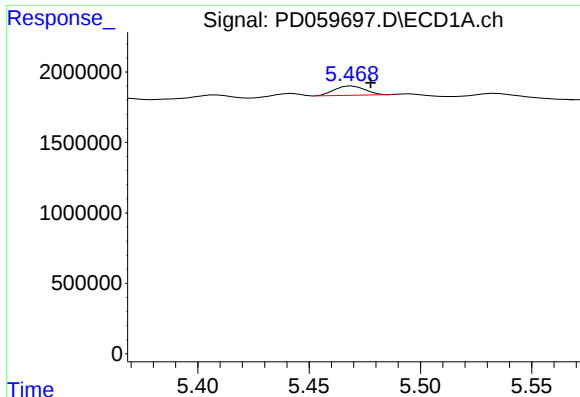

#25 Chlordane-3


R.T.: 5.469 min
Delta R.T.: -0.008 min
Response: 632289
Conc: 4.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

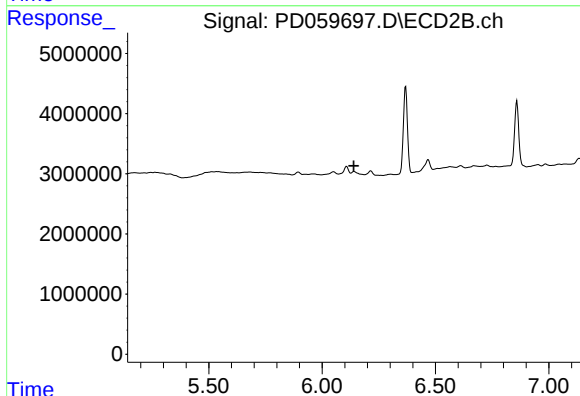


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.140 min
Response: 0
Conc: N.D.

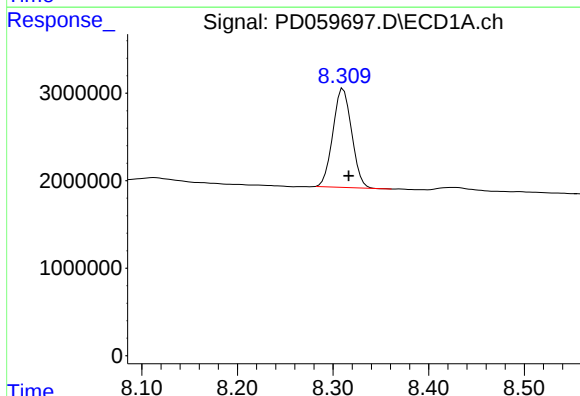

#28 Decachlorobiphenyl

R.T.: 8.311 min
Delta R.T.: -0.006 min
Response: 15375941
Conc: 13.84 ng/ml

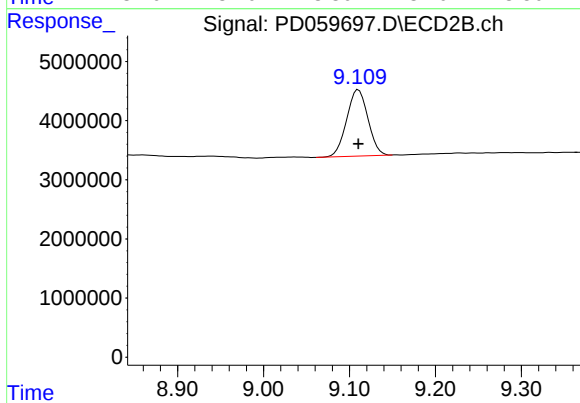

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 19336311
Conc: 12.00 ng/ml