

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101220\
 Data File : PD059686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2020 11:06
 Operator : DD\AJ
 Sample : L4330-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 S-1

Manual Integrations
 APPROVED

Ankita
 10/13/2020 12:26:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 13:27:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.510	4.023	23749877	34427559	16.472	15.836m
28)	SA Decachlor...	8.311	9.108	14223114	17918516	12.804	11.121

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101220\
Data File : PD059686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2020 11:06
Operator : DD\AJ
Sample : L4330-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
S-1


Manual Integrations
APPROVED

Ankita
10/13/2020 12:26:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 13:27:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

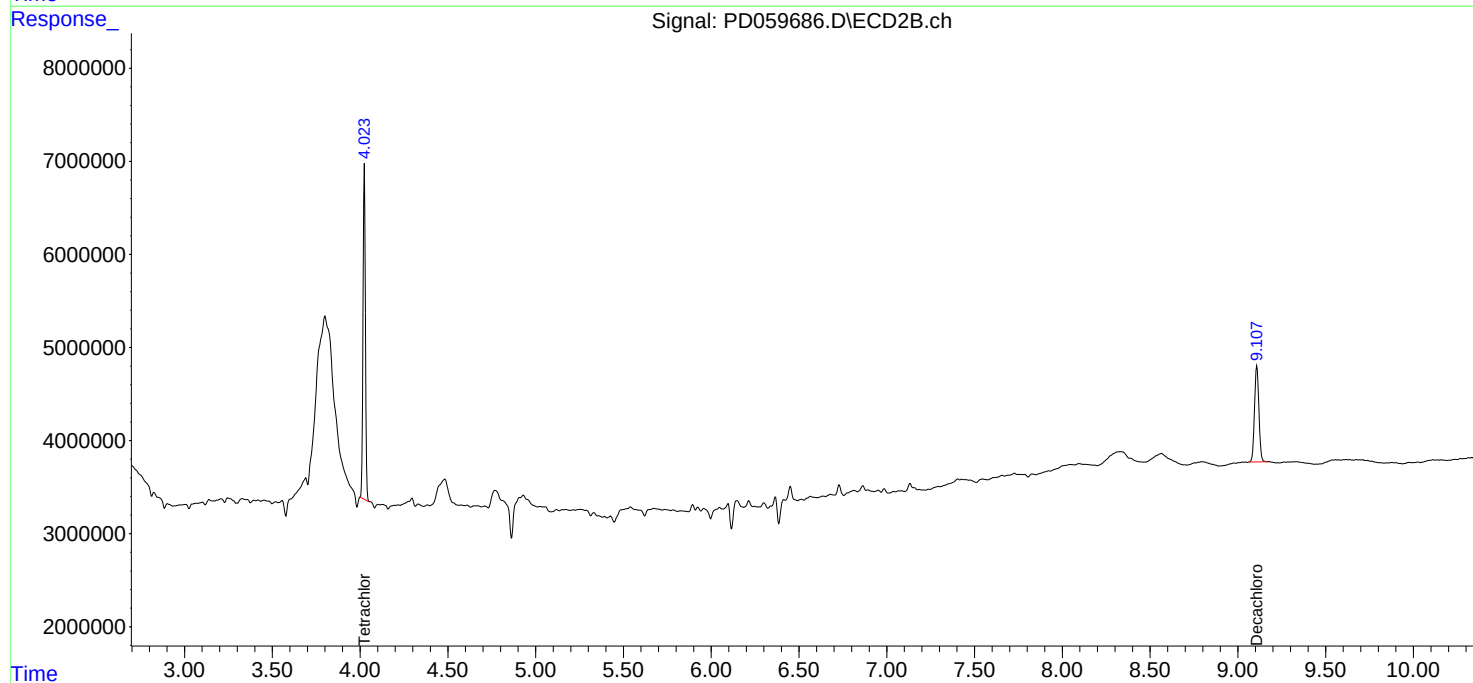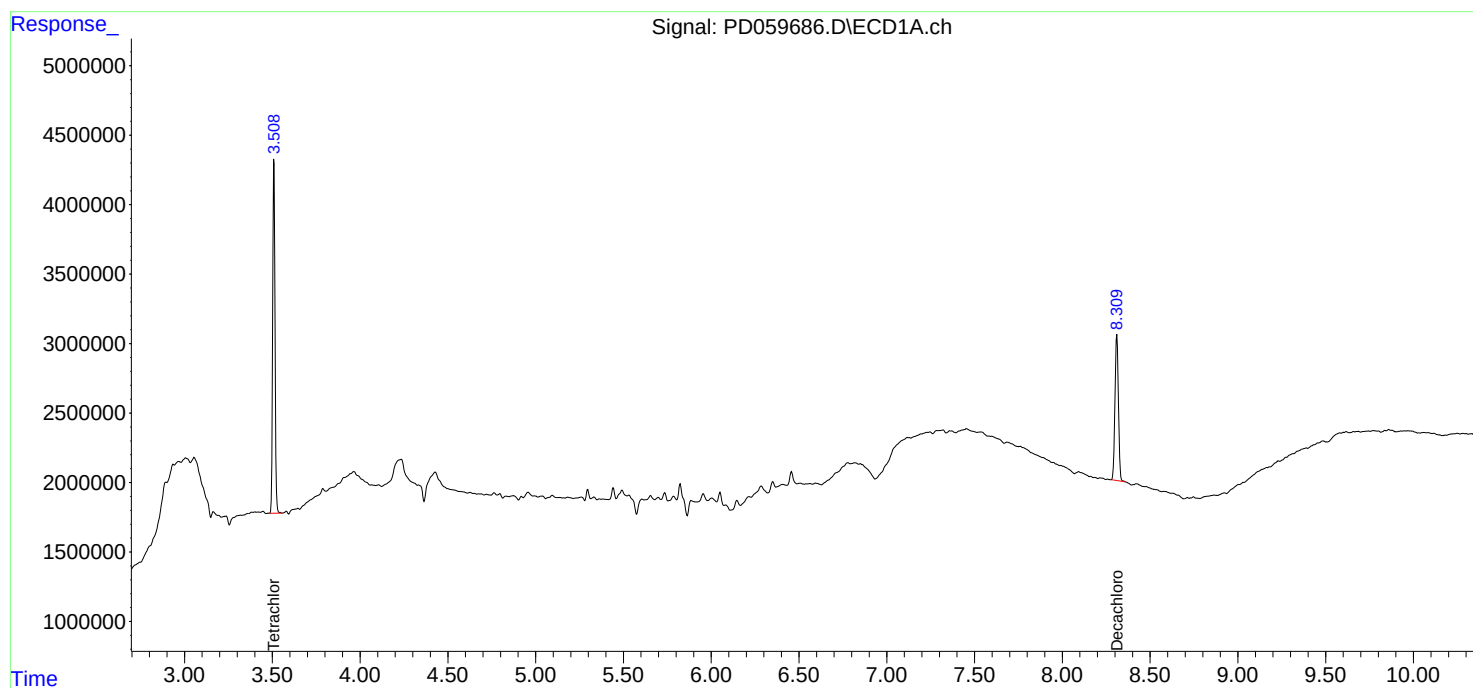

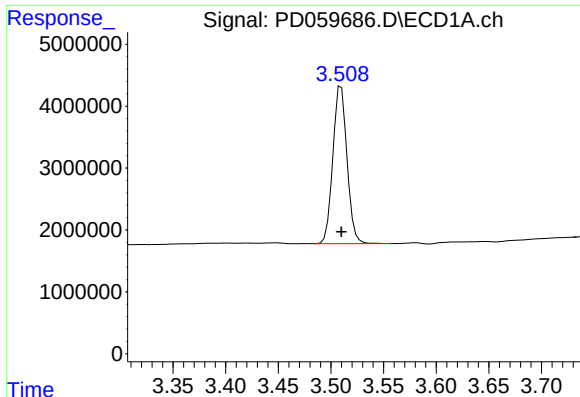


#1 Tetrachloro-m-xylene

R.T.: 3.510 min
Delta R.T.: 0.000 min
Response: 23749877
Conc: 16.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
S-1


Manual Integrations
APPROVED

Ankita
10/13/2020 12:26:24 PM

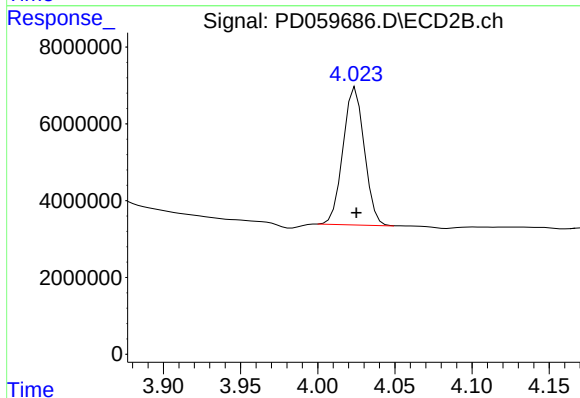


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: -0.002 min
Response: 34427559
Conc: 15.84 ng/ml m

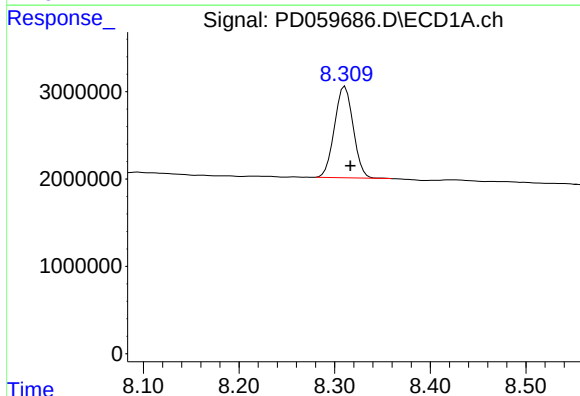

#28 Decachlorobiphenyl

R.T.: 8.311 min
Delta R.T.: -0.006 min
Response: 14223114
Conc: 12.80 ng/ml

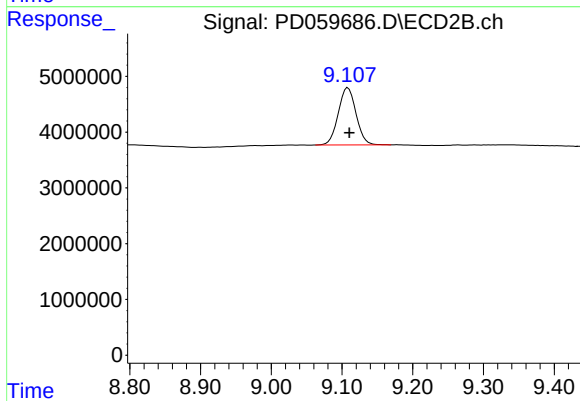

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: -0.002 min
Response: 17918516
Conc: 11.12 ng/ml