

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101220\
 Data File : PD059696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2020 14:34
 Operator : DD\AJ
 Sample : L4340-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A-2332-MH12

Manual Integrations
 APPROVED

Ankita
 10/13/2020 12:26:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 16:14:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 08 13:21:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.509	4.025	19901877	30018401	13.803	13.808
28)	SA Decachlor...	8.311	9.109	15746553	17714987	14.175m	10.994m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101220\
Data File : PD059696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2020 14:34
Operator : DD\AJ
Sample : L4340-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
A-2332-MH12


Manual Integrations
APPROVED

Ankita
10/13/2020 12:26:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 16:14:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100820.M
Quant Title : GC Extractables
QLast Update : Thu Oct 08 13:21:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

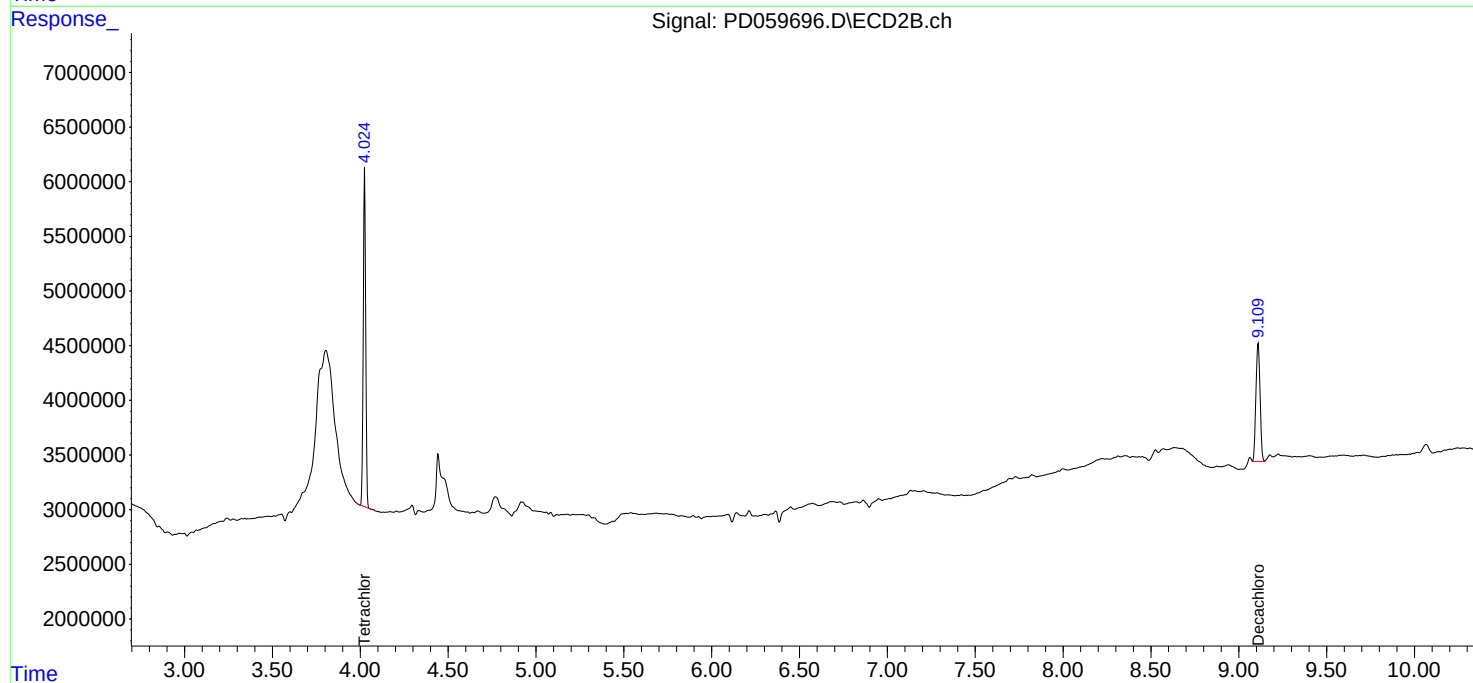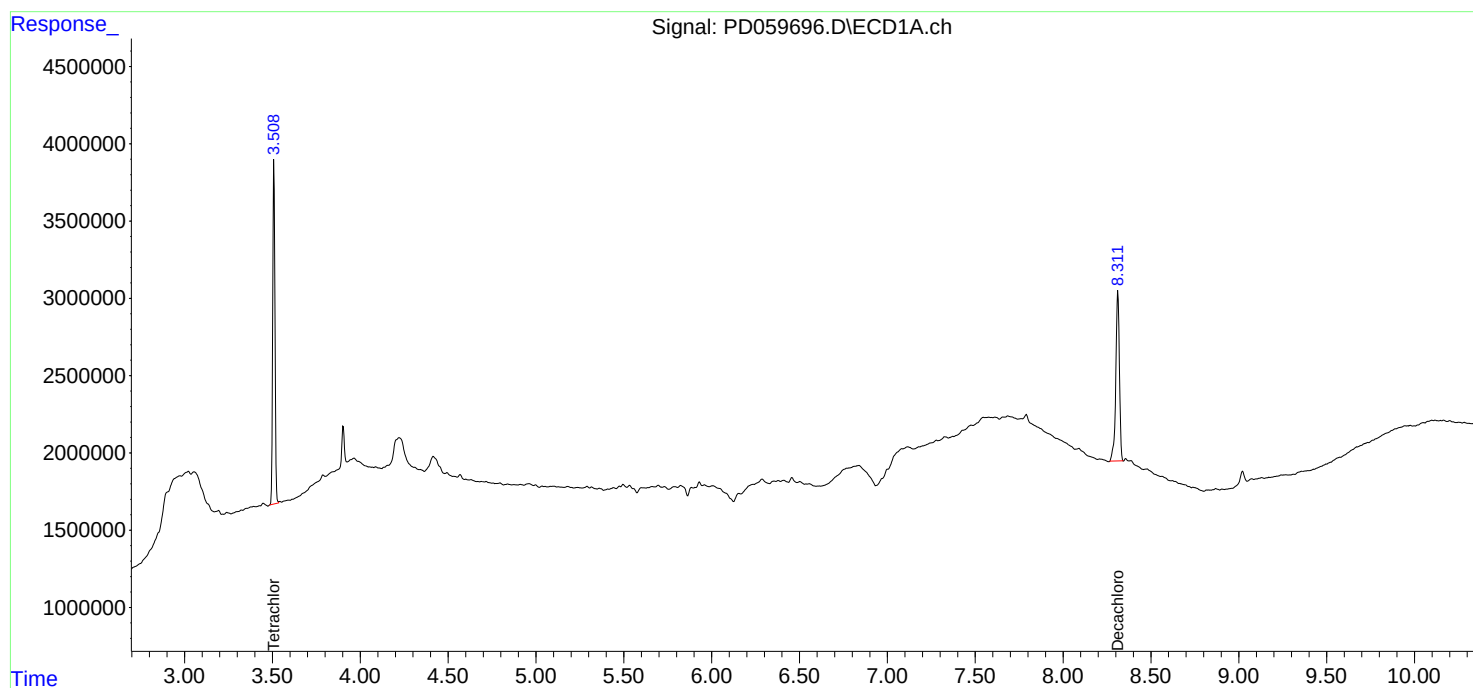

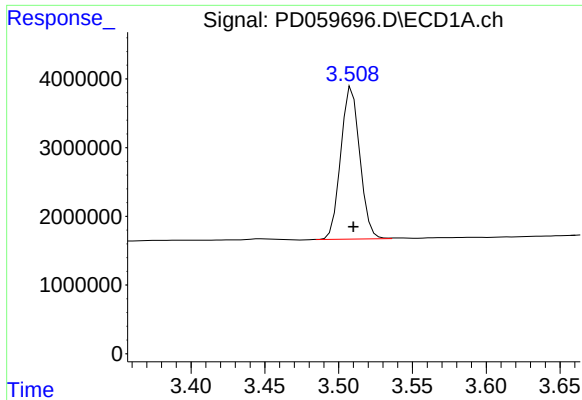


#1 Tetrachloro-m-xylene

R.T.: 3.509 min
Delta R.T.: 0.000 min
Response: 19901877
Conc: 13.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
A-2332-MH12


Manual Integrations
APPROVED

Ankita
10/13/2020 12:26:49 PM

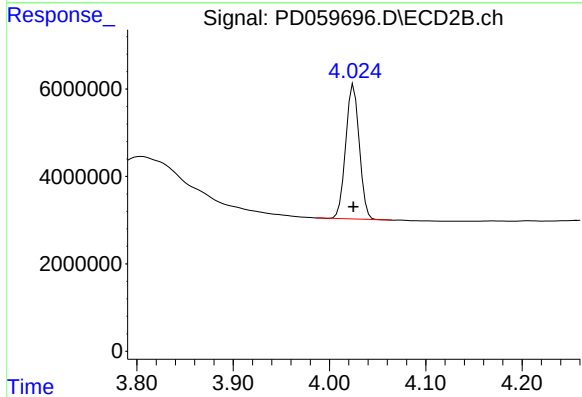


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.000 min
Response: 30018401
Conc: 13.81 ng/ml

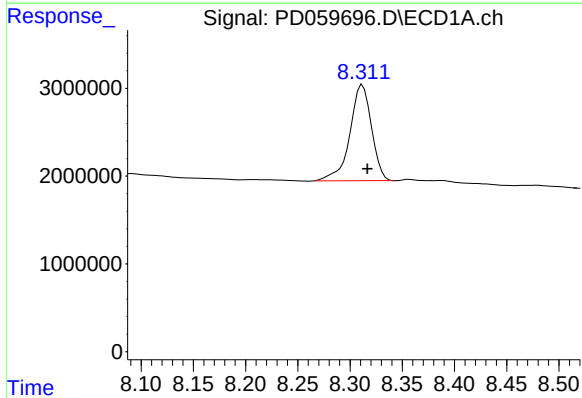

#28 Decachlorobiphenyl

R.T.: 8.311 min
Delta R.T.: -0.006 min
Response: 15746553
Conc: 14.18 ng/ml m

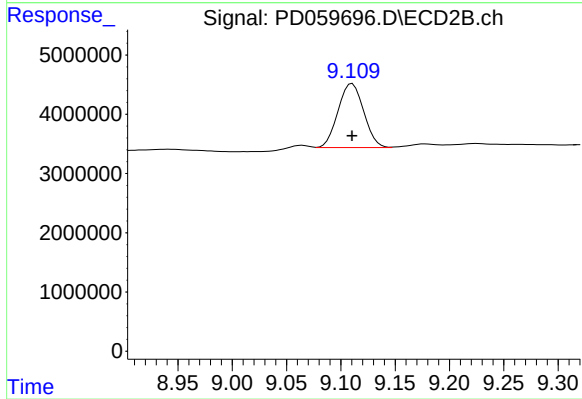

#28 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: -0.001 min
Response: 17714987
Conc: 10.99 ng/ml m